

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068857.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 09:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:21:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.569	8975344	23374553	21.698	23.022
28)	SA Decachlor...	10.405	11.487	12888216	21371881	22.426	22.027
Target Compounds							
3)	MA gamma-BHC...	5.768	0.000	1307665	0	2.409	N.D. #
4)	MA Heptachlor	6.154f	0.000	504345	0	0.859	N.D. #
6)	B beta-BHC	6.154	0.000	504345	0	1.789	N.D. #
8)	B Heptachlo...	0.000	8.036	0	1762874	N.D.	1.525 #
14)	MA Endrin	8.080f	0.000	673907	0	1.398	N.D. #
15)	B Endosulfa...	0.000	9.215	0	771982	N.D.	0.842 #
22)	Mirex	0.000	10.565f	0	220401	N.D.	0.279 #
23)	Chlordane-1	0.000	6.975f	0	1316511	N.D.	31.220 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068857.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 09:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:21:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

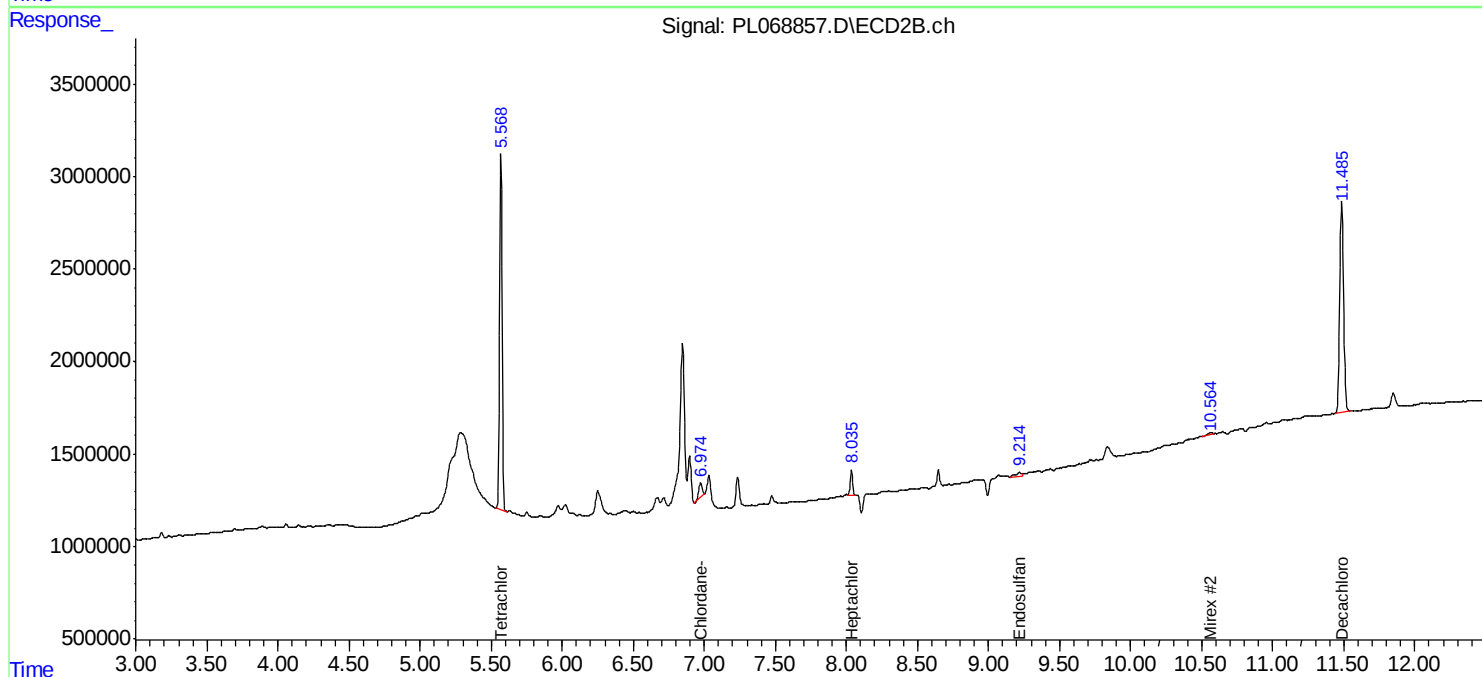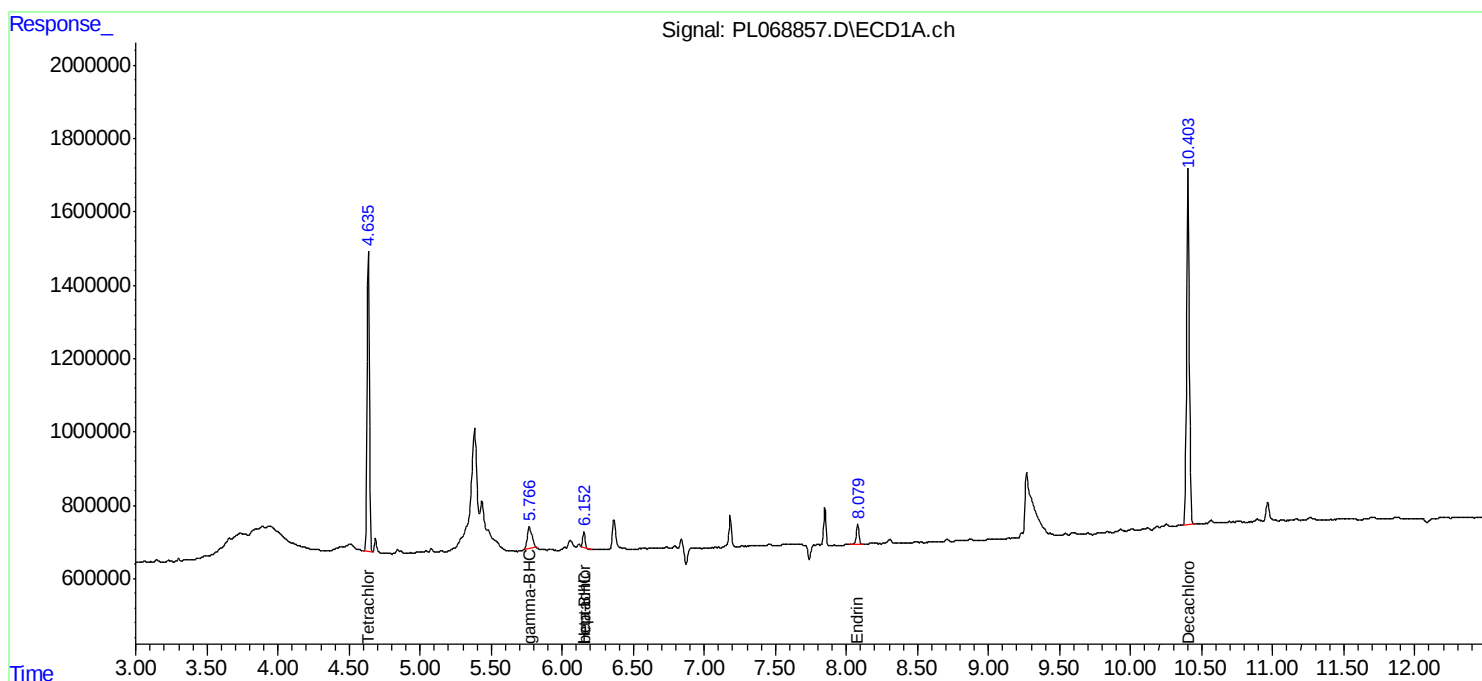


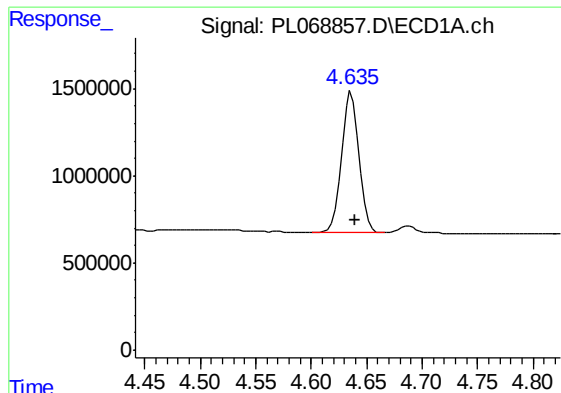

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 8975344
Conc: 21.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

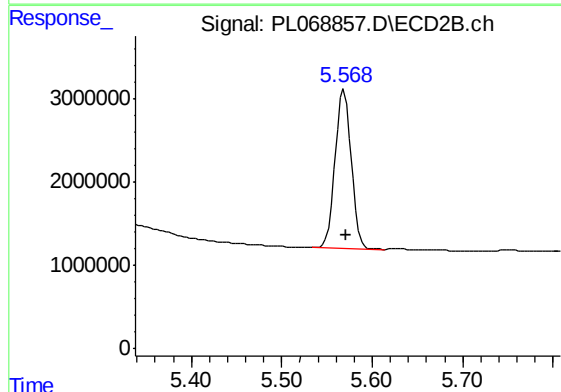


#1 Tetrachloro-m-xylene

R.T.: 5.569 min
Delta R.T.: -0.002 min
Response: 23374553
Conc: 23.02 ng/ml

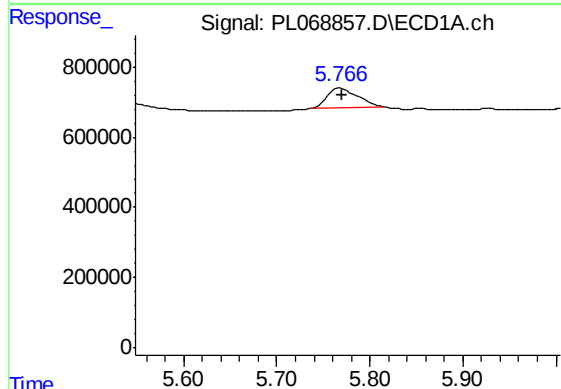


#3 gamma-BHC (Lindane)

R.T.: 5.768 min
Delta R.T.: -0.003 min
Response: 1307665
Conc: 2.41 ng/ml

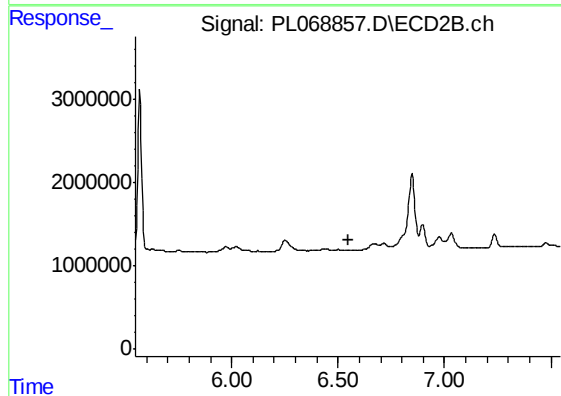

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.547 min
Response: 0
Conc: N.D.

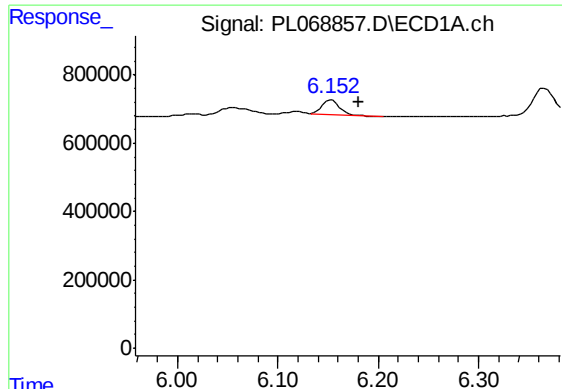

#4 Heptachlor


R.T.: 6.154 min
Delta R.T.: -0.027 min
Response: 504345
Conc: 0.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

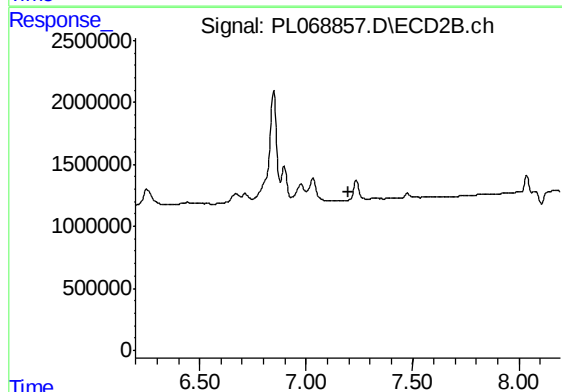


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 7.197 min
Response: 0
Conc: N.D.

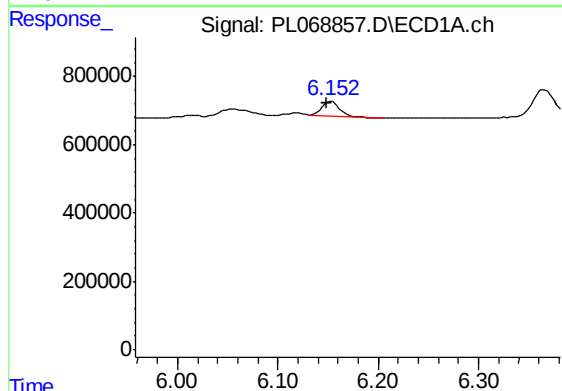


#6 beta-BHC

R.T.: 6.154 min
Delta R.T.: 0.005 min
Response: 504345
Conc: 1.79 ng/ml

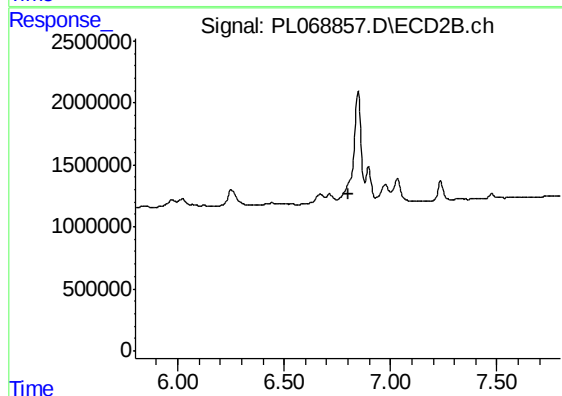

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

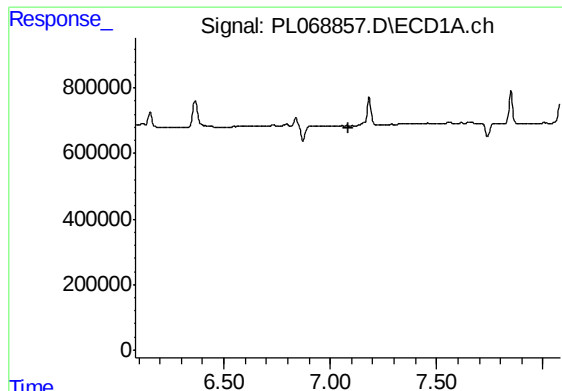

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

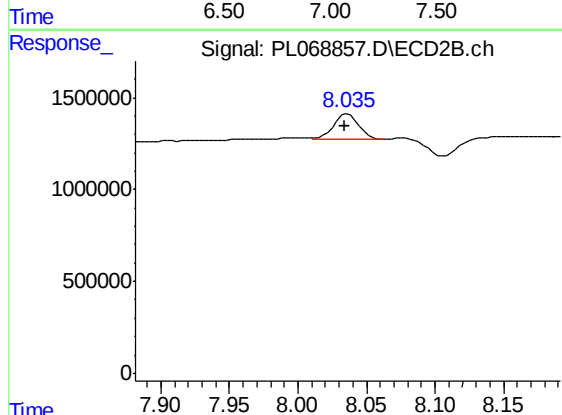


#8 Heptachlor epoxide

R.T.: 8.036 min
Delta R.T.: 0.002 min
Response: 1762874
Conc: 1.52 ng/ml

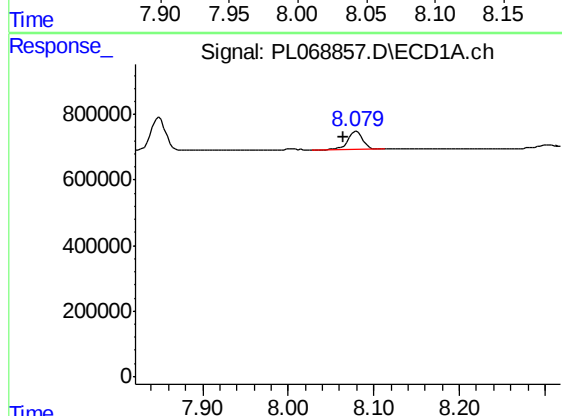


#14 Endrin

R.T.: 8.080 min
Delta R.T.: 0.016 min
Response: 673907
Conc: 1.40 ng/ml

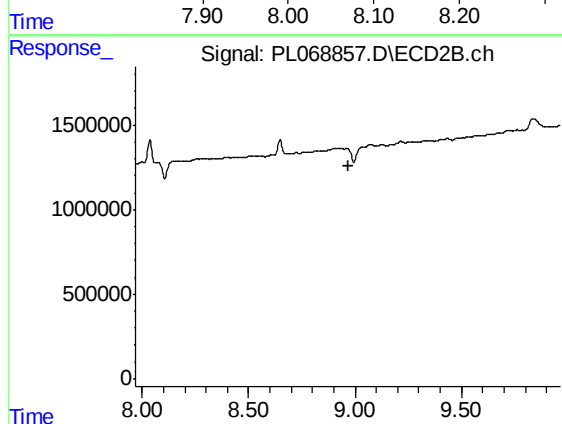

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

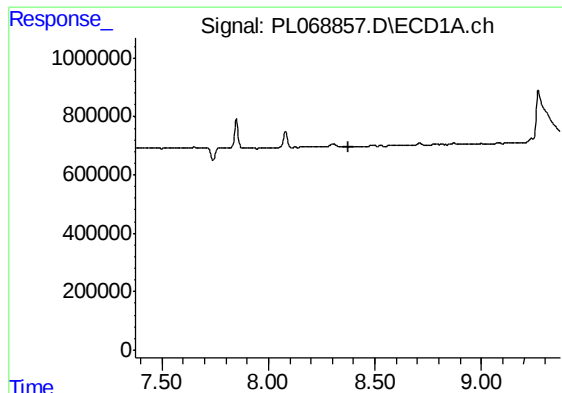

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

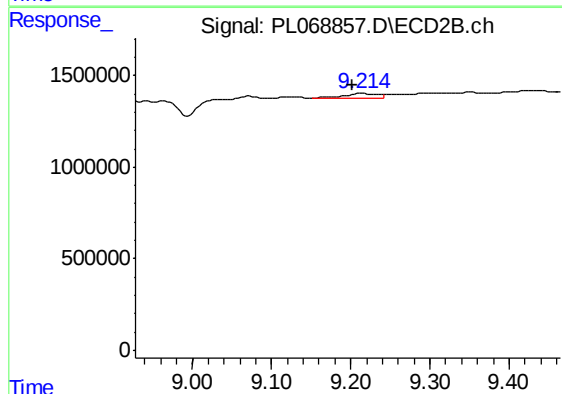


#15 Endosulfan II

R.T.: 9.215 min
Delta R.T.: 0.014 min
Response: 771982
Conc: 0.84 ng/ml

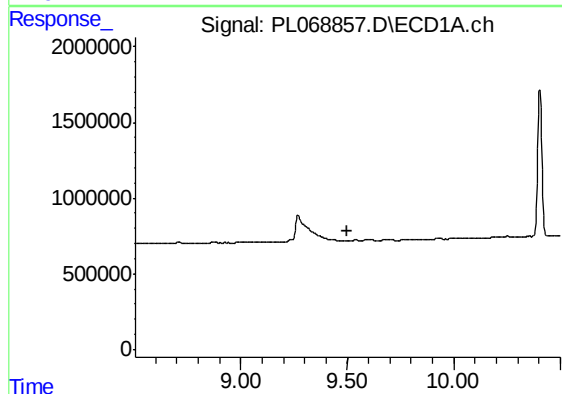


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

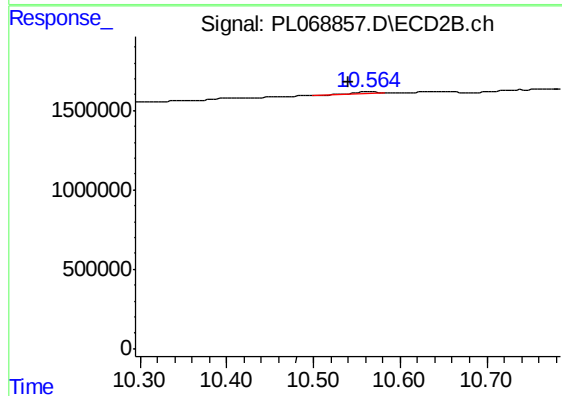

#22 Mirex


R.T.: 10.565 min
Delta R.T.: 0.025 min
Response: 220401
Conc: 0.28 ng/ml

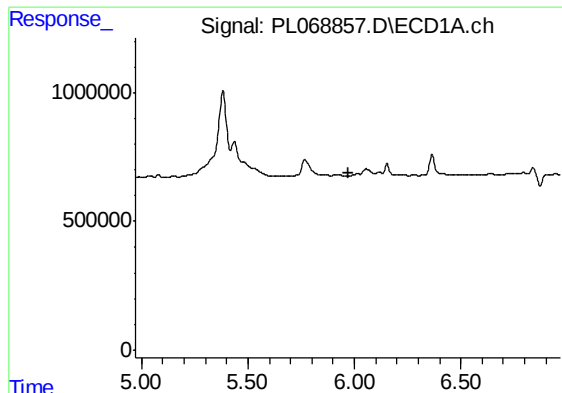

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

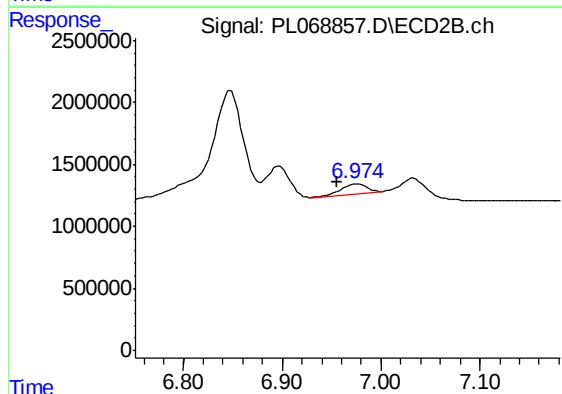


#23 Chlordane-1

R.T.: 6.975 min
Delta R.T.: 0.019 min
Response: 1316511
Conc: 31.22 ng/ml

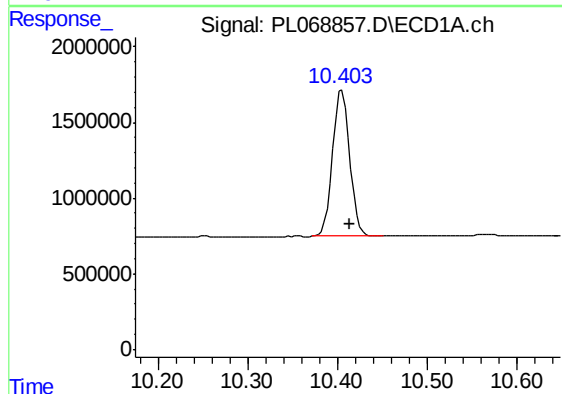

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.009 min
Response: 12888216
Conc: 22.43 ng/ml

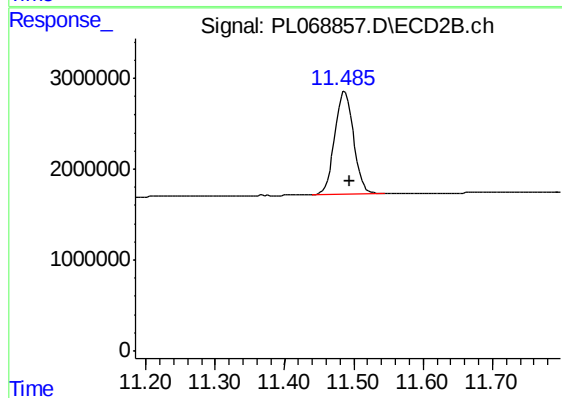

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 21371881
Conc: 22.03 ng/ml