

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 14:59
 Operator : AR\AJ
 Sample : M3333-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124055

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:28:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	7304934	19851652	17.660	19.552
28)	SA Decachlor...	10.406	11.487	8568379	14967521	14.909	15.427
Target Compounds							
2)	A alpha-BHC	0.000	6.181f	0	291527	N.D.	0.214 #
10)	B gamma-Chl...	0.000	8.297	0	456029	N.D.	0.398 #
11)	B alpha-Chl...	0.000	8.381	0	625563	N.D.	0.545 #
13)	MA Dieldrin	0.000	8.725	0	392688	N.D.	0.362 #
15)	B Endosulfa...	0.000	9.213	0	430507	N.D.	0.469 #
22)	Mirex	0.000	10.566f	0	191758	N.D.	0.242 #
23)	Chlordane-1	0.000	6.973f	0	248870	N.D.	5.902 #
25)	Chlordane-3	0.000	8.297	0	456029	N.D.	2.792 #
26)	Chlordane-4	0.000	8.381	0	625563	N.D.	3.154 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 14:59
Operator : AR\AJ
Sample : M3333-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
124055

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:28:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

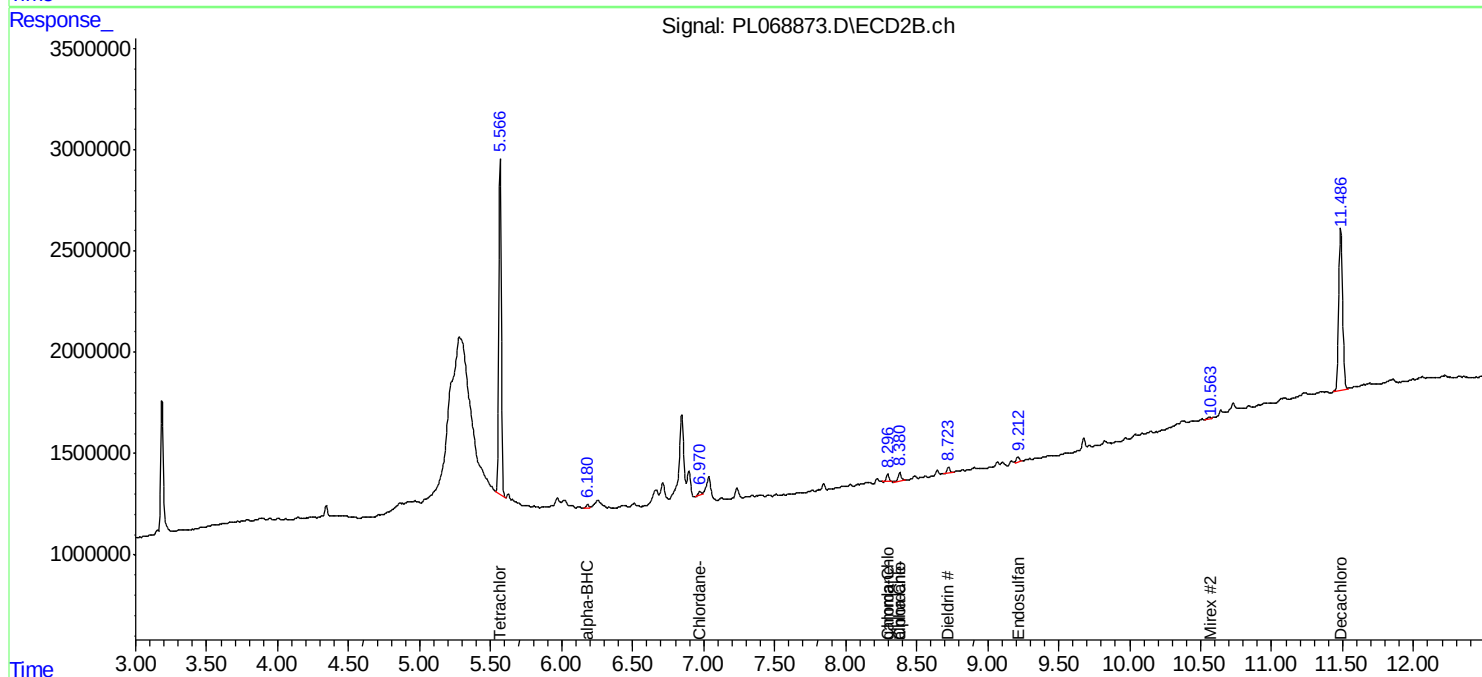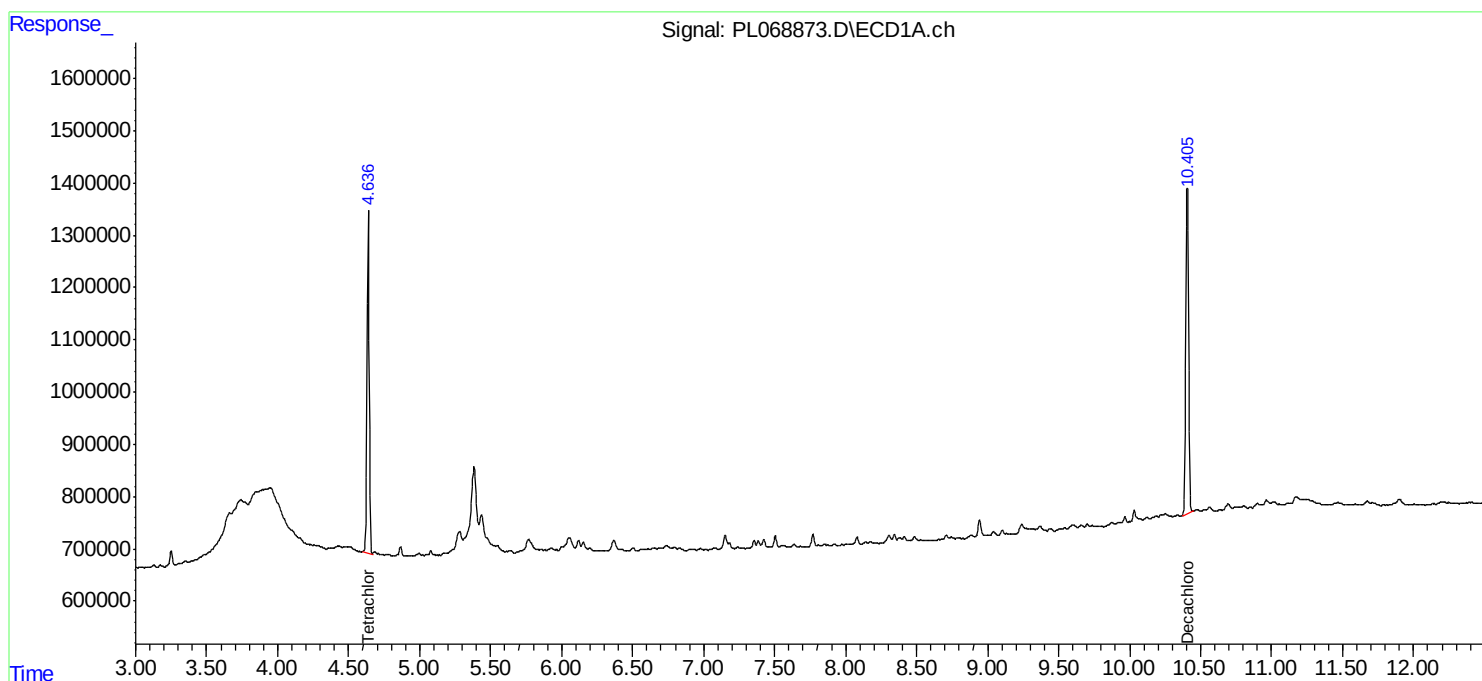


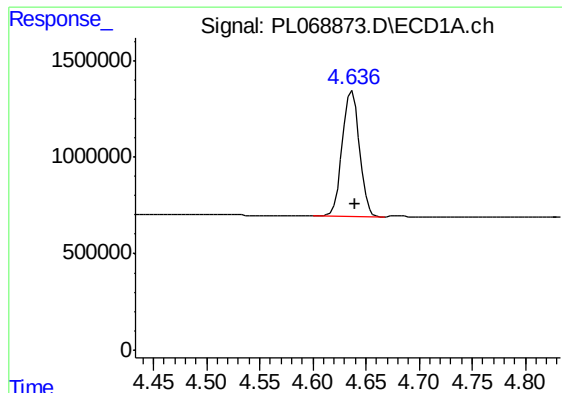

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 7304934
Conc: 17.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
124055

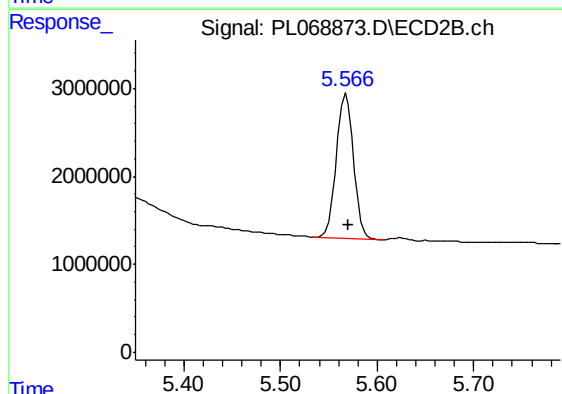


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 19851652
Conc: 19.55 ng/ml

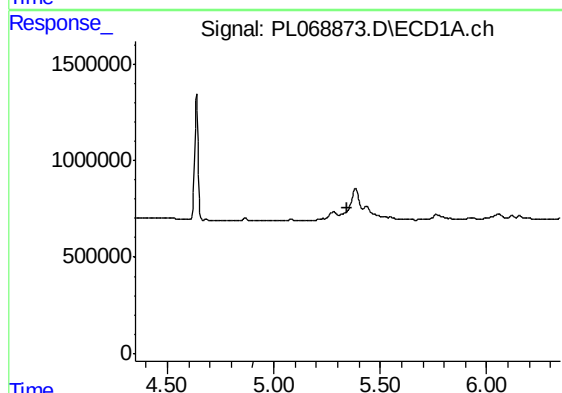


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

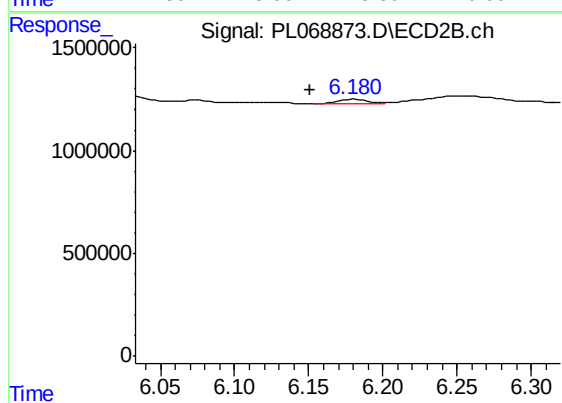

#2 alpha-BHC


R.T.: 6.181 min
Delta R.T.: 0.030 min
Response: 291527
Conc: 0.21 ng/ml

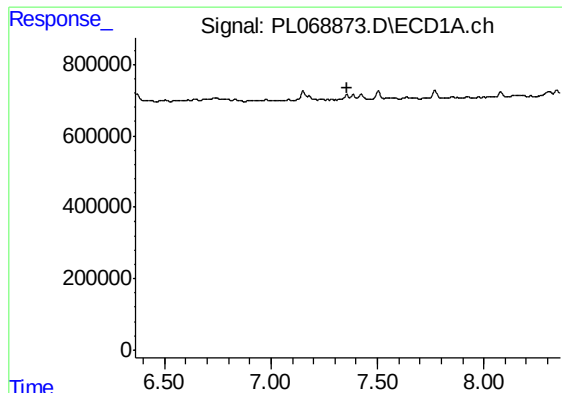

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
124055

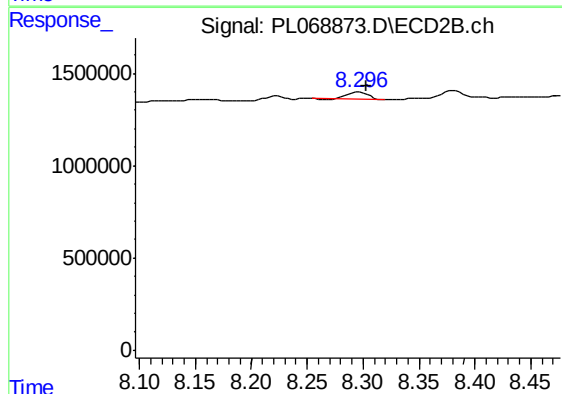


#10 gamma-Chlordane

R.T.: 8.297 min
Delta R.T.: -0.006 min
Response: 456029
Conc: 0.40 ng/ml

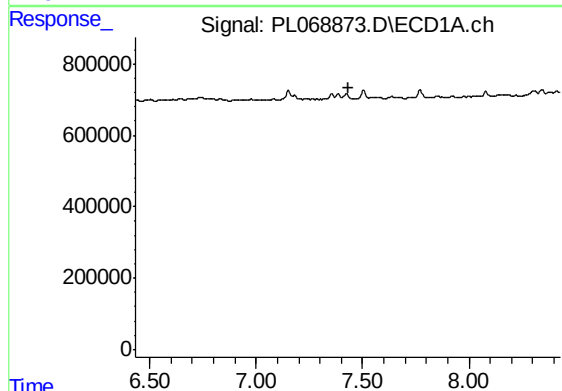


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

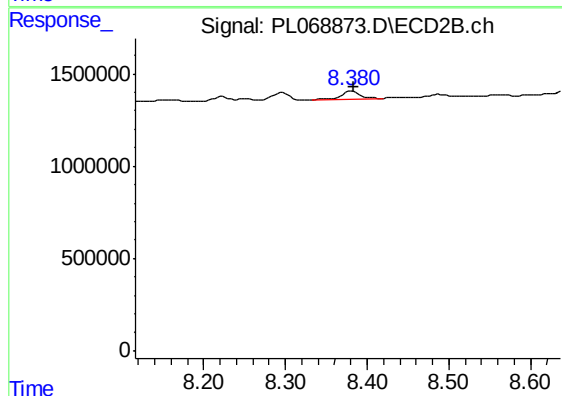

#11 alpha-Chlordane


R.T.: 8.381 min
Delta R.T.: -0.003 min
Response: 625563
Conc: 0.54 ng/ml

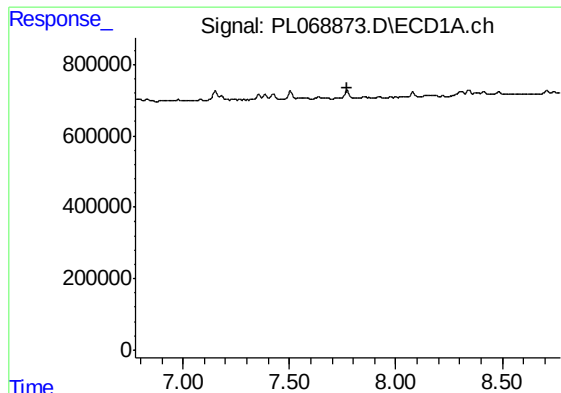

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
124055

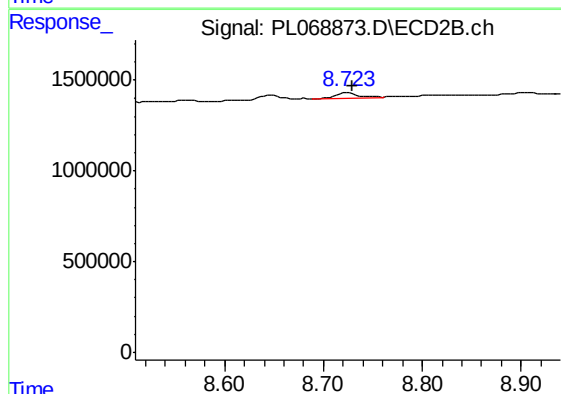


#13 Dielldrin

R.T.: 8.725 min
Delta R.T.: -0.004 min
Response: 392688
Conc: 0.36 ng/ml

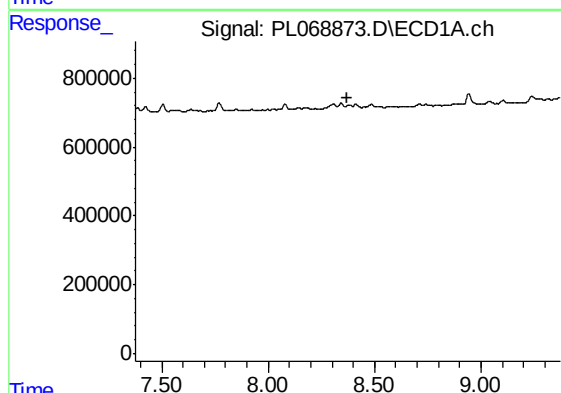


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

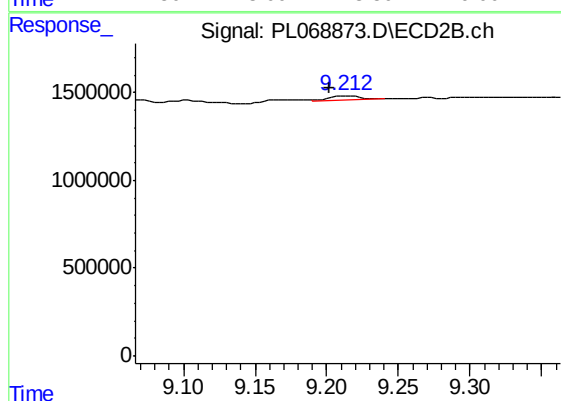

#15 Endosulfan II


R.T.: 9.213 min
Delta R.T.: 0.012 min
Response: 430507
Conc: 0.47 ng/ml

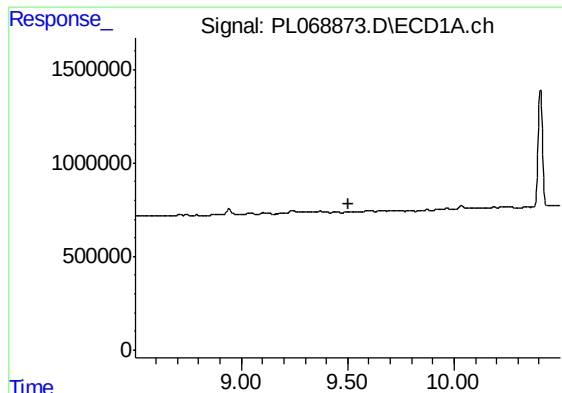

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
124055

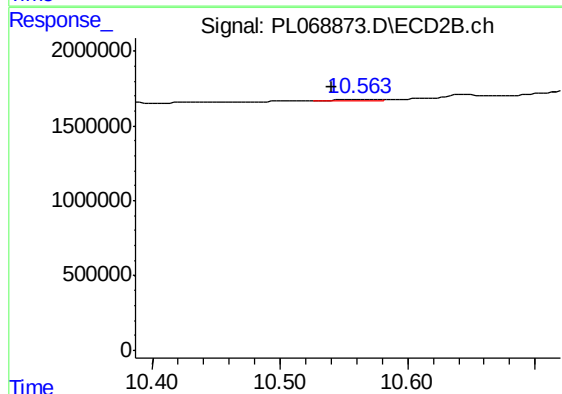


#22 Mirex

R.T.: 10.566 min
Delta R.T.: 0.026 min
Response: 191758
Conc: 0.24 ng/ml

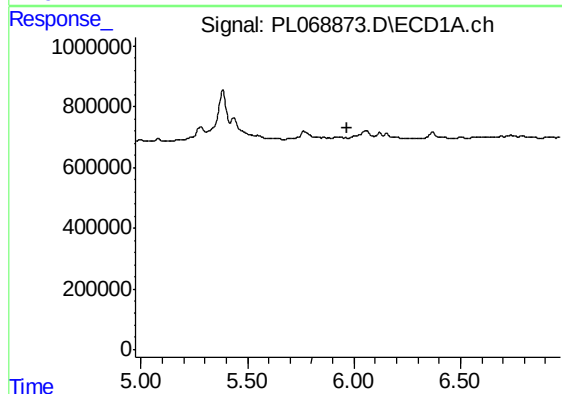


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

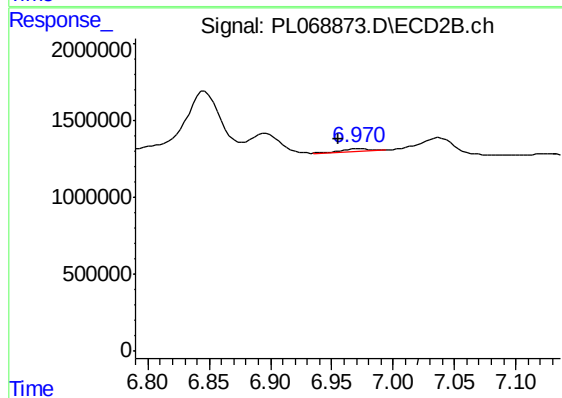

#23 Chlordane-1


R.T.: 6.973 min
Delta R.T.: 0.017 min
Response: 248870
Conc: 5.90 ng/ml

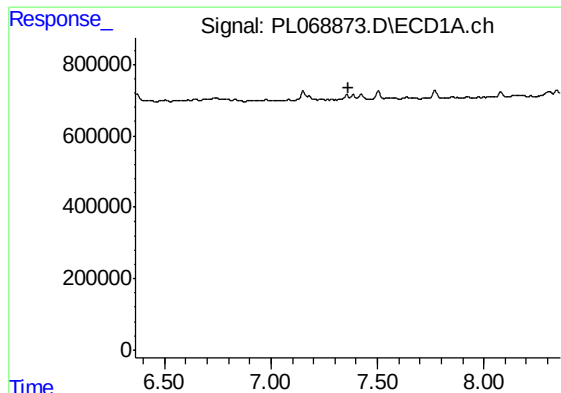

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
124055

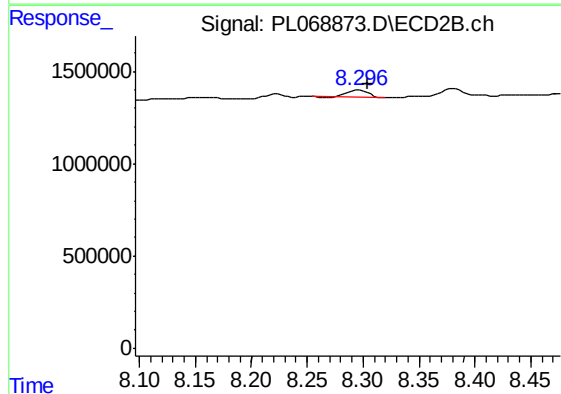


#25 Chlordane-3

R.T.: 8.297 min
Delta R.T.: -0.007 min
Response: 456029
Conc: 2.79 ng/ml

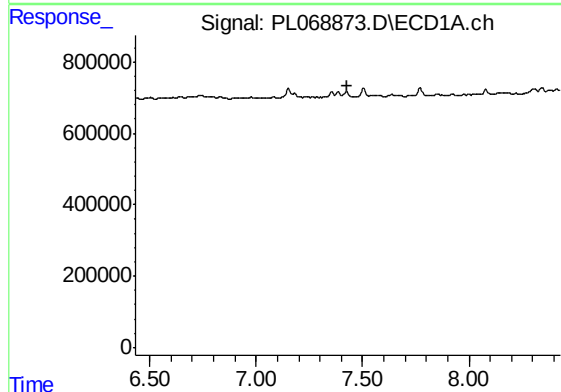


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.430 min
Response: 0
Conc: N.D.

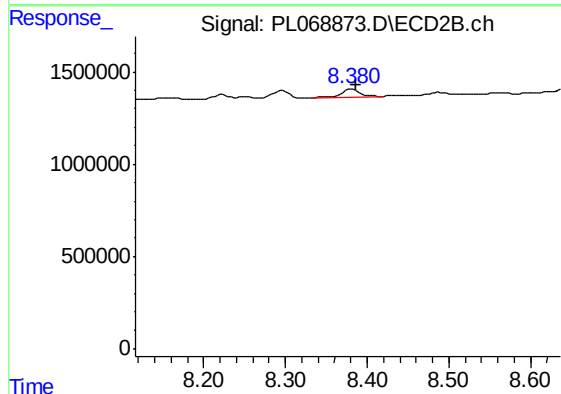

#26 Chlordane-4


R.T.: 8.381 min
Delta R.T.: -0.006 min
Response: 625563
Conc: 3.15 ng/ml

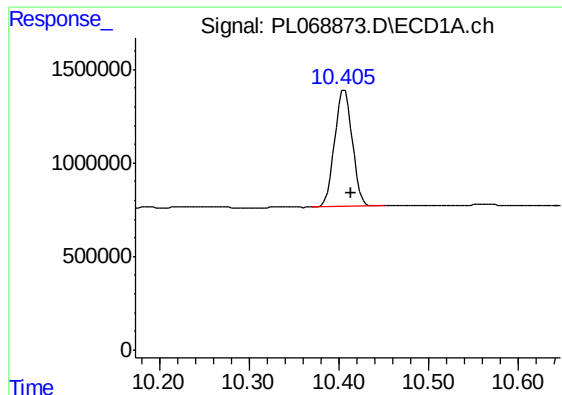

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.008 min
Response: 8568379
Conc: 14.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
124055

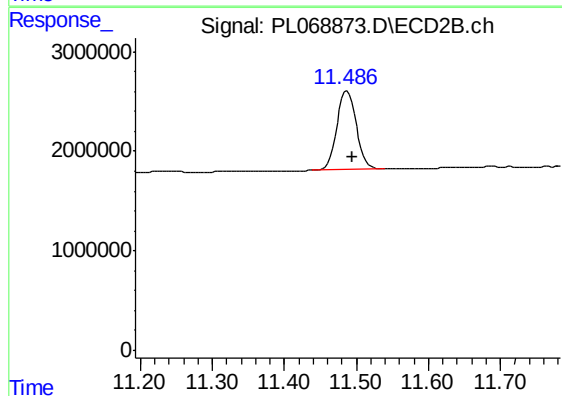

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 14967521
Conc: 15.43 ng/ml