

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 15:32
 Operator : AR\AJ
 Sample : PB138308BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB138308BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:28:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	8718303	24070189	21.077	23.707
28)	SA Decachlor...	10.405	11.487	12354360	21498730	21.497	22.158
Target Compounds							
8)	B Heptachlo...	0.000	8.035	0	3233046	N.D.	2.797 #
13)	MA Dieldrin	7.769	0.000	11654	0	0.023	N.D. #
14)	MA Endrin	8.081f	0.000	4686670	0	9.725	N.D. #
15)	B Endosulfa...	0.000	9.213	0	385524	N.D.	0.420 #
17)	MA 4,4'-DDT	0.000	9.430	0	363405	N.D.	0.384 #
21)	B Endrin ke...	0.000	10.086	0	226097	N.D.	0.222 #
22)	Mirex	0.000	10.563f	0	579548	N.D.	0.733 #
23)	Chlordane-1	0.000	6.978f	0	197697	N.D.	4.688 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 15:32
Operator : AR\AJ
Sample : PB138308BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB138308BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:28:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

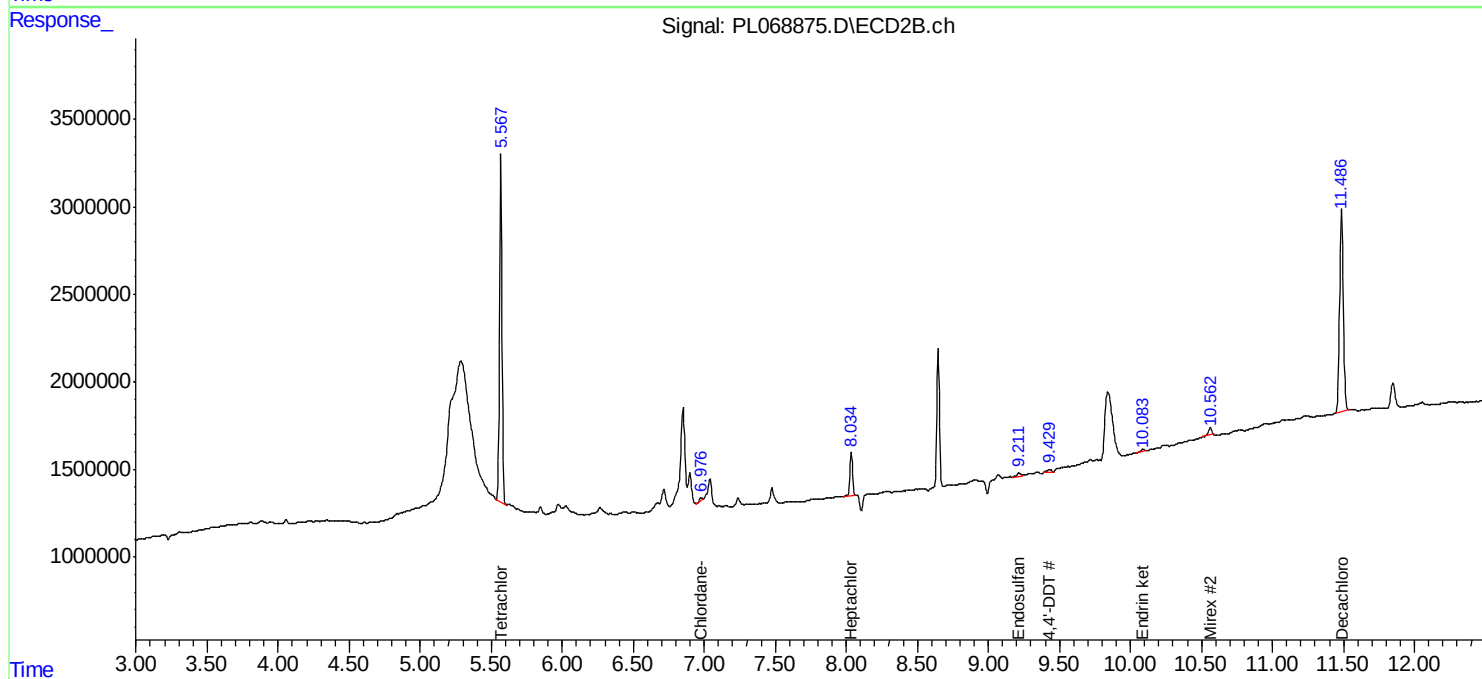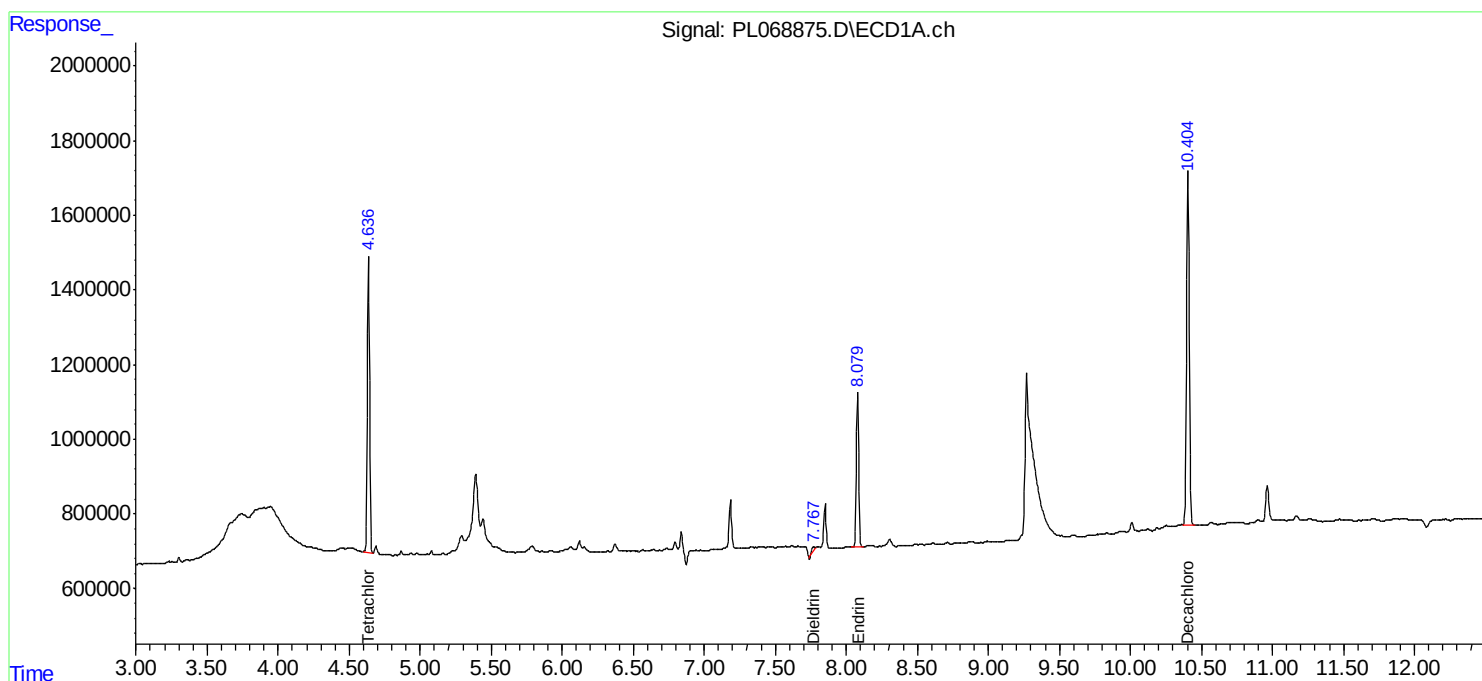


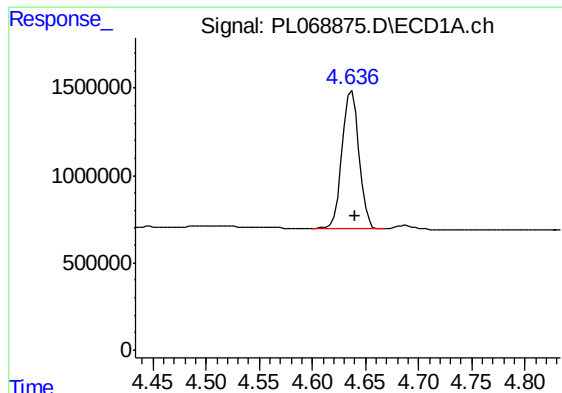

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 8718303
Conc: 21.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138308BL

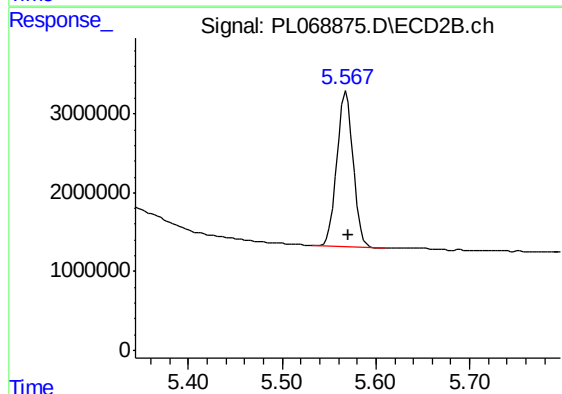


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 24070189
Conc: 23.71 ng/ml

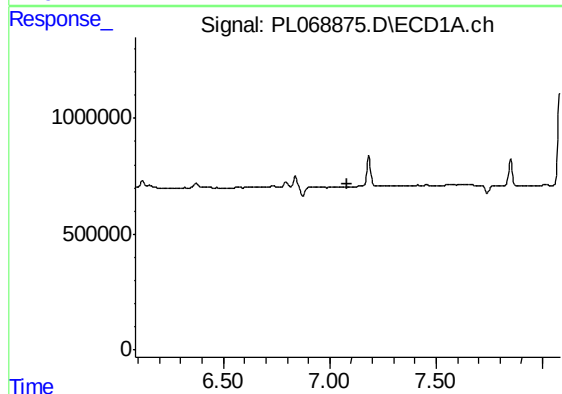


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

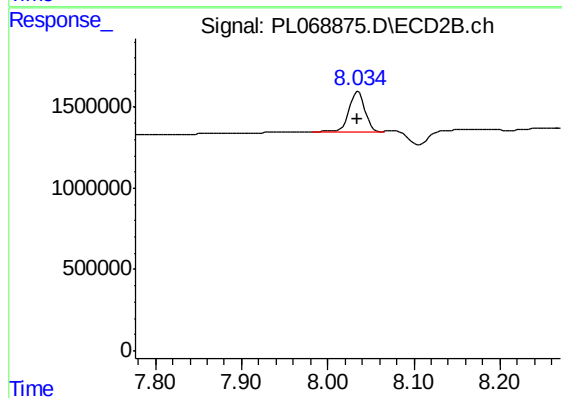

#8 Heptachlor epoxide


R.T.: 8.035 min
Delta R.T.: 0.001 min
Response: 3233046
Conc: 2.80 ng/ml

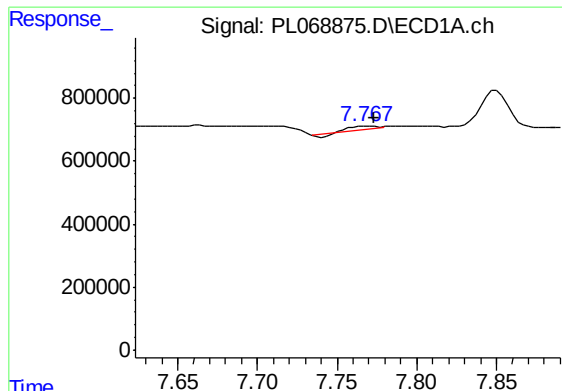

#13 Dielddrin


R.T.: 7.769 min
Delta R.T.: -0.004 min
Response: 11654
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB138308BL

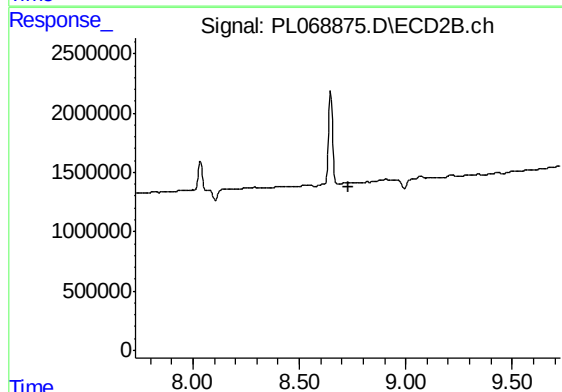


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 8.729 min
Response: 0
Conc: N.D.

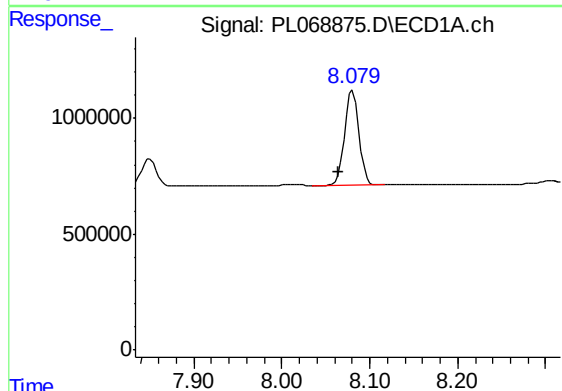


#14 Endrin

R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 4686670
Conc: 9.72 ng/ml

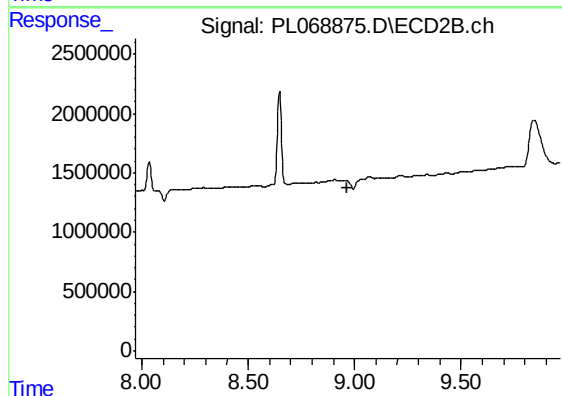

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

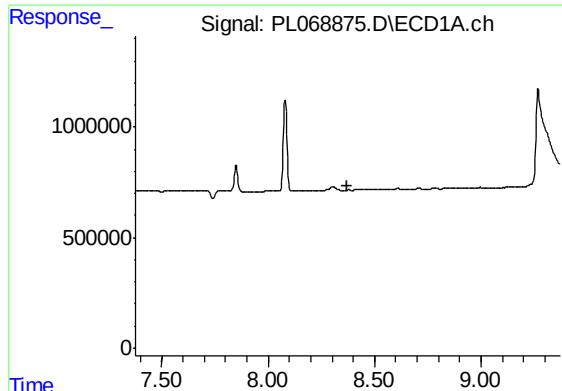

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138308BL

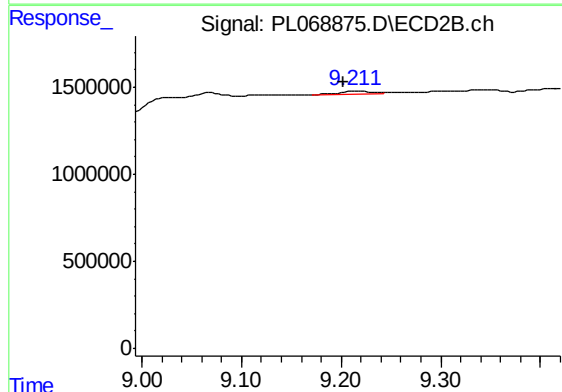


#15 Endosulfan II

R.T.: 9.213 min
Delta R.T.: 0.011 min
Response: 385524
Conc: 0.42 ng/ml

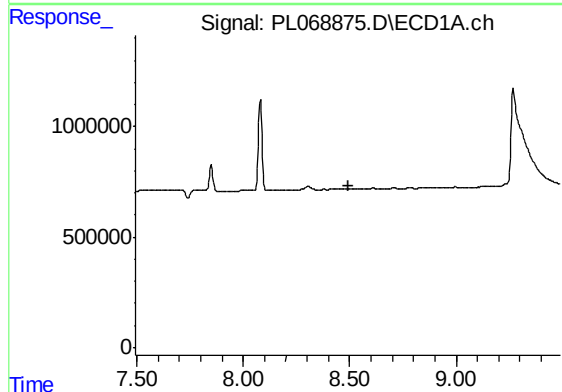


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.492 min
Response: 0
Conc: N.D.

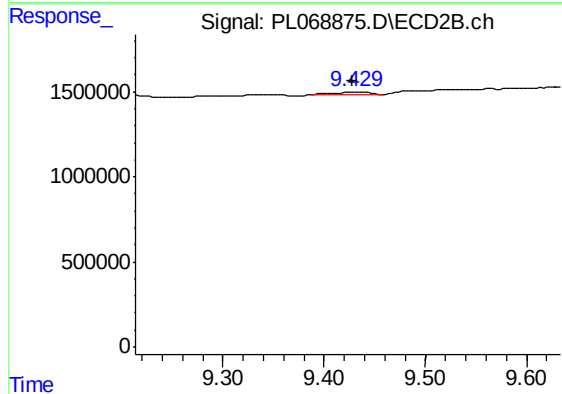

#17 4,4'-DDT


R.T.: 9.430 min
Delta R.T.: 0.002 min
Response: 363405
Conc: 0.38 ng/ml

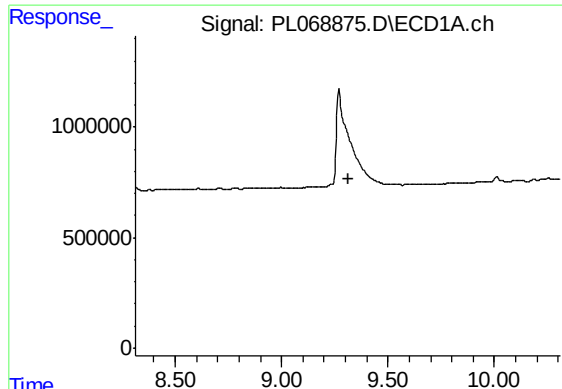

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138308BL

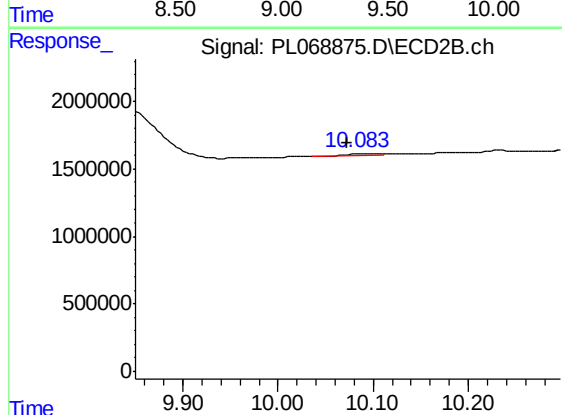


#21 Endrin ketone

R.T.: 10.086 min
Delta R.T.: 0.014 min
Response: 226097
Conc: 0.22 ng/ml

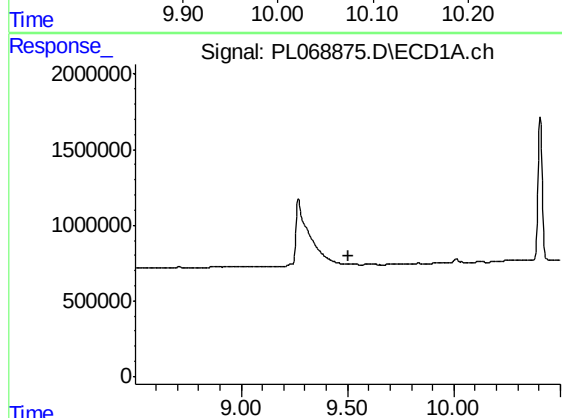


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 9.502 min
Response: 0
Conc: N.D.

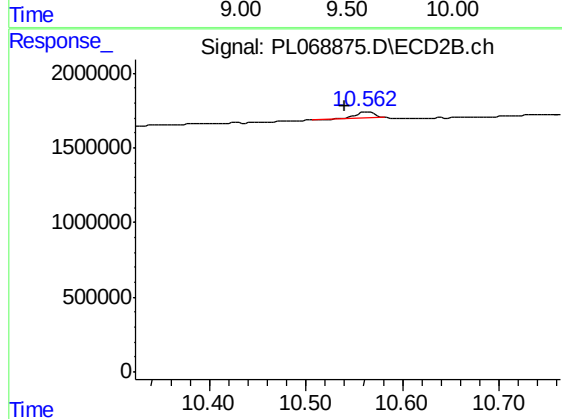

#22 Mirex


R.T.: 10.563 min
Delta R.T.: 0.023 min
Response: 579548
Conc: 0.73 ng/ml

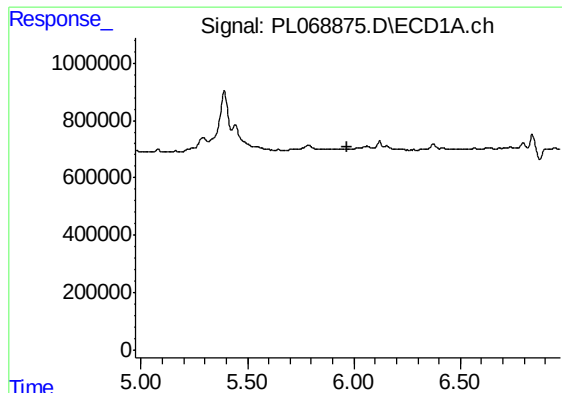

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB138308BL

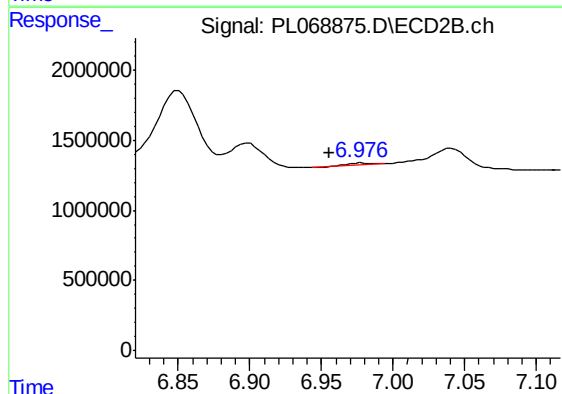


#23 Chlordane-1

R.T.: 6.978 min
Delta R.T.: 0.022 min
Response: 197697
Conc: 4.69 ng/ml

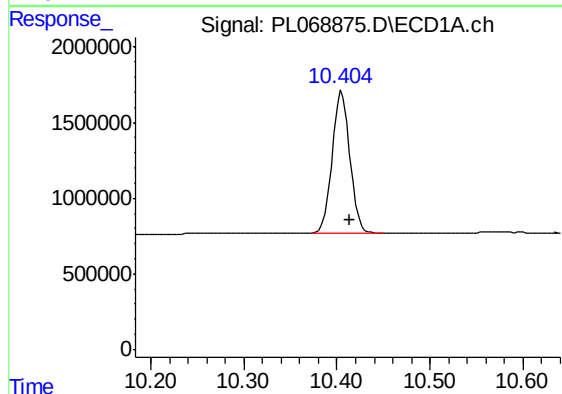

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.008 min
Response: 12354360
Conc: 21.50 ng/ml

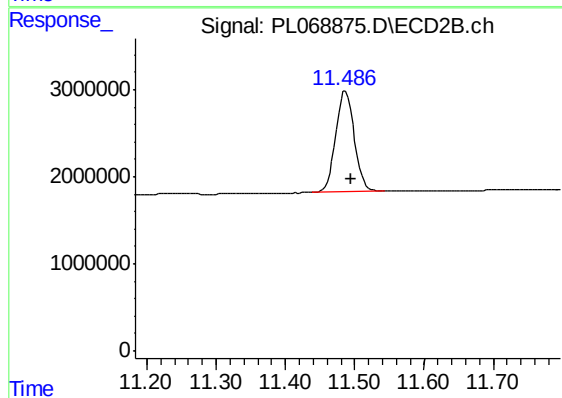

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.008 min
Response: 21498730
Conc: 22.16 ng/ml