

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 19:32
 Operator : AR\AJ
 Sample : M3331-13
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BSY1-WC-S-10-14-0-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:33:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	9008805	26216461	21.779	25.820
28)	SA Decachlor...	10.405	11.487	12769883	22516482	22.220	23.207
Target Compounds							
6)	B beta-BHC	6.119f	0.000	660831	0	2.344	N.D. #
7)	B delta-BHC	0.000	7.042f	0	91955	N.D.	0.073 #
11)	B alpha-Chl...	0.000	8.396	0	77304	N.D.	0.067 #
13)	MA Dieldrin	0.000	8.724	0	111027	N.D.	0.102 #
15)	B Endosulfa...	0.000	9.215	0	2123047	N.D.	2.315 #
21)	B Endrin ke...	0.000	10.090f	0	373922	N.D.	0.367 #
23)	Chlordane-1	0.000	6.975f	0	354816	N.D.	8.414 #
26)	Chlordane-4	0.000	8.396	0	77304	N.D.	0.390 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 19:32
Operator : AR\AJ
Sample : M3331-13
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:33:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

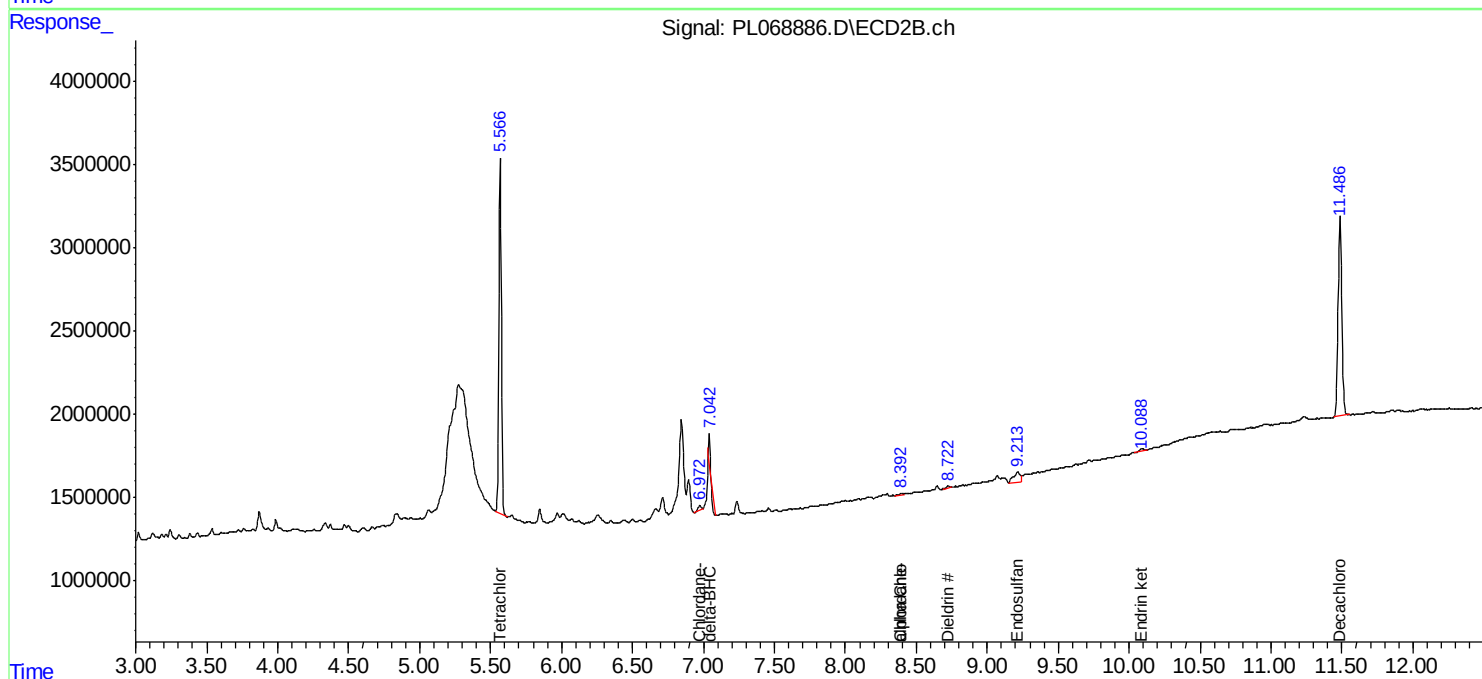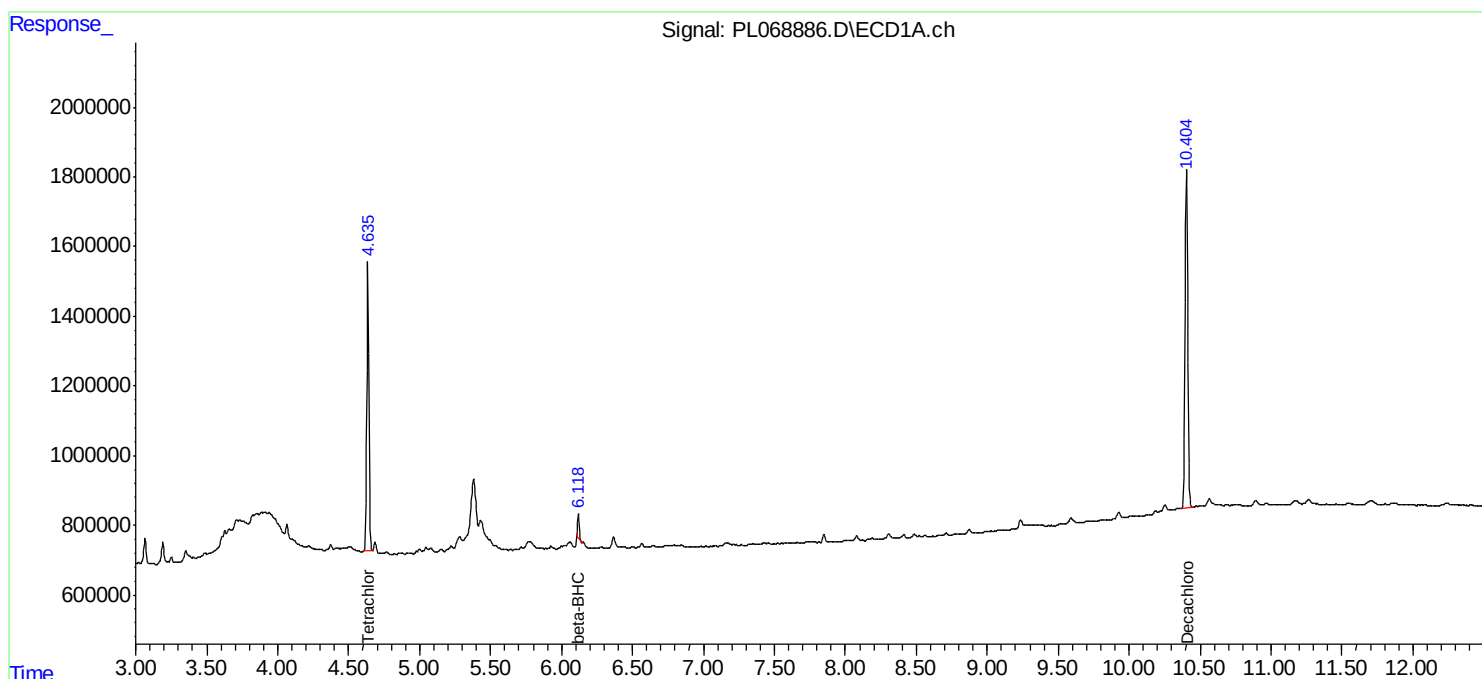


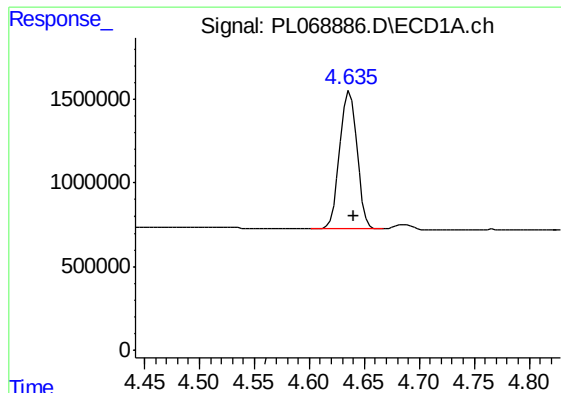

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 9008805
Conc: 21.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

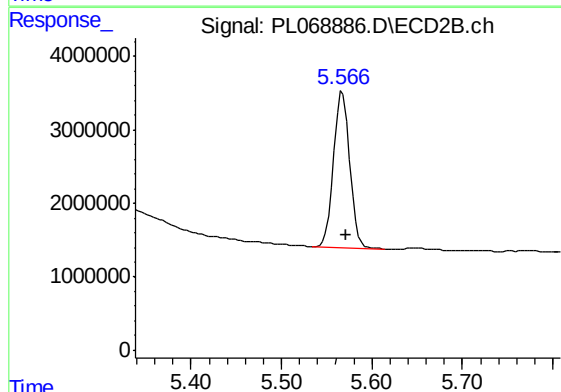


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 26216461
Conc: 25.82 ng/ml

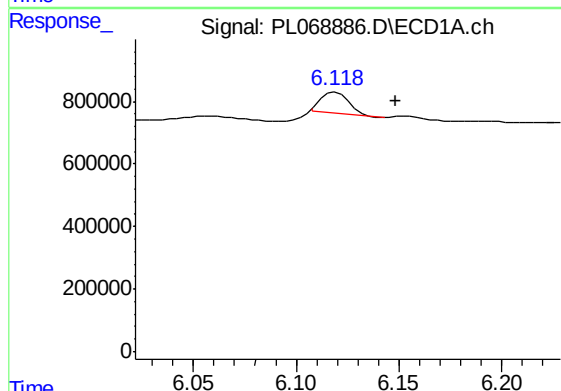


#6 beta-BHC

R.T.: 6.119 min
Delta R.T.: -0.029 min
Response: 660831
Conc: 2.34 ng/ml

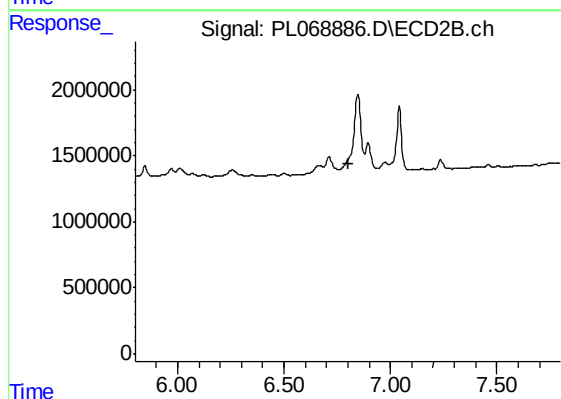

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 6.800 min
Response: 0
Conc: N.D.

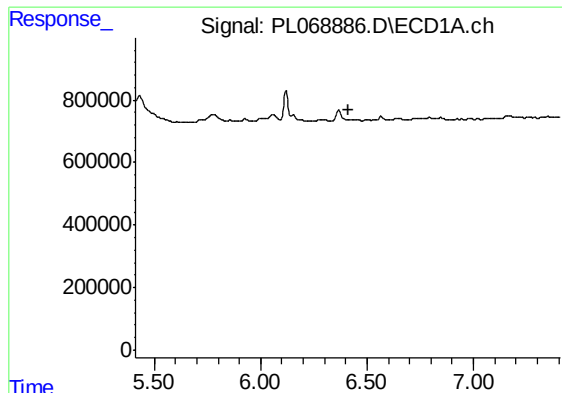

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

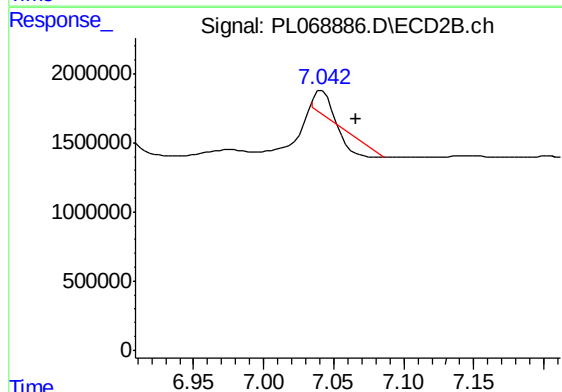


#7 delta-BHC

R.T.: 7.042 min
Delta R.T.: -0.024 min
Response: 91955
Conc: 0.07 ng/ml

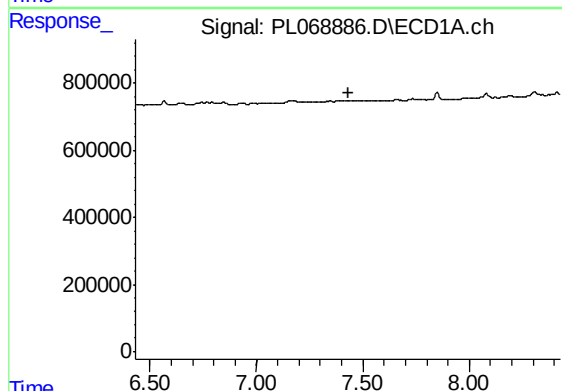


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.432 min
Response: 0
Conc: N.D.

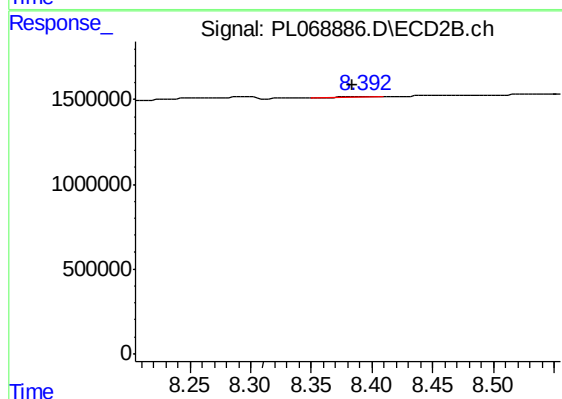

#11 alpha-Chlordane


R.T.: 8.396 min
Delta R.T.: 0.011 min
Response: 77304
Conc: 0.07 ng/ml

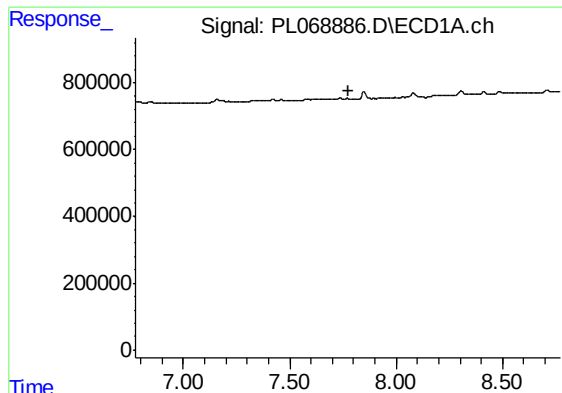

#13 Dielldrin


R.T.: 0.000 min
Exp R.T. : 7.774 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

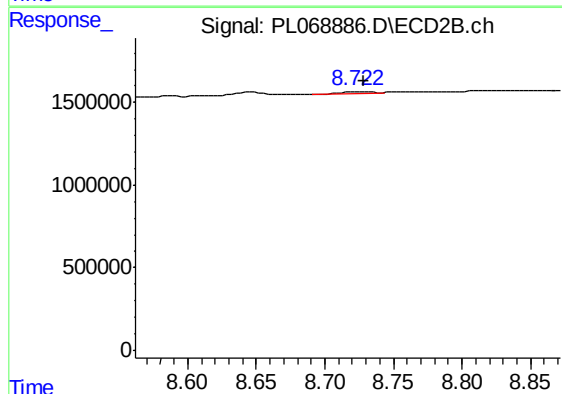


#13 Dielldrin

R.T.: 8.724 min
Delta R.T.: -0.004 min
Response: 111027
Conc: 0.10 ng/ml

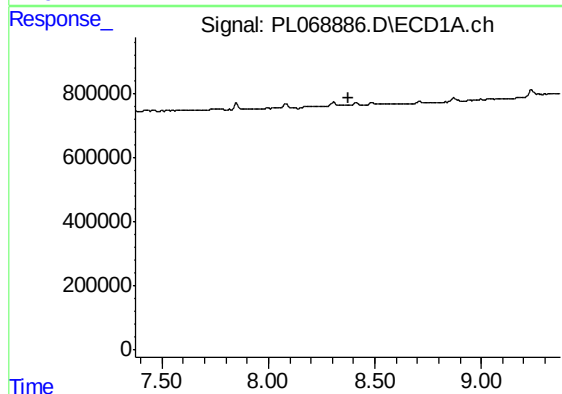


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

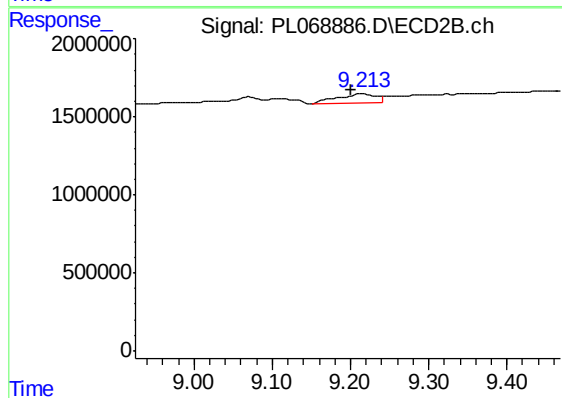

#15 Endosulfan II


R.T.: 9.215 min
Delta R.T.: 0.013 min
Response: 2123047
Conc: 2.31 ng/ml

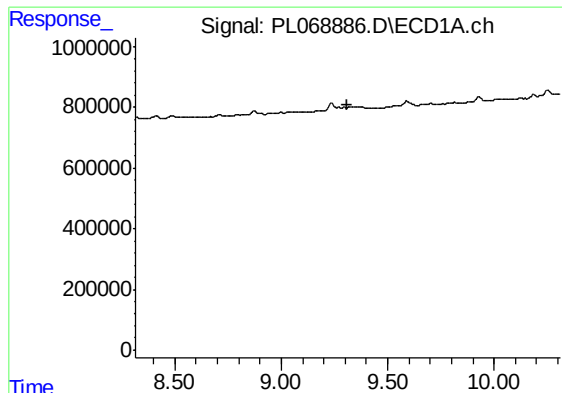

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 9.313 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

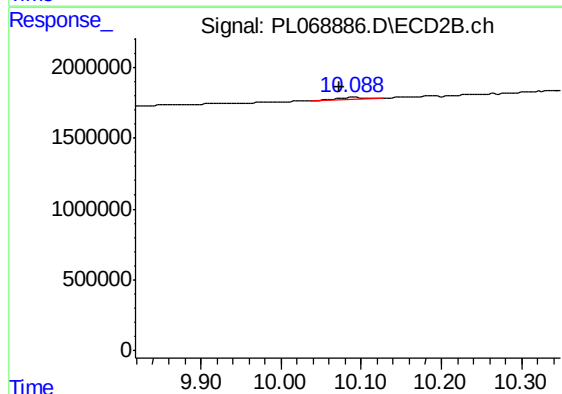


#21 Endrin ketone

R.T.: 10.090 min
Delta R.T.: 0.018 min
Response: 373922
Conc: 0.37 ng/ml

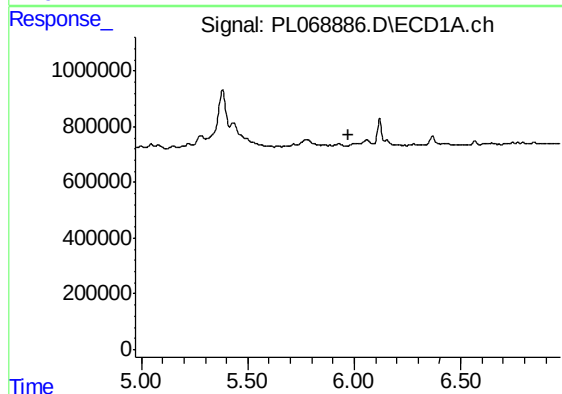


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

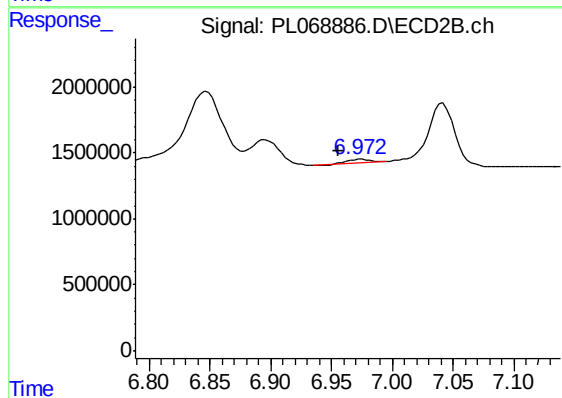

#23 Chlordane-1


R.T.: 6.975 min
Delta R.T.: 0.019 min
Response: 354816
Conc: 8.41 ng/ml

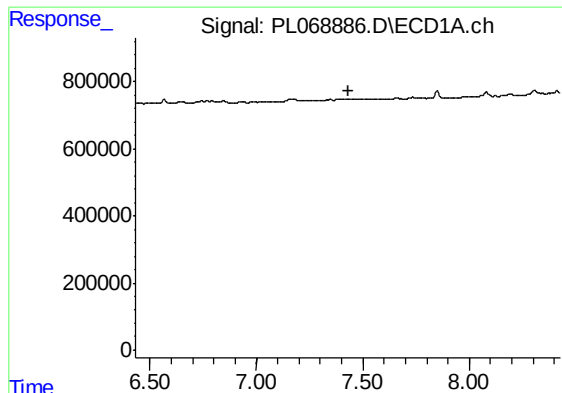

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BSY1-WC-S-10-14-0-10

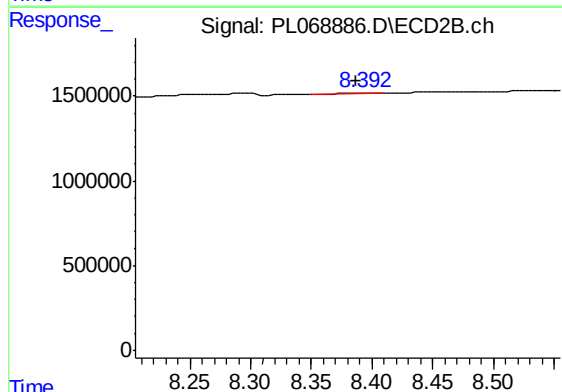


#26 Chlordane-4

R.T.: 8.396 min
Delta R.T.: 0.009 min
Response: 77304
Conc: 0.39 ng/ml

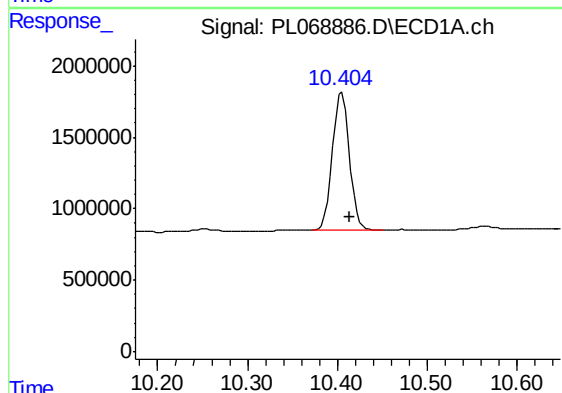

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.008 min
Response: 12769883
Conc: 22.22 ng/ml

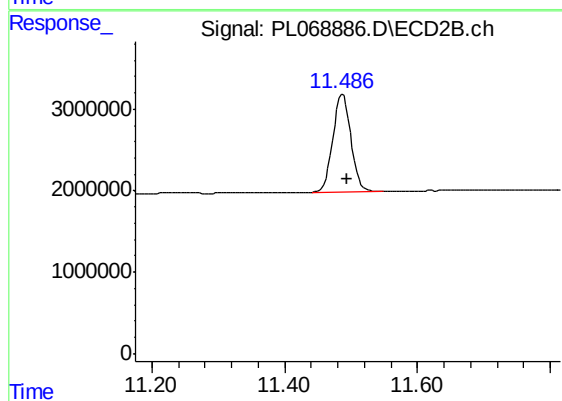

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 22516482
Conc: 23.21 ng/ml