

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068870.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 14:05
 Operator : AR\AJ
 Sample : M3328-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210566-COM-39

Manual Integrations
 APPROVED

Ankita
 8/11/2021 2:08:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:27:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.566	8374936	24199977	20.247m	23.834
28)	SA Decachlor...	10.412	11.492	10955249	19191626	19.063	19.780

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068870.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 14:05
Operator : AR\AJ
Sample : M3328-04
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
20210566-COM-39


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:27:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

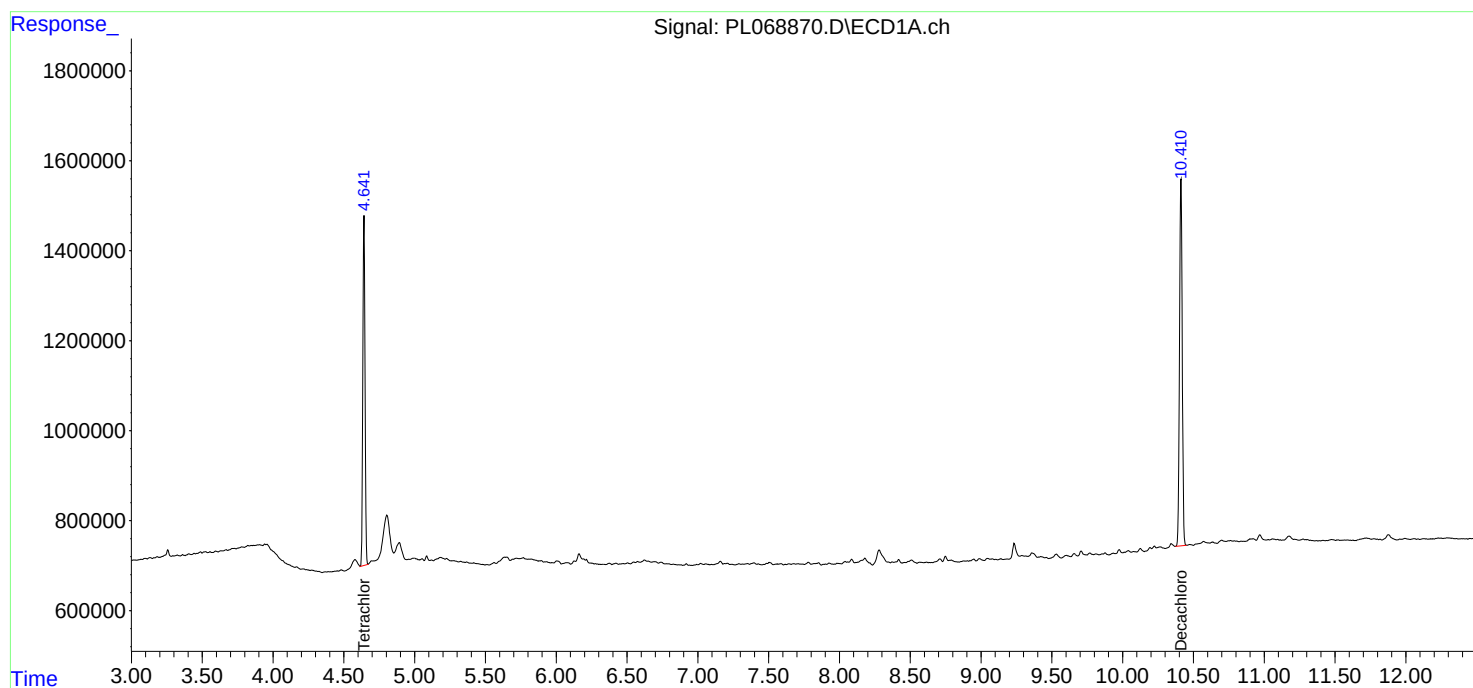

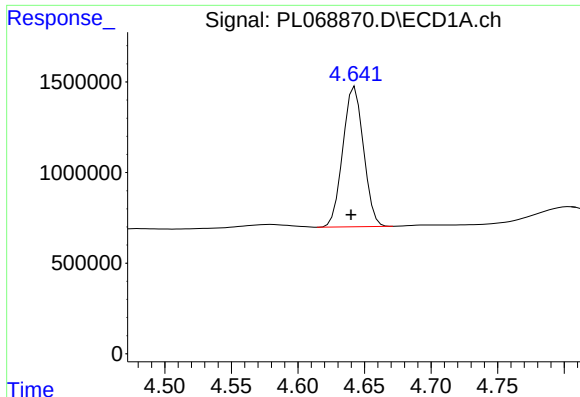


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: 0.001 min
Response: 8374936
Conc: 20.25 ng/ml m

Instrument :
ECD_L
ClientSampleId :
20210566-COM-39


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:42 PM

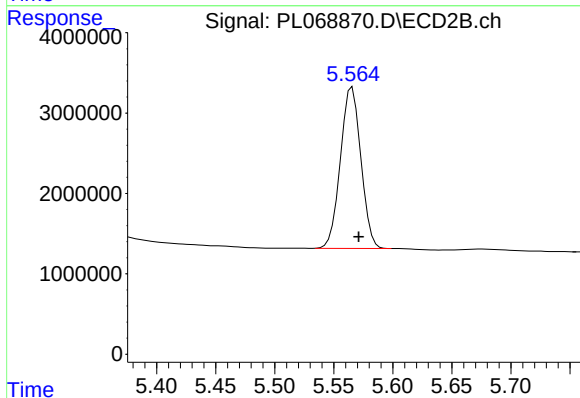


#1 Tetrachloro-m-xylene

R.T.: 5.566 min
Delta R.T.: -0.005 min
Response: 24199977
Conc: 23.83 ng/ml

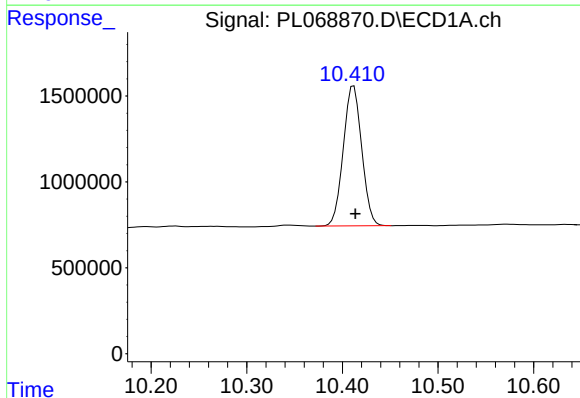

#28 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.002 min
Response: 10955249
Conc: 19.06 ng/ml

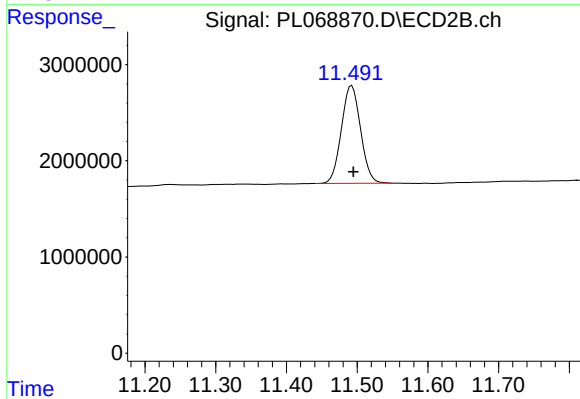

#28 Decachlorobiphenyl

R.T.: 11.492 min
Delta R.T.: -0.002 min
Response: 19191626
Conc: 19.78 ng/ml