

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068873.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 14:59
 Operator : AR\AJ
 Sample : M3333-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124055

Manual Integrations
 APPROVED

Ankita
 8/11/2021 2:08:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:28:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	7304934	19851652	17.660	19.552
28)	SA Decachlor...	10.406	11.487	8568379	14967521	14.909	15.427
Target Compounds							
10)	B gamma-Chl...	7.354	8.296	194185	538452	0.354m	0.470m#
11)	B alpha-Chl...	7.423	8.381	234525	625563	0.426m	0.545 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068873.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 14:59
Operator : AR\AJ
Sample : M3333-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
124055


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:28:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

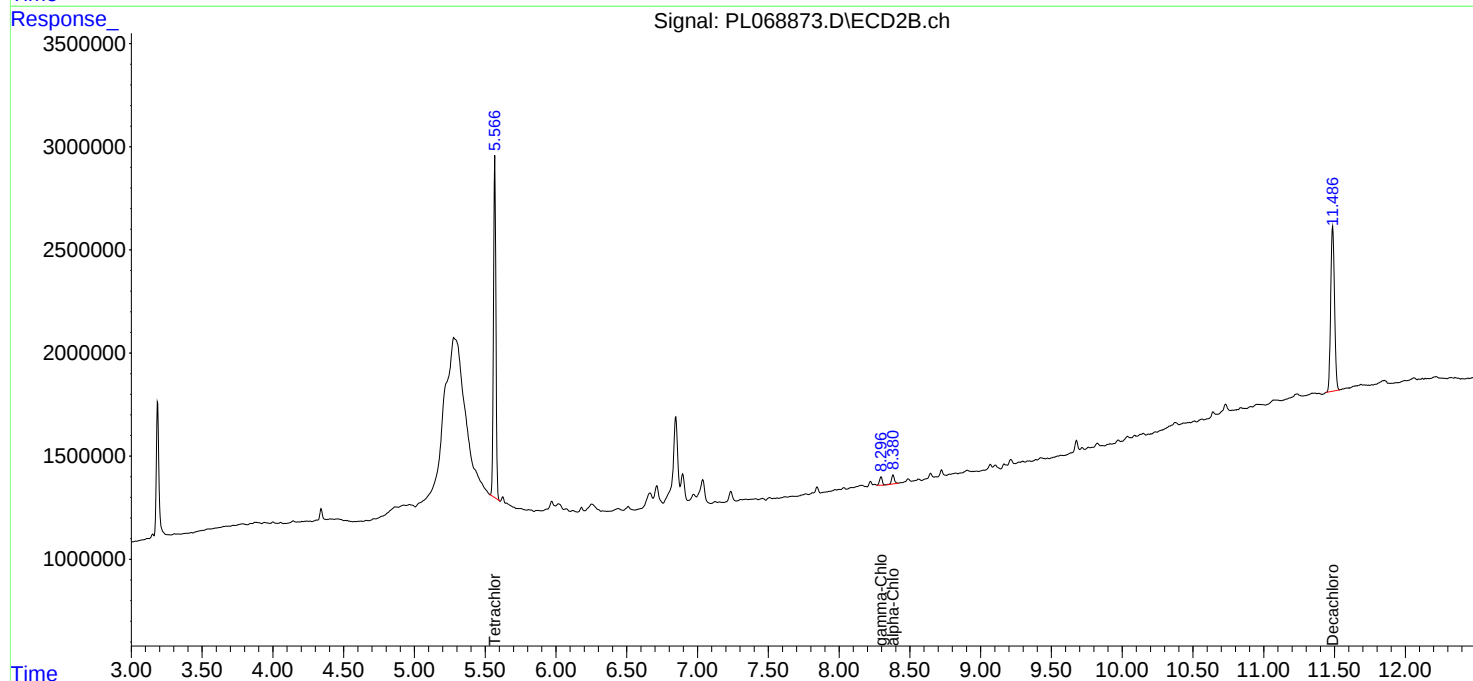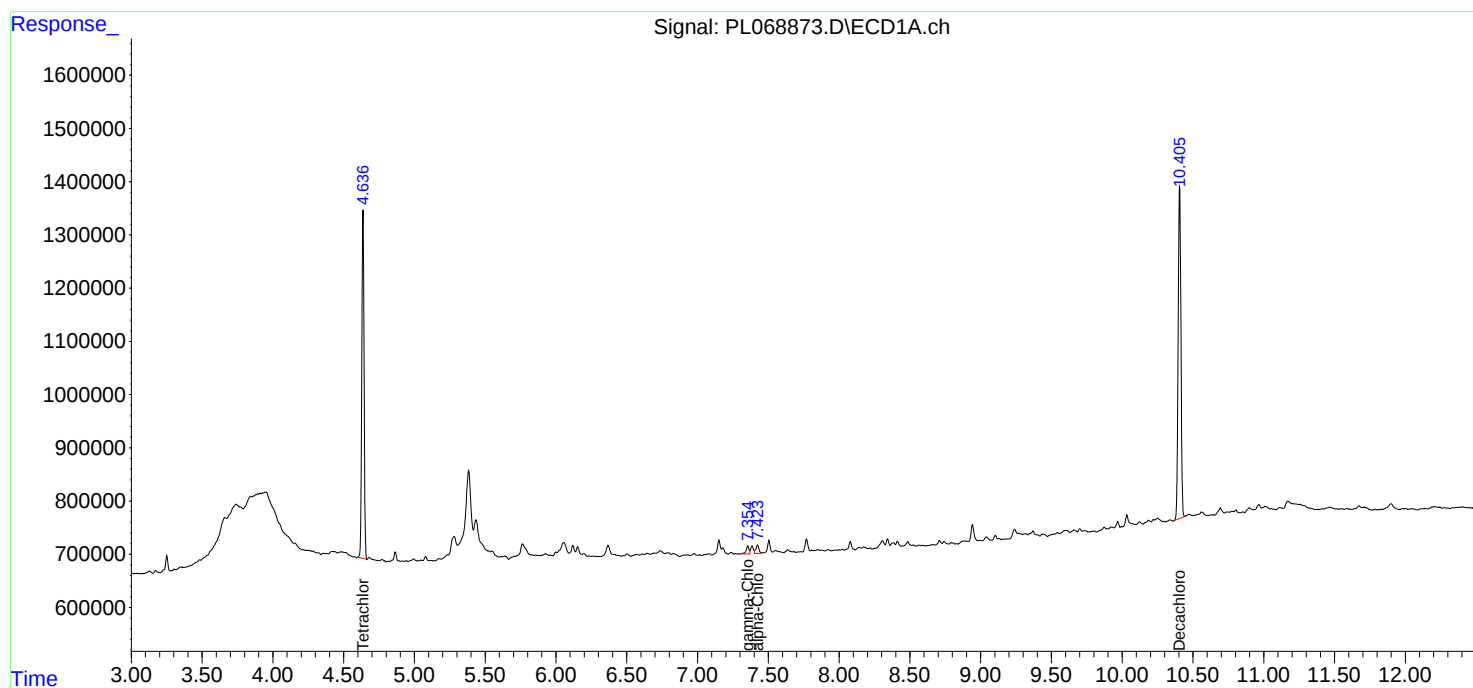

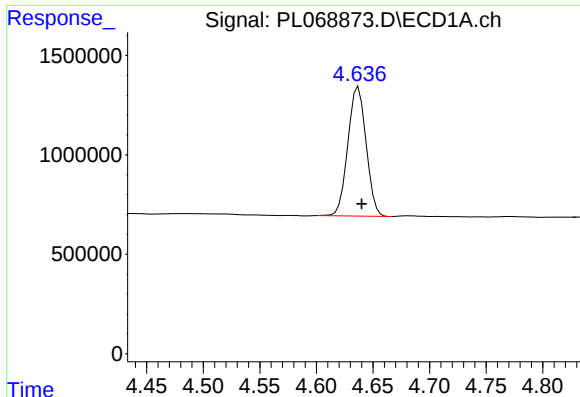


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 7304934
Conc: 17.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
124055


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:43 PM

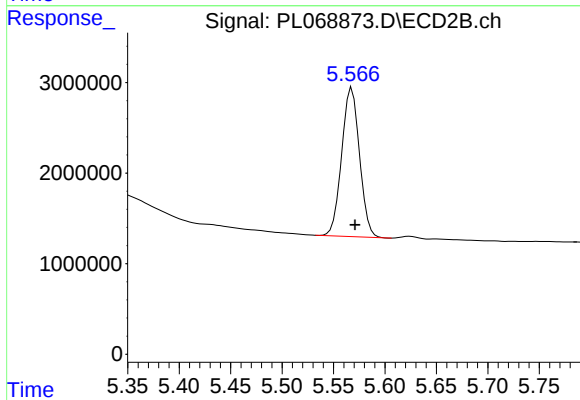


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 19851652
Conc: 19.55 ng/ml

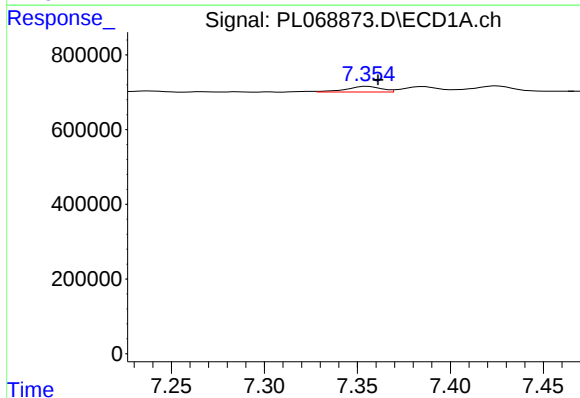


#10 gamma-Chlordane

R.T.: 7.354 min
Delta R.T.: -0.007 min
Response: 194185
Conc: 0.35 ng/ml m

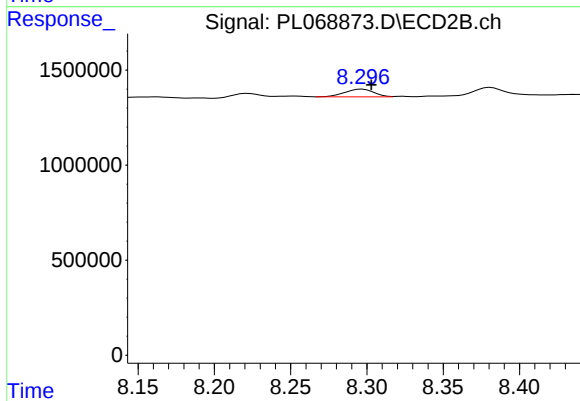

#10 gamma-Chlordane

R.T.: 8.296 min
Delta R.T.: -0.007 min
Response: 538452
Conc: 0.47 ng/ml m

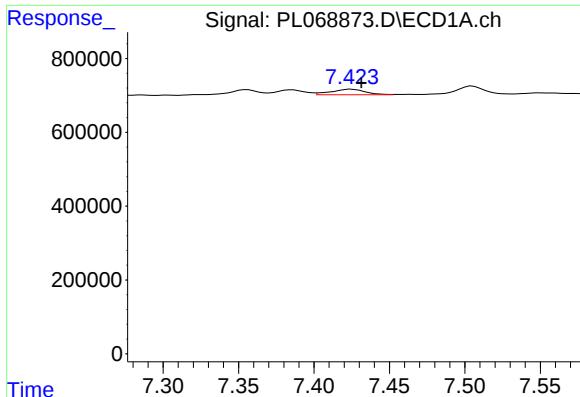


#11 alpha-Chlordane

R.T.: 7.423 min
Delta R.T.: -0.008 min
Response: 234525
Conc: 0.43 ng/ml m

Instrument :
ECD_L
ClientSampleId :
124055


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:43 PM

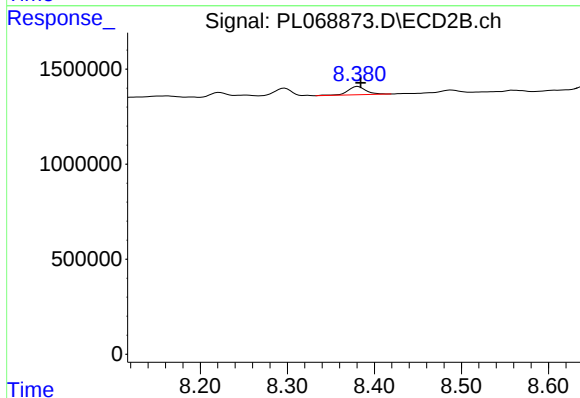


#11 alpha-Chlordane

R.T.: 8.381 min
Delta R.T.: -0.003 min
Response: 625563
Conc: 0.54 ng/ml

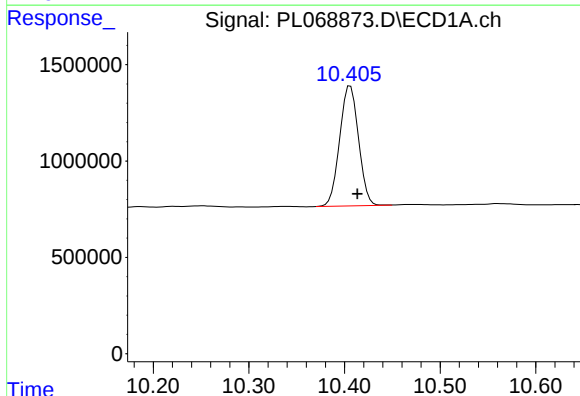

#28 Decachlorobiphenyl

R.T.: 10.406 min
Delta R.T.: -0.008 min
Response: 8568379
Conc: 14.91 ng/ml

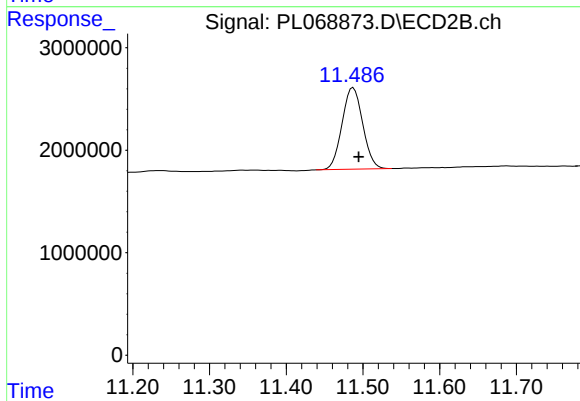

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 14967521
Conc: 15.43 ng/ml