

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 15:15
 Operator : AR\AJ
 Sample : M3333-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124030

Manual Integrations
 APPROVED

Ankita
 8/11/2021 2:07:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:28:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.638	5.568	5009706	13421412	12.111	13.219
28) SA Decachlor...	10.407	11.489	6709565	11645351	11.675	12.003
Target Compounds						
10) B gamma-Chl...	7.354	8.299	502982	1133398	0.918m	0.990
11) B alpha-Chl...	7.424	8.382	691296	1885076	1.256m	1.641 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 15:15
Operator : AR\AJ
Sample : M3333-03
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
124030


Manual Integrations
APPROVED

Ankita
8/11/2021 2:07:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:28:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

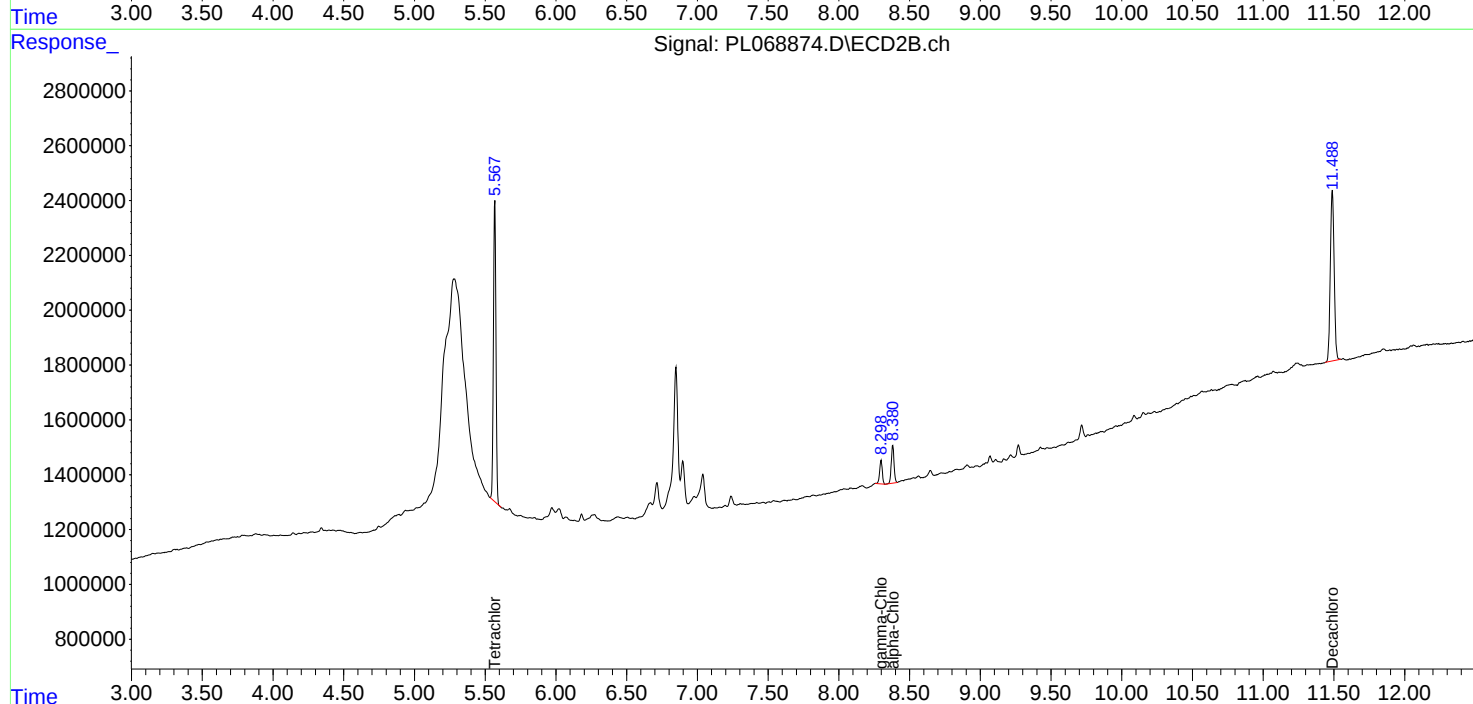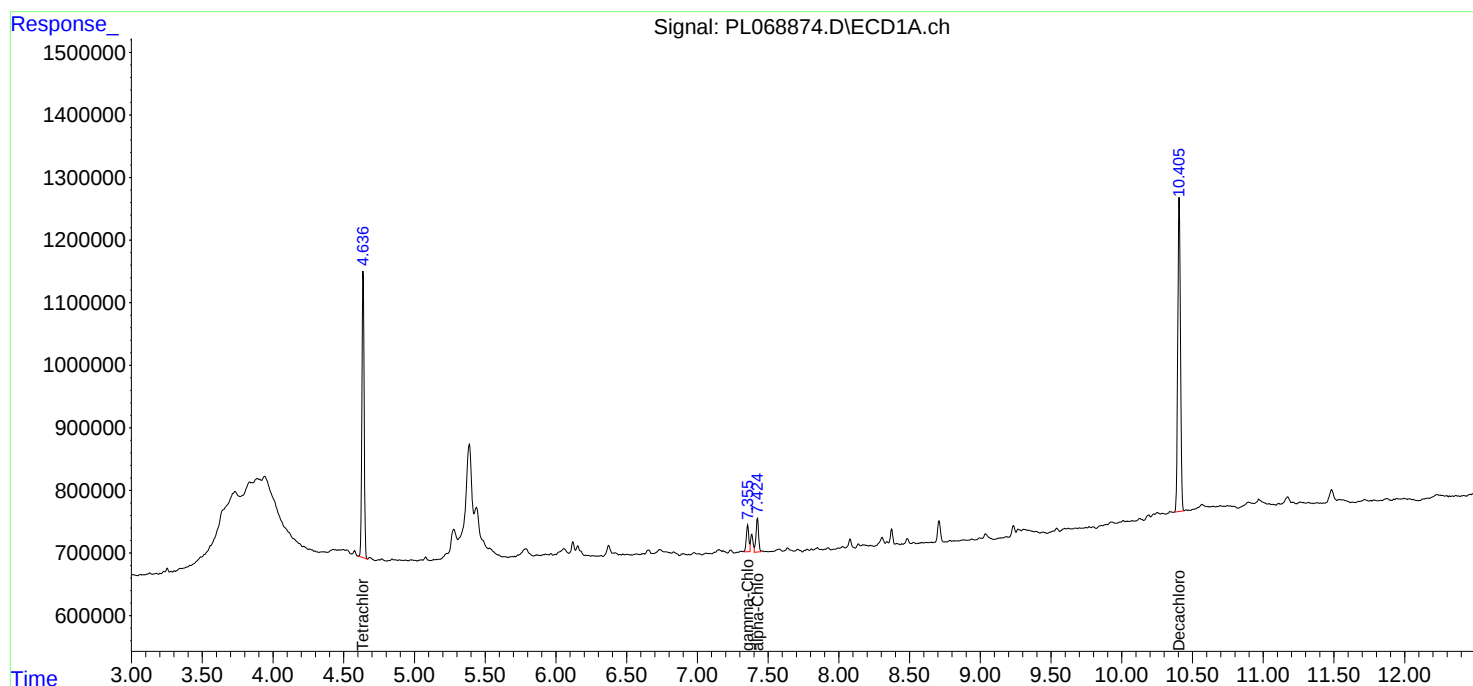

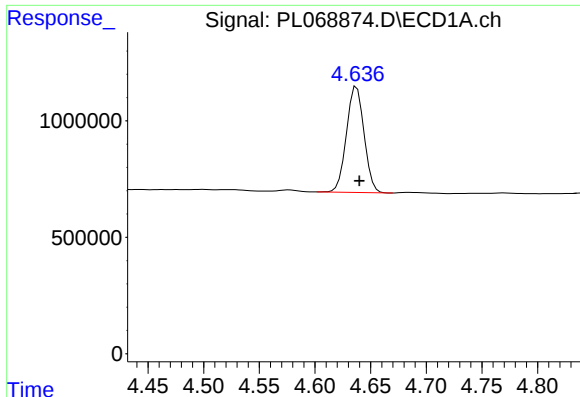


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: -0.002 min
Response: 5009706
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
124030


Manual Integrations
APPROVED

Ankita
8/11/2021 2:07:56 PM

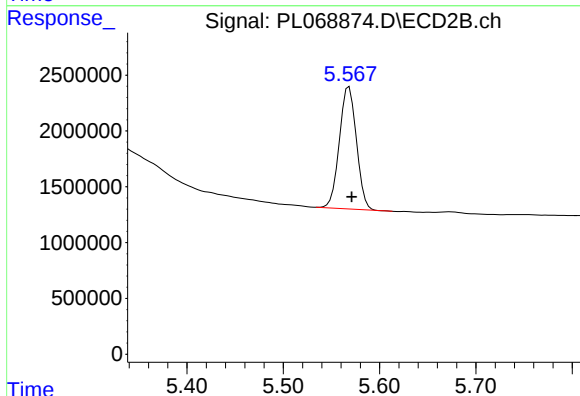


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 13421412
Conc: 13.22 ng/ml

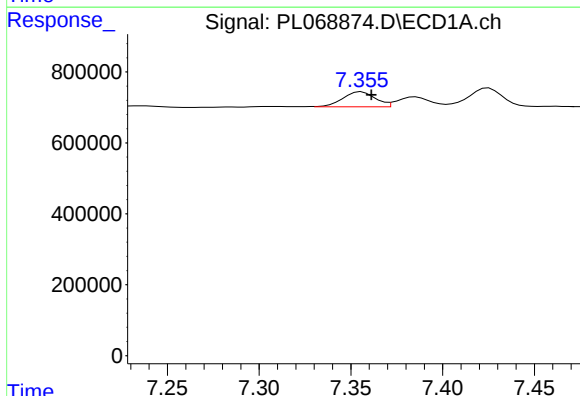


#10 gamma-Chlordane

R.T.: 7.354 min
Delta R.T.: -0.007 min
Response: 502982
Conc: 0.92 ng/ml m

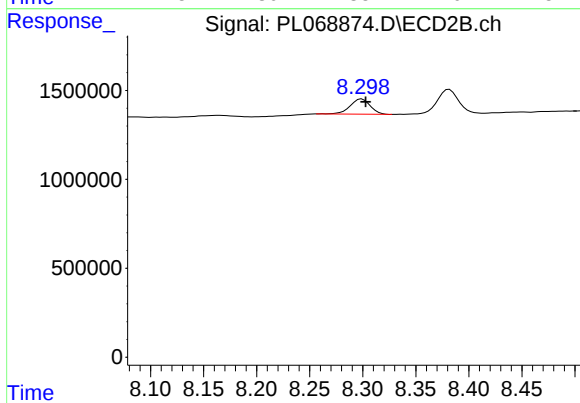

#10 gamma-Chlordane

R.T.: 8.299 min
Delta R.T.: -0.004 min
Response: 1133398
Conc: 0.99 ng/ml

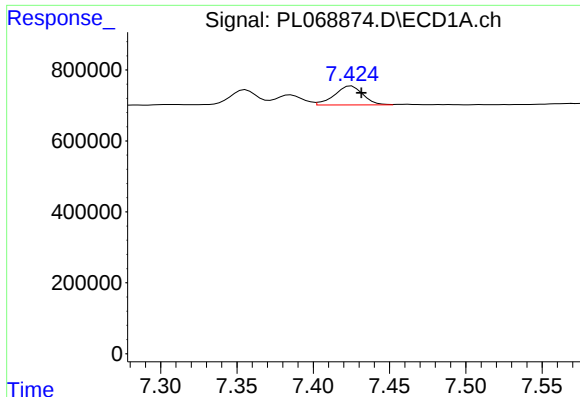


#11 alpha-Chlordane

R.T.: 7.424 min
Delta R.T.: -0.008 min
Response: 691296
Conc: 1.26 ng/ml m

Instrument :
ECD_L
ClientSampleId :
124030


Manual Integrations
APPROVED

Ankita
8/11/2021 2:07:56 PM

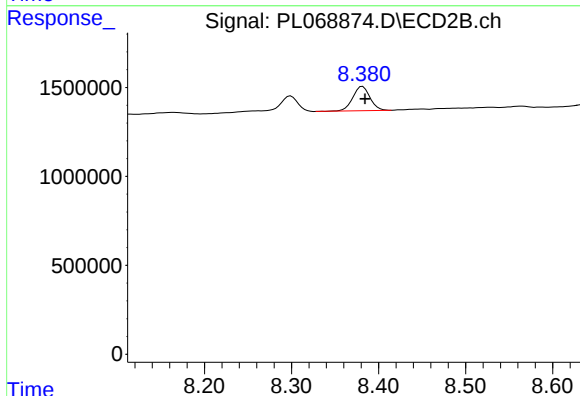


#11 alpha-Chlordane

R.T.: 8.382 min
Delta R.T.: -0.003 min
Response: 1885076
Conc: 1.64 ng/ml

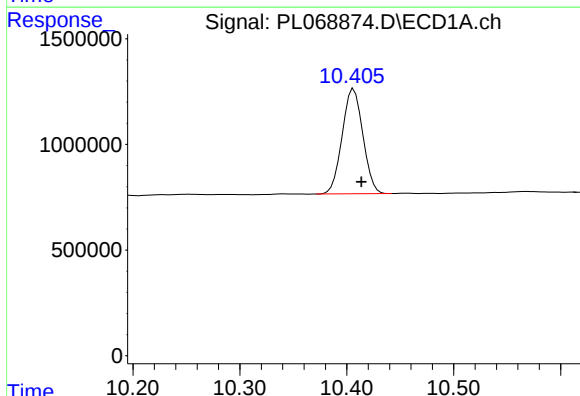

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.007 min
Response: 6709565
Conc: 11.68 ng/ml

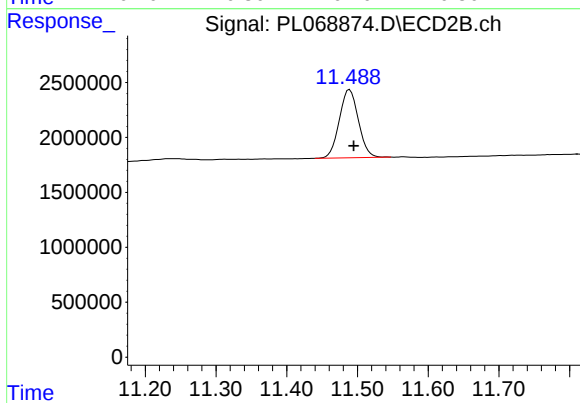

#28 Decachlorobiphenyl

R.T.: 11.489 min
Delta R.T.: -0.006 min
Response: 11645351
Conc: 12.00 ng/ml