

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
 Data File : PL068892.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2021 21:13
 Operator : AR\AJ
 Sample : M3333-11
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 124042

Manual Integrations
 APPROVED

Ankita
 8/11/2021 2:08:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:35:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.568	5072908	13747884	12.264	13.540
28)	SA Decachlor...	10.404	11.486	7288027	12832313	12.682	13.226
Target Compounds							
16)	A 4,4'-DDD	8.222	9.104	166605	744507	0.388m	0.871m#
17)	MA 4,4'-DDT	8.482	9.422	635784	661174	1.309	0.699m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081021\
Data File : PL068892.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2021 21:13
Operator : AR\AJ
Sample : M3333-11
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
124042


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

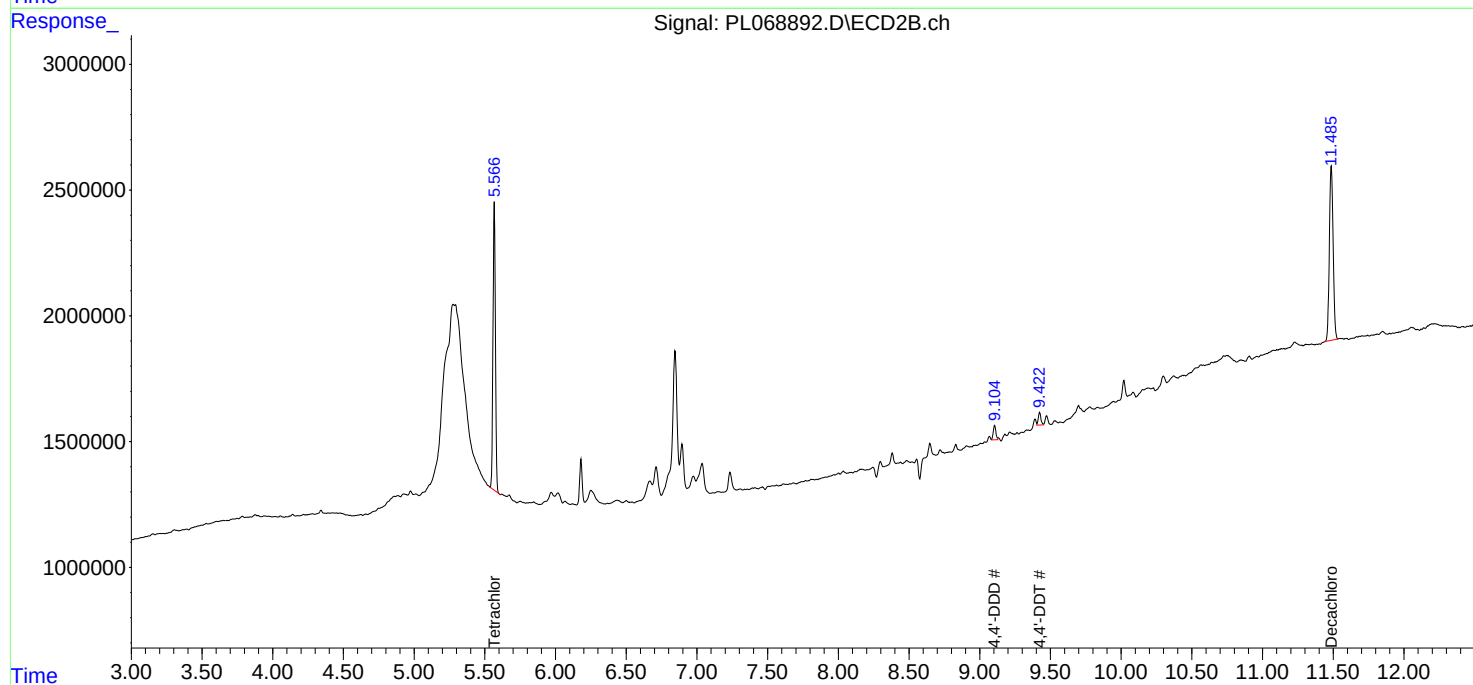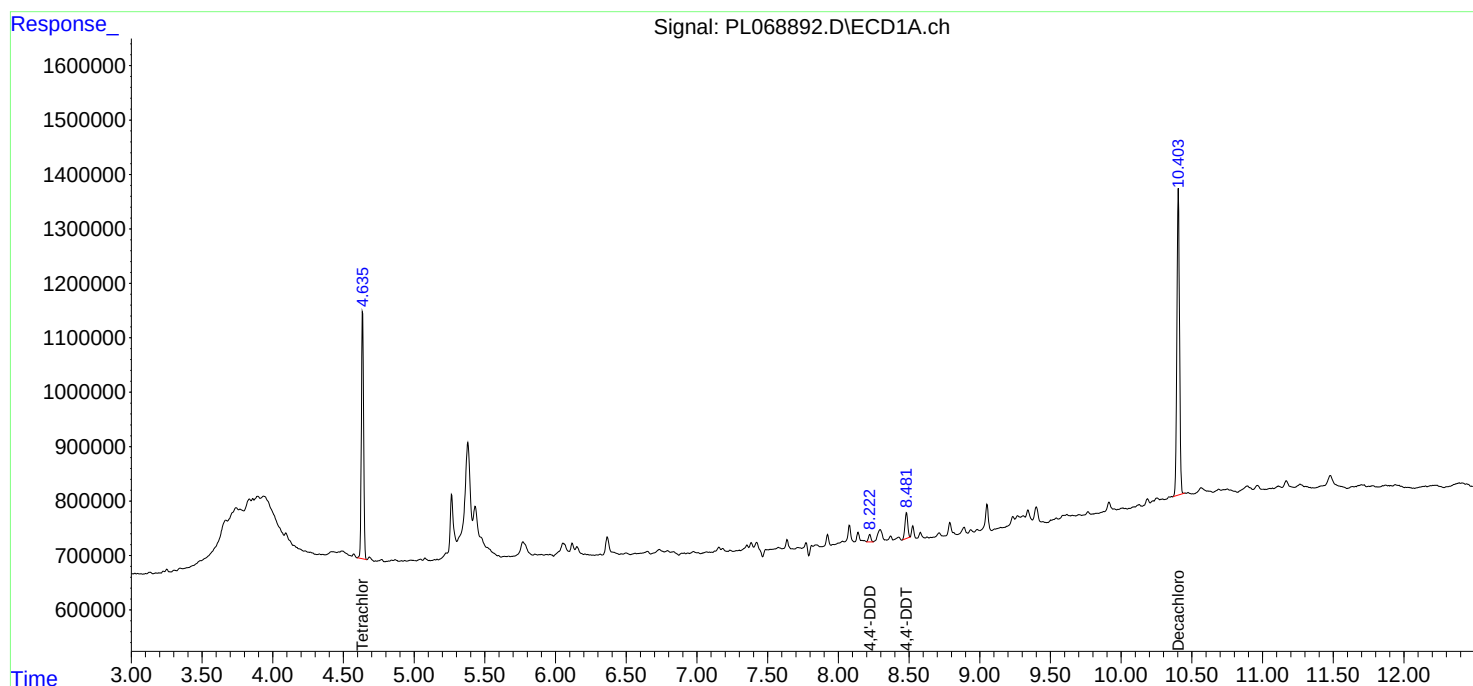

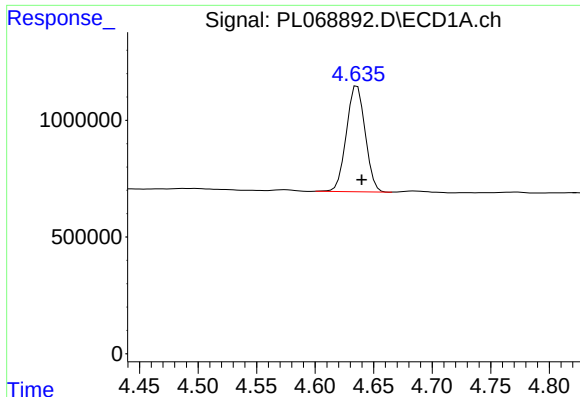


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.004 min
Response: 5072908
Conc: 12.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
124042


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:07 PM

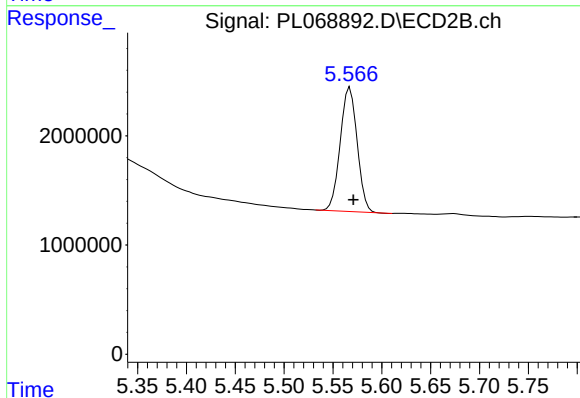


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.004 min
Response: 13747884
Conc: 13.54 ng/ml

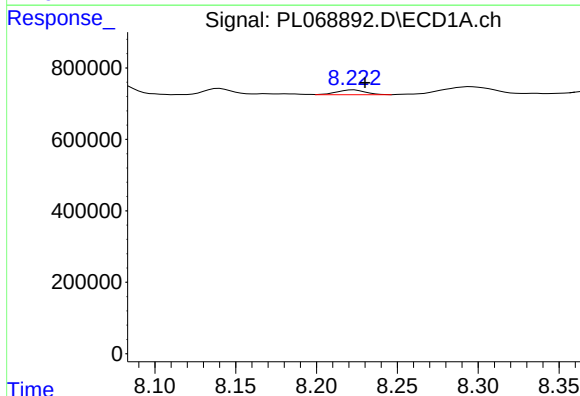


#16 4,4'-DDD

R.T.: 8.222 min
Delta R.T.: -0.008 min
Response: 166605
Conc: 0.39 ng/ml m

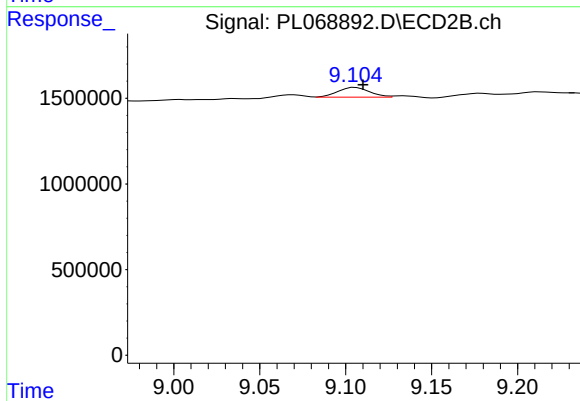

#16 4,4'-DDD

R.T.: 9.104 min
Delta R.T.: -0.006 min
Response: 744507
Conc: 0.87 ng/ml m

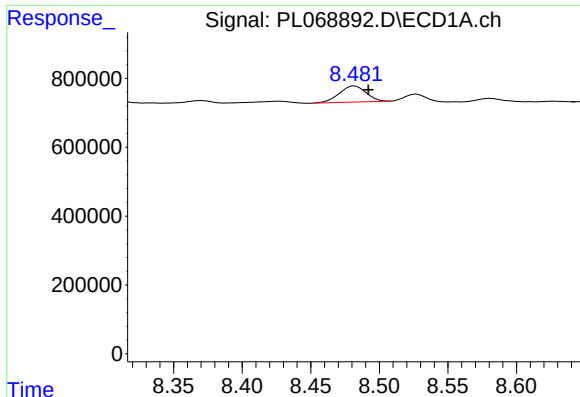


#17 4,4'-DDT

R.T.: 8.482 min
Delta R.T.: -0.010 min
Response: 635784
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
124042


Manual Integrations
APPROVED

Ankita
8/11/2021 2:08:07 PM

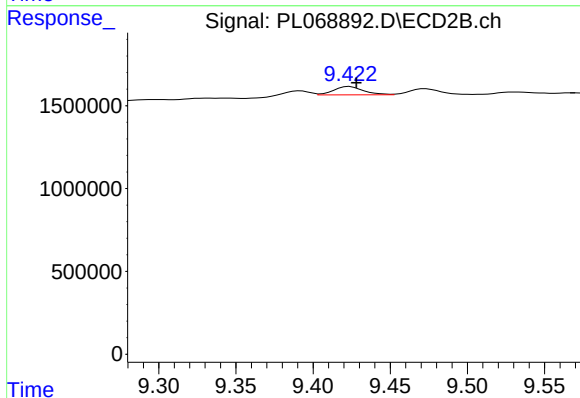


#17 4,4'-DDT

R.T.: 9.422 min
Delta R.T.: -0.006 min
Response: 661174
Conc: 0.70 ng/ml m

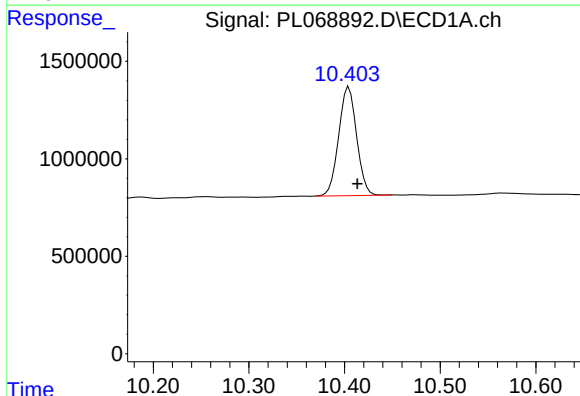

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.009 min
Response: 7288027
Conc: 12.68 ng/ml

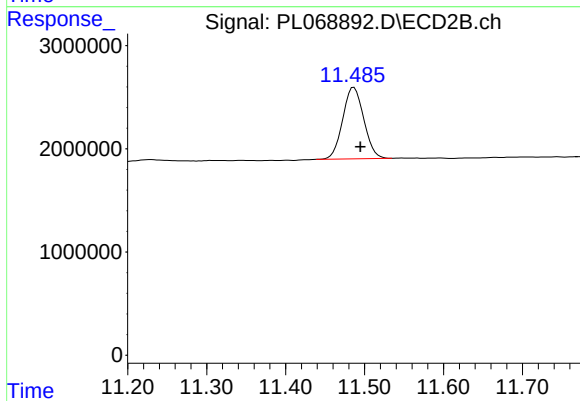

#28 Decachlorobiphenyl

R.T.: 11.486 min
Delta R.T.: -0.008 min
Response: 12832313
Conc: 13.23 ng/ml