

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL081022\  
 Data File : PL077013.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 10 Aug 2022 14:16  
 Operator : AR\AJ  
 Sample : N4119-01  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 10 15:33:36 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL080822.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Aug 09 09:13:15 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2   | Resp#1  | Resp#2   | ng/ml  | ng/ml    |
|-----------------------------|-----------------|-------|--------|---------|----------|--------|----------|
| -----                       |                 |       |        |         |          |        |          |
| System Monitoring Compounds |                 |       |        |         |          |        |          |
| 1)                          | SA Tetrachlo... | 3.421 | 2.638  | 9336501 | 25055949 | 9.522  | 8.753    |
| 28)                         | SA Decachlor... | 8.913 | 7.744  | 8748799 | 23172921 | 11.589 | 10.294   |
| Target Compounds            |                 |       |        |         |          |        |          |
| 5)                          | MB Aldrin       | 0.000 | 4.055  | 0       | 274450   | N.D.   | 0.077 #  |
| 6)                          | B beta-BHC      | 4.430 | 0.000  | 277680  | 0        | 0.495  | N.D. #   |
| 9)                          | A Endosulfan I  | 0.000 | 4.942f | 0       | 1595874  | N.D.   | 0.584 #  |
| 23)                         | Chlordane-1     | 0.000 | 3.615  | 0       | 2208430  | N.D.   | 22.675 # |
| -----                       |                 |       |        |         |          |        |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL081022\  
Data File : PL077013.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 10 Aug 2022 14:16  
Operator : AR\AJ  
Sample : N4119-01  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 10 15:33:36 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL080822.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 09 09:13:15 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

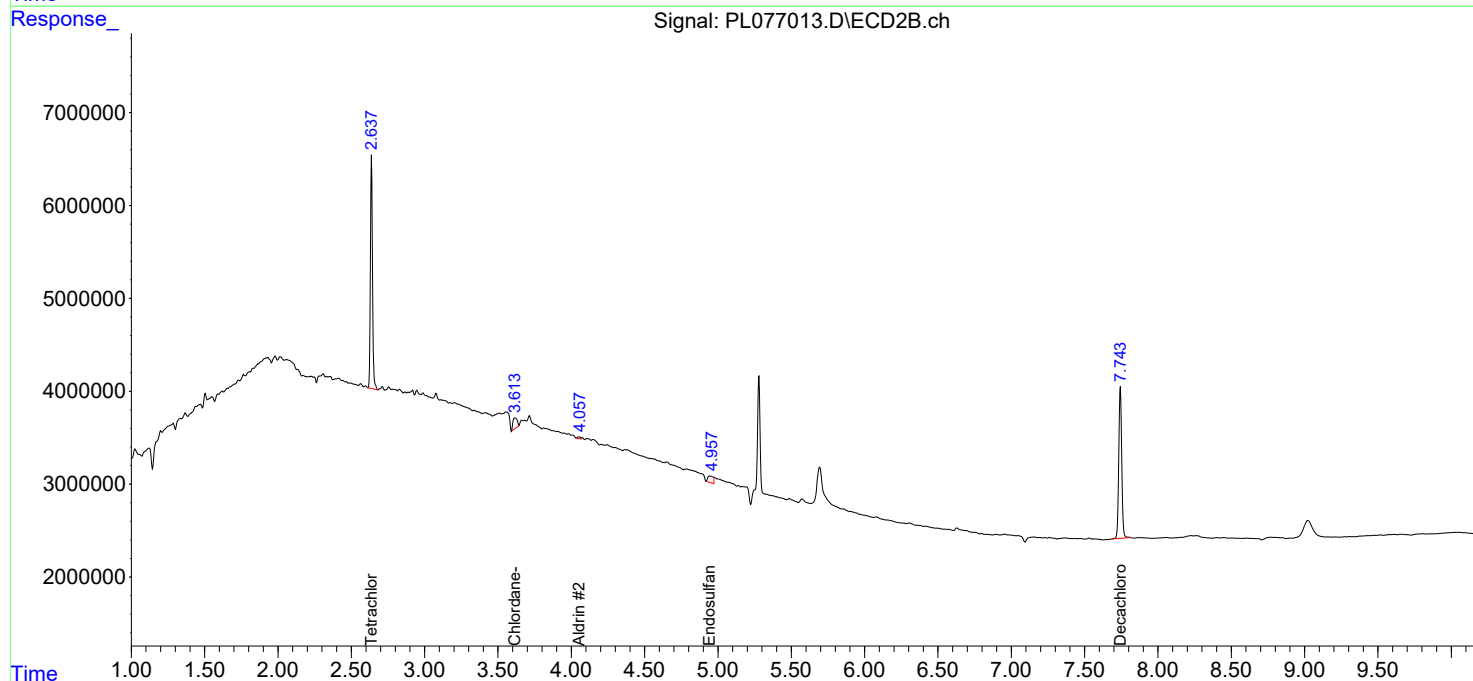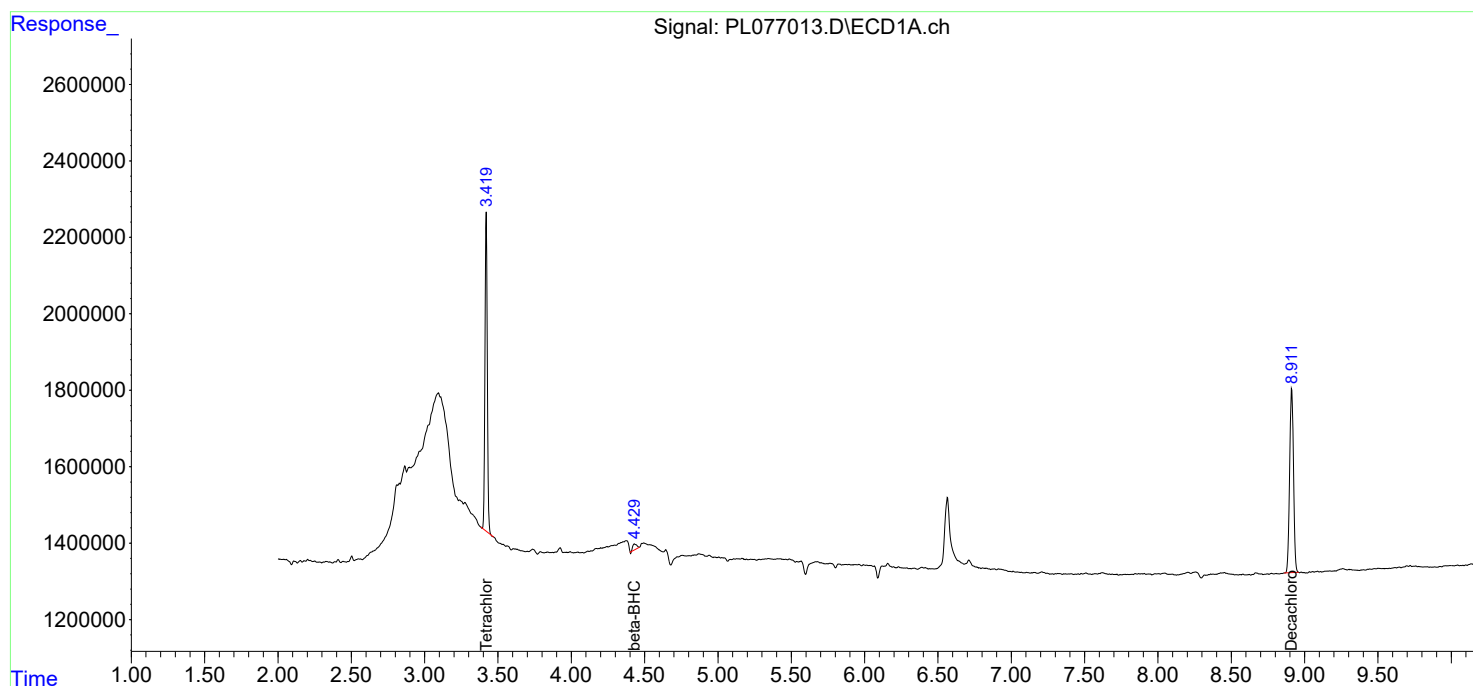


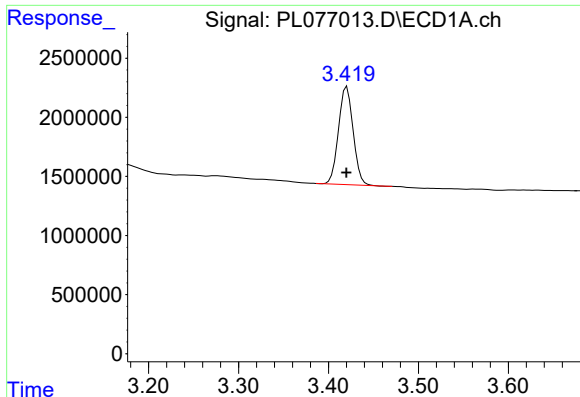

#1 Tetrachloro-m-xylene


R.T.: 3.421 min  
Delta R.T.: 0.000 min  
Response: 9336501  
Conc: 9.52 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

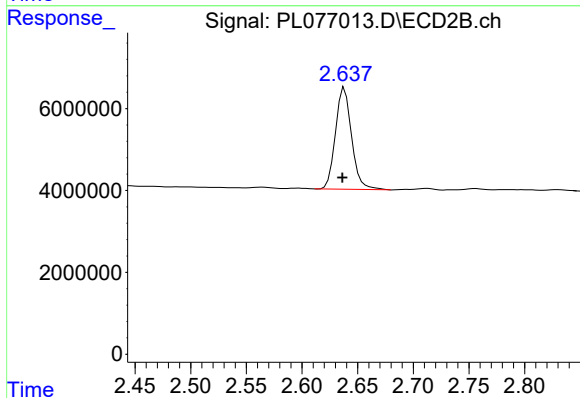


#1 Tetrachloro-m-xylene

R.T.: 2.638 min  
Delta R.T.: 0.002 min  
Response: 25055949  
Conc: 8.75 ng/ml

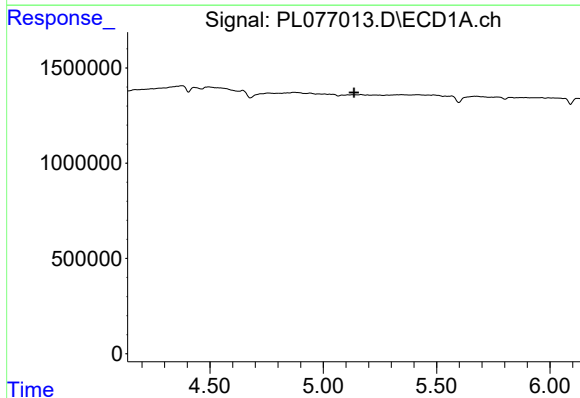


#5 Aldrin

R.T.: 0.000 min  
Exp R.T. : 5.136 min  
Response: 0  
Conc: N.D.

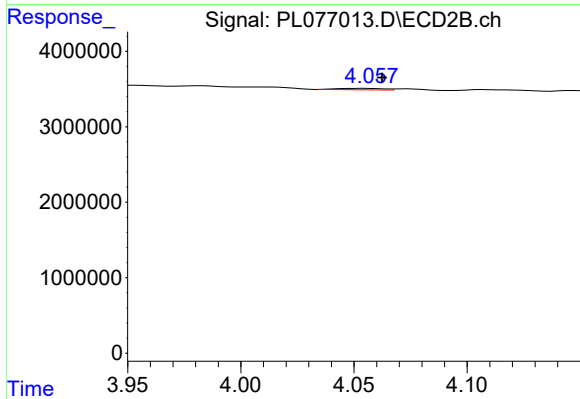

#5 Aldrin


R.T.: 4.055 min  
Delta R.T.: -0.008 min  
Response: 274450  
Conc: 0.08 ng/ml

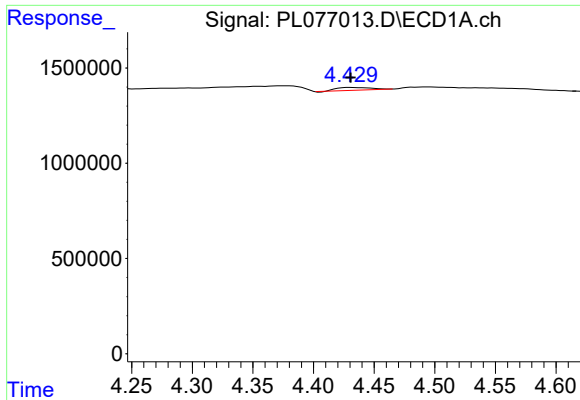

#6 beta-BHC


R.T.: 4.430 min  
Delta R.T.: 0.000 min  
Response: 277680  
Conc: 0.49 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

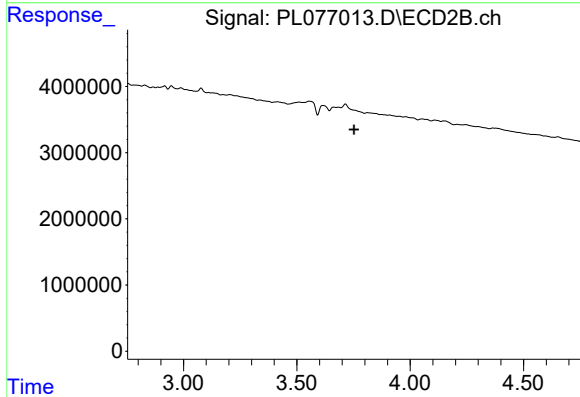


#6 beta-BHC

R.T.: 0.000 min  
Exp R.T. : 3.753 min  
Response: 0  
Conc: N.D.

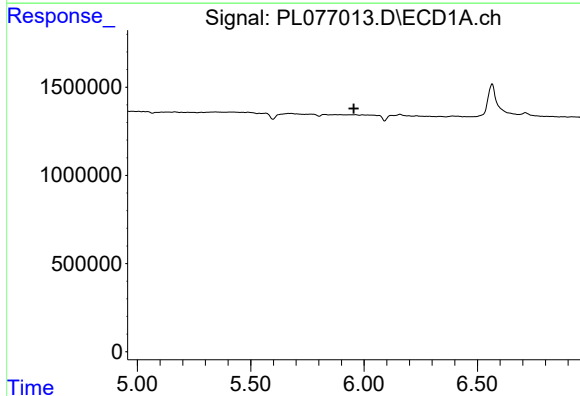


#9 Endosulfan I

R.T.: 0.000 min  
Exp R.T. : 5.954 min  
Response: 0  
Conc: N.D.

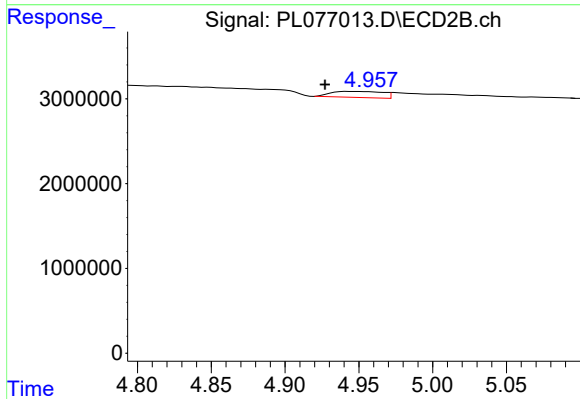

#9 Endosulfan I


R.T.: 4.942 min  
Delta R.T.: 0.015 min  
Response: 1595874  
Conc: 0.58 ng/ml

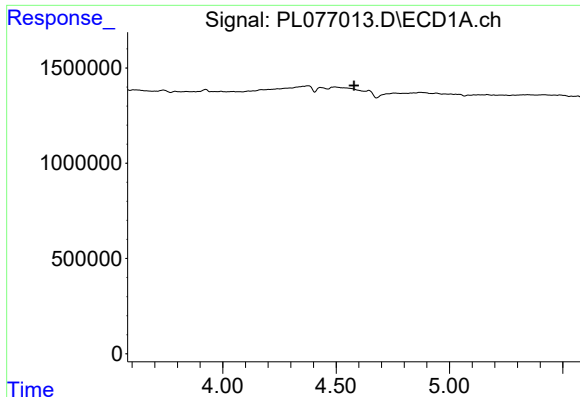

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T.: 4.579 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

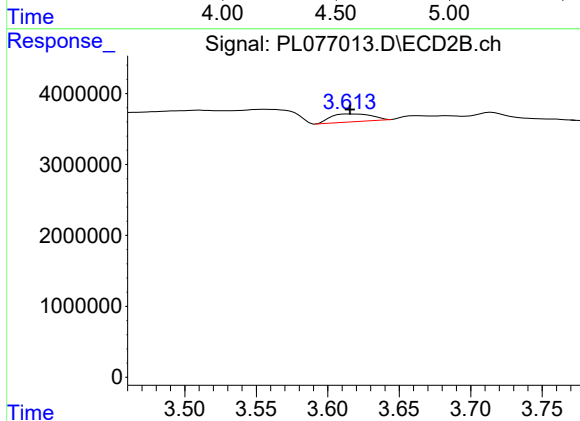


#23 Chlordane-1

R.T.: 3.615 min  
Delta R.T.: -0.001 min  
Response: 2208430  
Conc: 22.67 ng/ml

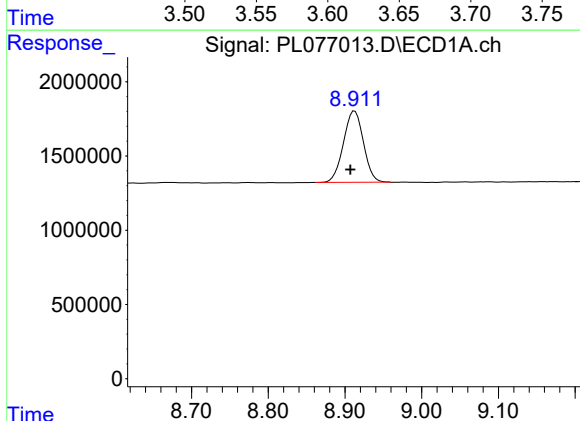

#28 Decachlorobiphenyl

R.T.: 8.913 min  
Delta R.T.: 0.005 min  
Response: 8748799  
Conc: 11.59 ng/ml

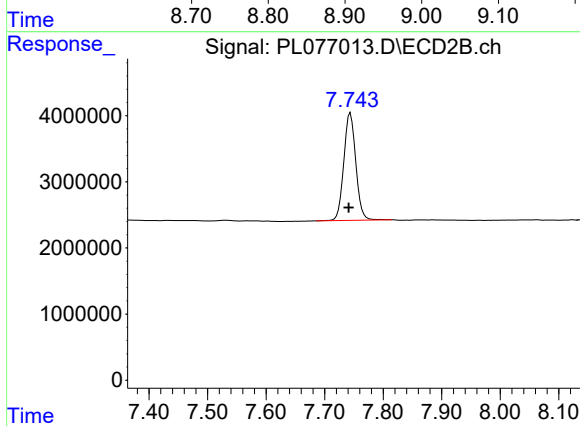

#28 Decachlorobiphenyl

R.T.: 7.744 min  
Delta R.T.: 0.003 min  
Response: 23172921  
Conc: 10.29 ng/ml