

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081022\
 Data File : PL077020.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Aug 2022 15:53
 Operator : AR\AJ
 Sample : N4127-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 10 16:13:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.639	9386129	24873046	9.572	8.689
28)	SA Decachlor...	8.912	7.744	8391787	20199292	11.116	8.973
Target Compounds							
9)	A Endosulfan I	0.000	4.937	0	111973	N.D.	0.041 #
14)	MA Endrin	0.000	5.486f	0	209343	N.D.	0.082 #
23)	Chlordane-1	0.000	3.610	0	693678	N.D.	7.122 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081022\
Data File : PL077020.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Aug 2022 15:53
Operator : AR\AJ
Sample : N4127-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 10 16:13:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

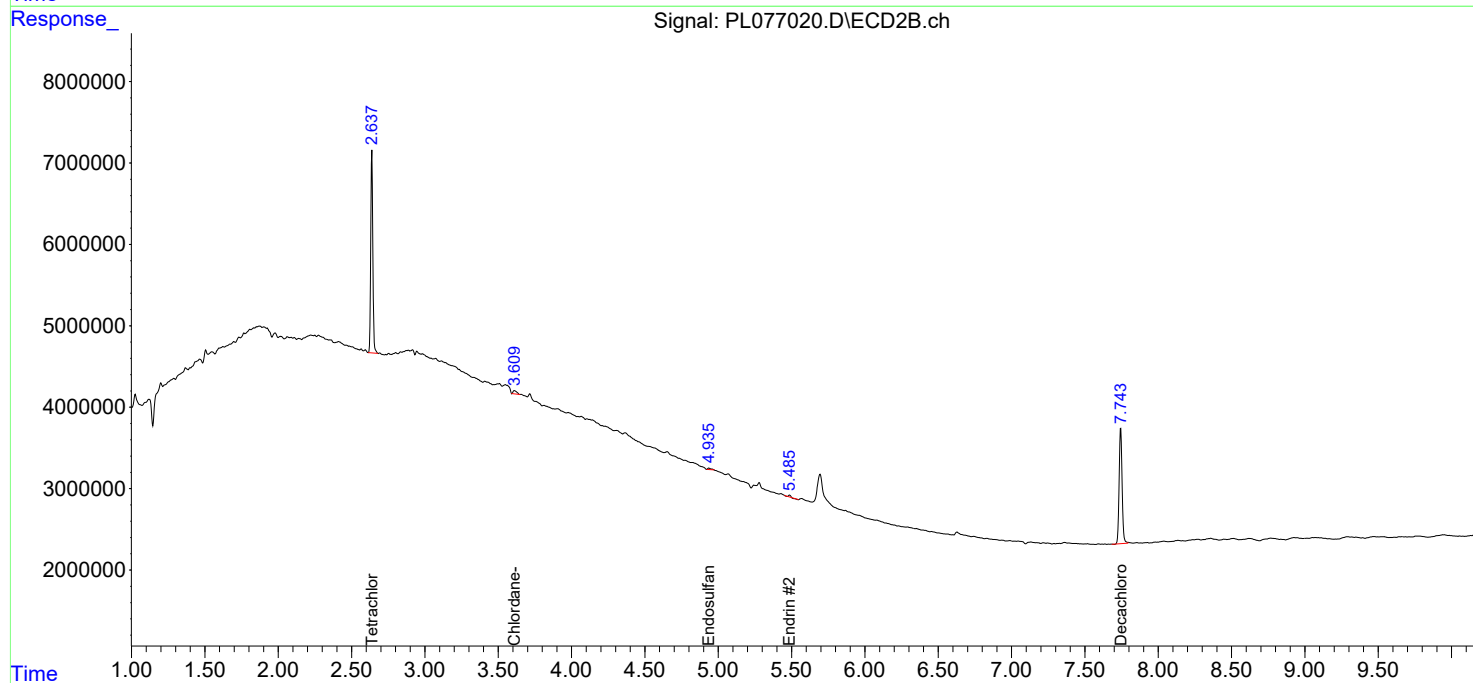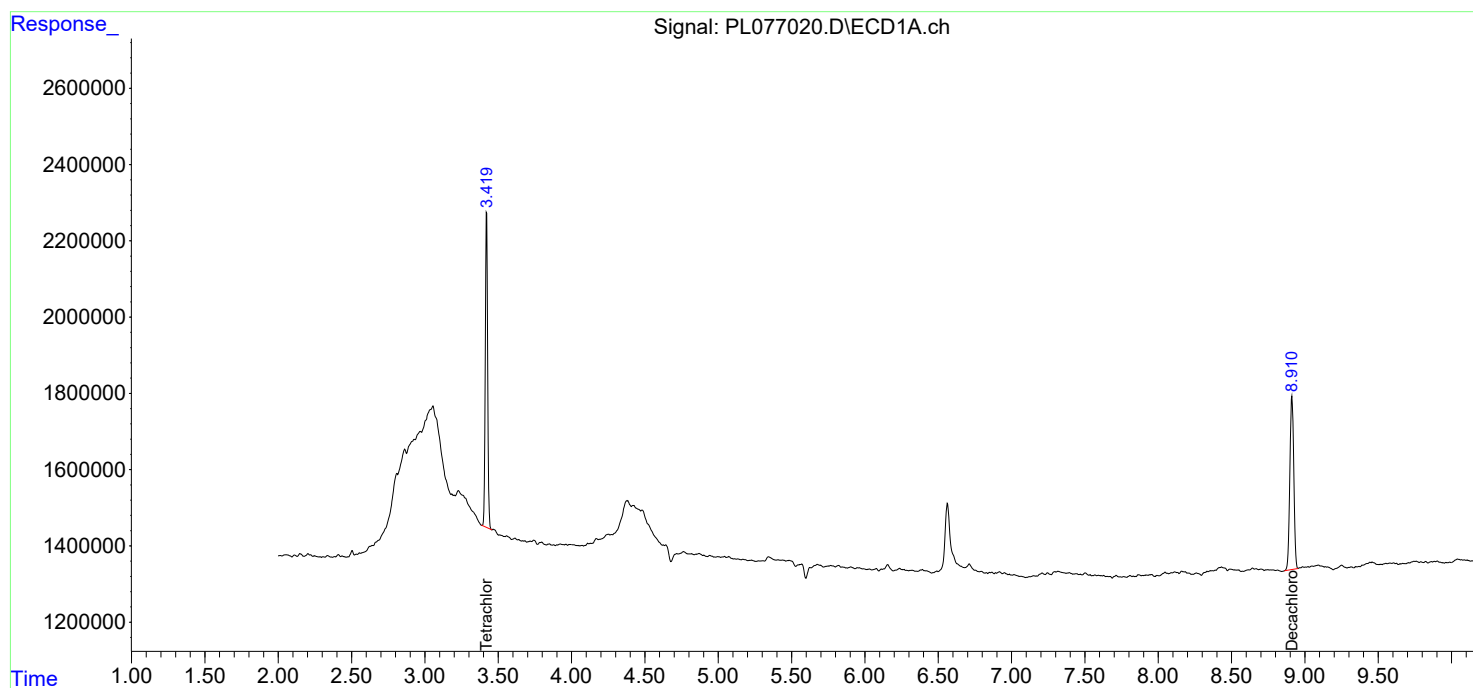


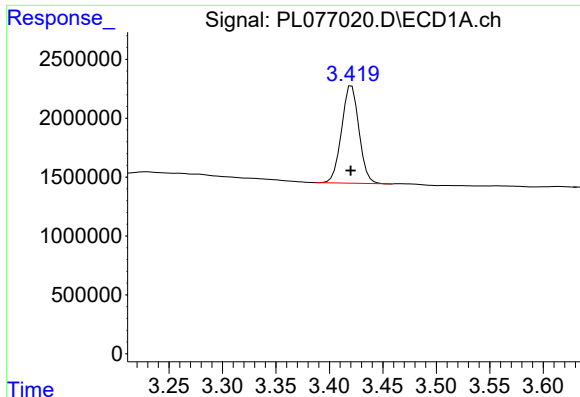

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 9386129
Conc: 9.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

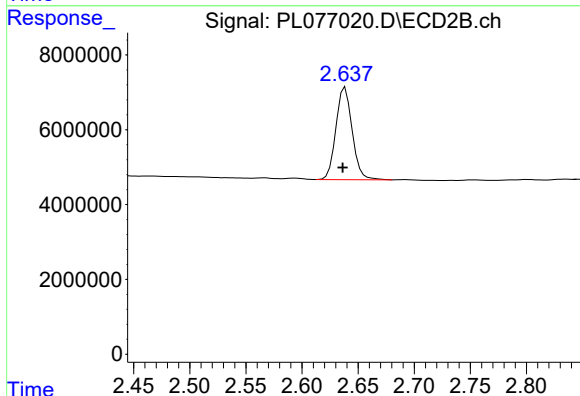


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.002 min
Response: 24873046
Conc: 8.69 ng/ml

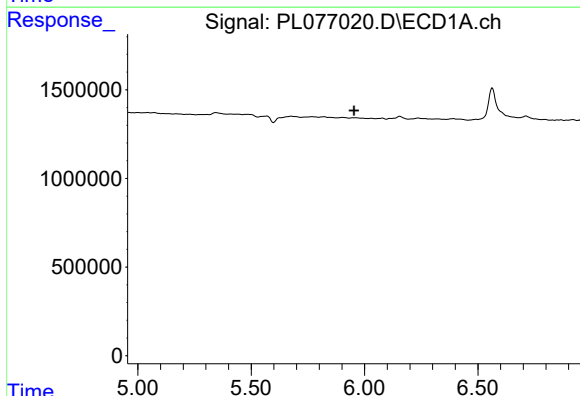


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

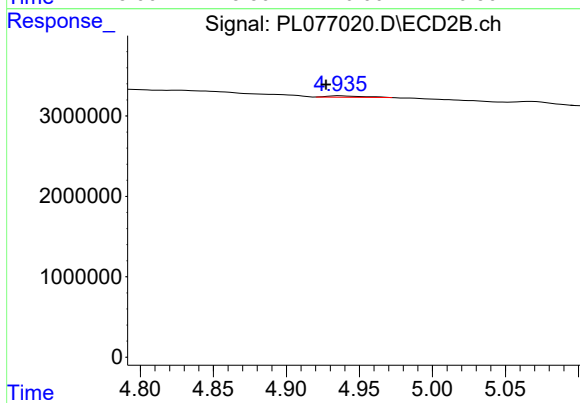

#9 Endosulfan I


R.T.: 4.937 min
Delta R.T.: 0.010 min
Response: 111973
Conc: 0.04 ng/ml

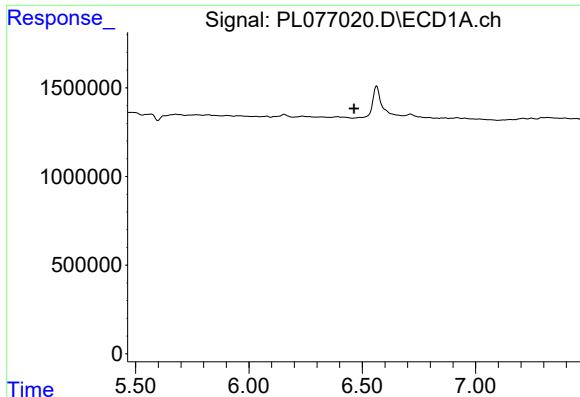

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

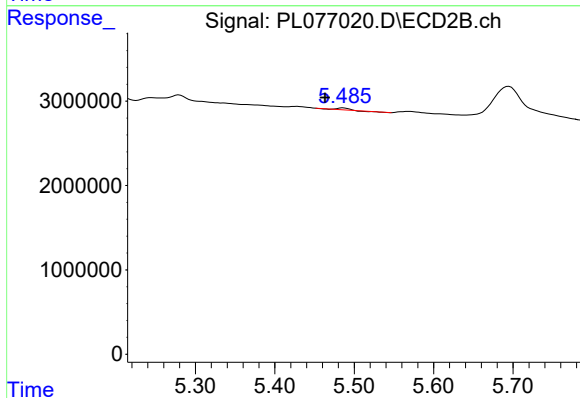


#14 Endrin

R.T.: 5.486 min
Delta R.T.: 0.023 min
Response: 209343
Conc: 0.08 ng/ml

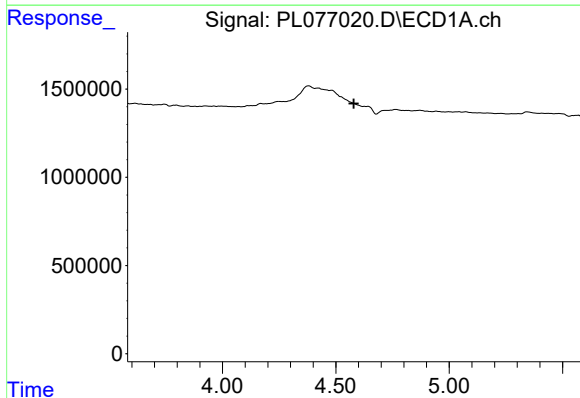


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.579 min
Response: 0
Conc: N.D.

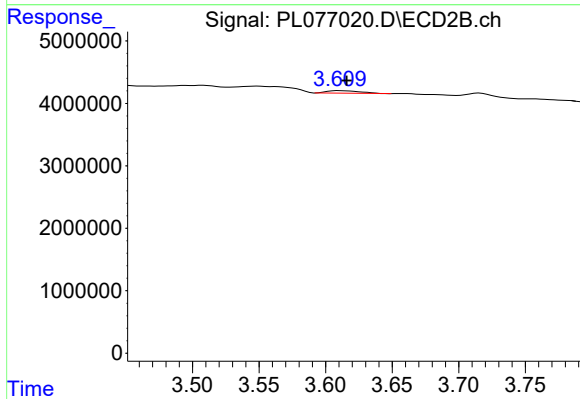

#23 Chlordane-1


R.T.: 3.610 min
Delta R.T.: -0.006 min
Response: 693678
Conc: 7.12 ng/ml

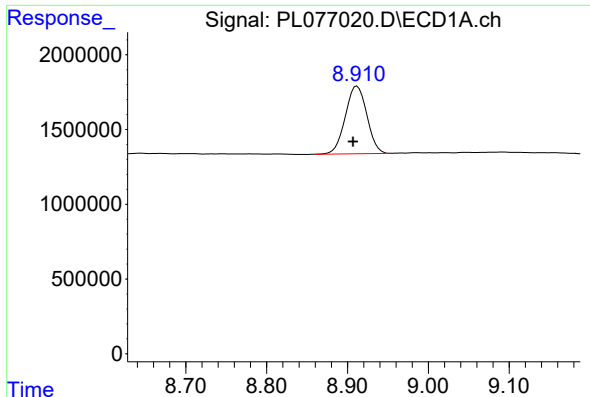

#28 Decachlorobiphenyl

R.T.: 8.912 min
Delta R.T.: 0.005 min
Response: 8391787
Conc: 11.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

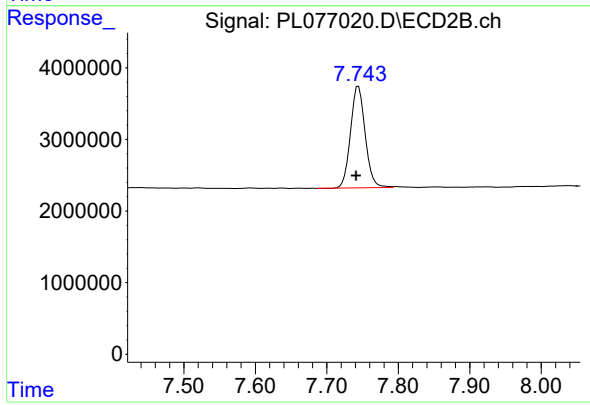

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 20199292
Conc: 8.97 ng/ml