

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081120\
 Data File : PL060600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2020 09:11
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 13:54:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) A	alpha-BHC	0.000	4.403	0	2543955	N.D. 0.619 #
3) MA	gamma-BHC...	0.000	4.689	0	2780649	N.D. 0.724 #
7) B	delta-BHC	0.000	5.080	0	2216884	N.D. 0.815 #
11) B	alpha-Chl...	0.000	6.205	0	2557490	N.D. 0.832 #
17) MA	4,4'-DDT	0.000	7.155	0	6803600	N.D. 3.112 #
26)	Chlordane-4	0.000	6.205	0	2557490	N.D. 5.900 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081120\
Data File : PL060600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2020 09:11
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 13:54:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

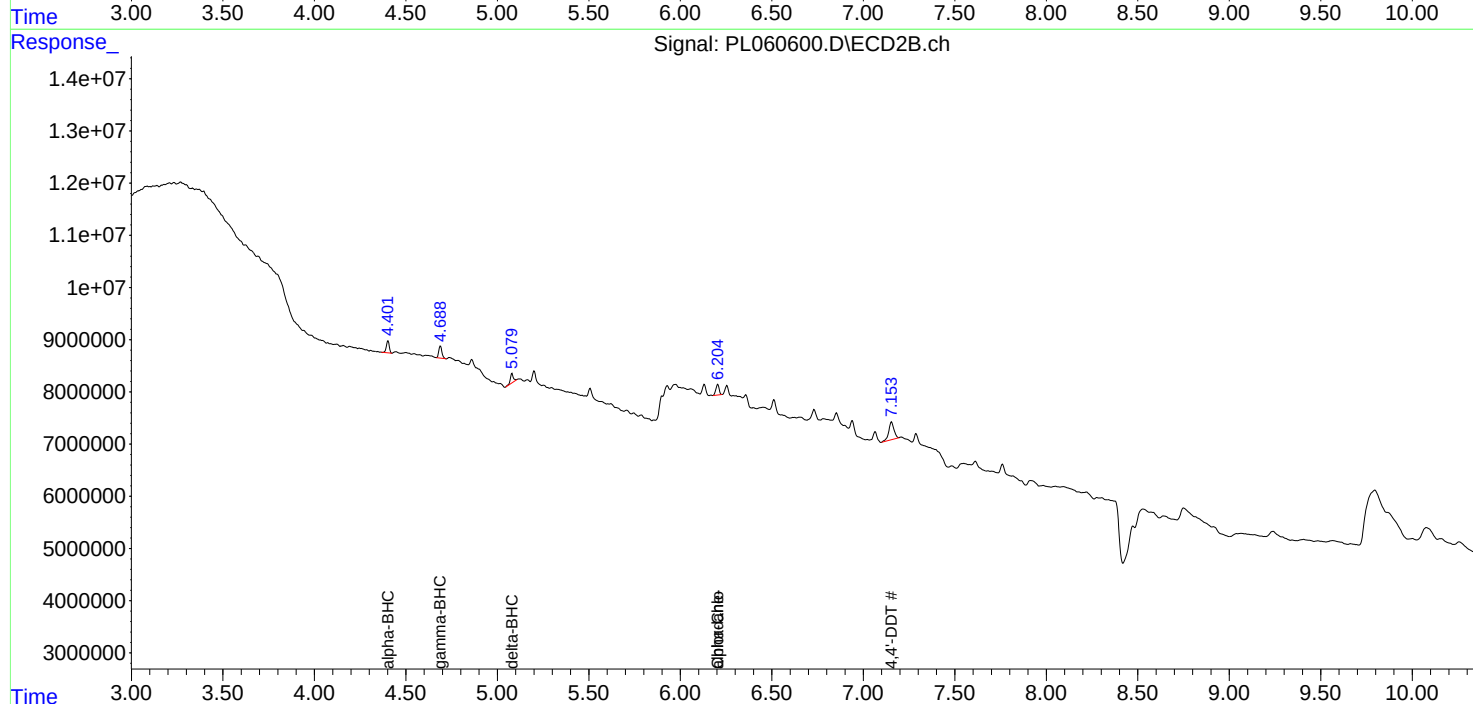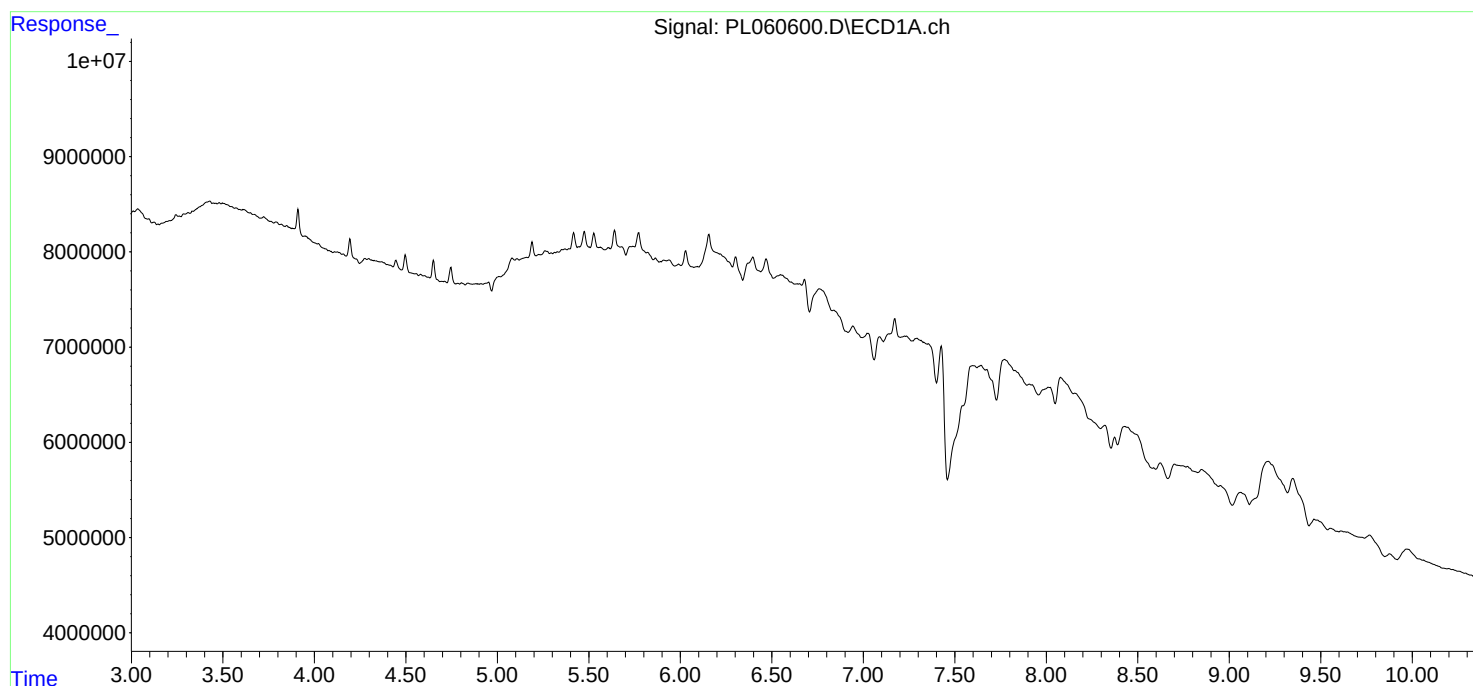


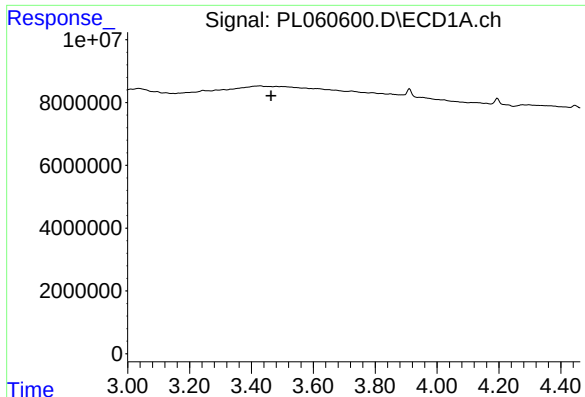

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

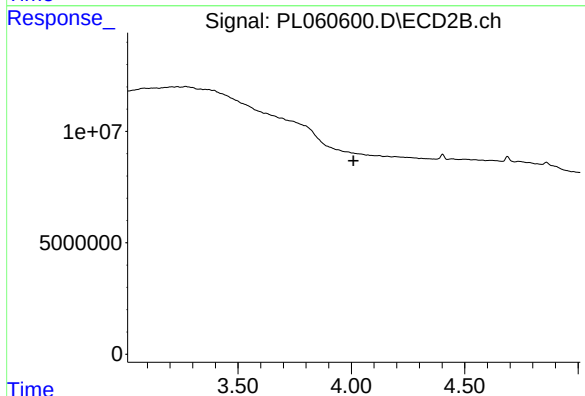


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.010 min
Response: 0
Conc: N.D.

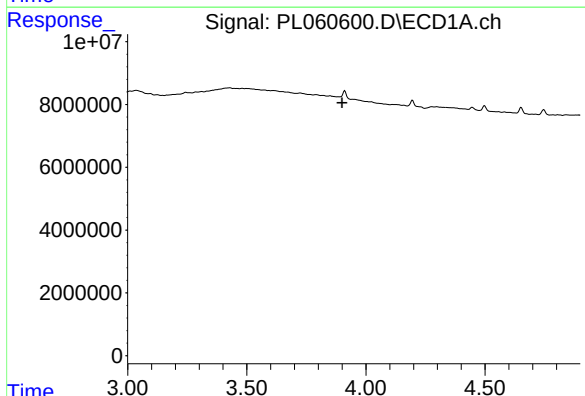


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.900 min
Response: 0
Conc: N.D.

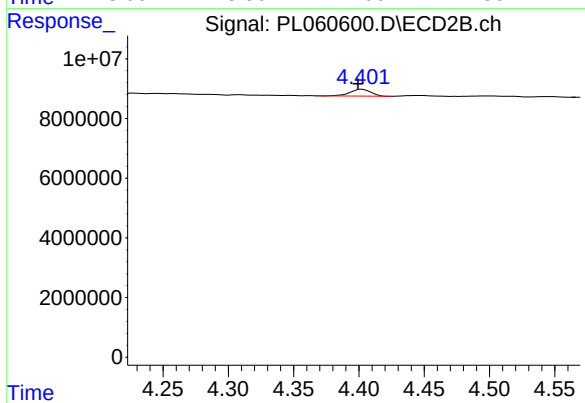

#2 alpha-BHC


R.T.: 4.403 min
Delta R.T.: 0.003 min
Response: 2543955
Conc: 0.62 ng/ml

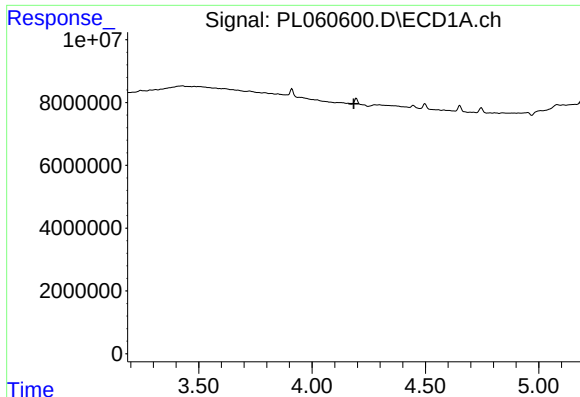

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.184 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

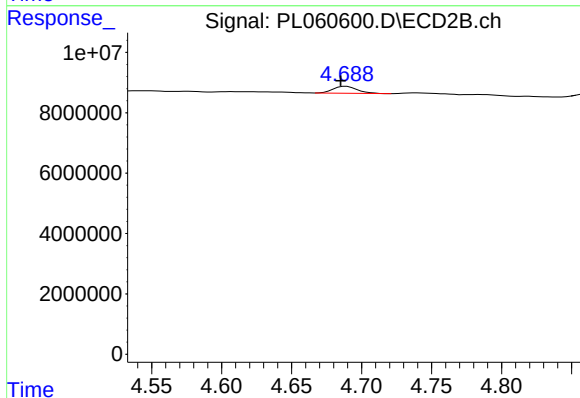


#3 gamma-BHC (Lindane)

R.T.: 4.689 min
Delta R.T.: 0.004 min
Response: 2780649
Conc: 0.72 ng/ml

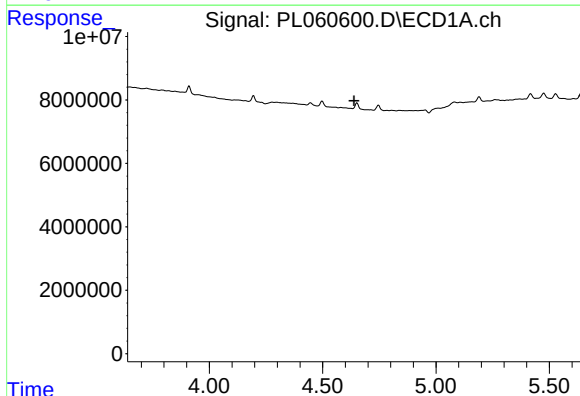


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.639 min
Response: 0
Conc: N.D.

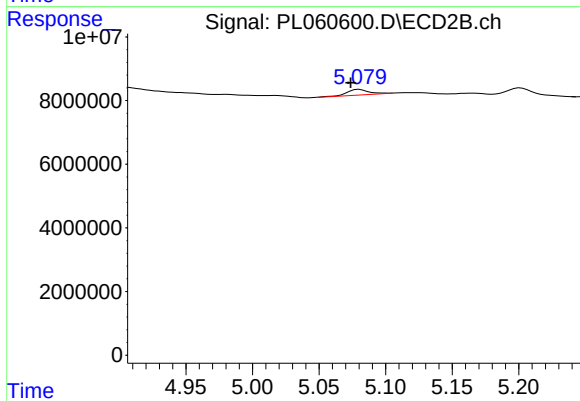

#7 delta-BHC


R.T.: 5.080 min
Delta R.T.: 0.006 min
Response: 2216884
Conc: 0.82 ng/ml

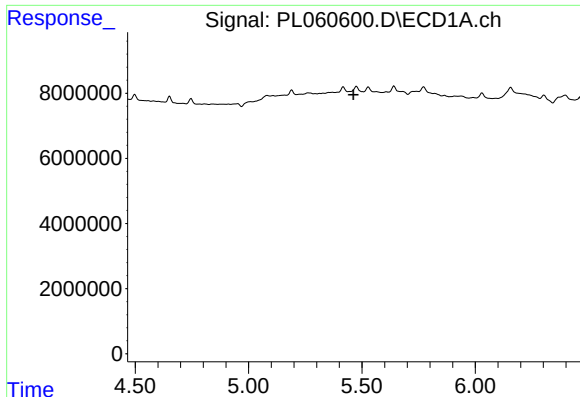

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

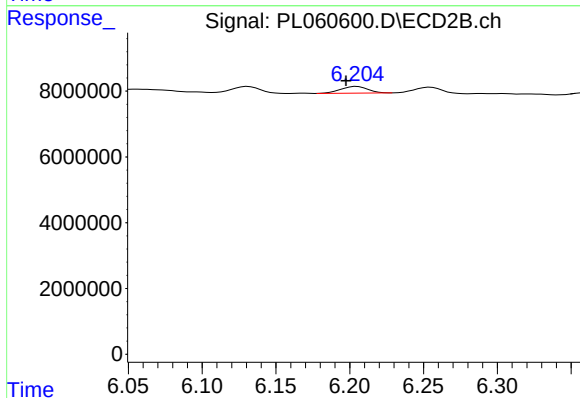


#11 alpha-Chlordane

R.T.: 6.205 min
Delta R.T.: 0.007 min
Response: 2557490
Conc: 0.83 ng/ml

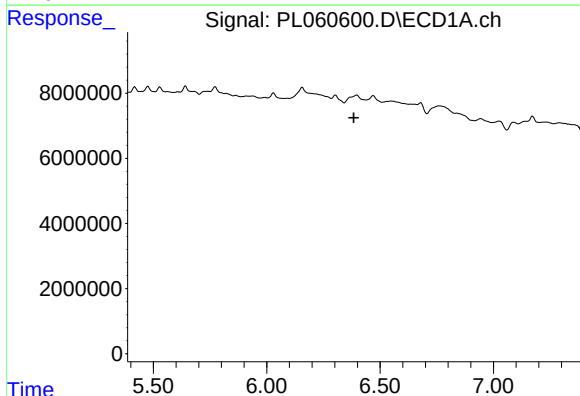


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.385 min
Response: 0
Conc: N.D.

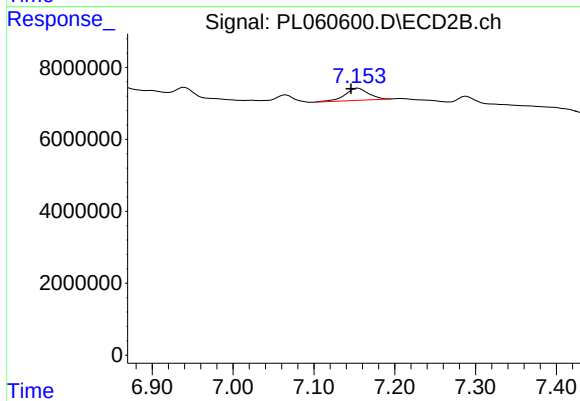

#17 4,4'-DDT


R.T.: 7.155 min
Delta R.T.: 0.009 min
Response: 6803600
Conc: 3.11 ng/ml

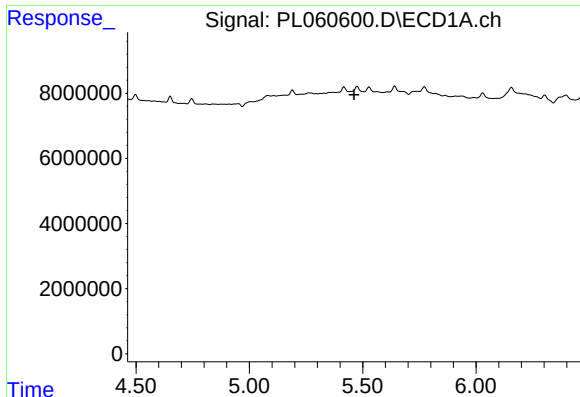

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

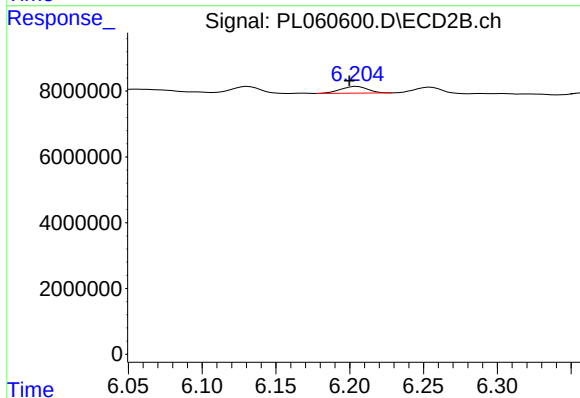


#26 Chlordane-4

R.T.: 6.205 min
Delta R.T.: 0.005 min
Response: 2557490
Conc: 5.90 ng/ml

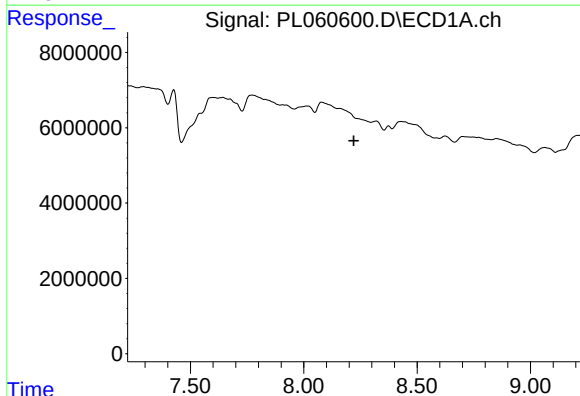

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.220 min
Response: 0
Conc: N.D.

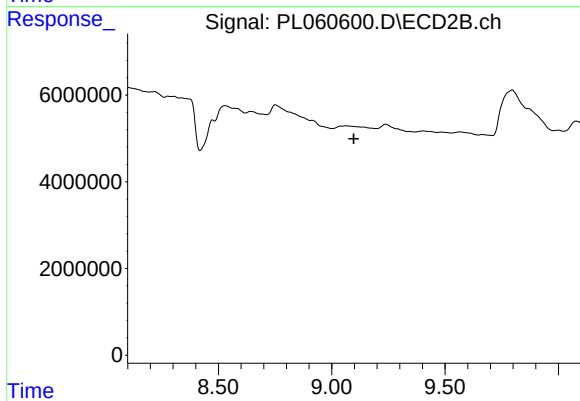

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.098 min
Response: 0
Conc: N.D.