

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081120\
 Data File : PL060608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2020 13:09
 Operator : DD\AJ
 Sample : L3623-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 13:55:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	42137552	56906309	22.477	21.400
28)	SA Decachlor...	8.220	9.099	38357814	38722976	21.015	20.639
Target Compounds							
3)	MA gamma-BHC...	4.188	4.666f	4549966	5748573	1.718	1.498
9)	A Endosulfan I	5.536f	0.000	21918800	0	11.119	N.D. #
10)	B gamma-Chl...	0.000	6.112	0	8363434	N.D.	2.766 #
15)	B Endosulfa...	0.000	6.946	0	11626413	N.D.	4.457 #
16)	A 4,4'-DDD	0.000	6.842	0	9985961	N.D.	4.352 #
23)	Chlordane-1	4.336	0.000	4357843	0	80.096	N.D. #
25)	Chlordane-3	0.000	6.112	0	8363434	N.D.	23.097 #
27)	Chlordane-5	0.000	6.992	0	1120586	N.D.	15.289 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081120\
Data File : PL060608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2020 13:09
Operator : DD\AJ
Sample : L3623-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 13:55:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

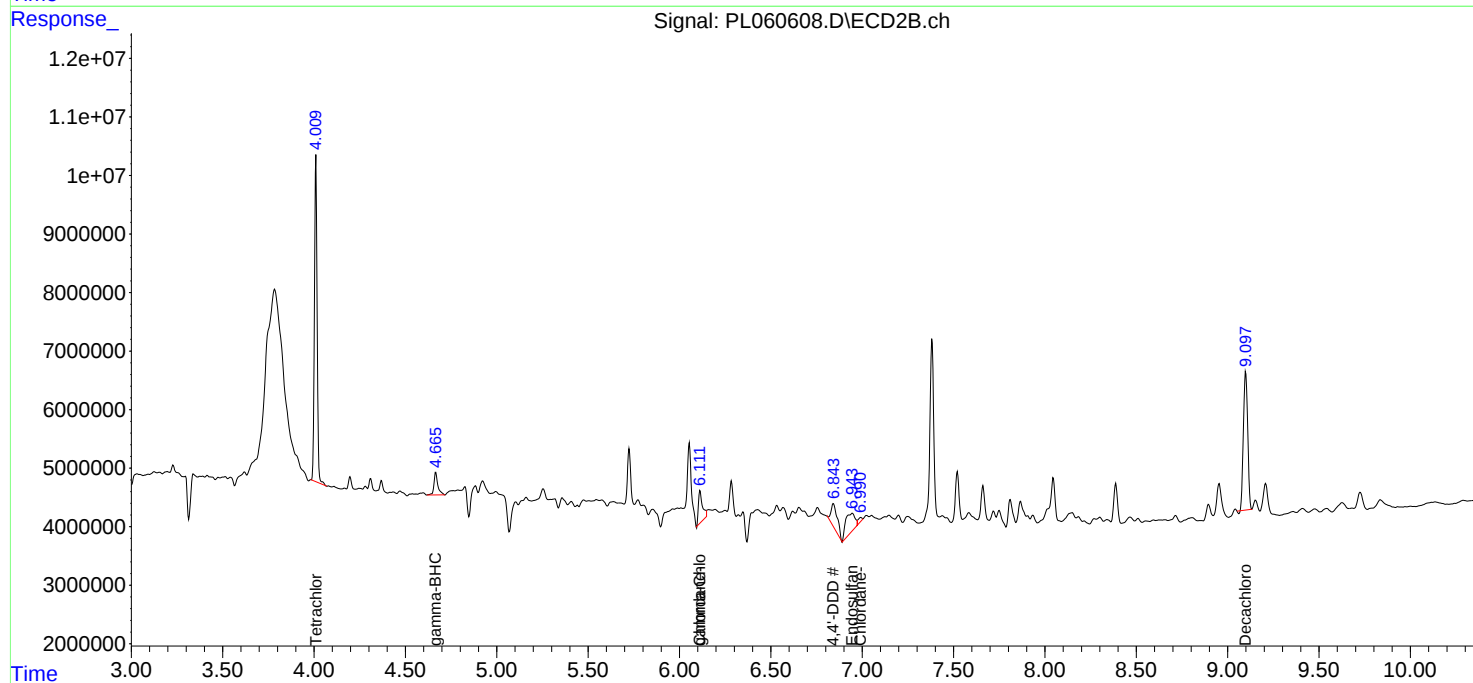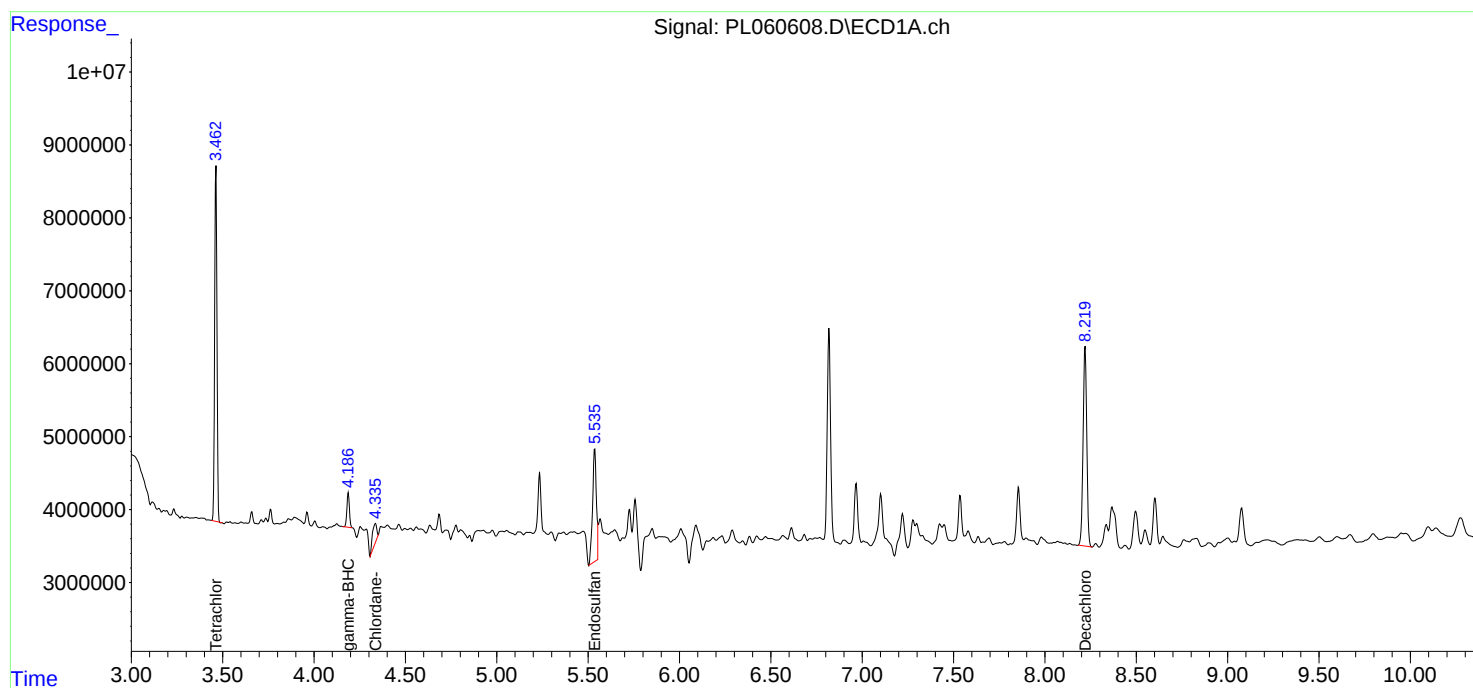


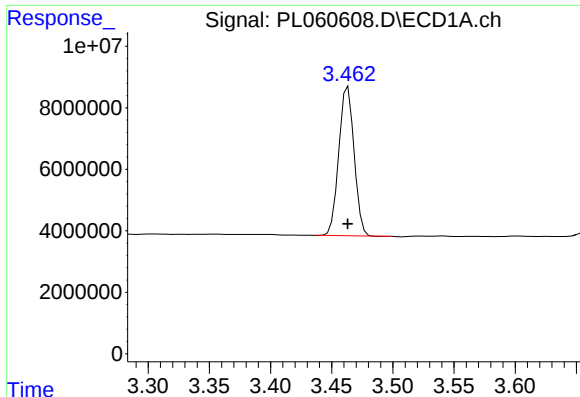

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 42137552
Conc: 22.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

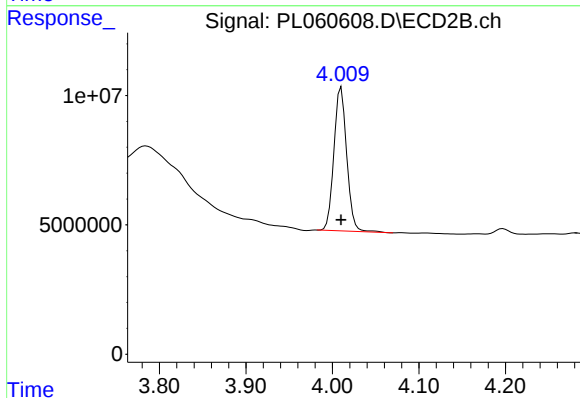


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 56906309
Conc: 21.40 ng/ml

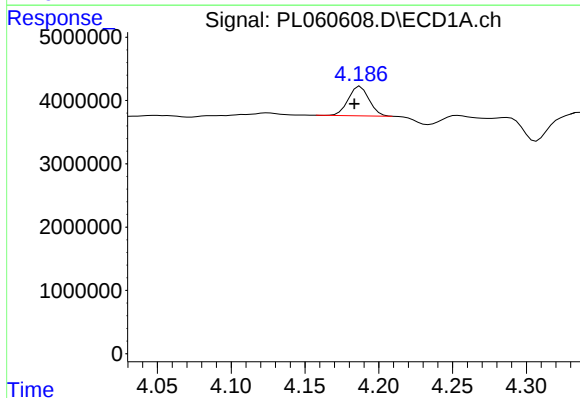


#3 gamma-BHC (Lindane)

R.T.: 4.188 min
Delta R.T.: 0.004 min
Response: 4549966
Conc: 1.72 ng/ml

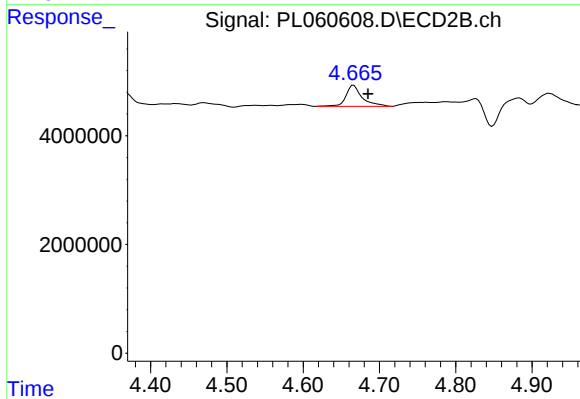

#3 gamma-BHC (Lindane)


R.T.: 4.666 min
Delta R.T.: -0.019 min
Response: 5748573
Conc: 1.50 ng/ml

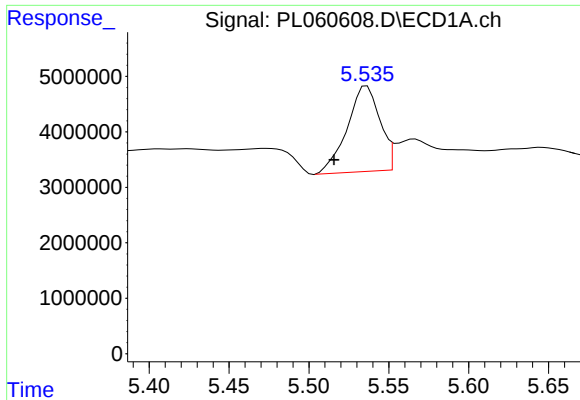

#9 Endosulfan I


R.T.: 5.536 min
Delta R.T.: 0.021 min
Response: 21918800
Conc: 11.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

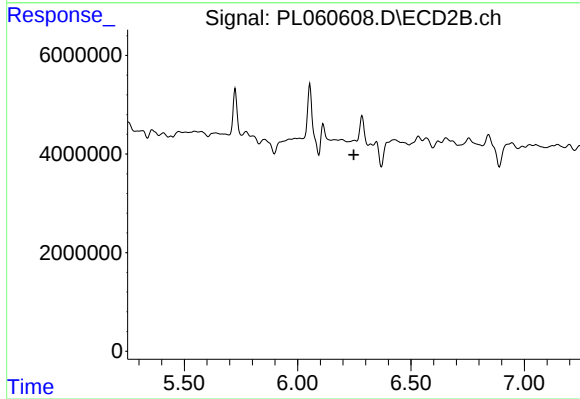


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

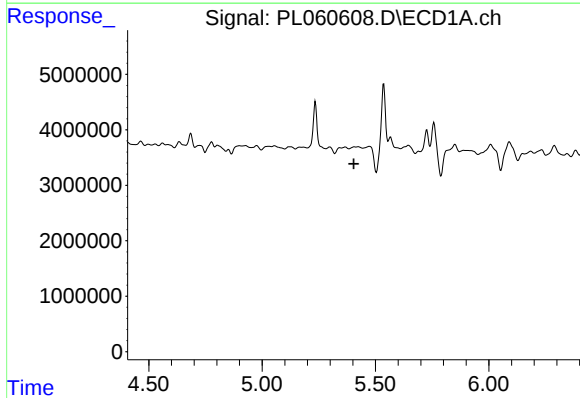


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

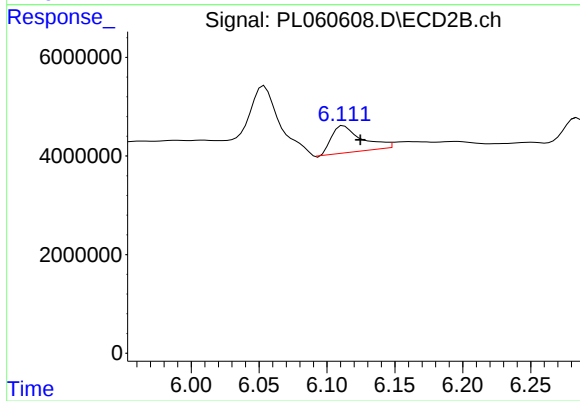

#10 gamma-Chlordane


R.T.: 6.112 min
Delta R.T.: -0.012 min
Response: 8363434
Conc: 2.77 ng/ml

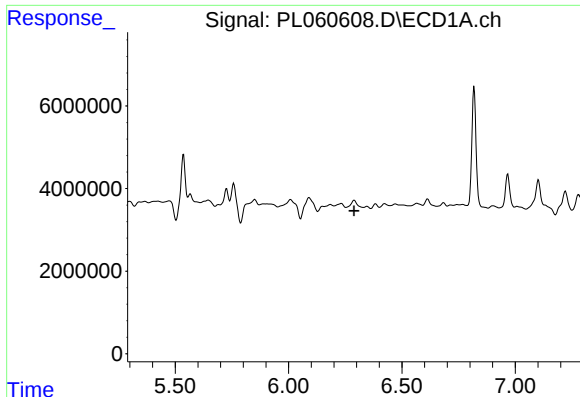

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

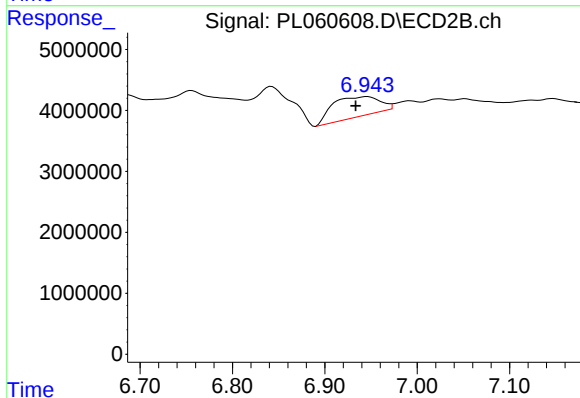


#15 Endosulfan II

R.T.: 6.946 min
Delta R.T.: 0.013 min
Response: 11626413
Conc: 4.46 ng/ml

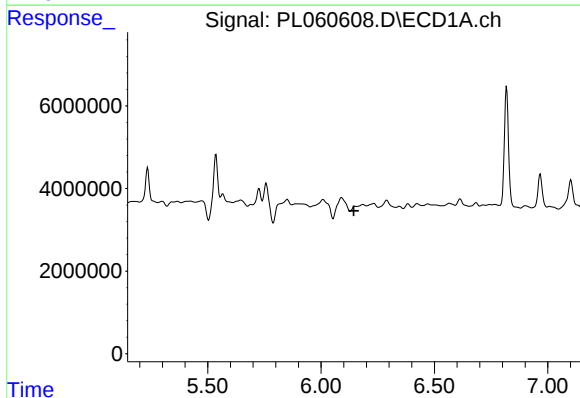


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.144 min
Response: 0
Conc: N.D.

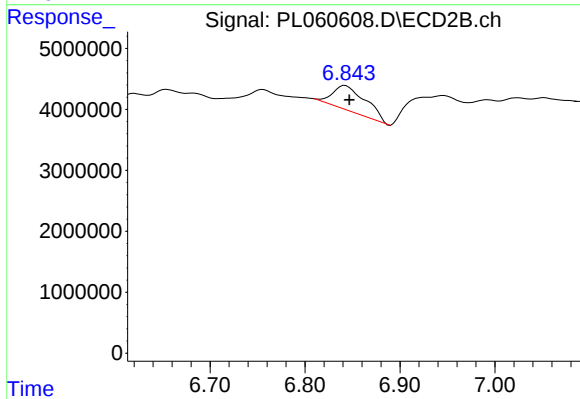

#16 4,4'-DDD


R.T.: 6.842 min
Delta R.T.: -0.005 min
Response: 9985961
Conc: 4.35 ng/ml

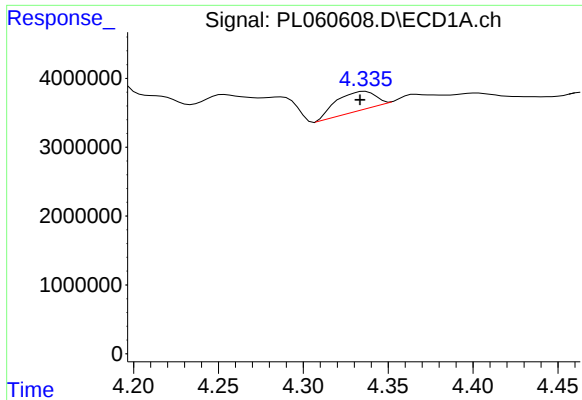

#23 Chlordane-1


R.T.: 4.336 min
Delta R.T.: 0.003 min
Response: 4357843
Conc: 80.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

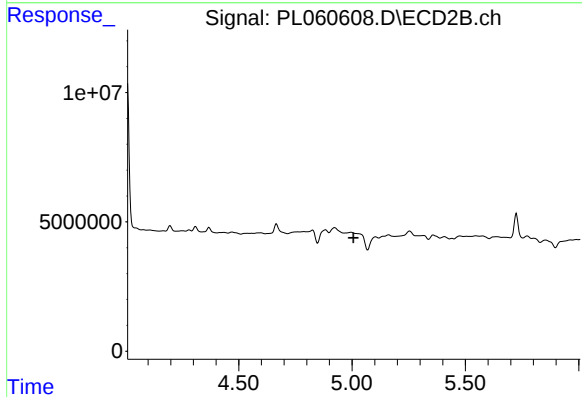


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.007 min
Response: 0
Conc: N.D.

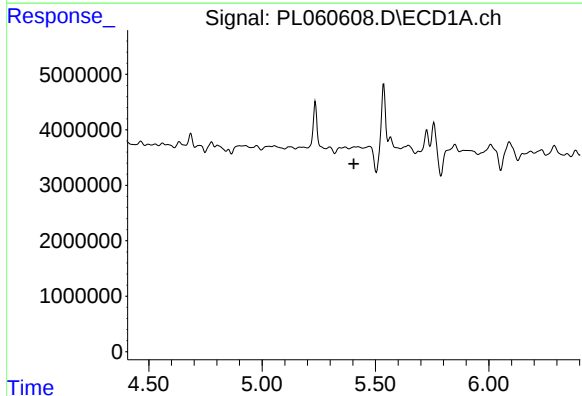


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.404 min
Response: 0
Conc: N.D.

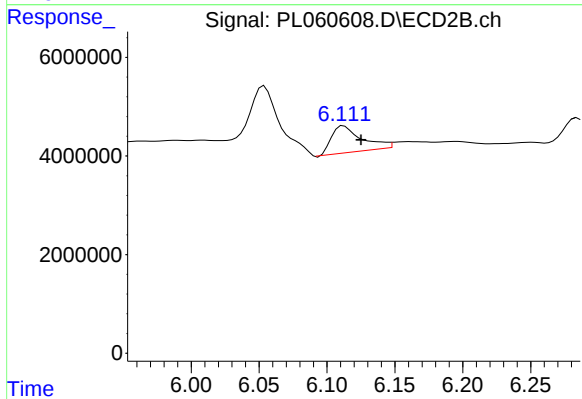

#25 Chlordane-3


R.T.: 6.112 min
Delta R.T.: -0.013 min
Response: 8363434
Conc: 23.10 ng/ml

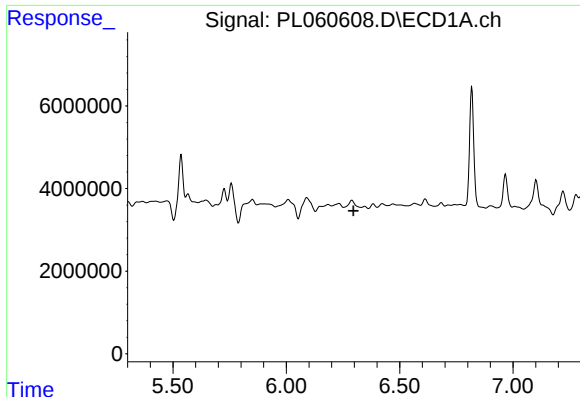

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.297 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

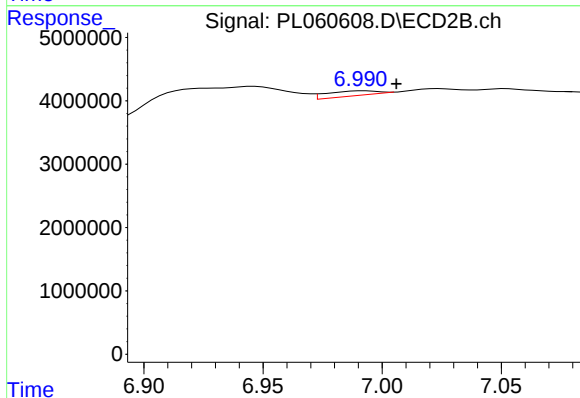


#27 Chlordane-5

R.T.: 6.992 min
Delta R.T.: -0.014 min
Response: 1120586
Conc: 15.29 ng/ml

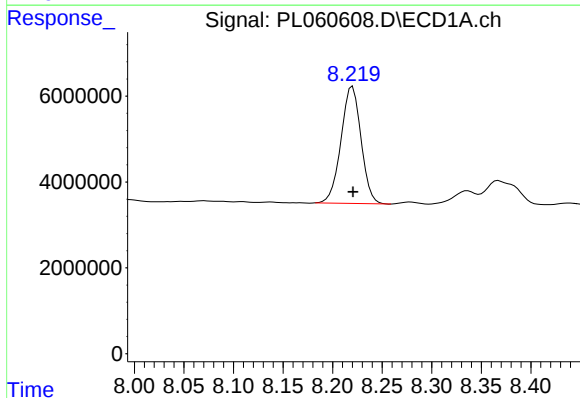

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 38357814
Conc: 21.01 ng/ml

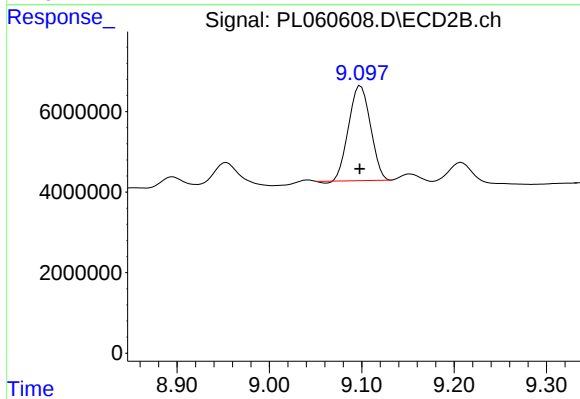

#28 Decachlorobiphenyl

R.T.: 9.099 min
Delta R.T.: 0.001 min
Response: 38722976
Conc: 20.64 ng/ml