

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL081120\  
 Data File : PL060608.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 11 Aug 2020 13:09  
 Operator : DD\AJ  
 Sample : L3623-03  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 STP-7A

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Aug 11 13:55:44 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL081020.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Aug 11 01:39:18 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|--------|
| -----                       |                 |       |       |          |          |        |        |
| System Monitoring Compounds |                 |       |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.463 | 4.010 | 42137552 | 56906309 | 22.477 | 21.400 |
| 28)                         | SA Decachlor... | 8.220 | 9.099 | 38357814 | 38722976 | 21.015 | 20.639 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL081120\  
Data File : PL060608.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 11 Aug 2020 13:09  
Operator : DD\AJ  
Sample : L3623-03  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
STP-7A

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Aug 11 13:55:44 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL081020.M  
Quant Title : GC Extractables  
QLast Update : Tue Aug 11 01:39:18 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

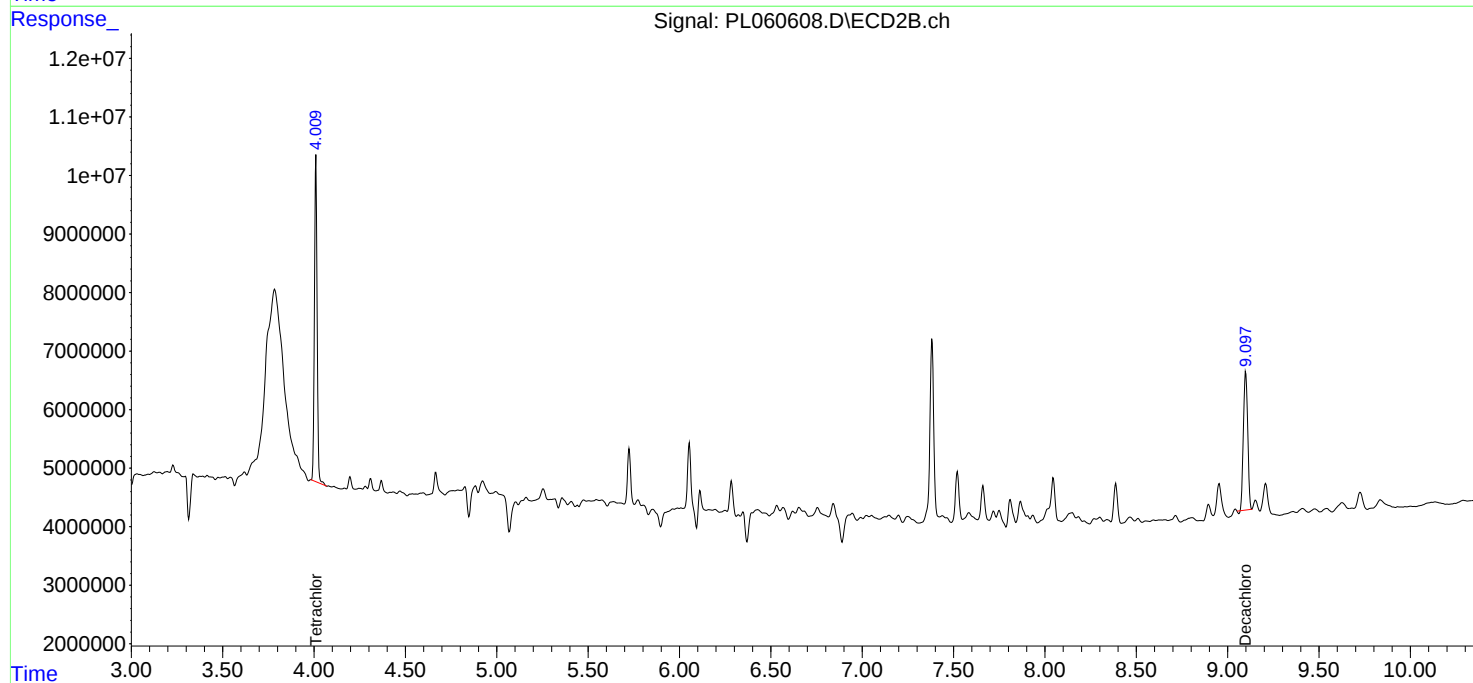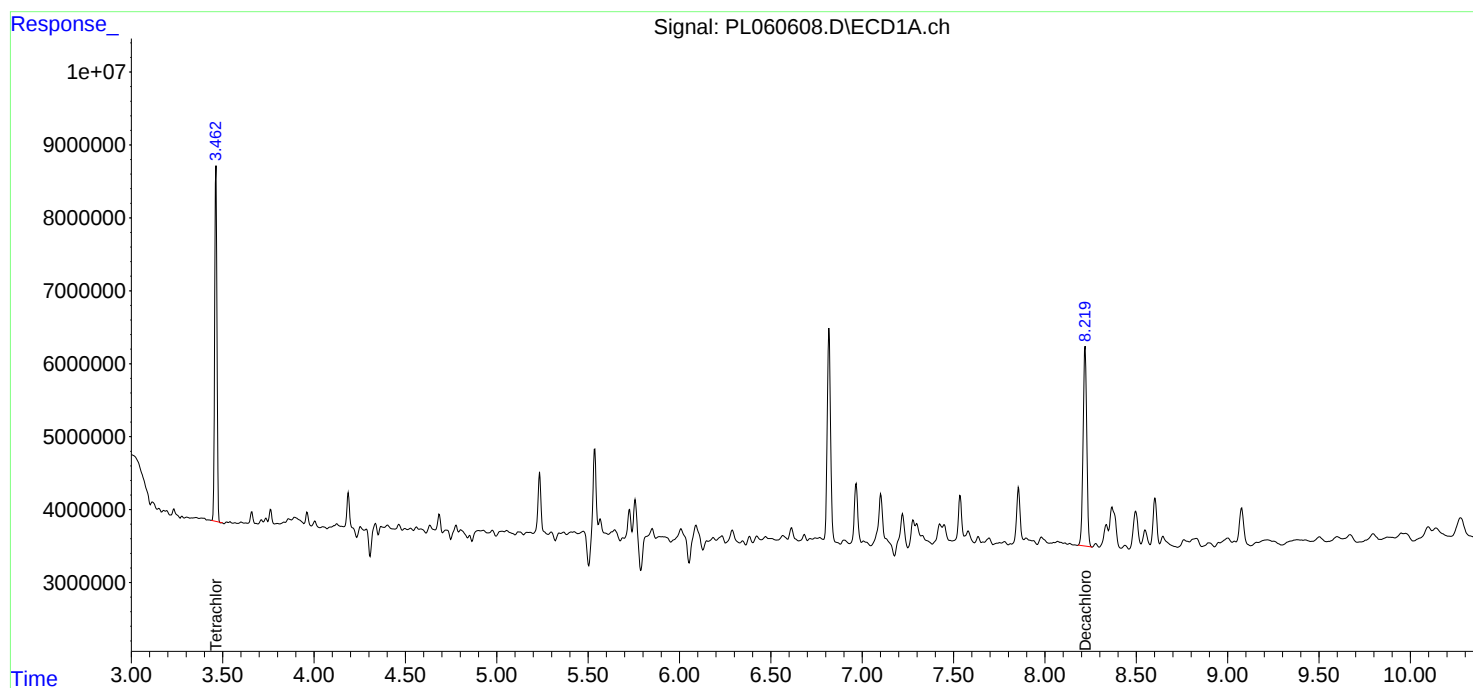


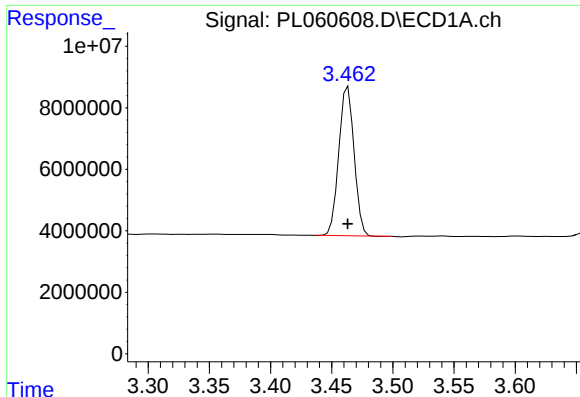

#1 Tetrachloro-m-xylene


R.T.: 3.463 min  
Delta R.T.: 0.000 min  
Response: 42137552  
Conc: 22.48 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
STP-7A

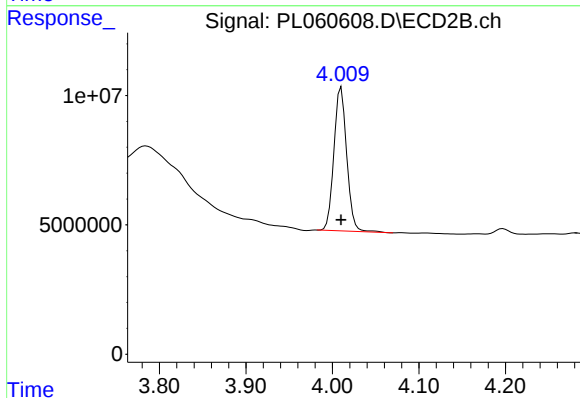


#1 Tetrachloro-m-xylene

R.T.: 4.010 min  
Delta R.T.: 0.000 min  
Response: 56906309  
Conc: 21.40 ng/ml

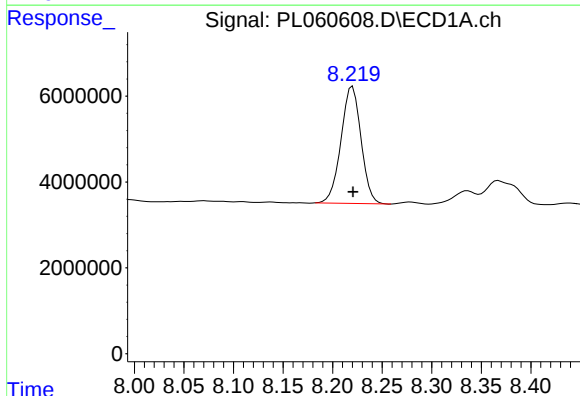

#28 Decachlorobiphenyl

R.T.: 8.220 min  
Delta R.T.: 0.000 min  
Response: 38357814  
Conc: 21.01 ng/ml

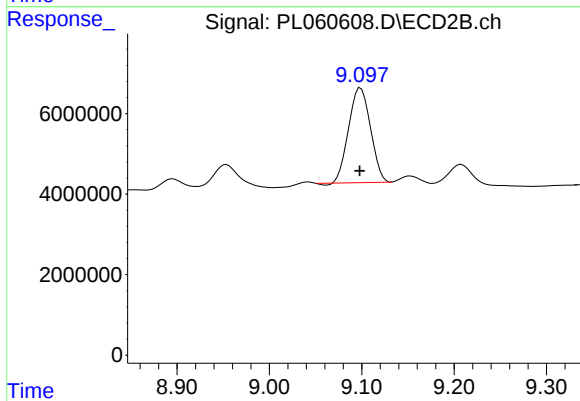

#28 Decachlorobiphenyl

R.T.: 9.099 min  
Delta R.T.: 0.001 min  
Response: 38722976  
Conc: 20.64 ng/ml