

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081121\
 Data File : PL068921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2021 18:38
 Operator : AR\AJ
 Sample : M3343-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210548-COM-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 07:24:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	8255340	23211246	19.958	22.861
28)	SA Decachlor...	10.406	11.489	9772259	17371768	17.004	17.905
Target Compounds							
3)	MA gamma-BHC...	5.776	0.000	598129	0	1.102	N.D. #
8)	B Heptachlo...	0.000	8.034	0	159505	N.D.	0.138 #
9)	A Endosulfan I	0.000	8.452	0	127148	N.D.	0.121 #
10)	B gamma-Chl...	0.000	8.321f	0	287325	N.D.	0.251 #
14)	MA Endrin	8.080f	0.000	316650	0	0.657	N.D. #
15)	B Endosulfa...	0.000	9.214	0	976168	N.D.	1.064 #
18)	B Endrin al...	0.000	9.332	0	124262	N.D.	0.177 #
19)	B Endosulfa...	0.000	9.571	0	196193	N.D.	0.215 #
23)	Chlordane-1	0.000	6.975f	0	645937	N.D.	15.318 #
25)	Chlordane-3	0.000	8.321f	0	287325	N.D.	1.759 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081121\
Data File : PL068921.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2021 18:38
Operator : AR\AJ
Sample : M3343-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
20210548-COM-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 07:24:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

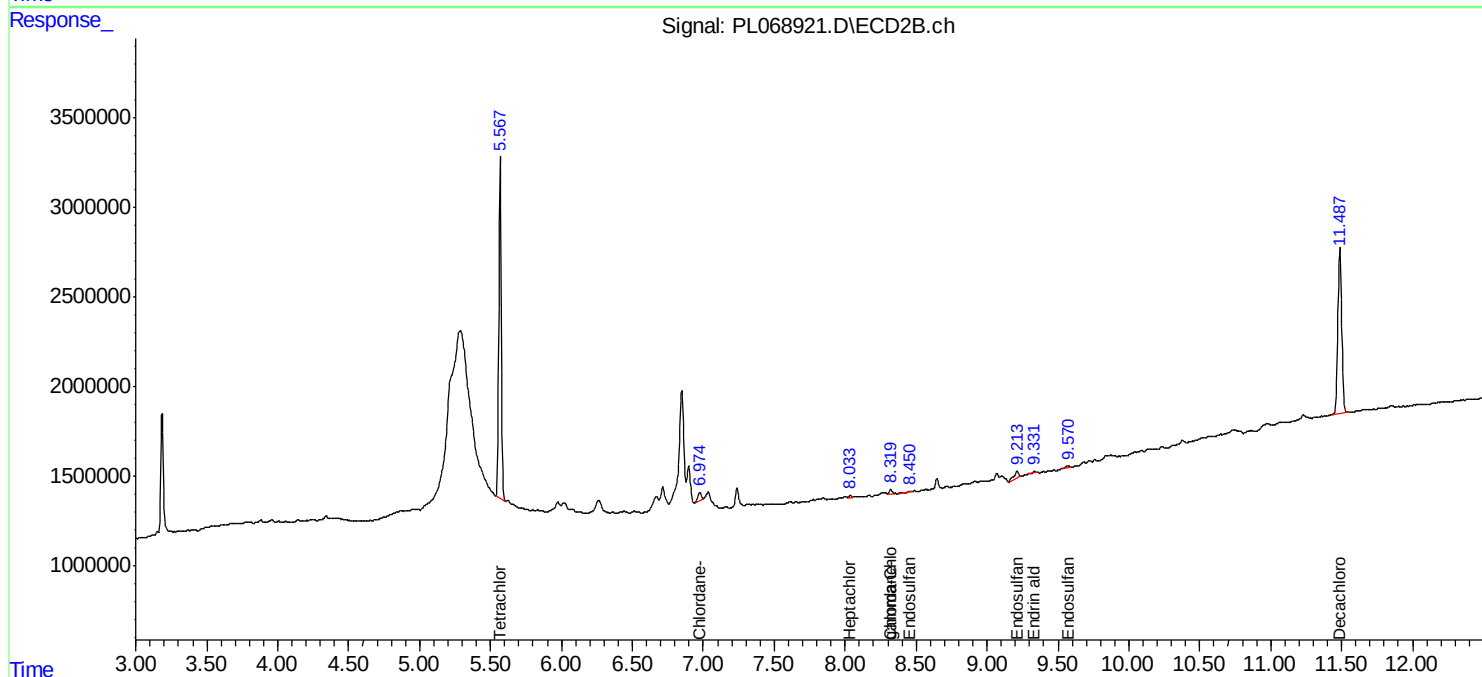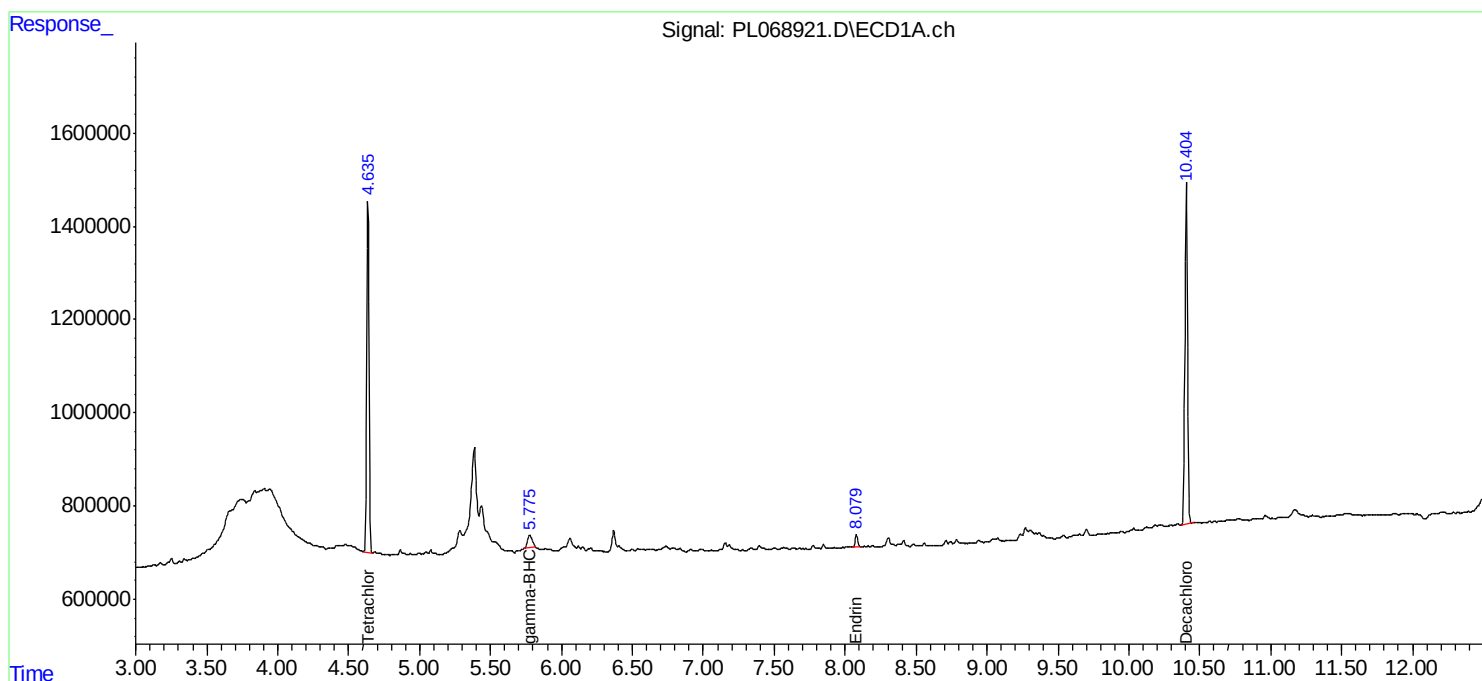


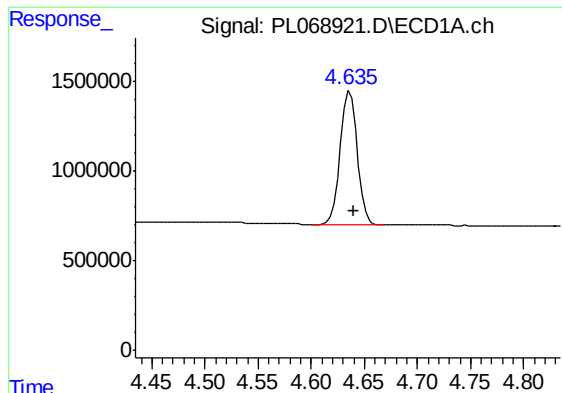

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 8255340
Conc: 19.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210548-COM-21

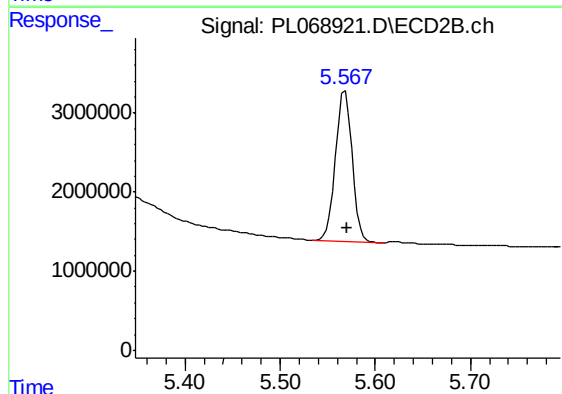


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 23211246
Conc: 22.86 ng/ml

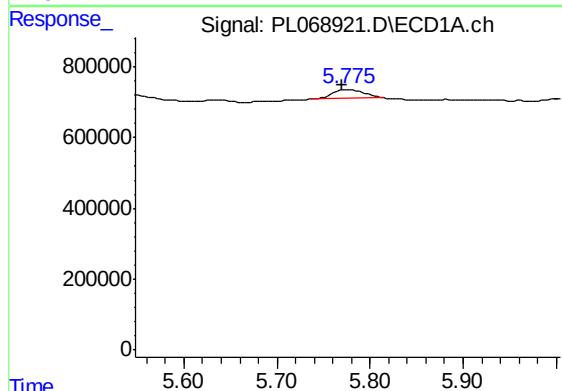


#3 gamma-BHC (Lindane)

R.T.: 5.776 min
Delta R.T.: 0.006 min
Response: 598129
Conc: 1.10 ng/ml

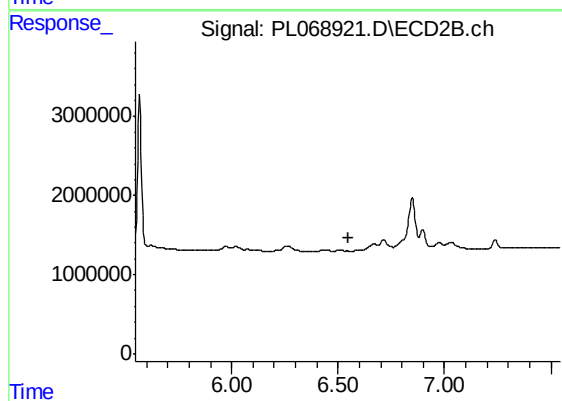

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.547 min
Response: 0
Conc: N.D.

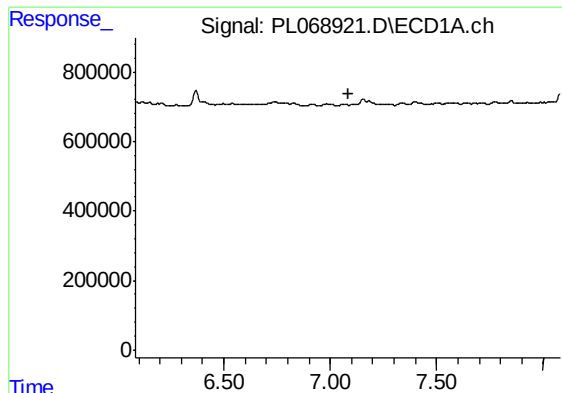

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210548-COM-21

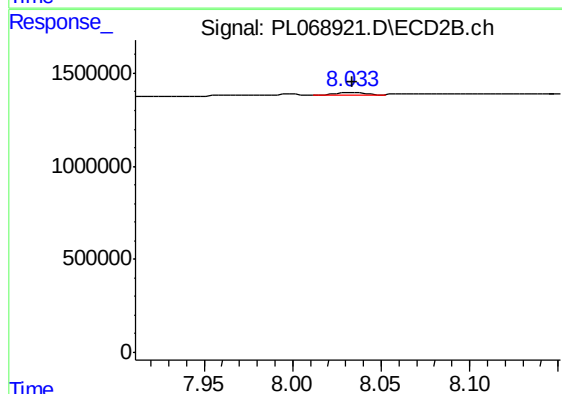


#8 Heptachlor epoxide

R.T.: 8.034 min
Delta R.T.: 0.000 min
Response: 159505
Conc: 0.14 ng/ml

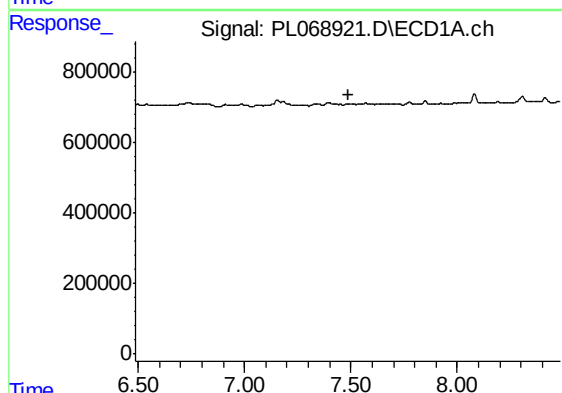


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.487 min
Response: 0
Conc: N.D.

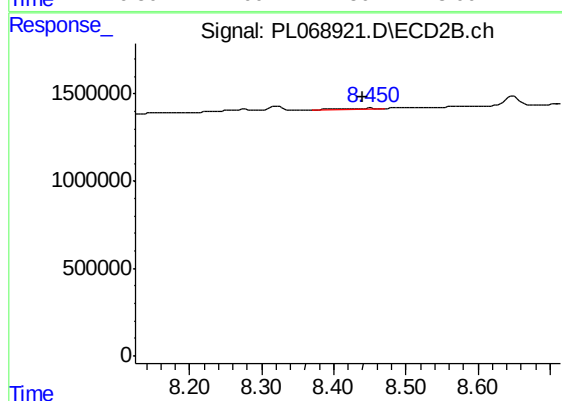

#9 Endosulfan I


R.T.: 8.452 min
Delta R.T.: 0.012 min
Response: 127148
Conc: 0.12 ng/ml

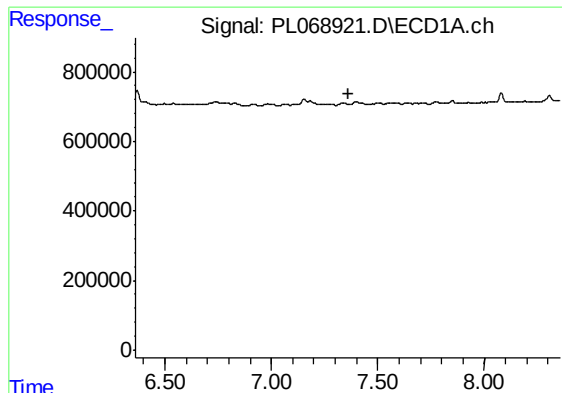

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210548-COM-21

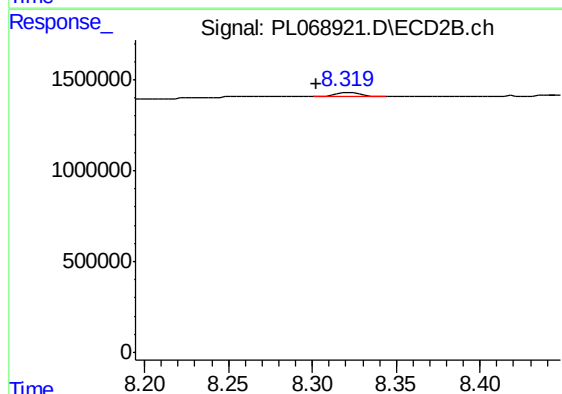


#10 gamma-Chlordane

R.T.: 8.321 min
Delta R.T.: 0.018 min
Response: 287325
Conc: 0.25 ng/ml

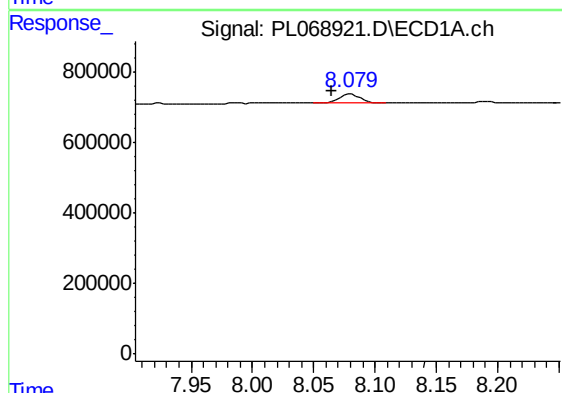


#14 Endrin

R.T.: 8.080 min
Delta R.T.: 0.016 min
Response: 316650
Conc: 0.66 ng/ml

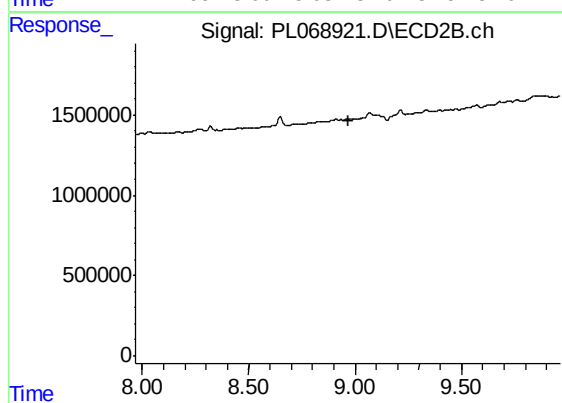

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

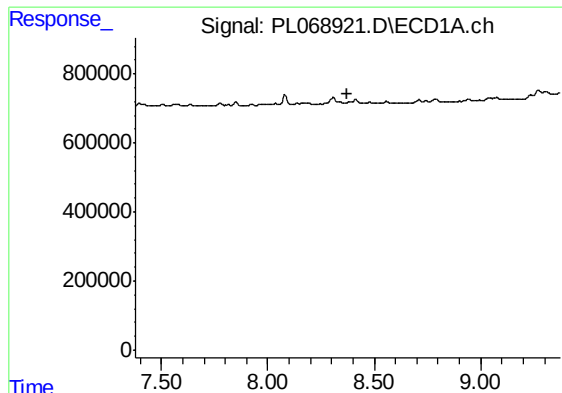

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210548-COM-21

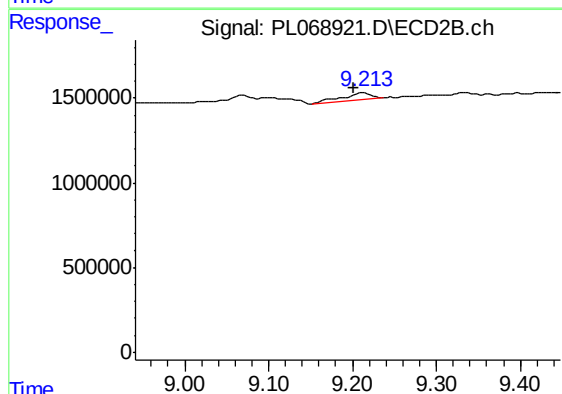


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.012 min
Response: 976168
Conc: 1.06 ng/ml

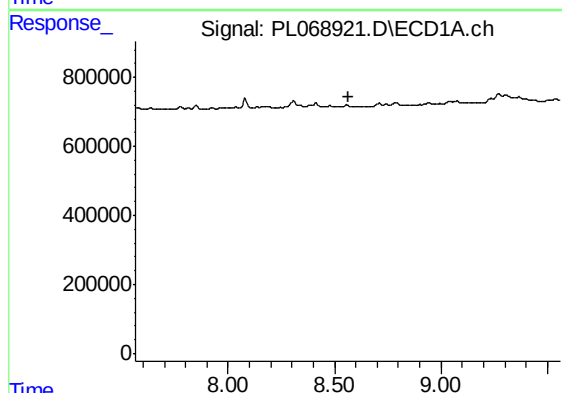


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.564 min
Response: 0
Conc: N.D.

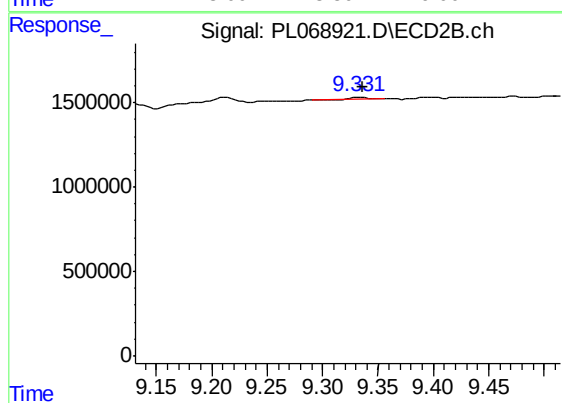

#18 Endrin aldehyde


R.T.: 9.332 min
Delta R.T.: -0.004 min
Response: 124262
Conc: 0.18 ng/ml

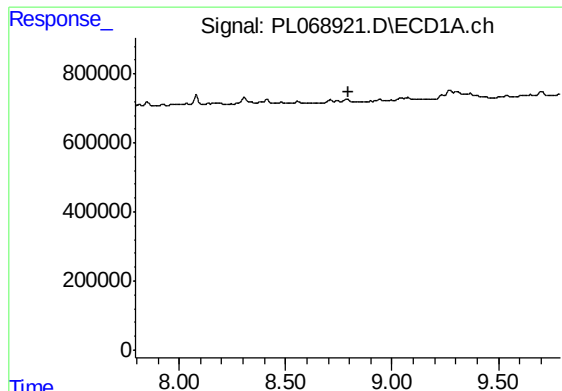

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210548-COM-21

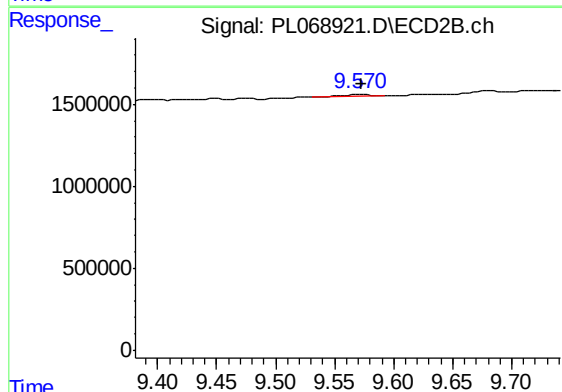


#19 Endosulfan Sulfate

R.T.: 9.571 min
Delta R.T.: -0.002 min
Response: 196193
Conc: 0.22 ng/ml

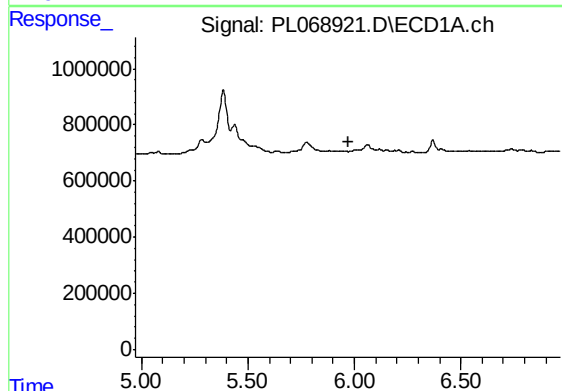

#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.971 min
Response: 0
Conc: N.D.

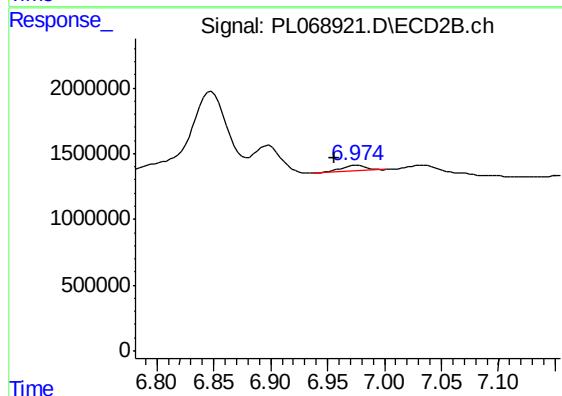

#23 Chlordane-1

R.T.: 6.975 min
Delta R.T.: 0.020 min
Response: 645937
Conc: 15.32 ng/ml

