

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081121\
 Data File : PL068926.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2021 20:01
 Operator : AR\AJ
 Sample : M3343-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20210591-AMENDED-COM-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 07:25:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.637	5.568	7477227	21076759	18.077	20.758
28)	SA Decachlor...	10.405	11.488	9096504	16321268	15.828	16.822
Target Compounds							
2)	A alpha-BHC	0.000	6.140	0	413104	N.D.	0.303 #
8)	B Heptachlo...	0.000	8.031	0	203903	N.D.	0.176 #
10)	B gamma-Chl...	0.000	8.321f	0	966648	N.D.	0.844 #
15)	B Endosulfa...	0.000	9.216	0	1323251	N.D.	1.443 #
18)	B Endrin al...	0.000	9.334	0	148479	N.D.	0.212 #
23)	Chlordane-1	0.000	6.978f	0	564216	N.D.	13.380 #
25)	Chlordane-3	0.000	8.321f	0	966648	N.D.	5.917 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081121\
Data File : PL068926.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2021 20:01
Operator : AR\AJ
Sample : M3343-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 07:25:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

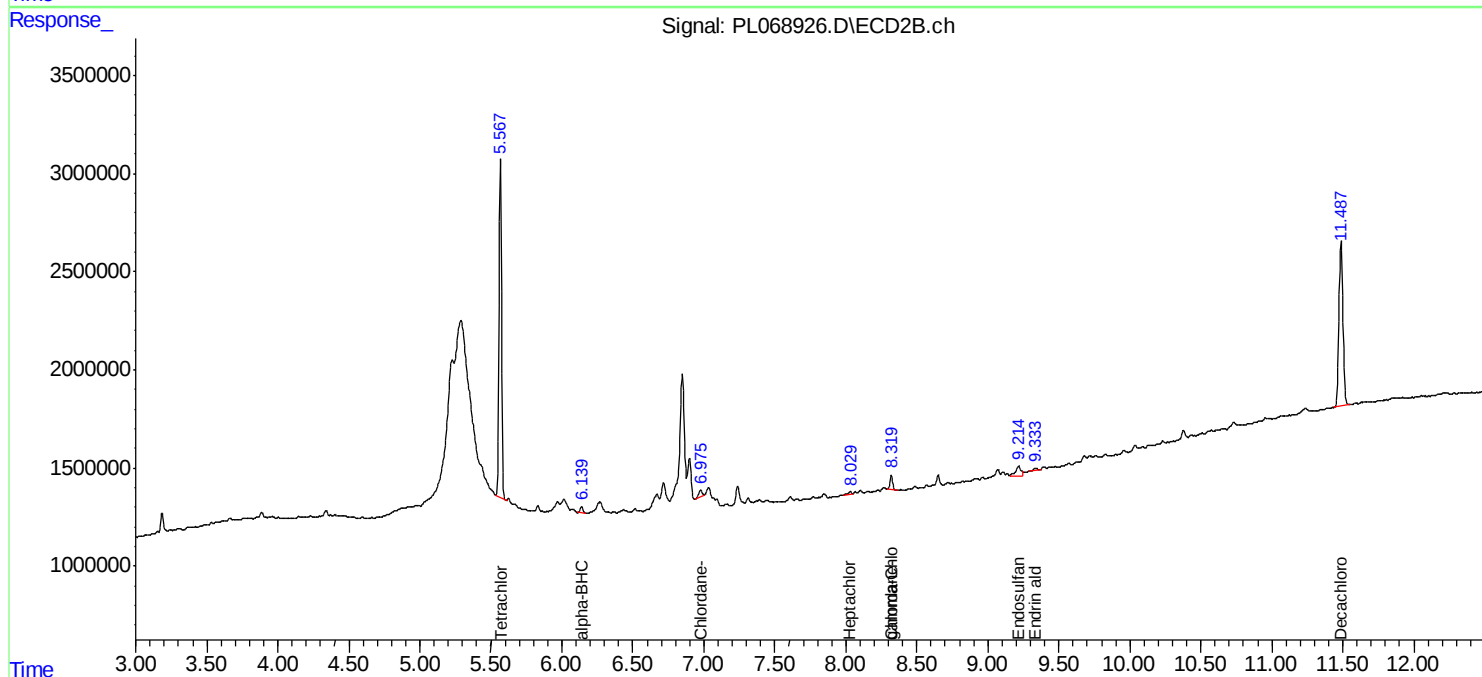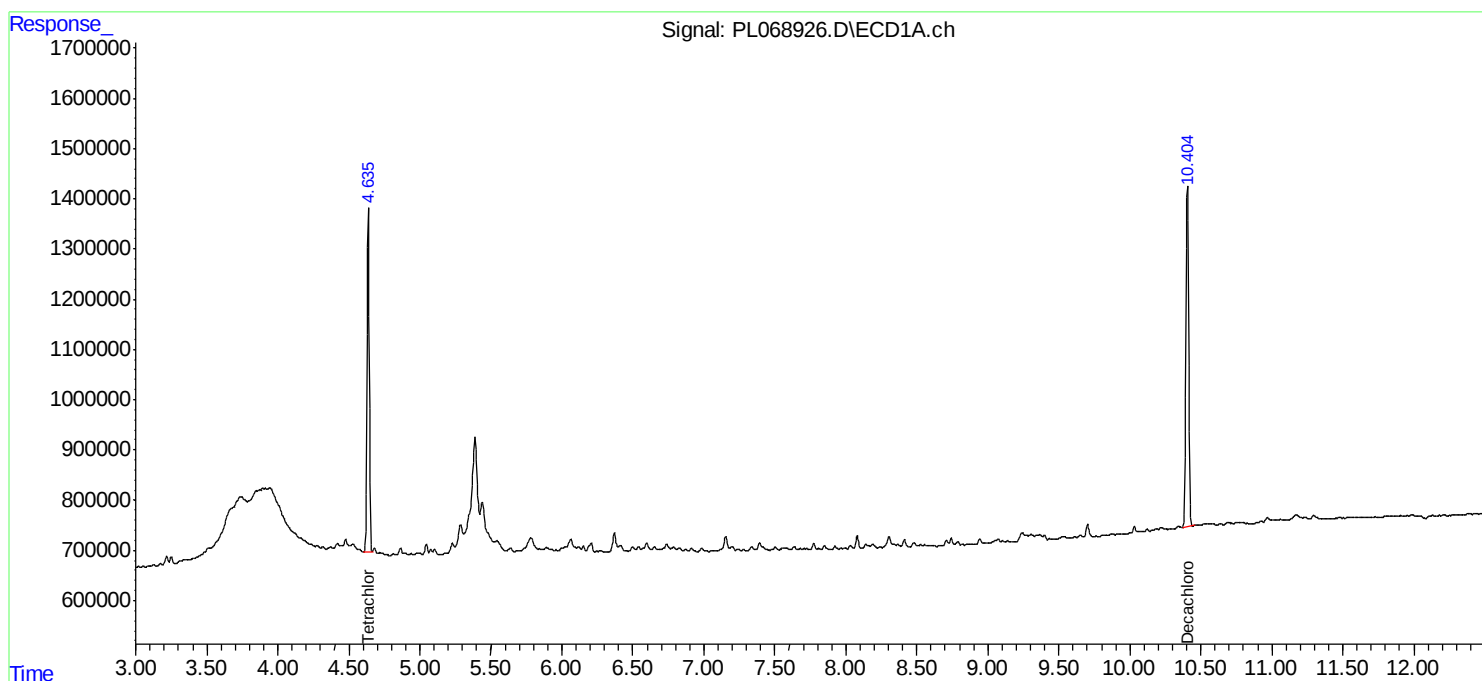


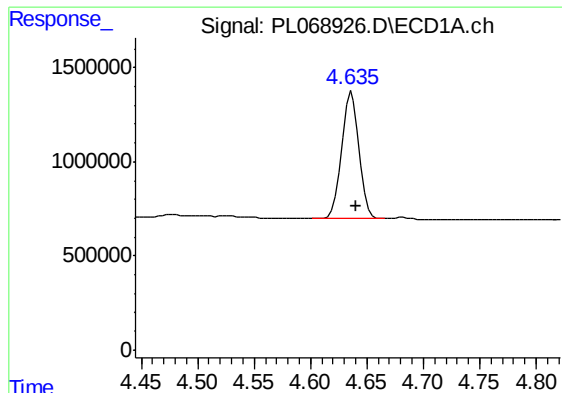

#1 Tetrachloro-m-xylene


R.T.: 4.637 min
Delta R.T.: -0.003 min
Response: 7477227
Conc: 18.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

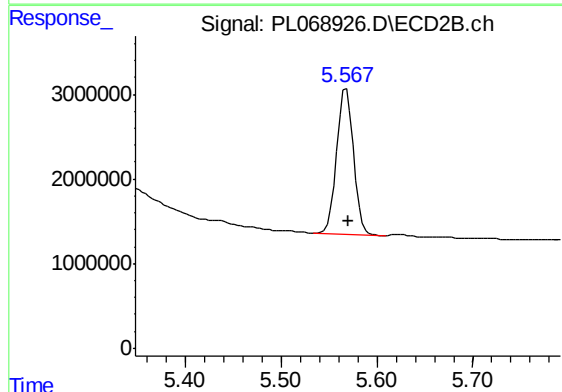


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 21076759
Conc: 20.76 ng/ml

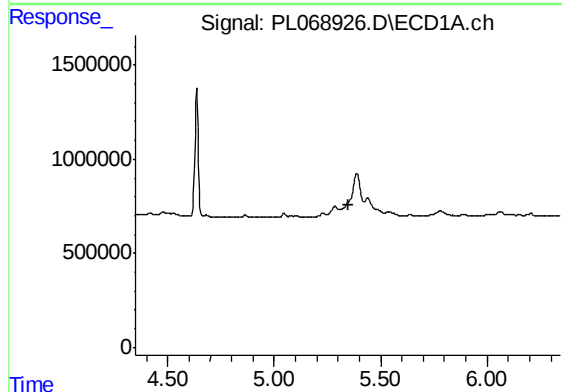


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

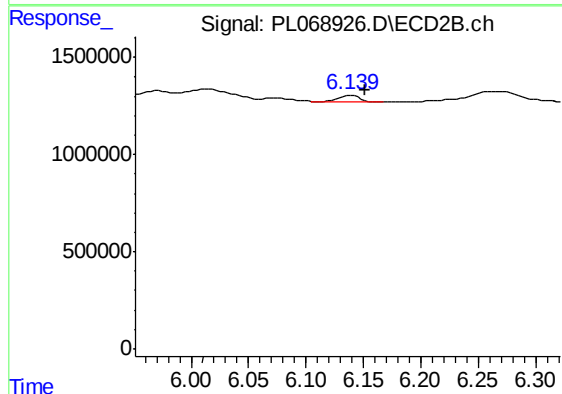

#2 alpha-BHC


R.T.: 6.140 min
Delta R.T.: -0.011 min
Response: 413104
Conc: 0.30 ng/ml

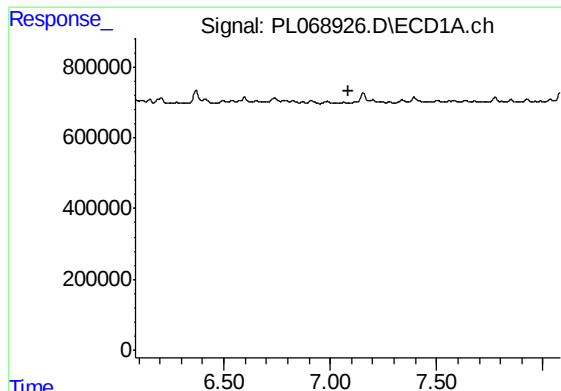

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

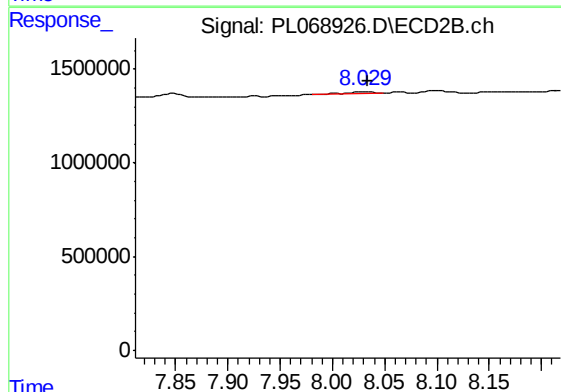


#8 Heptachlor epoxide

R.T.: 8.031 min
Delta R.T.: -0.003 min
Response: 203903
Conc: 0.18 ng/ml

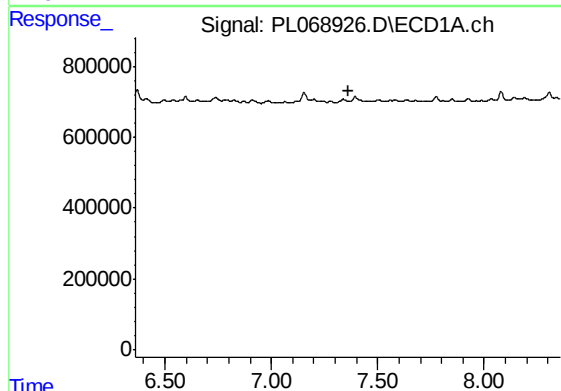


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.361 min
Response: 0
Conc: N.D.

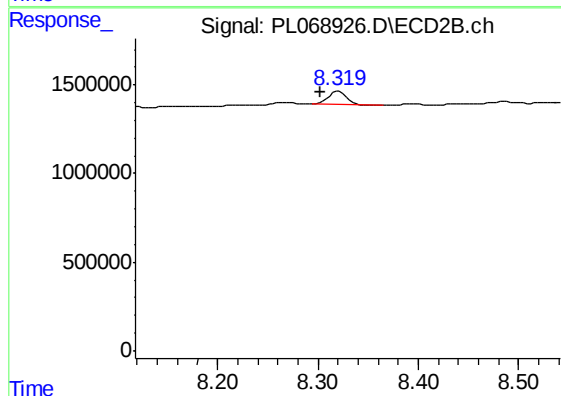

#10 gamma-Chlordane


R.T.: 8.321 min
Delta R.T.: 0.018 min
Response: 966648
Conc: 0.84 ng/ml

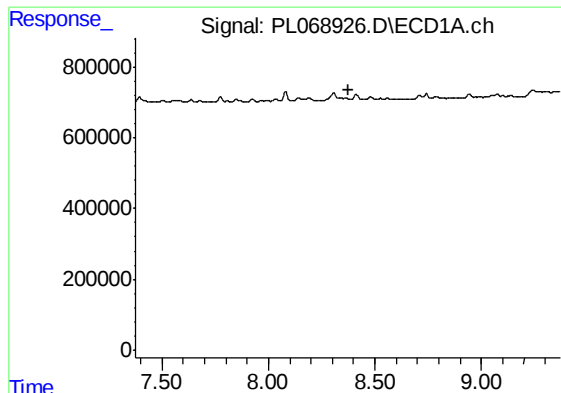

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

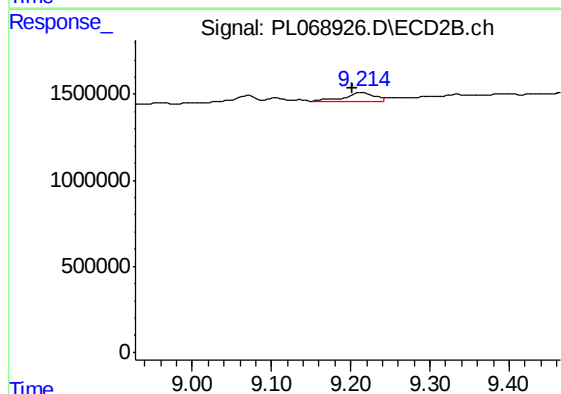


#15 Endosulfan II

R.T.: 9.216 min
Delta R.T.: 0.014 min
Response: 1323251
Conc: 1.44 ng/ml

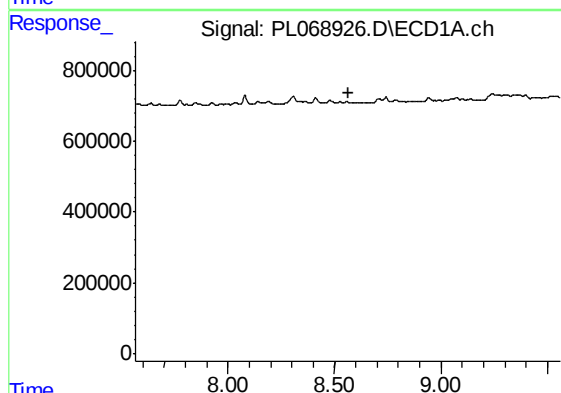


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.564 min
Response: 0
Conc: N.D.

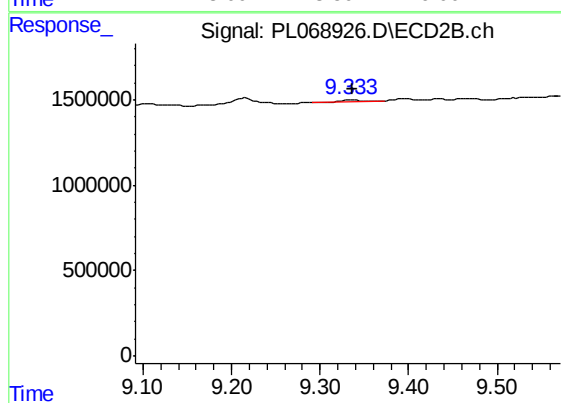

#18 Endrin aldehyde


R.T.: 9.334 min
Delta R.T.: -0.002 min
Response: 148479
Conc: 0.21 ng/ml

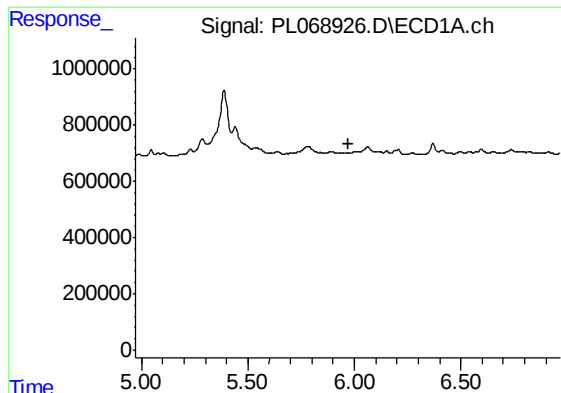

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

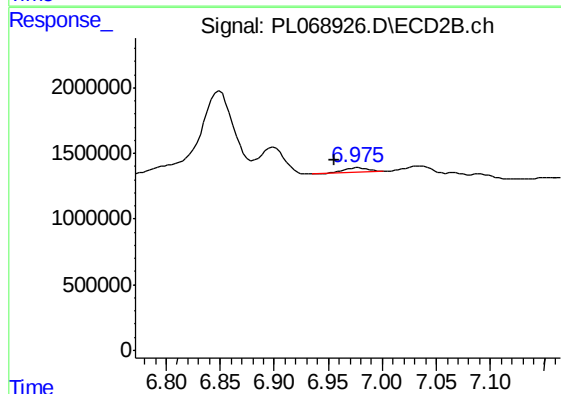


#23 Chlordane-1

R.T.: 6.978 min
Delta R.T.: 0.022 min
Response: 564216
Conc: 13.38 ng/ml

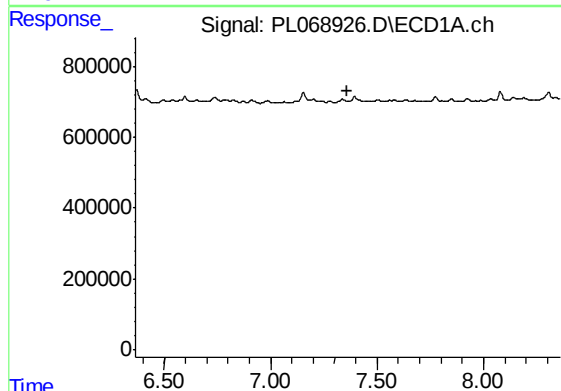


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

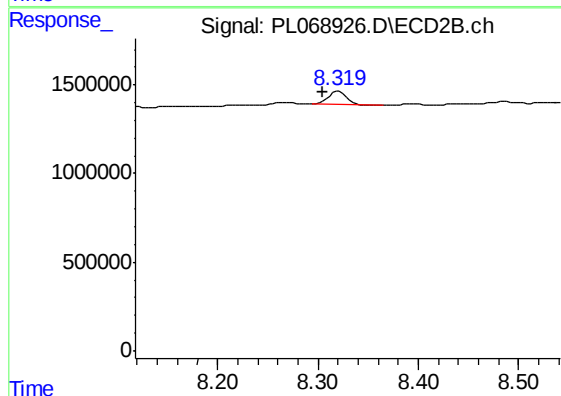

#25 Chlordane-3


R.T.: 8.321 min
Delta R.T.: 0.016 min
Response: 966648
Conc: 5.92 ng/ml

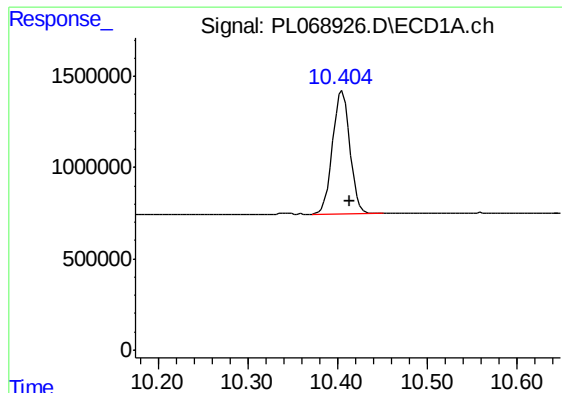

#28 Decachlorobiphenyl

R.T.: 10.405 min
Delta R.T.: -0.008 min
Response: 9096504
Conc: 15.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
20210591-AMENDED-COM-5

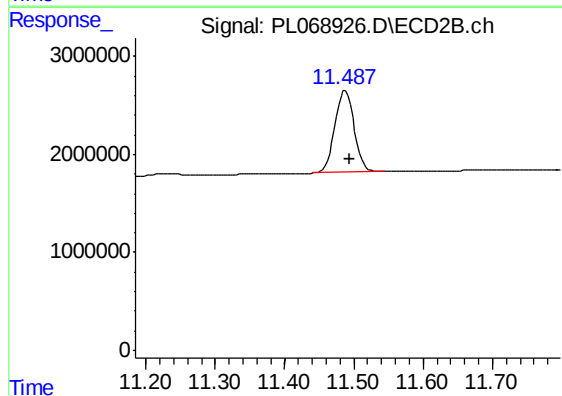

#28 Decachlorobiphenyl

R.T.: 11.488 min
Delta R.T.: -0.007 min
Response: 16321268
Conc: 16.82 ng/ml