

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
 Data File : PL077023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 09:27
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:05:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.665f	0	188326	N.D.	0.066 #
28)	SA Decachlor...	0.000	7.723f	0	181876	N.D.	0.081 #
Target Compounds							
8)	B Heptachlo...	5.574	0.000	5953178	0	5.896	N.D. #
9)	A Endosulfan I	0.000	4.953f	0	102312	N.D.	0.037 #
14)	MA Endrin	0.000	5.489f	0	2370075	N.D.	0.933 #
15)	B Endosulfa...	0.000	5.761	0	503575	N.D.	0.192 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
Data File : PL077023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 09:27
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:05:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

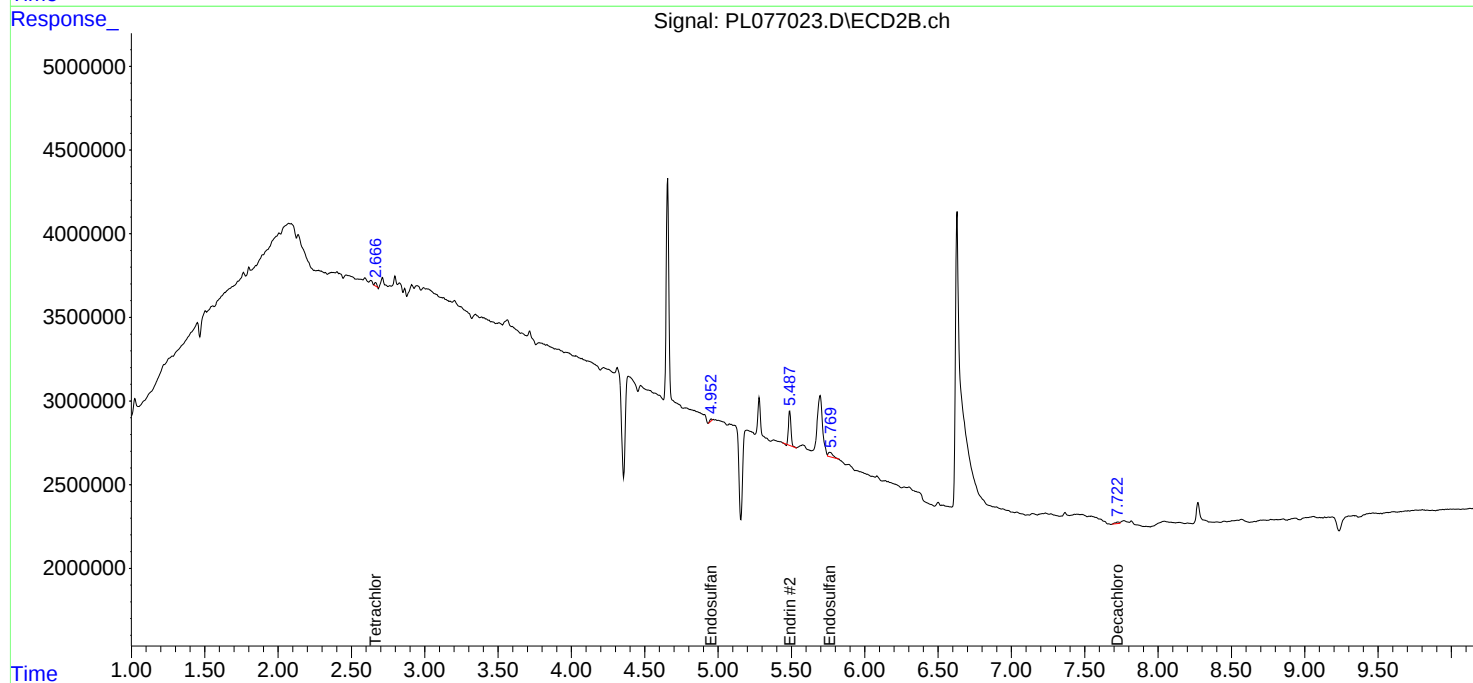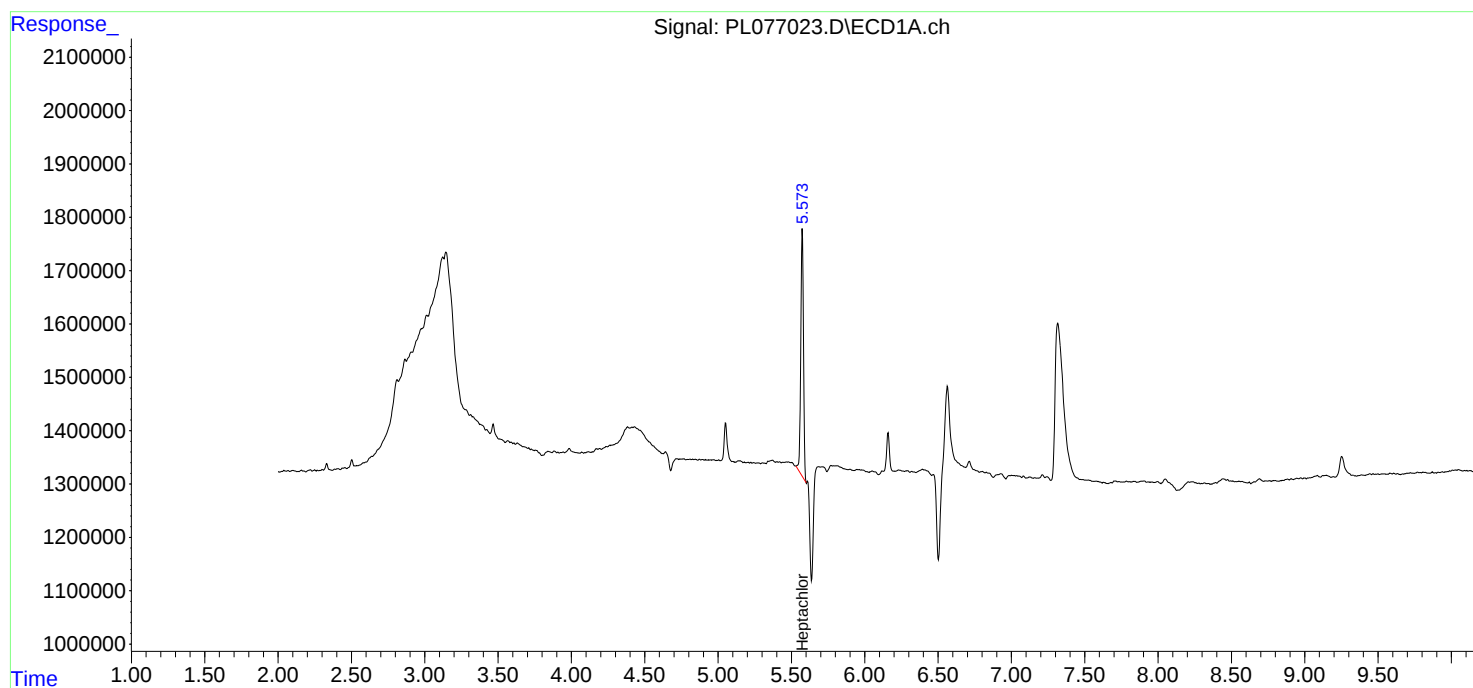


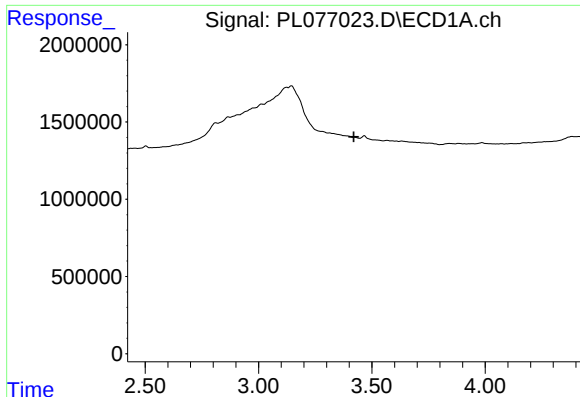

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.420 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

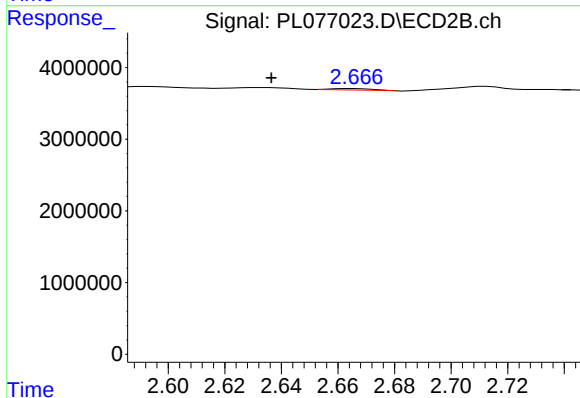


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: 0.028 min
Response: 188326
Conc: 0.07 ng/ml

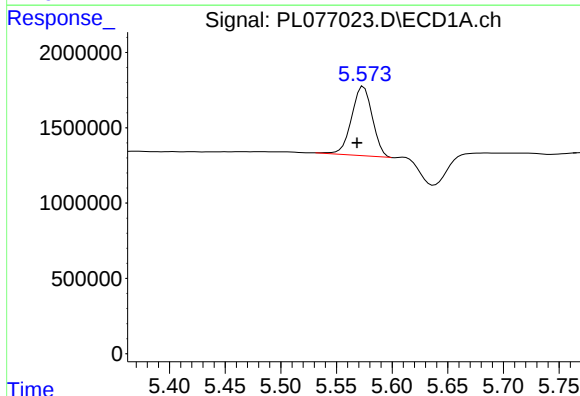


#8 Heptachlor epoxide

R.T.: 5.574 min
Delta R.T.: 0.006 min
Response: 5953178
Conc: 5.90 ng/ml

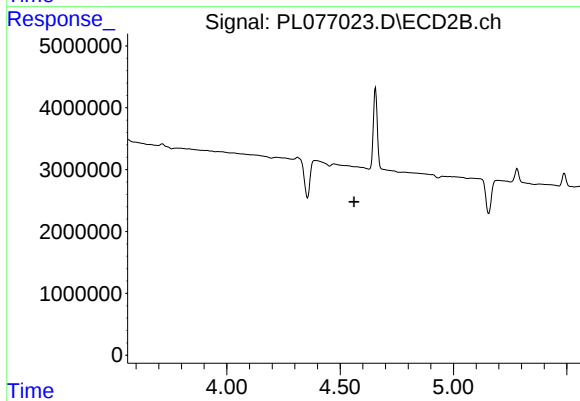

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.561 min
Response: 0
Conc: N.D.

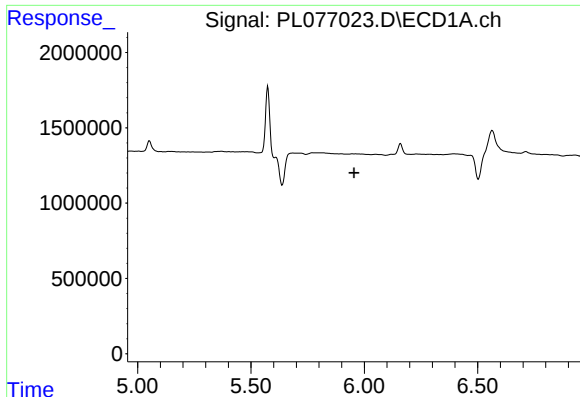

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

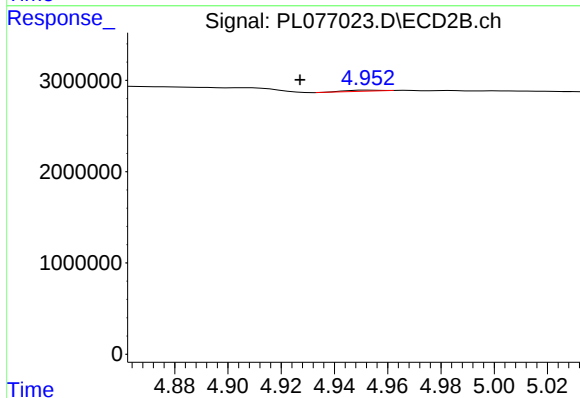


#9 Endosulfan I

R.T.: 4.953 min
Delta R.T.: 0.026 min
Response: 102312
Conc: 0.04 ng/ml

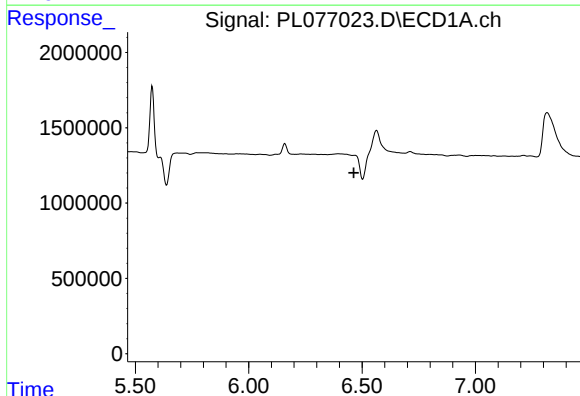


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

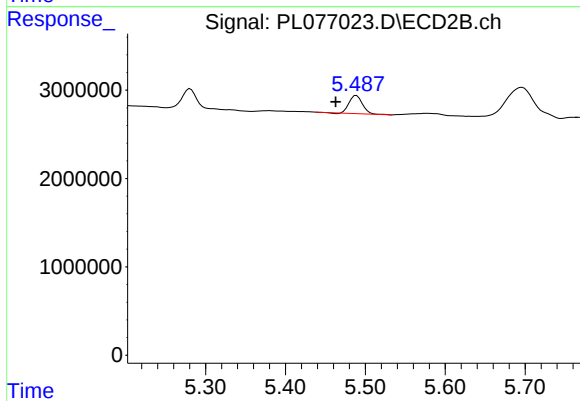

#14 Endrin


R.T.: 5.489 min
Delta R.T.: 0.026 min
Response: 2370075
Conc: 0.93 ng/ml

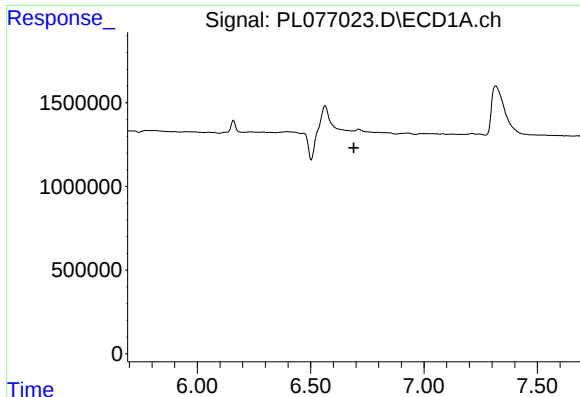

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.691 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

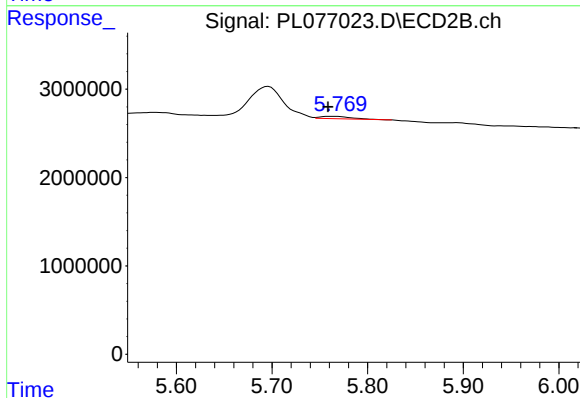


#15 Endosulfan II

R.T.: 5.761 min
Delta R.T.: 0.002 min
Response: 503575
Conc: 0.19 ng/ml

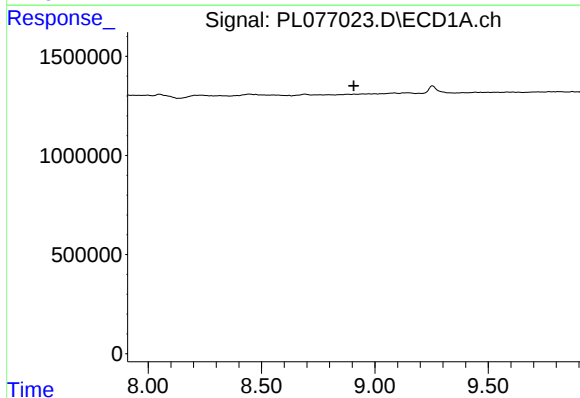

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.907 min
Response: 0
Conc: N.D.

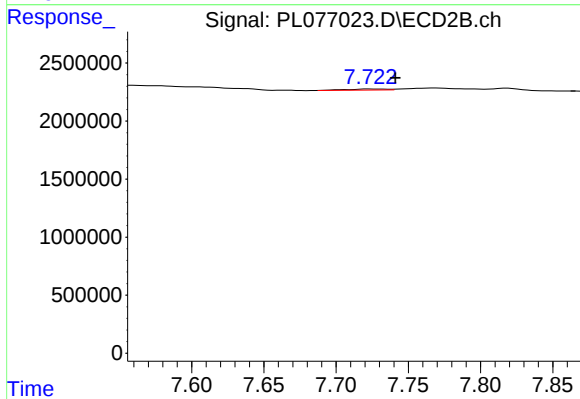

#28 Decachlorobiphenyl

R.T.: 7.723 min
Delta R.T.: -0.018 min
Response: 181876
Conc: 0.08 ng/ml