

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
 Data File : PL077024.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 09:41
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:05:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.639	17410151	46567540	17.756	16.268
28)	SA Decachlor...	8.913	7.745	15307896	38439039	20.277	17.075
Target Compounds							
13)	MA Dieldrin	0.000	5.188	0	122341	N.D.	0.041 #
14)	MA Endrin	0.000	5.489f	0	365845	N.D.	0.144 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
Data File : PL077024.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 09:41
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:05:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

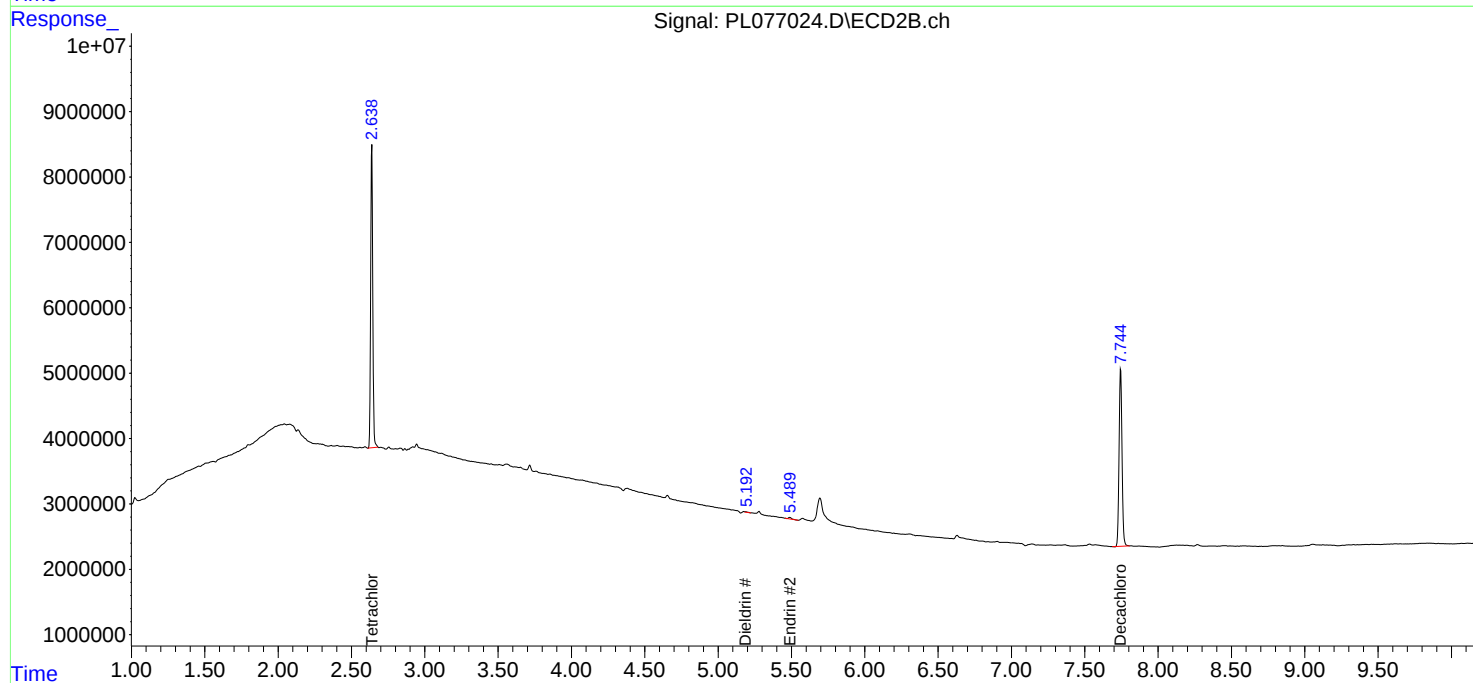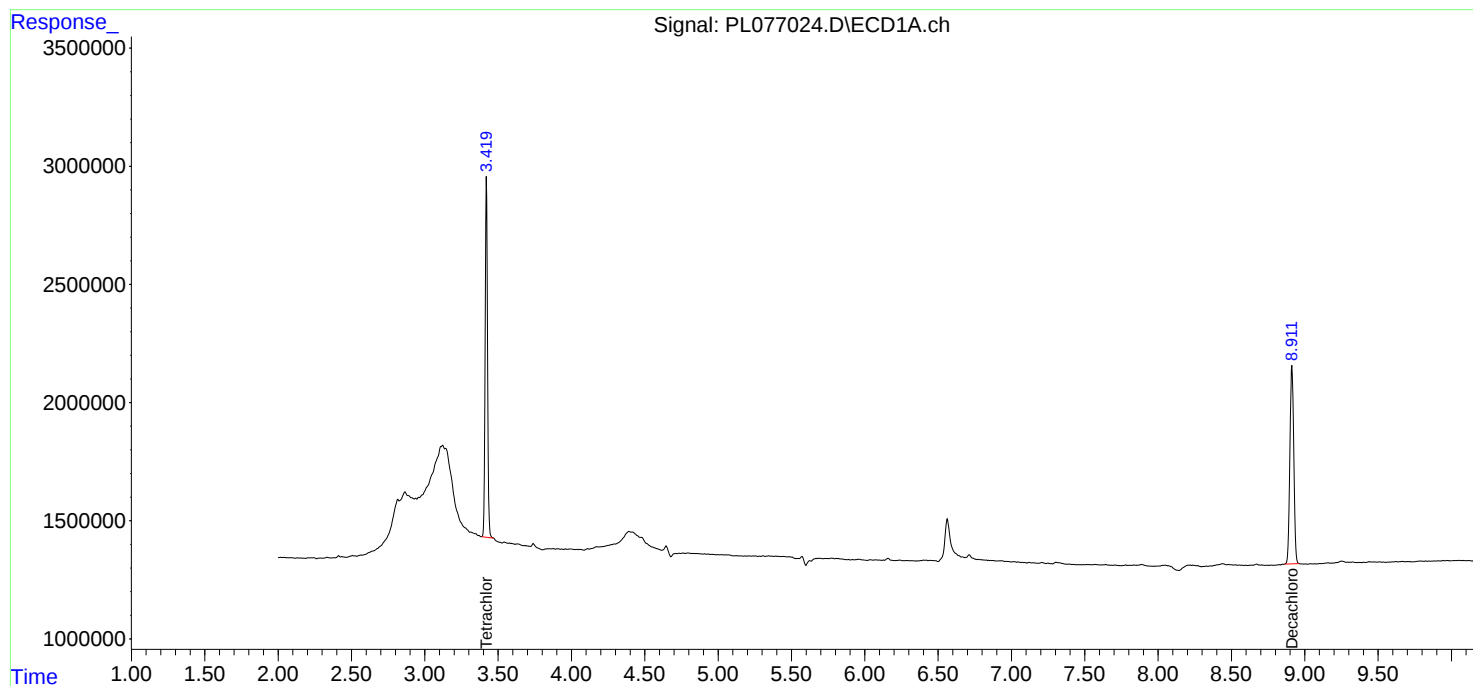


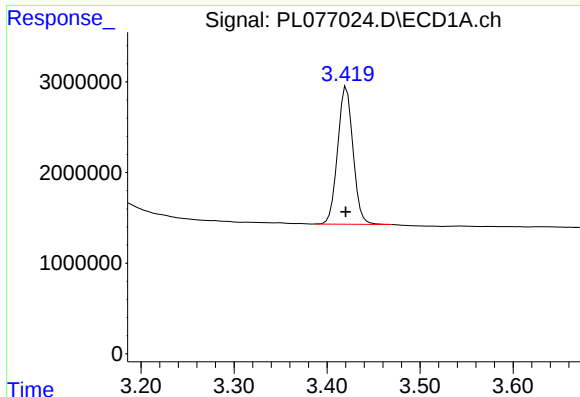

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 17410151
Conc: 17.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

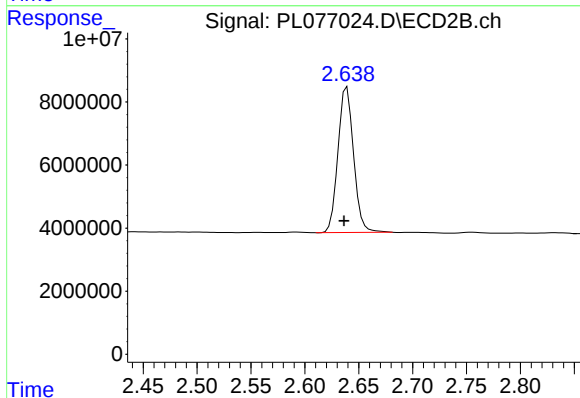


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.003 min
Response: 46567540
Conc: 16.27 ng/ml

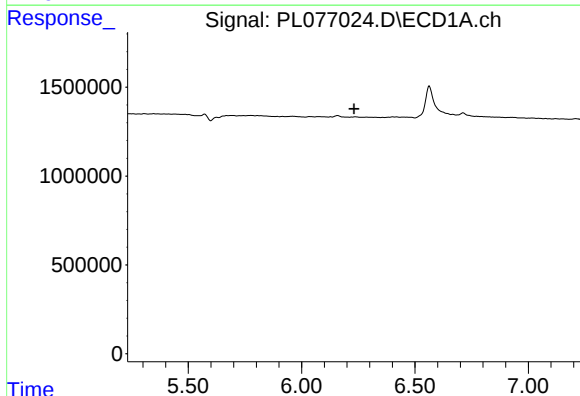


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.232 min
Response: 0
Conc: N.D.

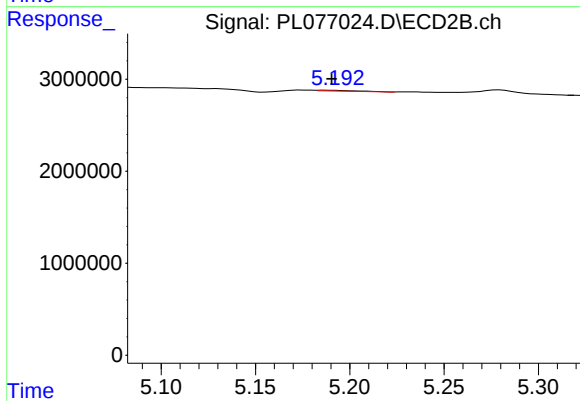

#13 Dieldrin


R.T.: 5.188 min
Delta R.T.: -0.003 min
Response: 122341
Conc: 0.04 ng/ml

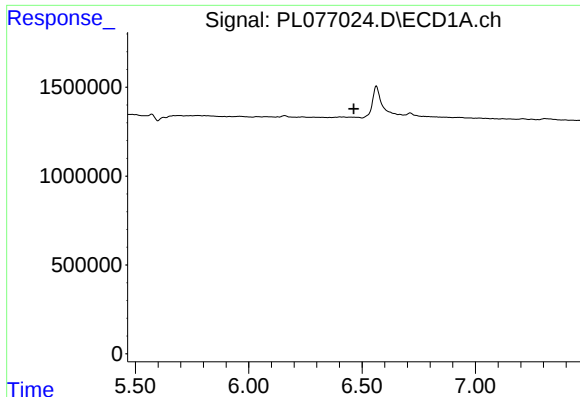

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

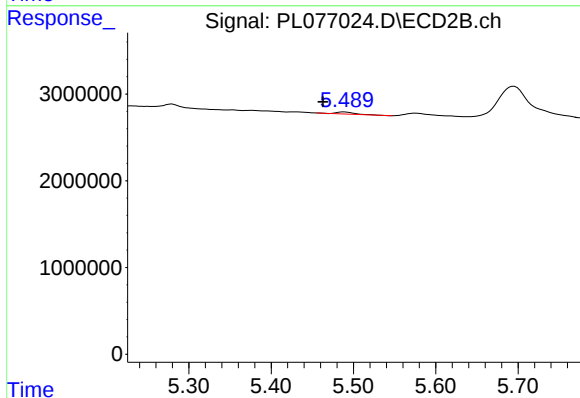


#14 Endrin

R.T.: 5.489 min
Delta R.T.: 0.026 min
Response: 365845
Conc: 0.14 ng/ml

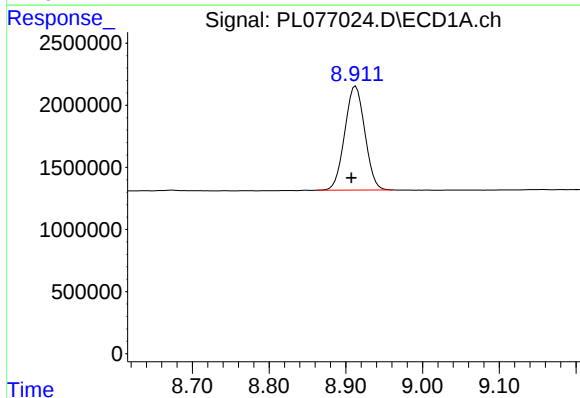

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.006 min
Response: 15307896
Conc: 20.28 ng/ml

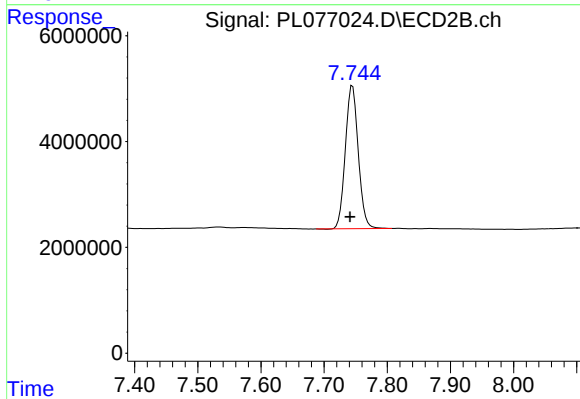

#28 Decachlorobiphenyl

R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 38439039
Conc: 17.07 ng/ml