

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
 Data File : PL077030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 14:04
 Operator : AR\AJ
 Sample : N4082-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:08:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	2.639	9760276	25107298	9.954	8.771
28)	SA Decachlor...	8.915	7.745	10787823	27778431	14.290	12.339
Target Compounds							
12)	B 4,4'-DDE	6.082	5.069	242227	644875	0.278	0.224
24)	Chlordane-2	0.000	4.188	0	329971	N.D.	2.869 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
Data File : PL077030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 14:04
Operator : AR\AJ
Sample : N4082-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:08:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

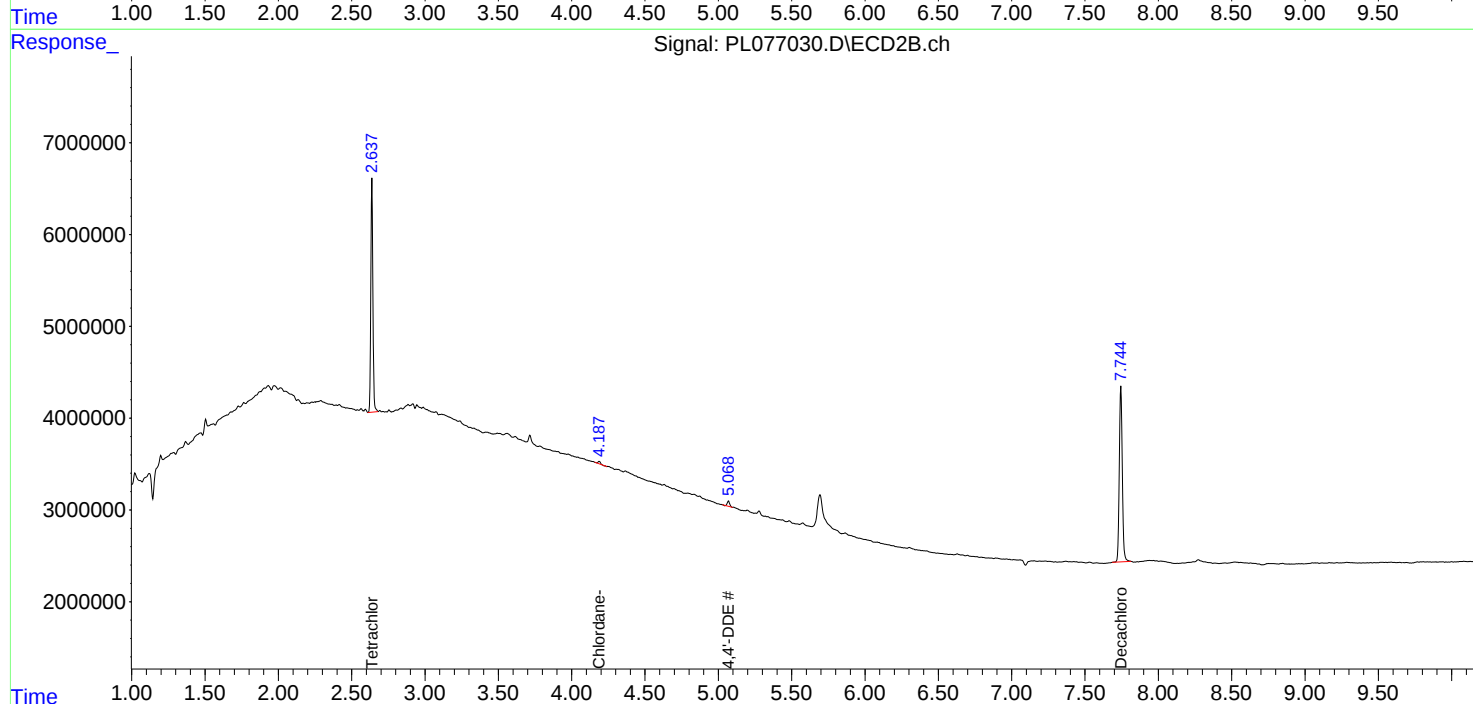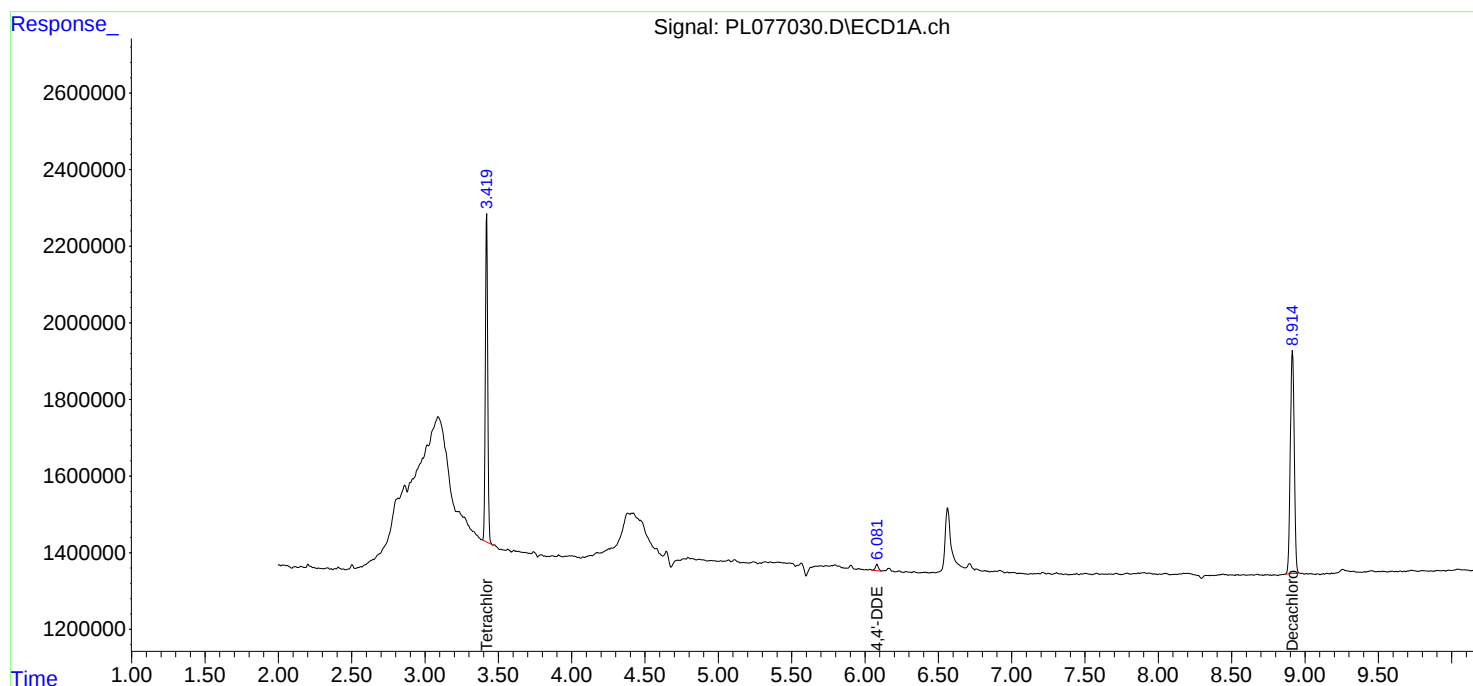


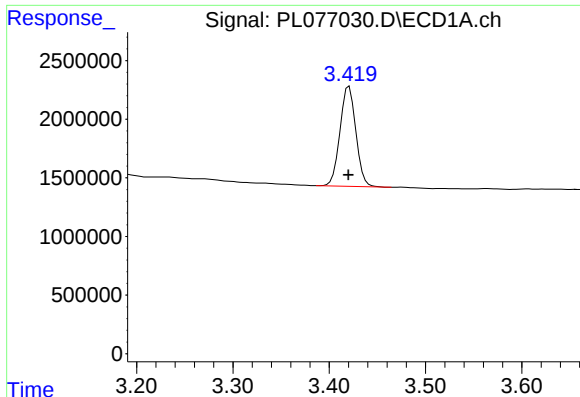

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 9760276
Conc: 9.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

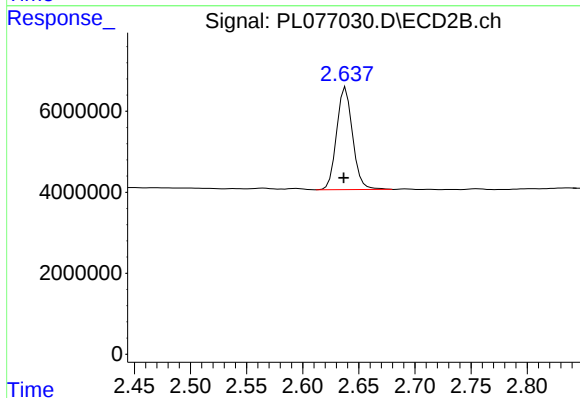


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.002 min
Response: 25107298
Conc: 8.77 ng/ml

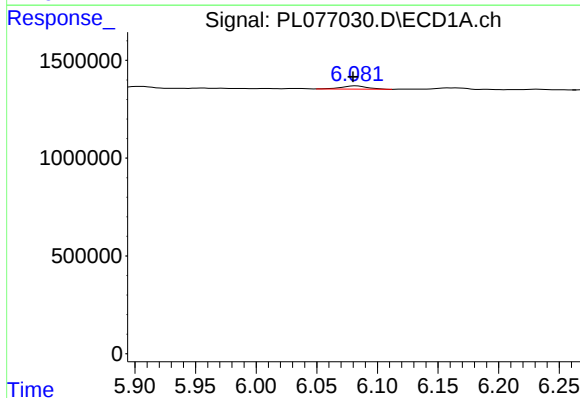


#12 4,4'-DDE

R.T.: 6.082 min
Delta R.T.: 0.003 min
Response: 242227
Conc: 0.28 ng/ml

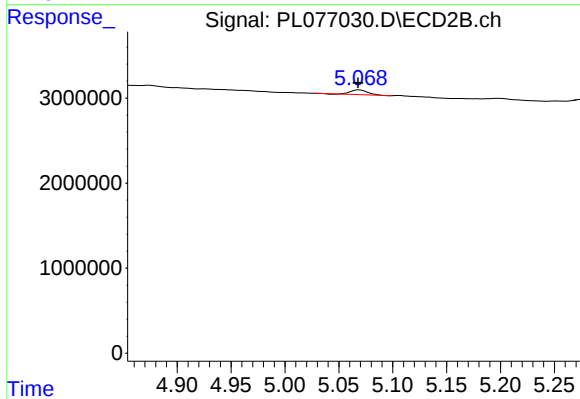

#12 4,4'-DDE


R.T.: 5.069 min
Delta R.T.: 0.001 min
Response: 644875
Conc: 0.22 ng/ml

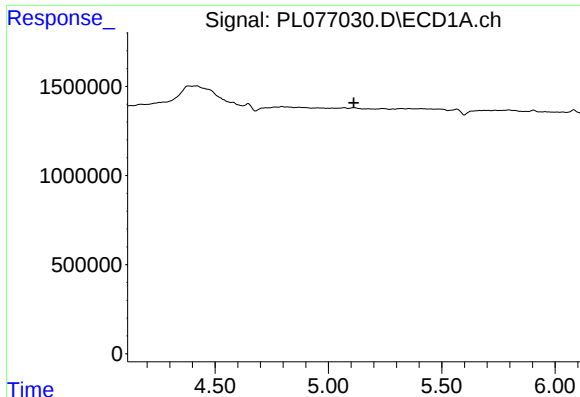

#24 Chlorodane-2


R.T.: 0.000 min
Exp R.T.: 5.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

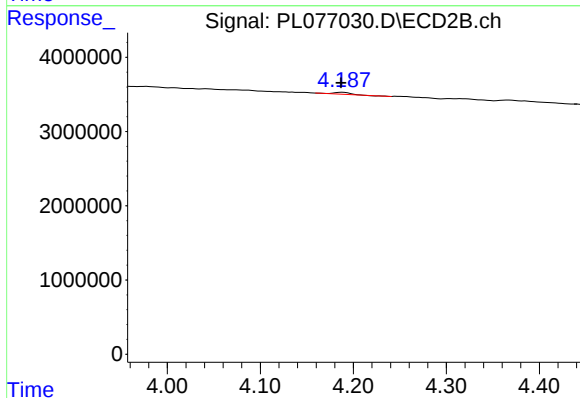


#24 Chlorodane-2

R.T.: 4.188 min
Delta R.T.: 0.001 min
Response: 329971
Conc: 2.87 ng/ml

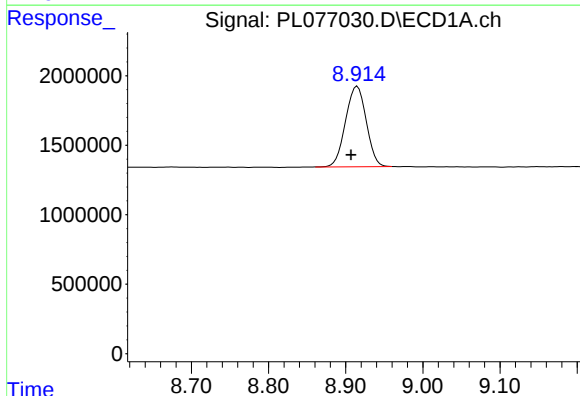

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.008 min
Response: 10787823
Conc: 14.29 ng/ml

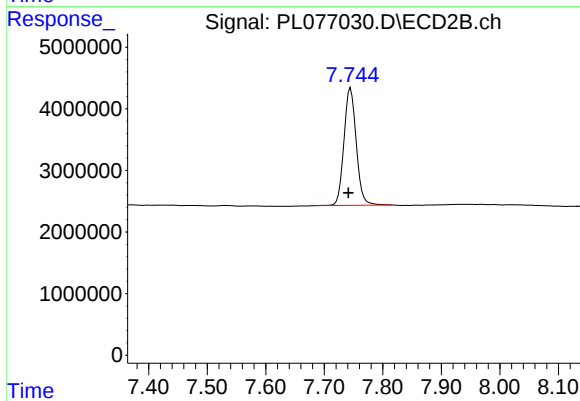

#28 Decachlorobiphenyl

R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 27778431
Conc: 12.34 ng/ml