

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
 Data File : PL077031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 14:18
 Operator : AR\AJ
 Sample : N4084-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:08:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.638	9833398	25643346	10.028	8.958
28)	SA Decachlor...	8.915	7.745	11376473	29456443	15.069	13.085
Target Compounds							
4)	MA Heptachlor	0.000	3.789	0	377097	N.D.	0.105 #
12)	B 4,4'-DDE	6.081	5.069	198965	493185	0.228	0.171 #
23)	Chlordane-1	0.000	3.617	0	227441	N.D.	2.335 #
24)	Chlordane-2	0.000	4.187	0	457006	N.D.	3.974 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
Data File : PL077031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 14:18
Operator : AR\AJ
Sample : N4084-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:08:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

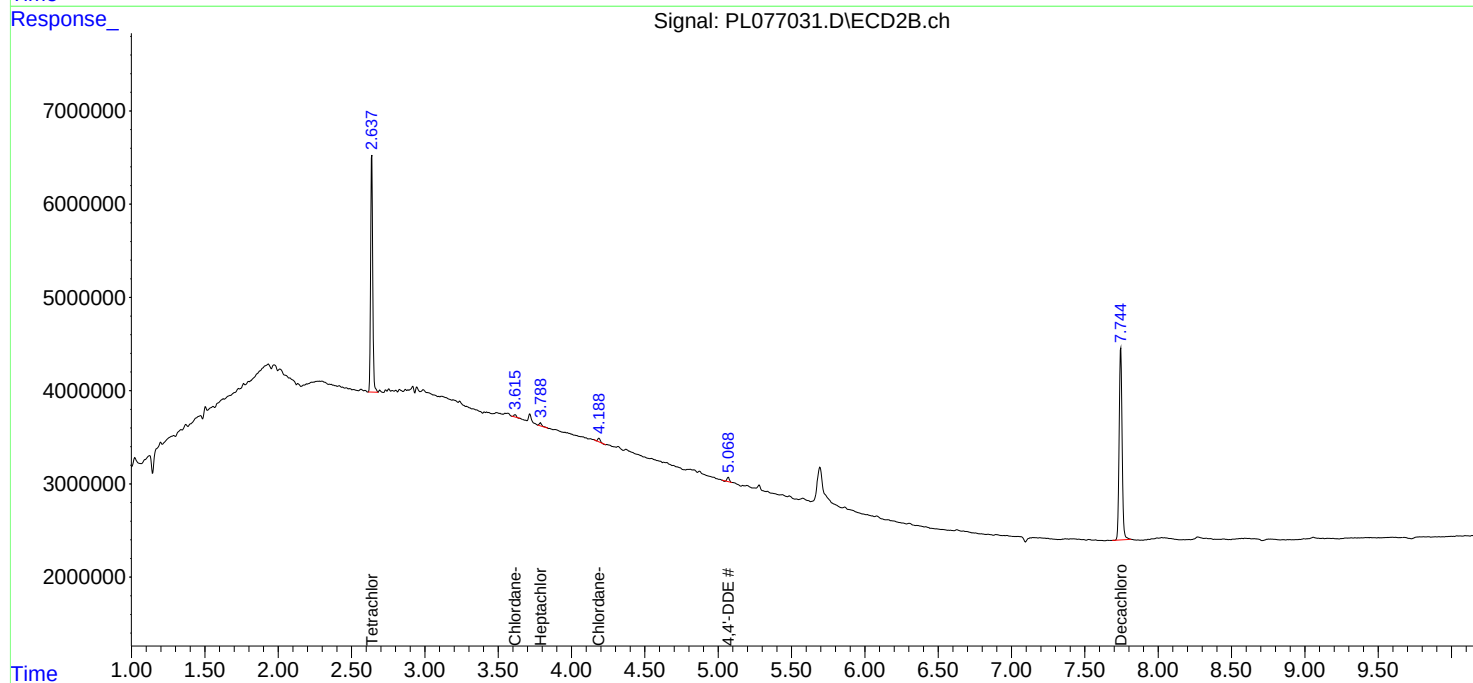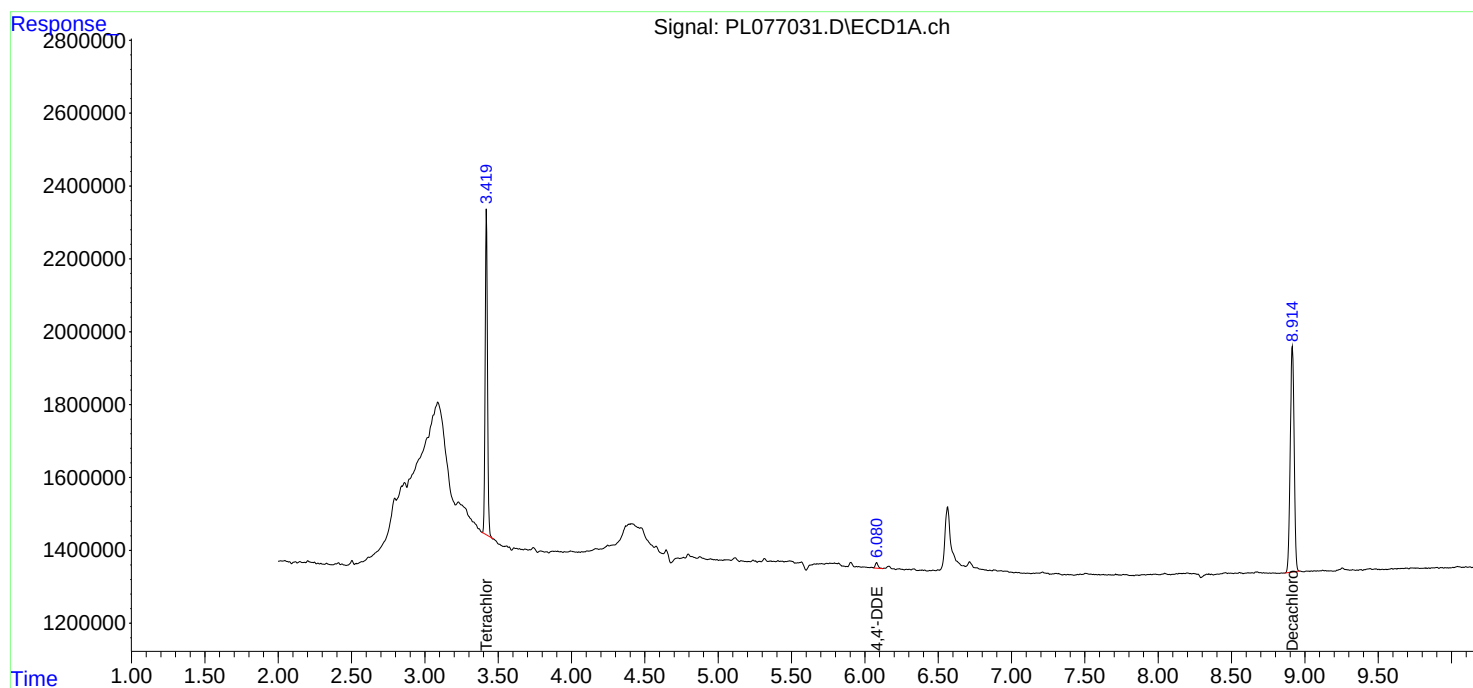


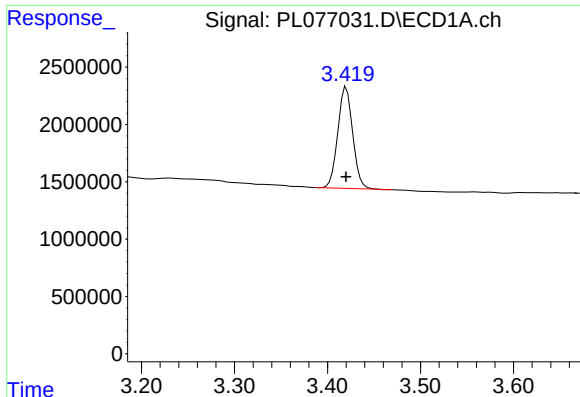

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 9833398
Conc: 10.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

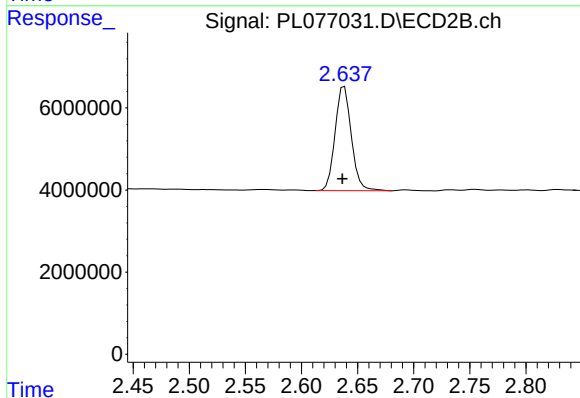


#1 Tetrachloro-m-xylene

R.T.: 2.638 min
Delta R.T.: 0.002 min
Response: 25643346
Conc: 8.96 ng/ml

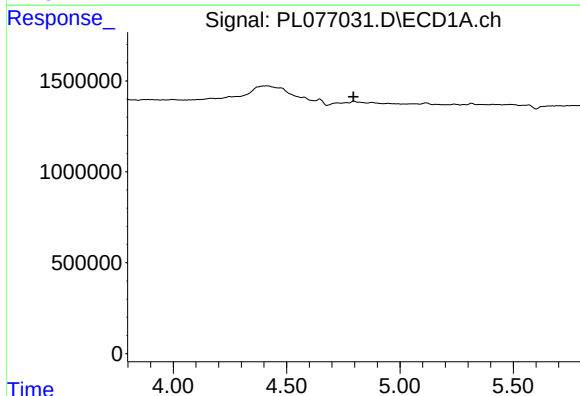


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.795 min
Response: 0
Conc: N.D.

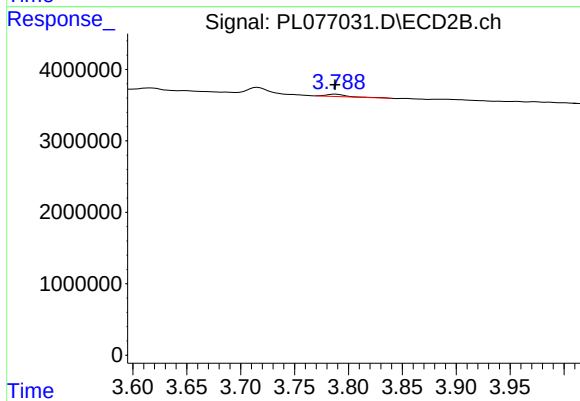

#4 Heptachlor


R.T.: 3.789 min
Delta R.T.: 0.001 min
Response: 377097
Conc: 0.11 ng/ml

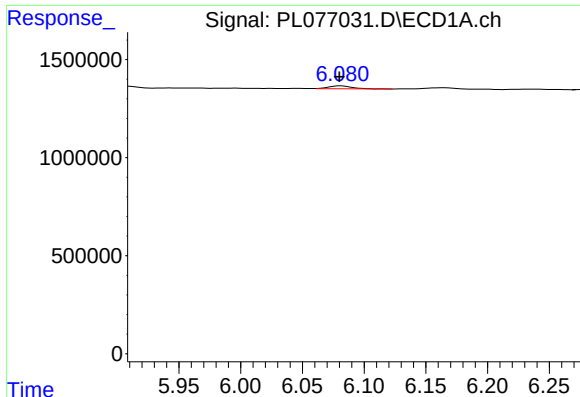

#12 4,4'-DDE


R.T.: 6.081 min
Delta R.T.: 0.001 min
Response: 198965
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

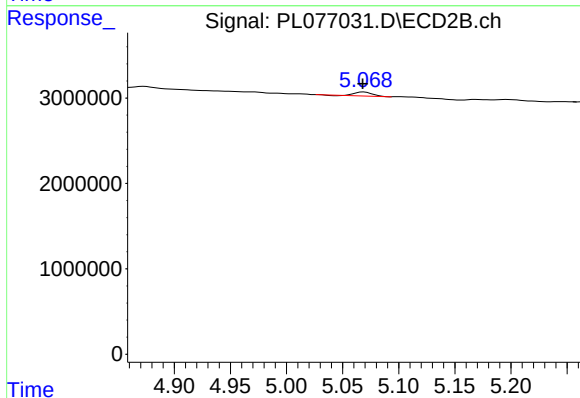


#12 4,4'-DDE

R.T.: 5.069 min
Delta R.T.: 0.001 min
Response: 493185
Conc: 0.17 ng/ml

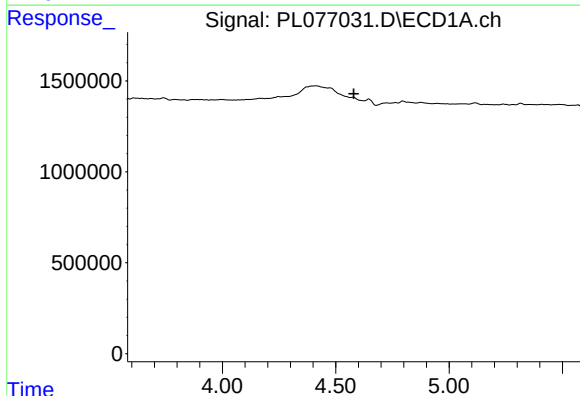


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.579 min
Response: 0
Conc: N.D.

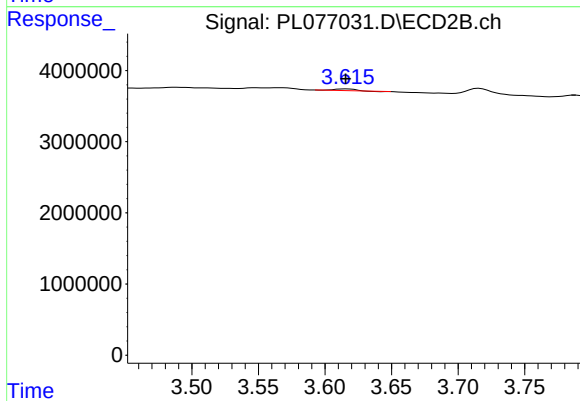

#23 Chlordane-1


R.T.: 3.617 min
Delta R.T.: 0.000 min
Response: 227441
Conc: 2.34 ng/ml

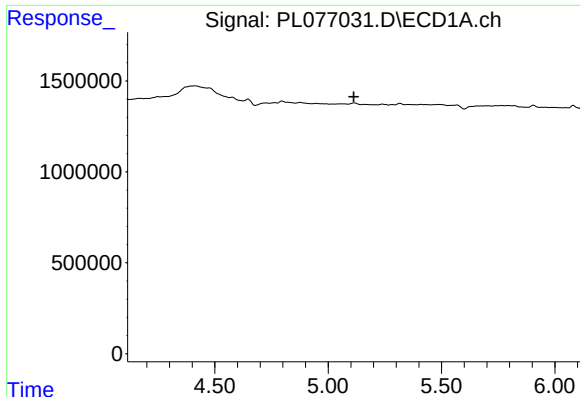

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.113 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

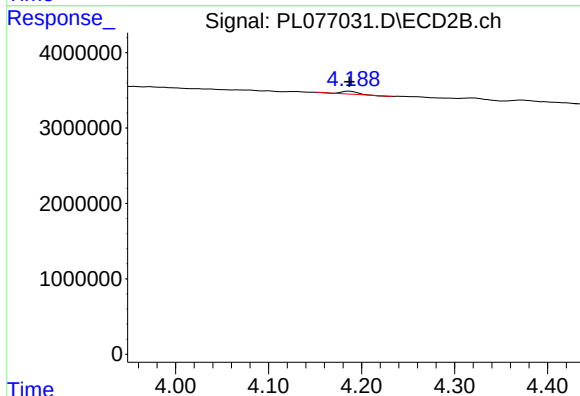


#24 Chlordane-2

R.T.: 4.187 min
Delta R.T.: 0.000 min
Response: 457006
Conc: 3.97 ng/ml

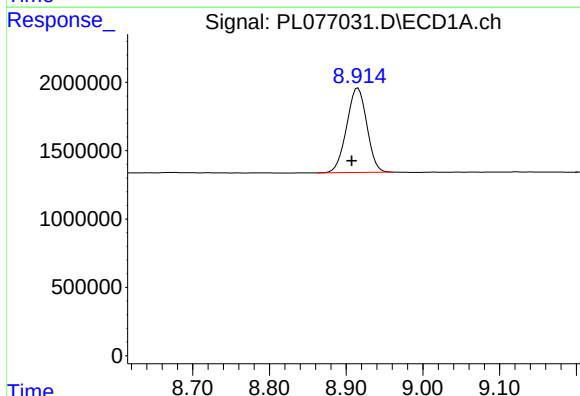

#28 Decachlorobiphenyl

R.T.: 8.915 min
Delta R.T.: 0.008 min
Response: 11376473
Conc: 15.07 ng/ml

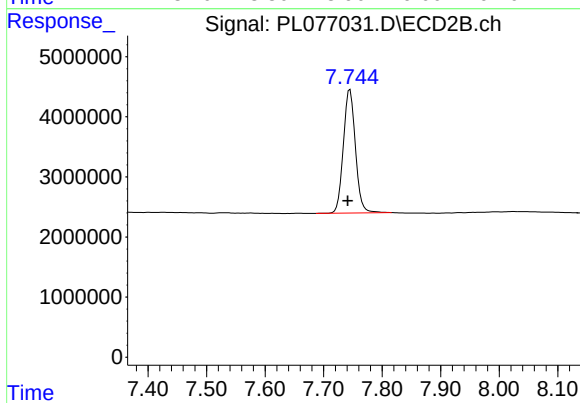

#28 Decachlorobiphenyl

R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 29456443
Conc: 13.08 ng/ml