

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
 Data File : PL077036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Aug 2022 15:27
 Operator : AR\AJ
 Sample : N4143-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-24051

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/12/2022
 Supervised By :Ankita Jodhani 08/12/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 23:13:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.639	7107260	18290401	7.248m	6.389
2)	SA Decachlor...	8.914	7.745	9619452	28567345	12.742	12.690

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081122\
Data File : PL077036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Aug 2022 15:27
Operator : AR\AJ
Sample : N4143-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CHRT-24051


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2022
Supervised By :Ankita Jodhani 08/12/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 23:13:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

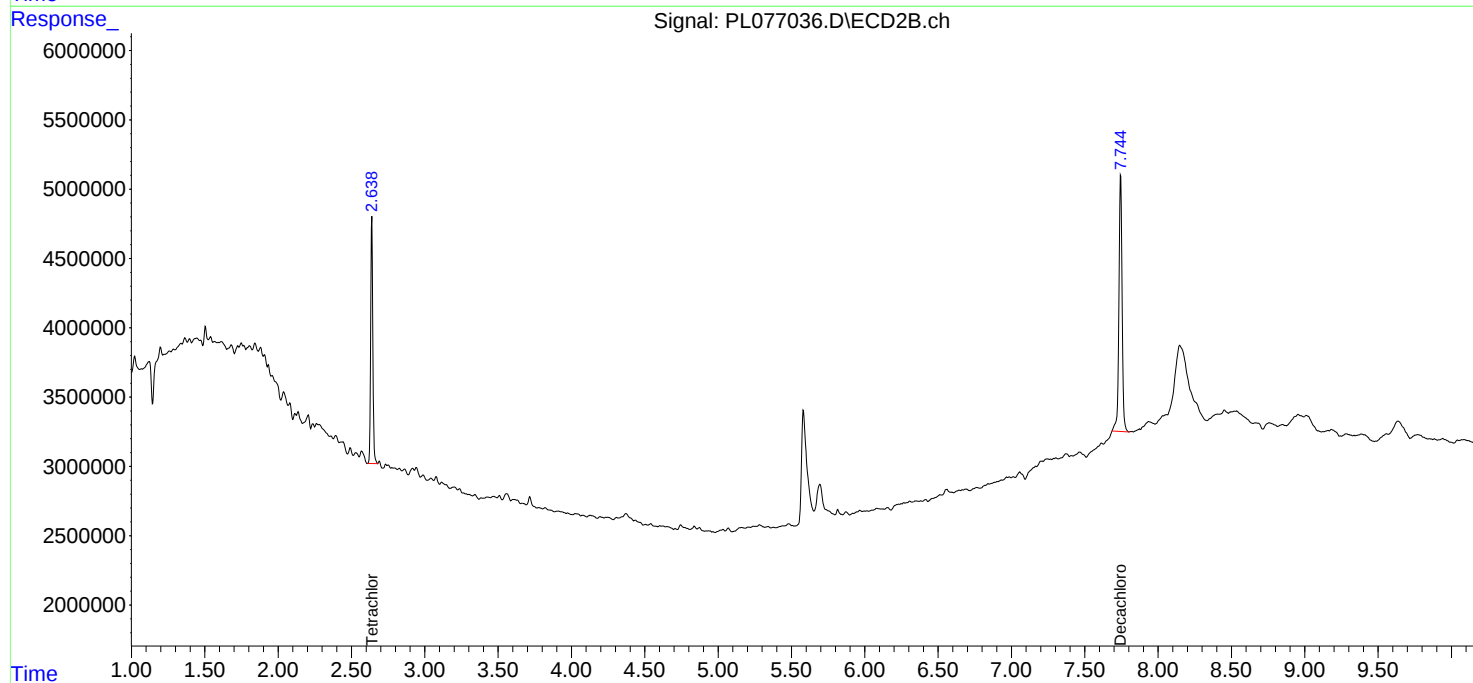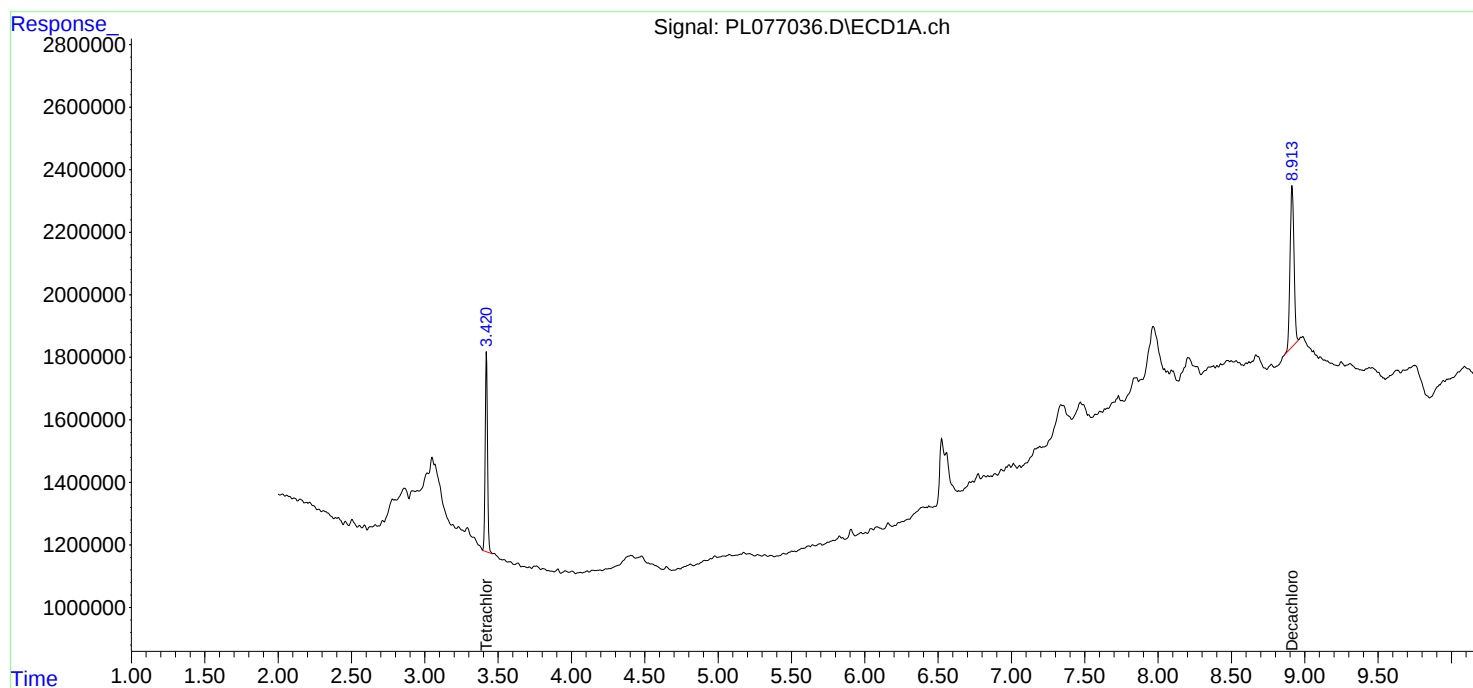

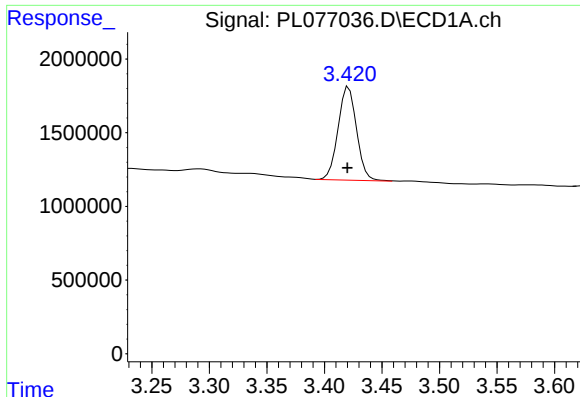


#1 Tetrachloro-m-xylene

R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 7107260
Conc: 7.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-24051


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/12/2022
Supervised By :Ankita Jodhani 08/12/2022

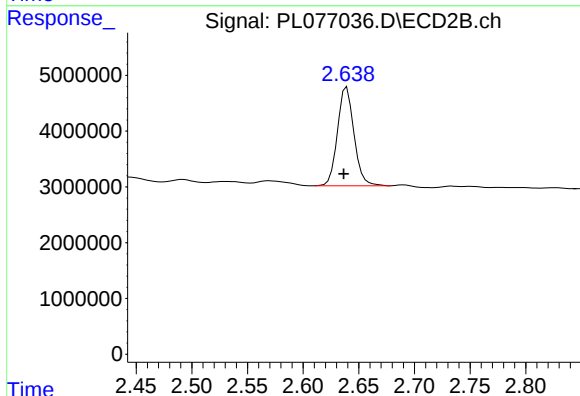


#1 Tetrachloro-m-xylene

R.T.: 2.639 min
Delta R.T.: 0.003 min
Response: 18290401
Conc: 6.39 ng/ml

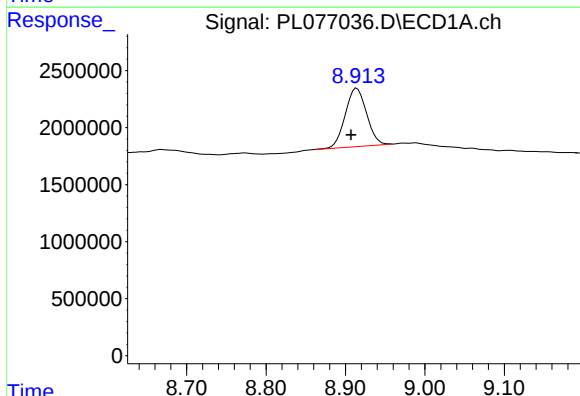

#28 Decachlorobiphenyl

R.T.: 8.914 min
Delta R.T.: 0.007 min
Response: 9619452
Conc: 12.74 ng/ml

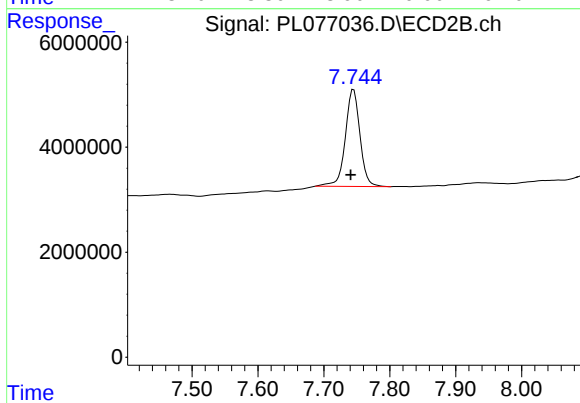

#28 Decachlorobiphenyl

R.T.: 7.745 min
Delta R.T.: 0.004 min
Response: 28567345
Conc: 12.69 ng/ml