

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 13:53
 Operator : SM\AJ
 Sample : K4240-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-035-B242-080619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:44:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.926	280.5E6	72106667	27.920	25.272
28)	SA Decachlor...	7.976	8.954	230.9E6	58808513	22.805	20.796
Target Compounds							
6)	B beta-BHC	0.000	4.801f	0	1319237	N.D.	0.763 #
9)	A Endosulfan I	5.334f	6.150	4578707	8829201	0.315	2.567 #
11)	B alpha-Chl...	5.264	0.000	79378085	0	5.203	N.D. #
16)	A 4,4'-DDD	5.941	0.000	3093797	0	0.258	N.D. #
20)	A Methoxychlor	0.000	7.487f	0	4988560	N.D.	3.400 #
21)	B Endrin ke...	0.000	7.642	0	22964356	N.D.	7.943 #
22)	Mirex	7.104	8.111	4343420	73485282	0.443	31.992 #
26)	Chlordane-4	5.264	0.000	79378085	0	60.181	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 13:53
Operator : SM\AJ
Sample : K4240-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:44:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

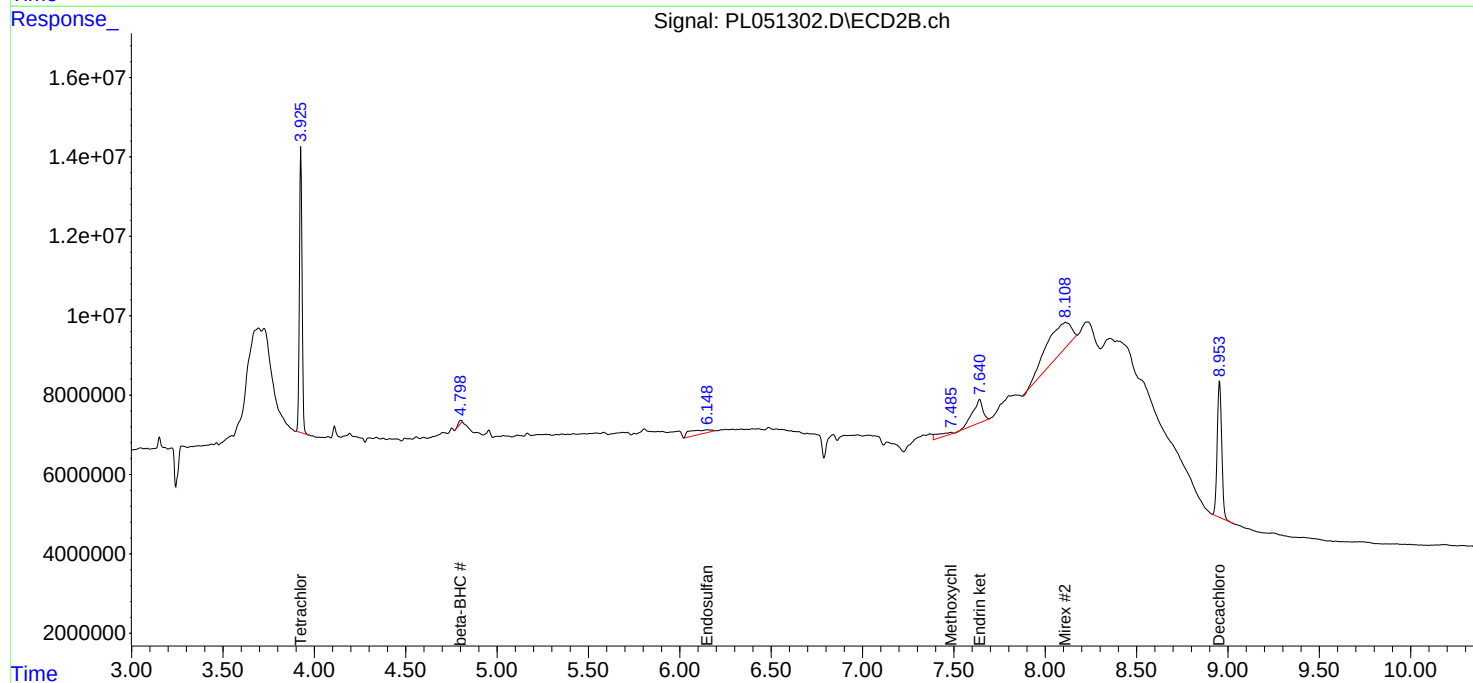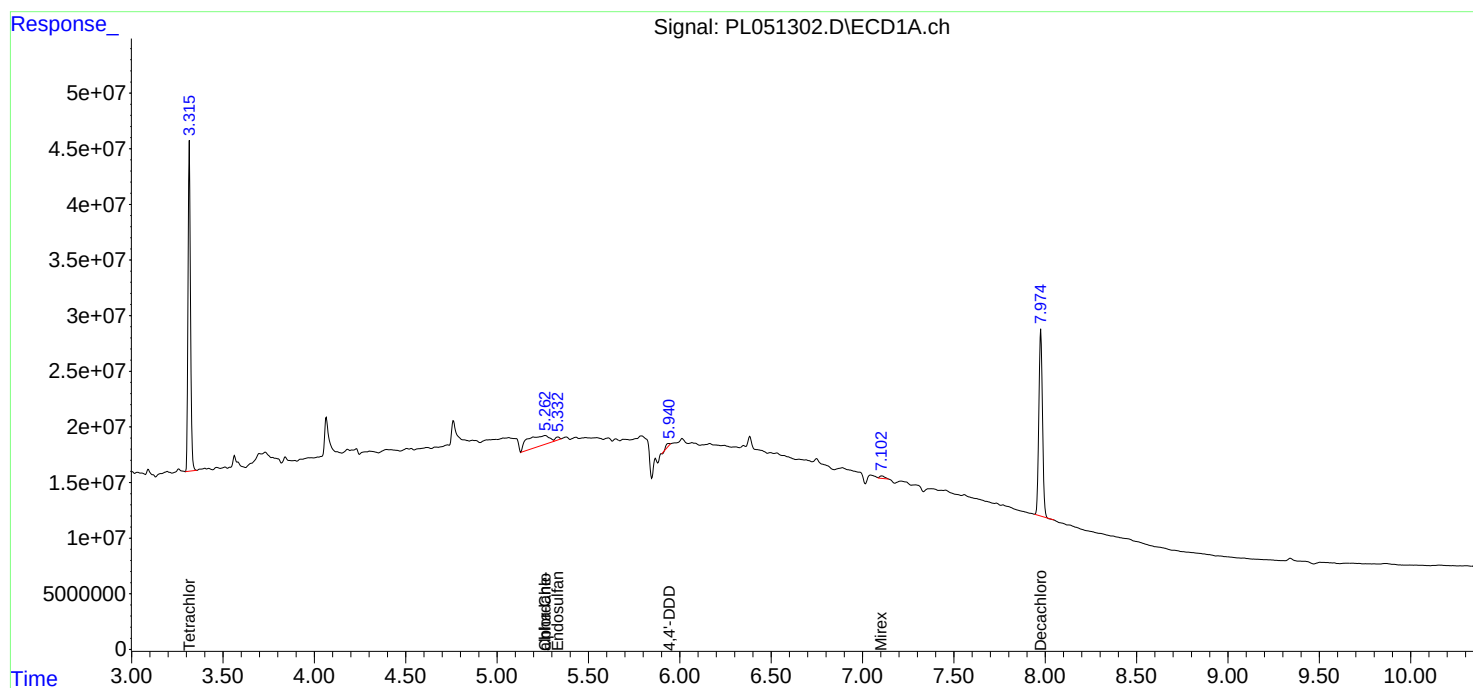


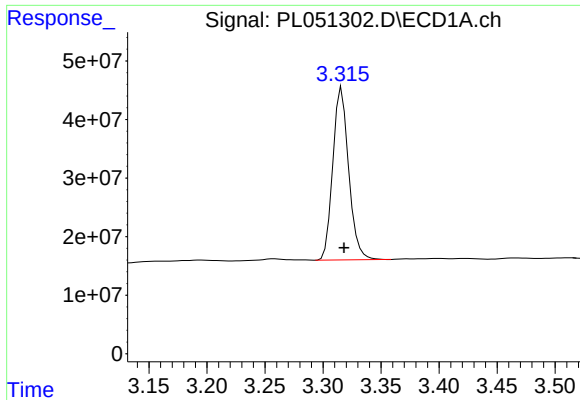

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 280540701
Conc: 27.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

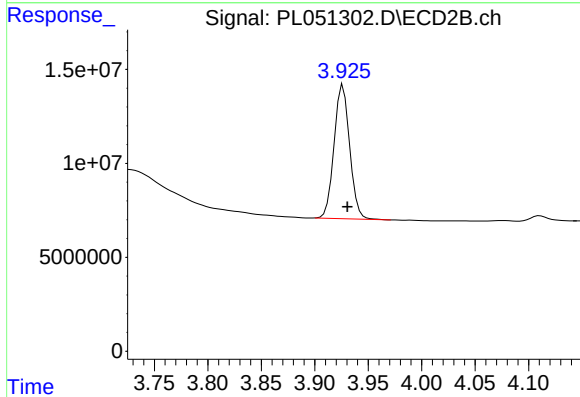


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.004 min
Response: 72106667
Conc: 25.27 ng/ml

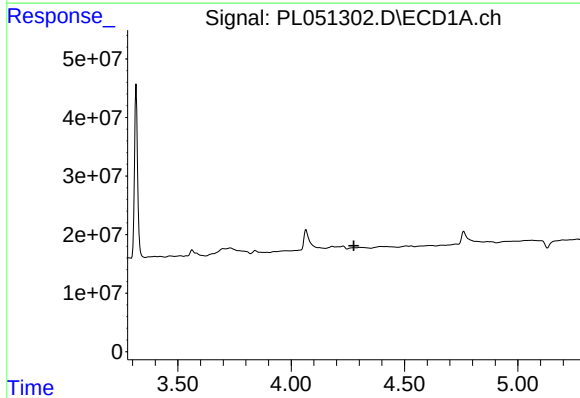


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

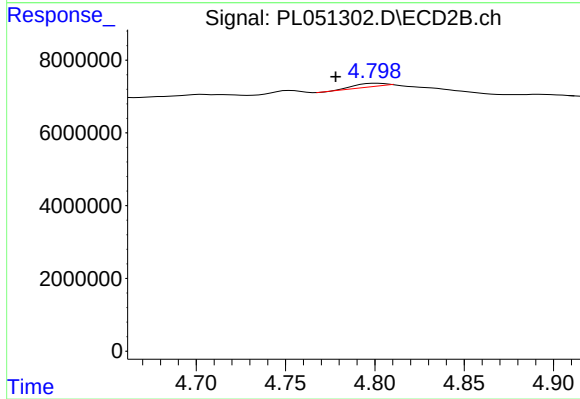

#6 beta-BHC


R.T.: 4.801 min
Delta R.T.: 0.023 min
Response: 1319237
Conc: 0.76 ng/ml

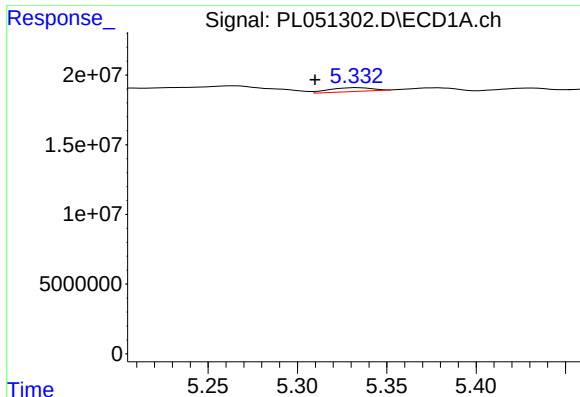

#9 Endosulfan I


R.T.: 5.334 min
Delta R.T.: 0.024 min
Response: 4578707
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

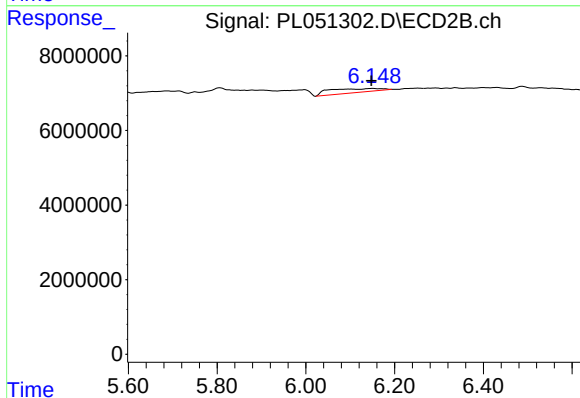


#9 Endosulfan I

R.T.: 6.150 min
Delta R.T.: 0.002 min
Response: 8829201
Conc: 2.57 ng/ml

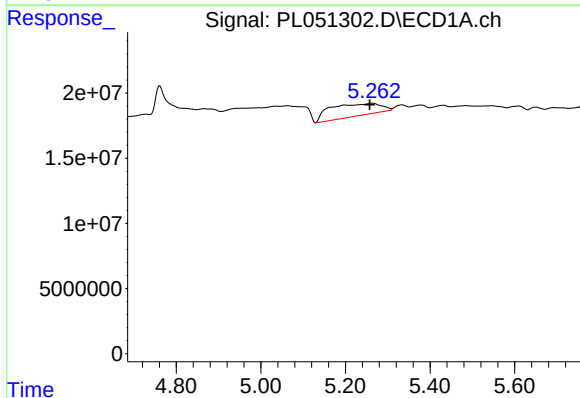


#11 alpha-Chlordane

R.T.: 5.264 min
Delta R.T.: 0.007 min
Response: 79378085
Conc: 5.20 ng/ml

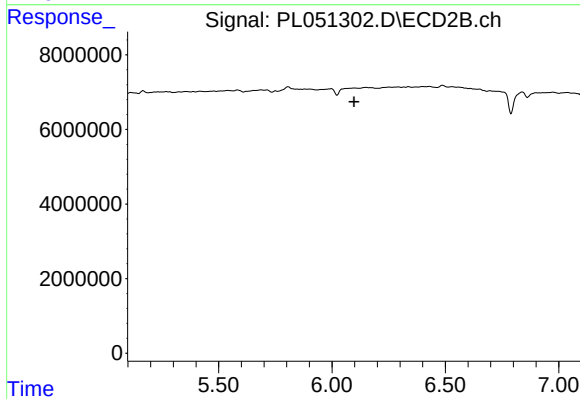

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

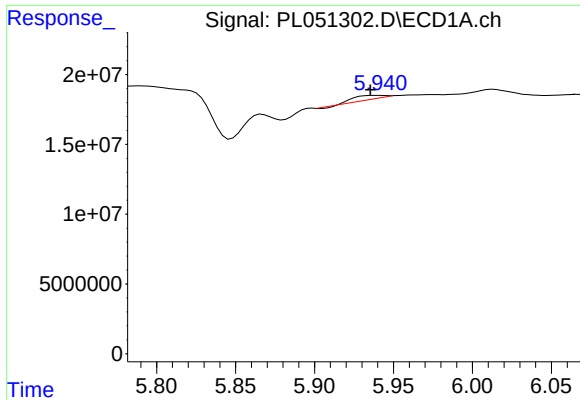

#16 4,4'-DDD


R.T.: 5.941 min
Delta R.T.: 0.006 min
Response: 3093797
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

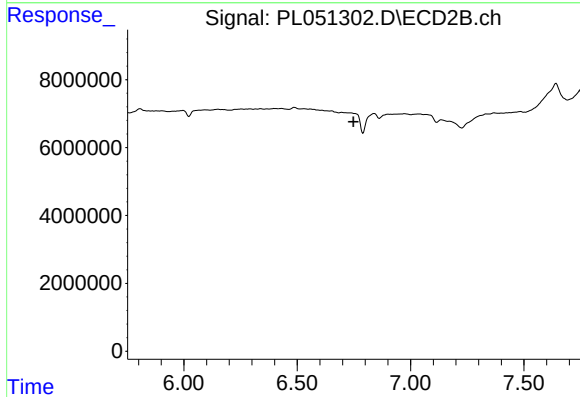


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

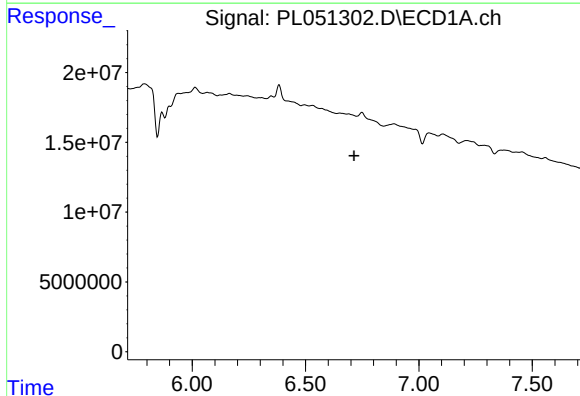


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.714 min
Response: 0
Conc: N.D.

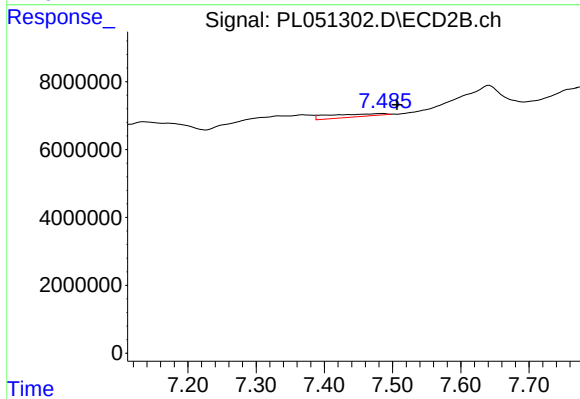

#20 Methoxychlor


R.T.: 7.487 min
Delta R.T.: -0.020 min
Response: 4988560
Conc: 3.40 ng/ml

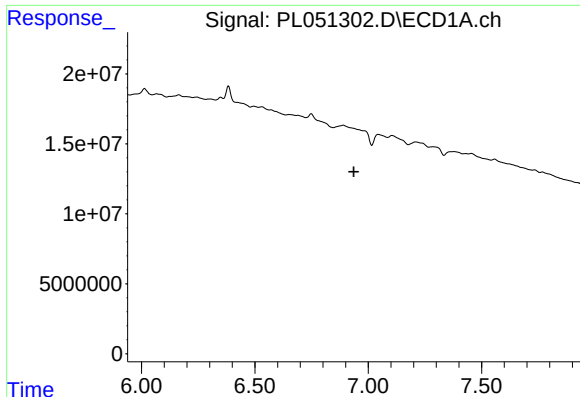

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 6.936 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

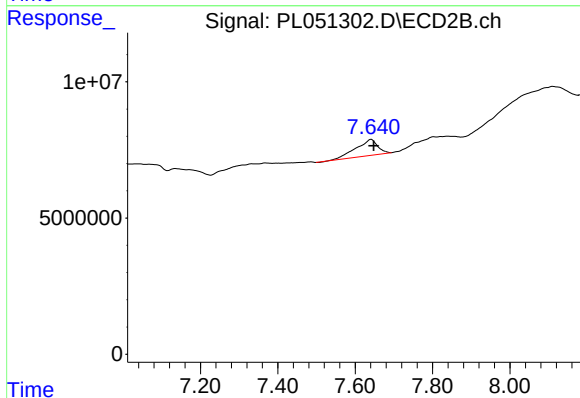


#21 Endrin ketone

R.T.: 7.642 min
Delta R.T.: -0.006 min
Response: 22964356
Conc: 7.94 ng/ml

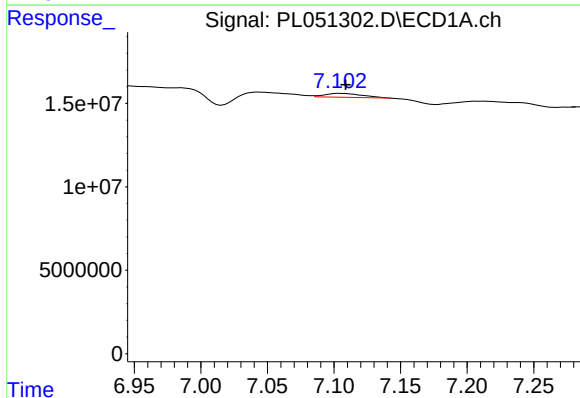


#22 Mirex

R.T.: 7.104 min
Delta R.T.: -0.005 min
Response: 4343420
Conc: 0.44 ng/ml

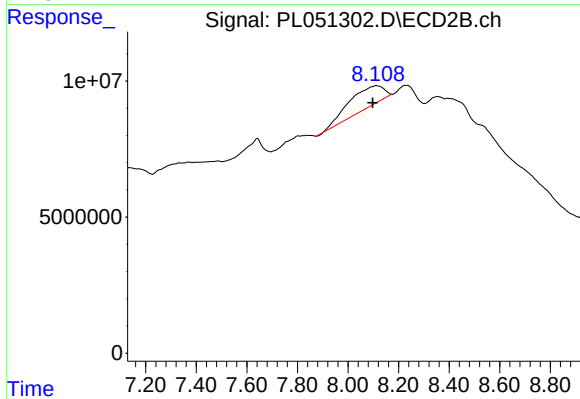

#22 Mirex


R.T.: 8.111 min
Delta R.T.: 0.014 min
Response: 73485282
Conc: 31.99 ng/ml

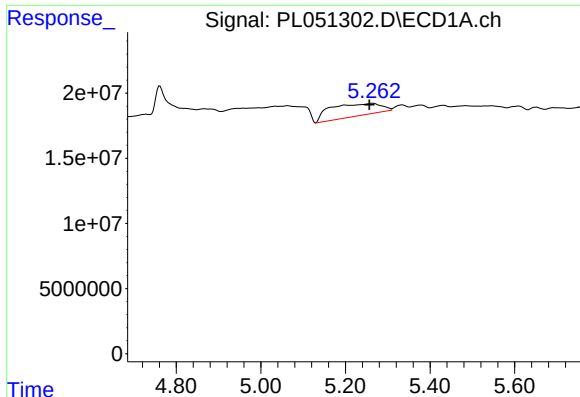

#26 Chlordane-4


R.T.: 5.264 min
Delta R.T.: 0.007 min
Response: 79378085
Conc: 60.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B242-080619

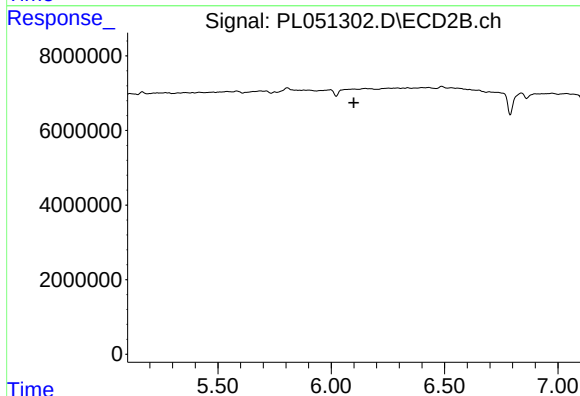


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

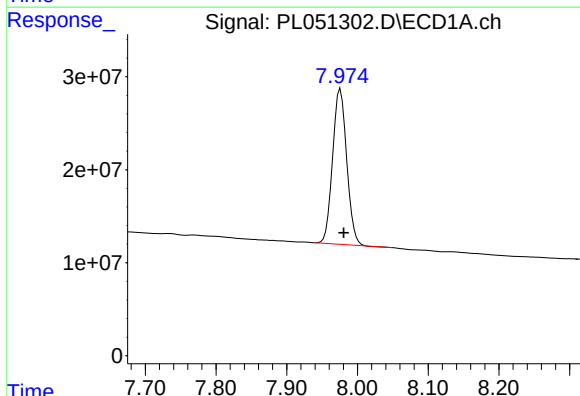

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 230911414
Conc: 22.81 ng/ml

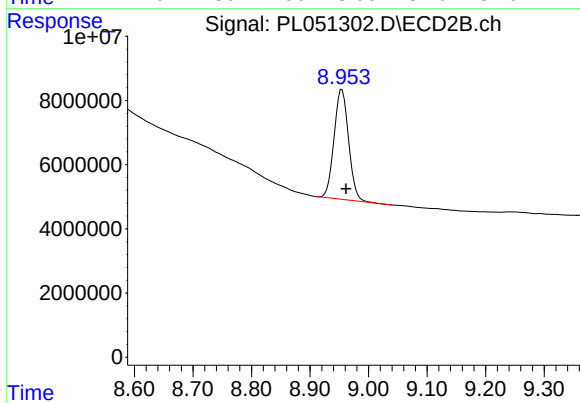

#28 Decachlorobiphenyl

R.T.: 8.954 min
Delta R.T.: -0.007 min
Response: 58808513
Conc: 20.80 ng/ml