

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 18:54
 Operator : SM\AJ
 Sample : K4230-12
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2S-J-(0-1)-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:49:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	220.8E6	59723846	21.976	20.932
28)	SA Decachlor...	7.976	8.955	225.2E6	57751373	22.236	20.422
Target Compounds							
6)	B beta-BHC	0.000	4.806f	0	501491	N.D.	0.290 #
9)	A Endosulfan I	5.337f	0.000	12711518	0	0.874	N.D. #
10)	B gamma-Chl...	5.202	0.000	37472917	0	2.374	N.D. #
11)	B alpha-Chl...	5.247	0.000	71633786	0	4.695	N.D. #
15)	B Endosulfa...	0.000	6.845	0	9242001	N.D.	2.907 #
25)	Chlordane-3	5.202	0.000	37472917	0	26.770	N.D. #
26)	Chlordane-4	5.247	0.000	71633786	0	54.310	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 18:54
Operator : SM\AJ
Sample : K4230-12
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:49:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

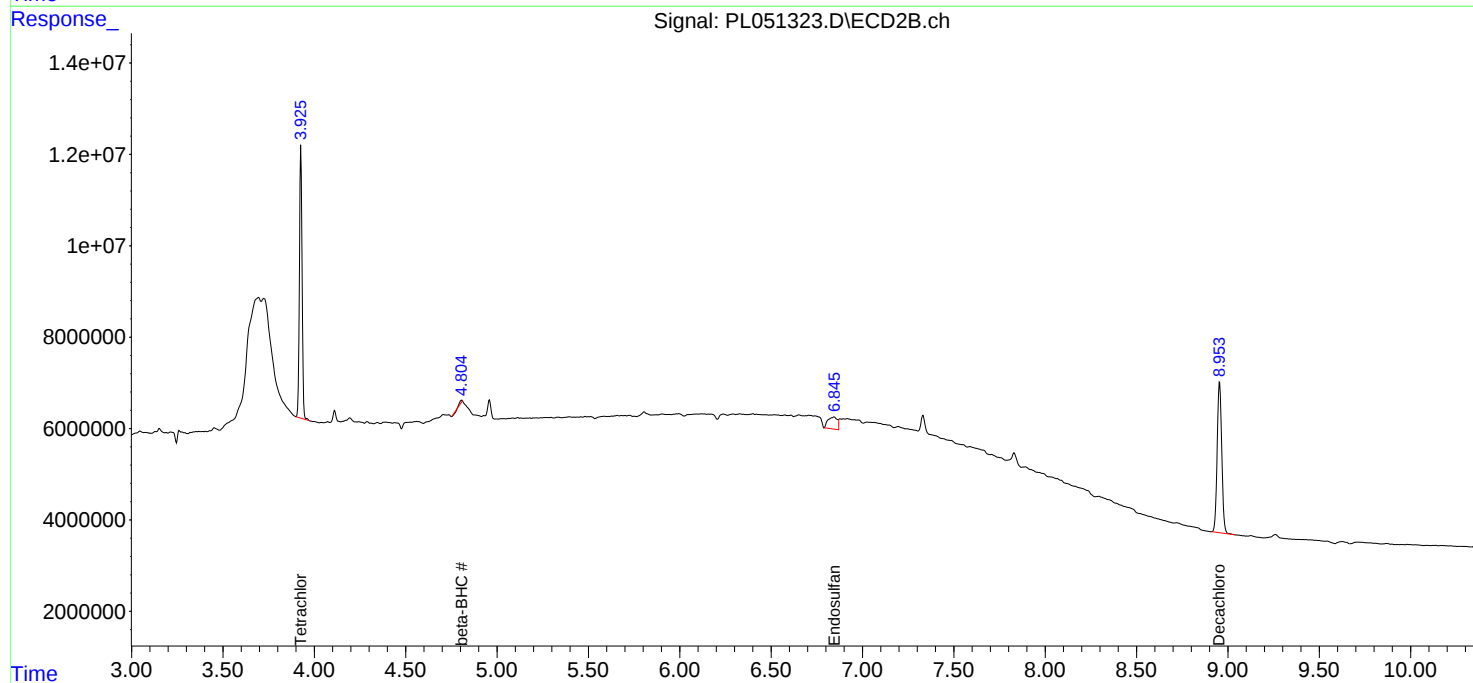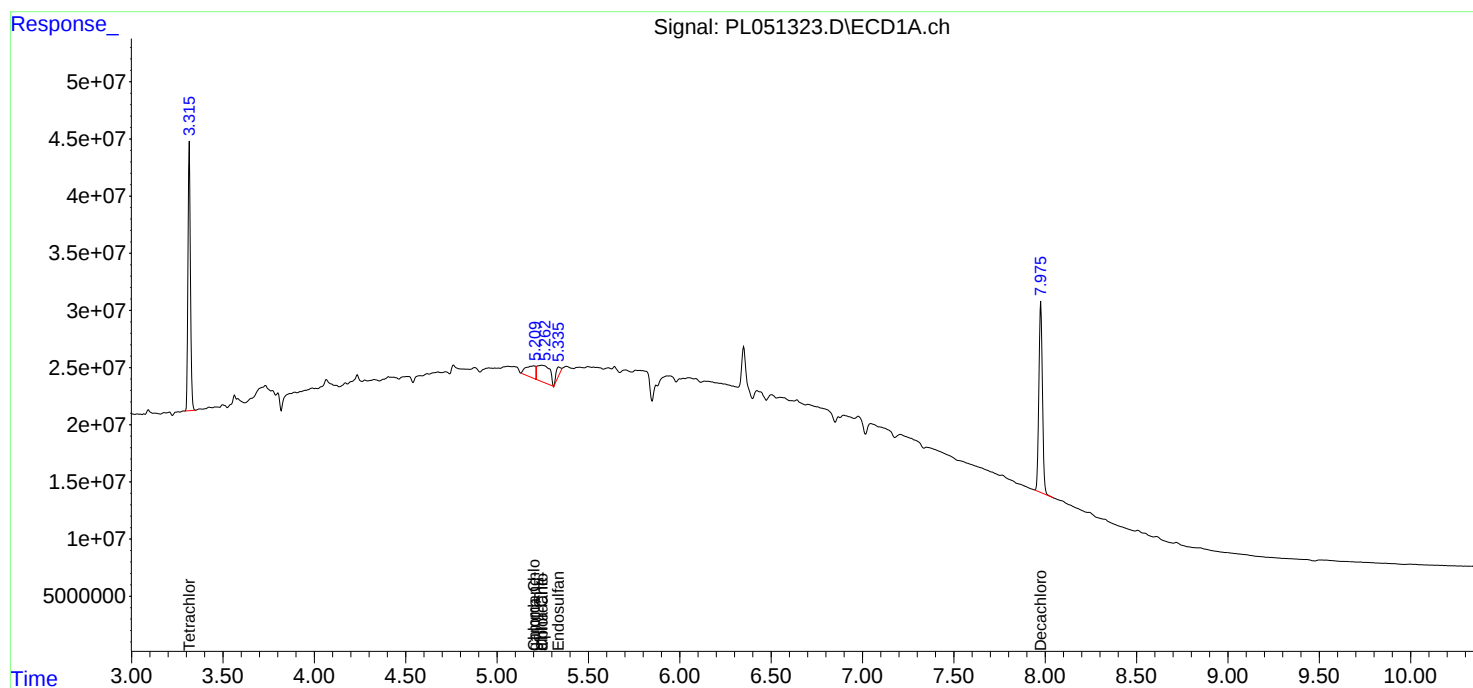


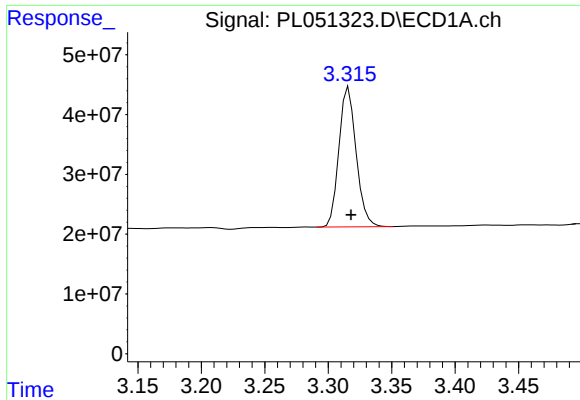

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 220806485
Conc: 21.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

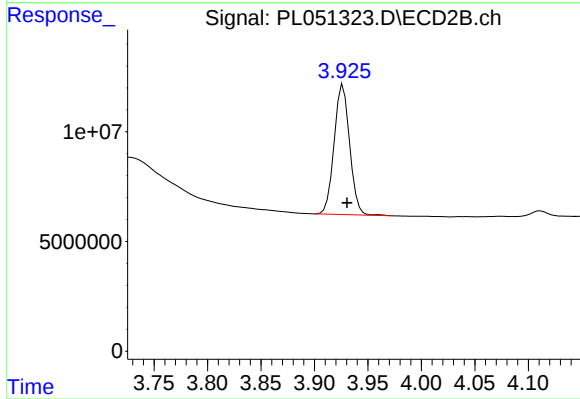


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 59723846
Conc: 20.93 ng/ml

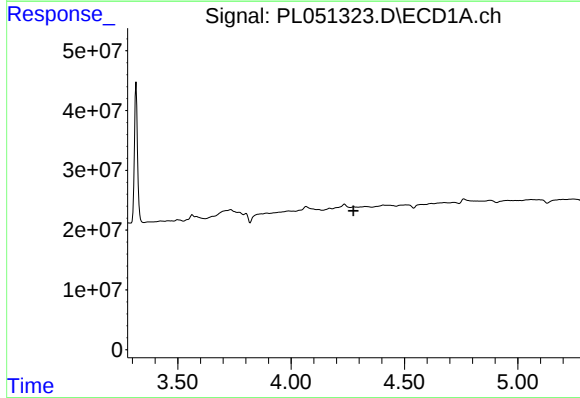


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

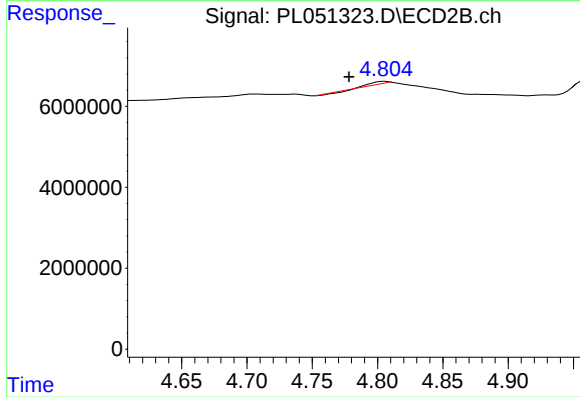

#6 beta-BHC

R.T.: 4.806 min
Delta R.T.: 0.028 min
Response: 501491
Conc: 0.29 ng/ml

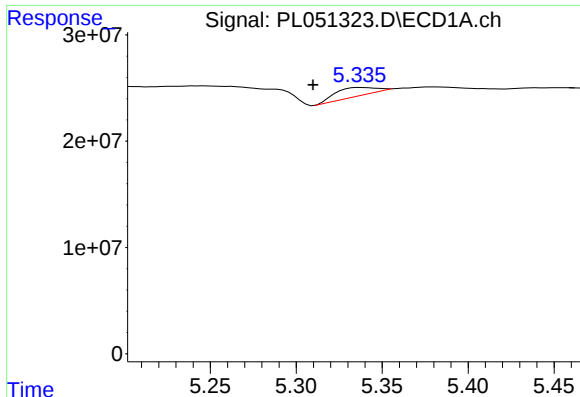


#9 Endosulfan I

R.T.: 5.337 min
Delta R.T.: 0.027 min
Response: 12711518
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

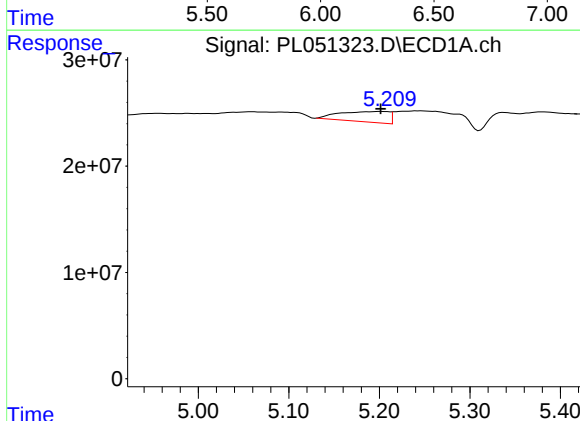


#10 gamma-Chlordane

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 37472917
Conc: 2.37 ng/ml

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

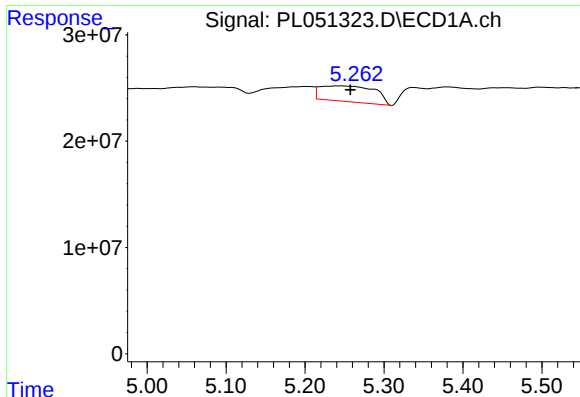

#11 alpha-Chlordane


R.T.: 5.247 min
Delta R.T.: -0.010 min
Response: 71633786
Conc: 4.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

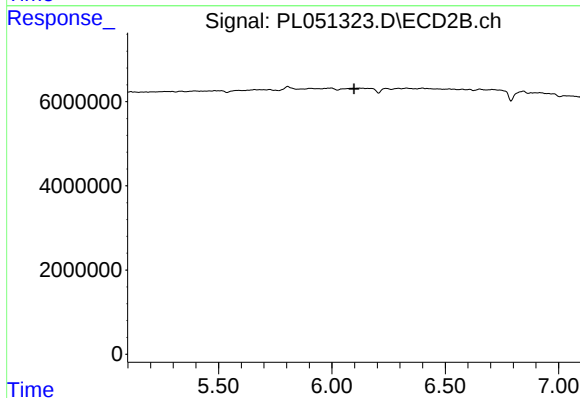


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

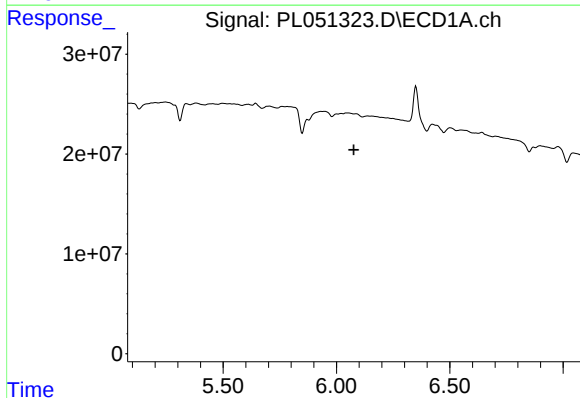


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

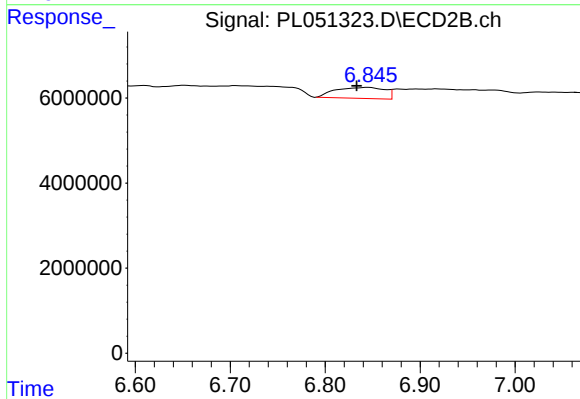

#15 Endosulfan II


R.T.: 6.845 min
Delta R.T.: 0.012 min
Response: 9242001
Conc: 2.91 ng/ml

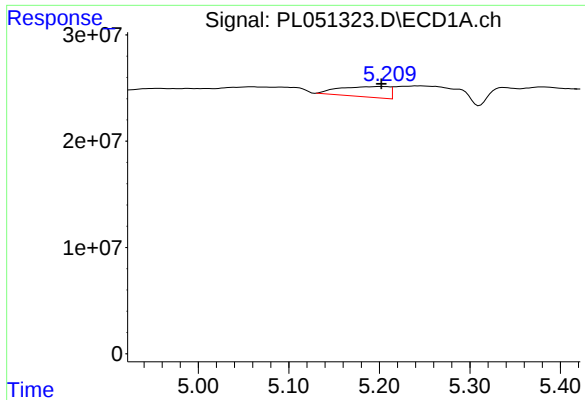

#25 Chlordane-3


R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 37472917
Conc: 26.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

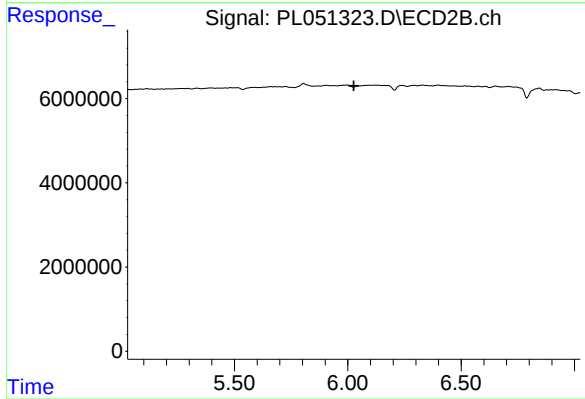


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

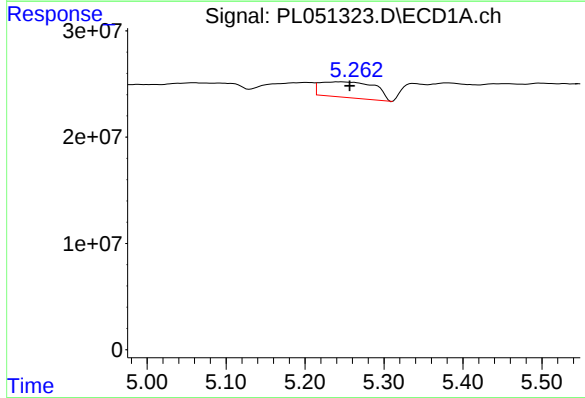


#26 Chlordane-4

R.T.: 5.247 min
Delta R.T.: -0.010 min
Response: 71633786
Conc: 54.31 ng/ml

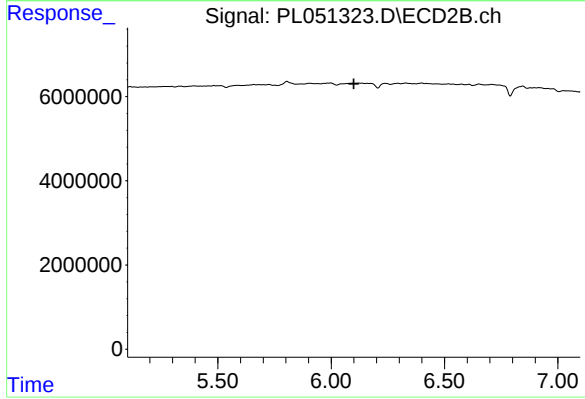

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

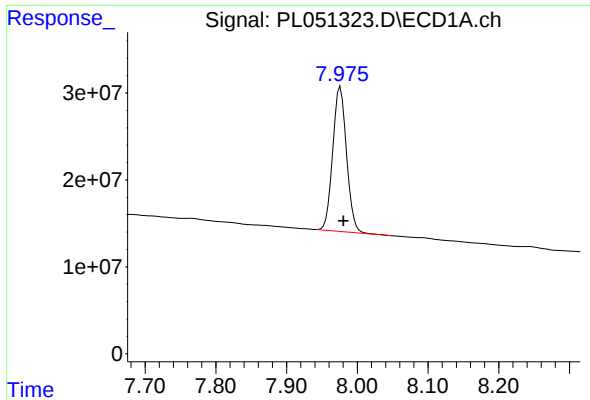

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.004 min
Response: 225151628
Conc: 22.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
2S-J-(0-1)-COMP

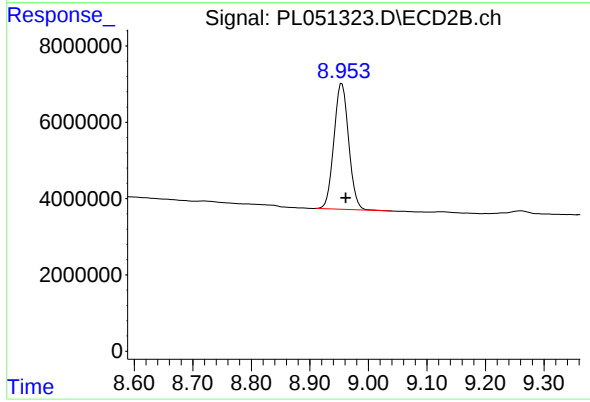

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.007 min
Response: 57751373
Conc: 20.42 ng/ml