

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051327.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 19:50
 Operator : SM\AJ
 Sample : K4231-05
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 REACTOR-3-B(0-3)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:49:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	244.4E6	66439948	24.327	23.286
28)	SA Decachlor...	7.976	8.956	278.9E6	70487193	27.540	24.926
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	4197899	N.D.	2.428 #
9)	A Endosulfan I	5.338f	0.000	9432795	0	0.649	N.D. #
10)	B gamma-Chl...	5.202	0.000	34915313	0	2.212	N.D. #
11)	B alpha-Chl...	5.244	0.000	54312108	0	3.560	N.D. #
25)	Chlordane-3	5.202	0.000	34915313	0	24.943	N.D. #
26)	Chlordane-4	5.244	0.000	54312108	0	41.177	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051327.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 19:50
Operator : SM\AJ
Sample : K4231-05
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
REACTOR-3-B(0-3)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:49:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

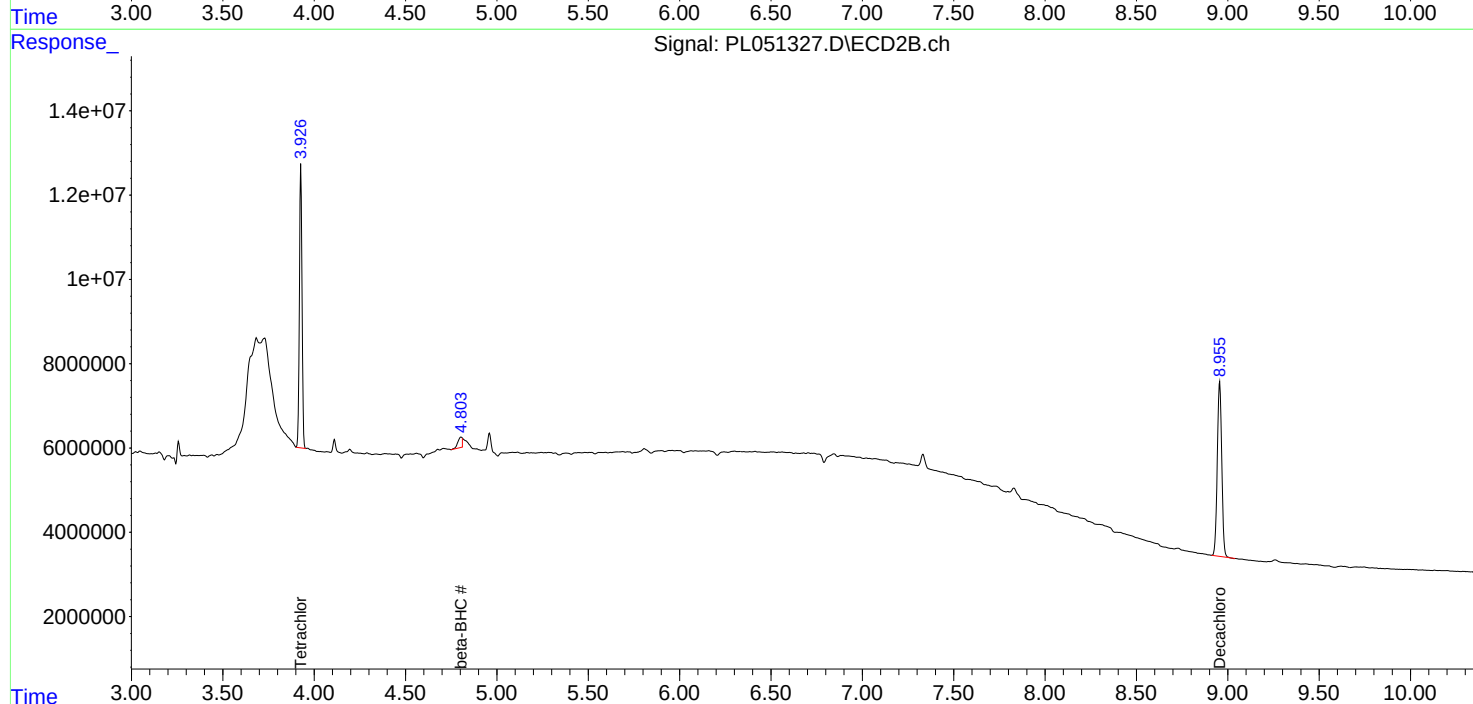


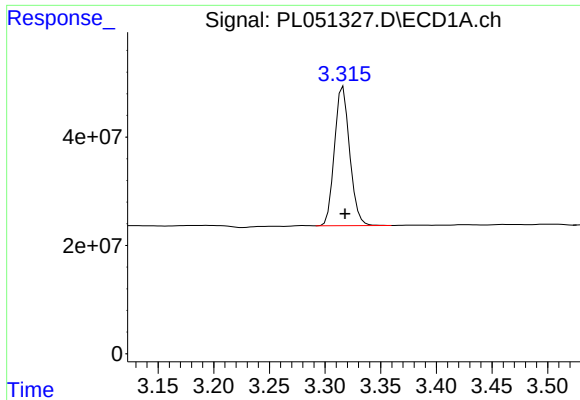

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 244438222
Conc: 24.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
REACTOR-3-B(0-3)

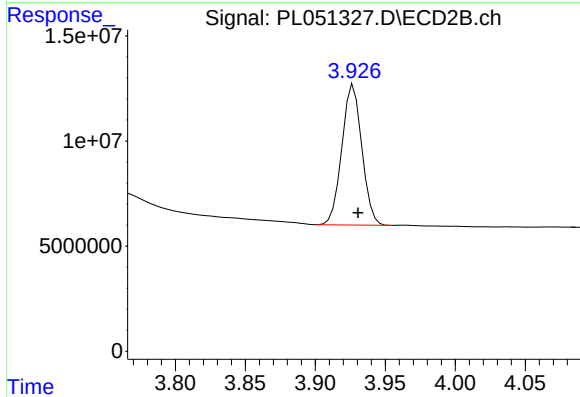


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 66439948
Conc: 23.29 ng/ml

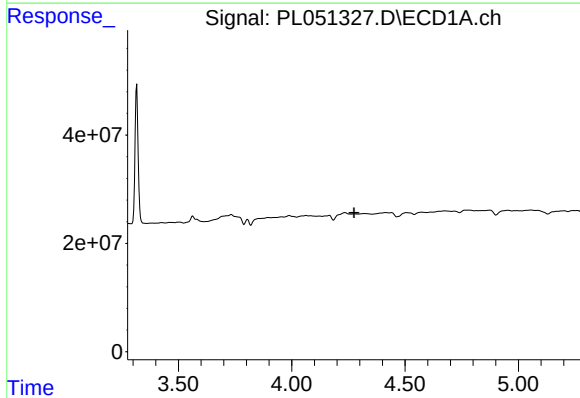


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

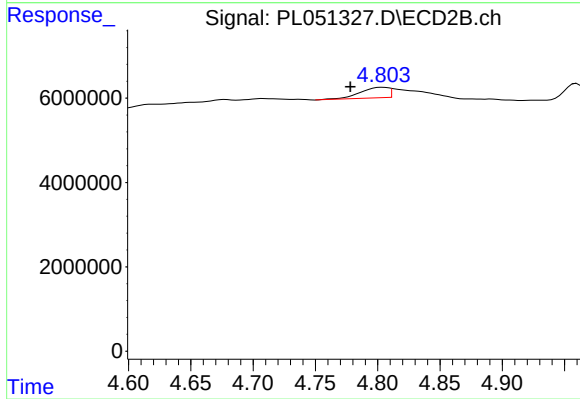

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 4197899
Conc: 2.43 ng/ml

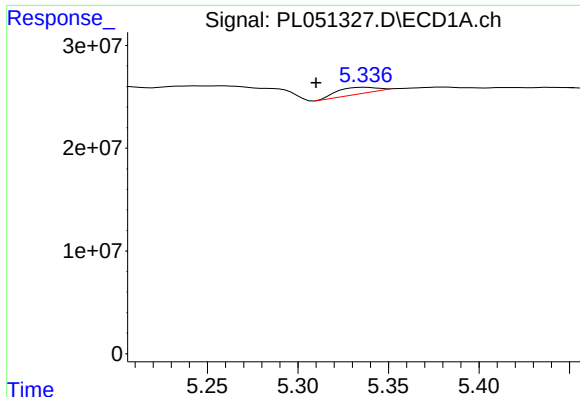

#9 Endosulfan I


R.T.: 5.338 min
Delta R.T.: 0.028 min
Response: 9432795
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
REACTOR-3-B(0-3)

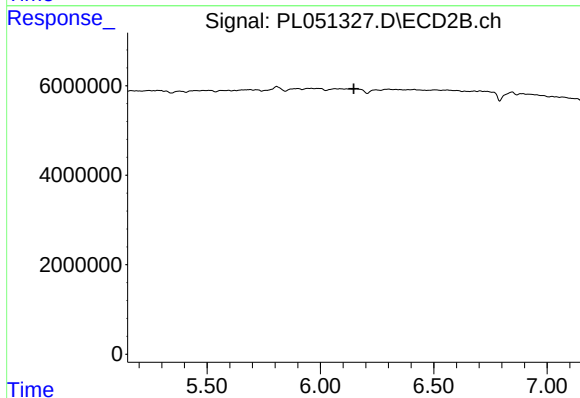


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.148 min
Response: 0
Conc: N.D.

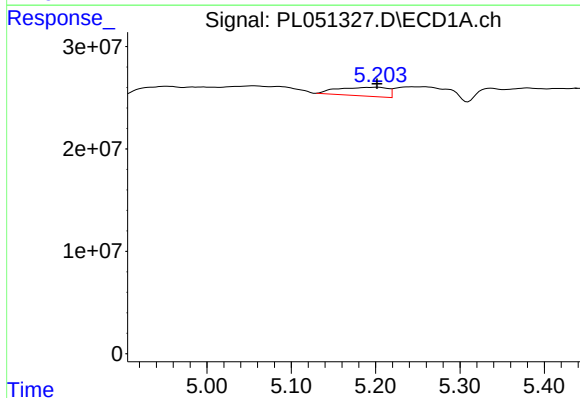


#10 gamma-Chlordane

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 34915313
Conc: 2.21 ng/ml

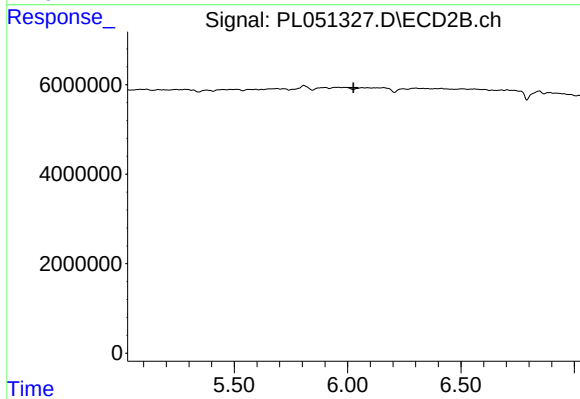

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

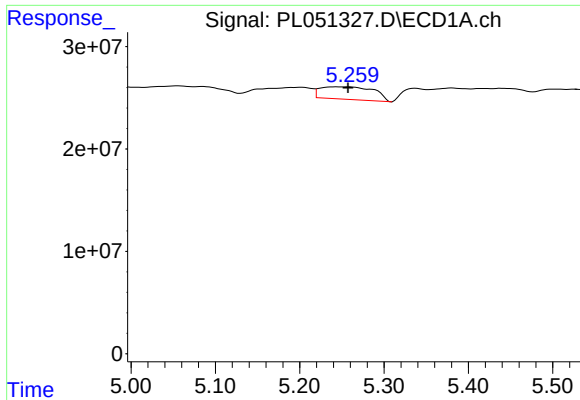

#11 alpha-Chlordane


R.T.: 5.244 min
Delta R.T.: -0.014 min
Response: 54312108
Conc: 3.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
REACTOR-3-B(0-3)

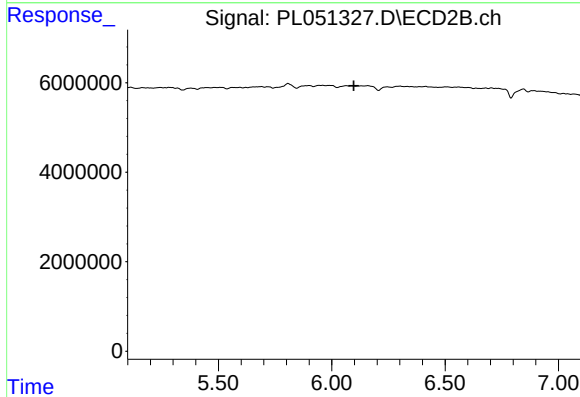


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

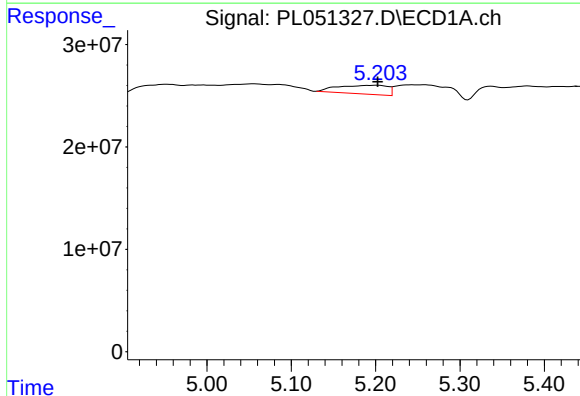


#25 Chlordane-3

R.T.: 5.202 min
Delta R.T.: 0.000 min
Response: 34915313
Conc: 24.94 ng/ml

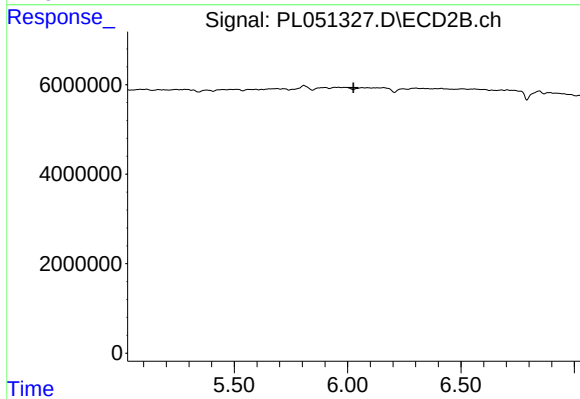

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

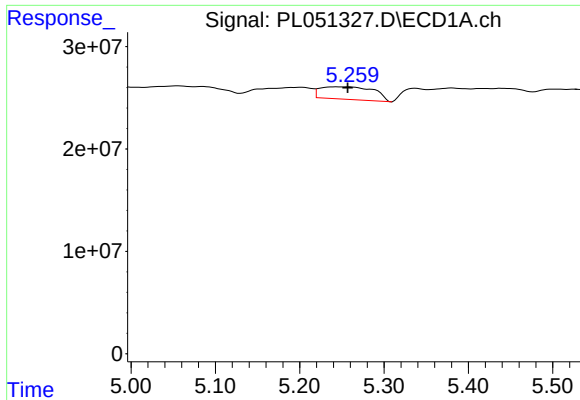

#26 Chlordane-4


R.T.: 5.244 min
Delta R.T.: -0.013 min
Response: 54312108
Conc: 41.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
REACTOR-3-B(0-3)

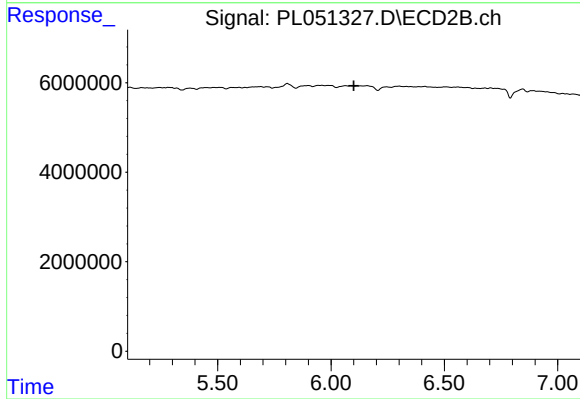


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

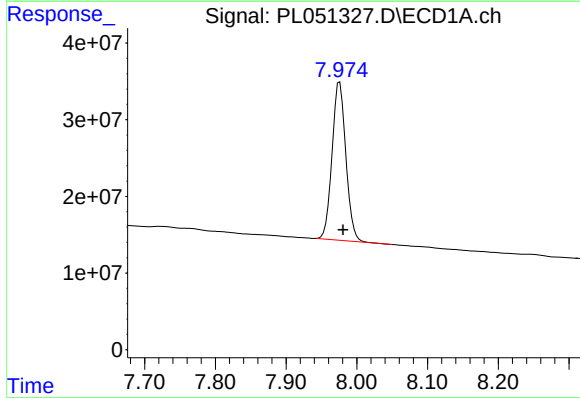

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 278857031
Conc: 27.54 ng/ml

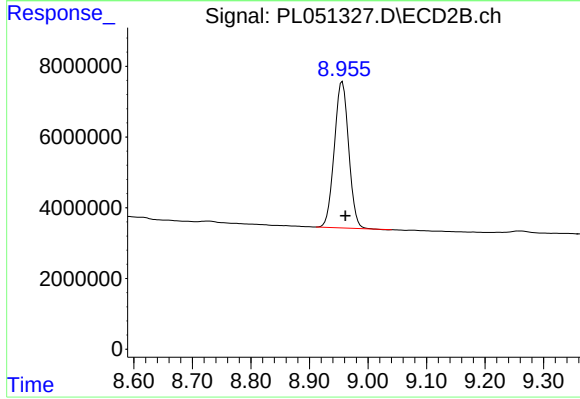

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 70487193
Conc: 24.93 ng/ml