

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2019 23:23
 Operator : SM\AJ
 Sample : K4090-05
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-080919-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:53:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	130.9E6	34262518	13.031	12.008
28)	SA Decachlor...	7.976	8.955	108.1E6	35164579	10.678	12.435
Target Compounds							
6)	B beta-BHC	0.000	4.796f	0	9247846	N.D.	5.349 #
10)	B gamma-Chl...	5.217f	0.000	8281008	0	0.525	N.D. #
11)	B alpha-Chl...	0.000	6.094	0	3990024	N.D.	1.089 #
23)	Chlordane-1	4.156	0.000	12475732	0	33.906	N.D. #
24)	Chlordane-2	4.643	0.000	8010662	0	17.897	N.D. #
25)	Chlordane-3	5.217	0.000	8281008	0	5.916	N.D. #
26)	Chlordane-4	0.000	6.094	0	3990024	N.D.	6.868 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2019 23:23
Operator : SM\AJ
Sample : K4090-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:53:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

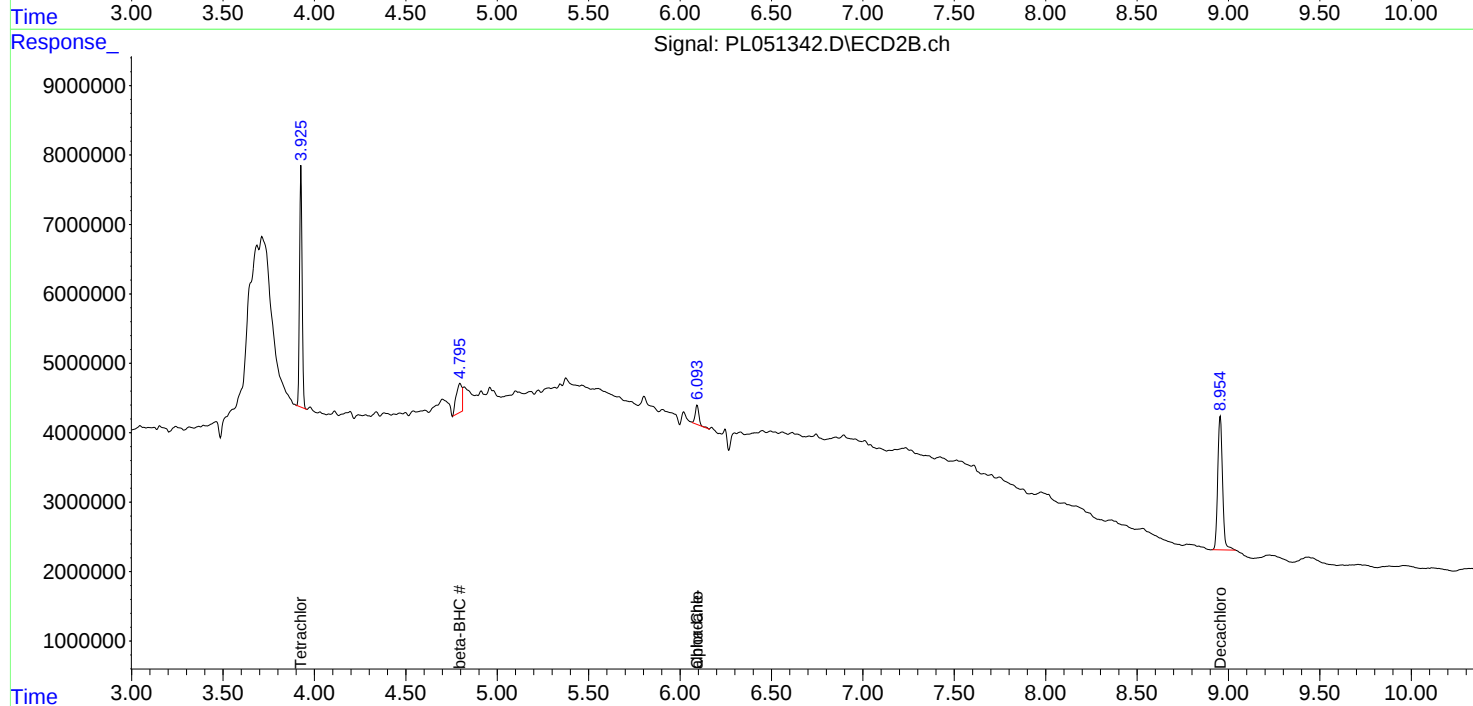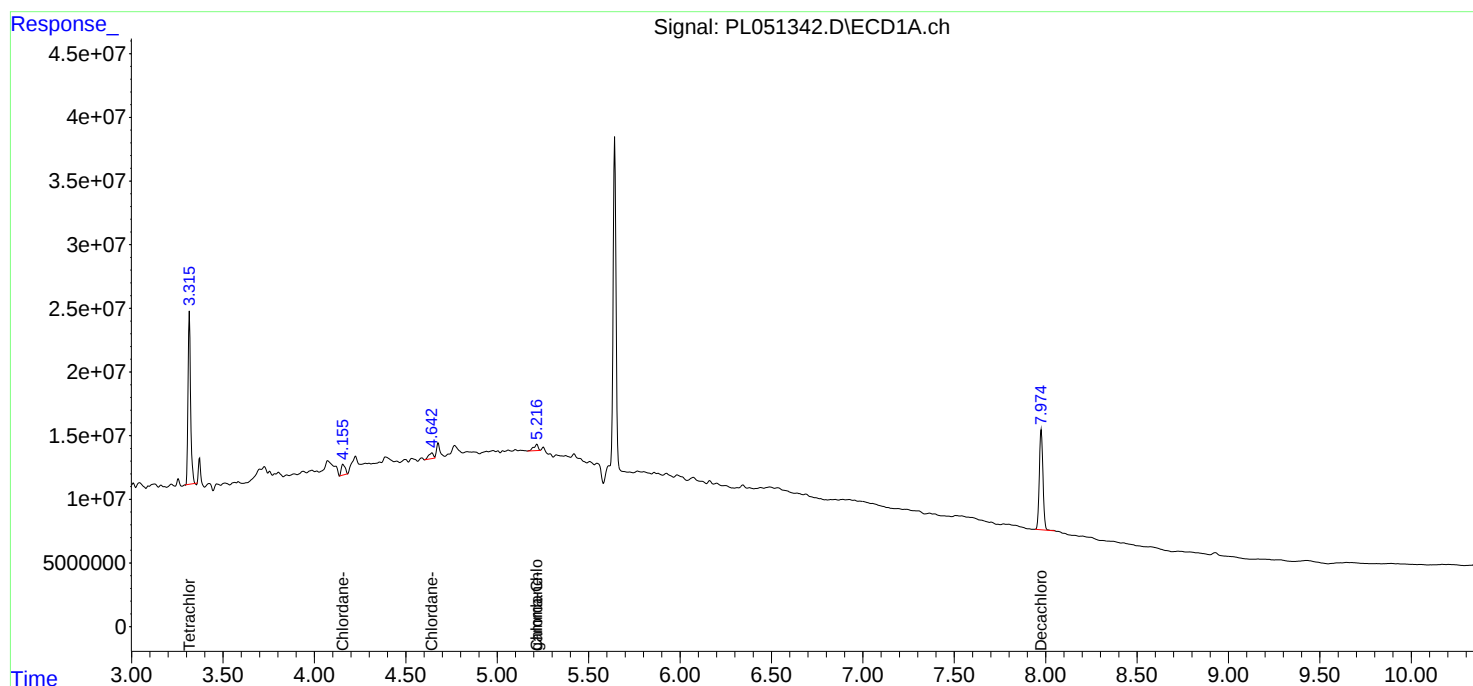


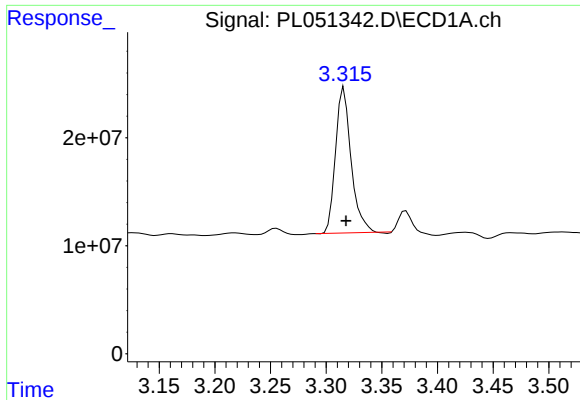

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 130934046
Conc: 13.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

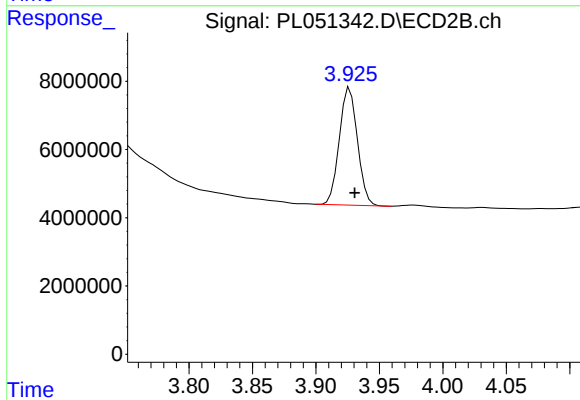


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 34262518
Conc: 12.01 ng/ml

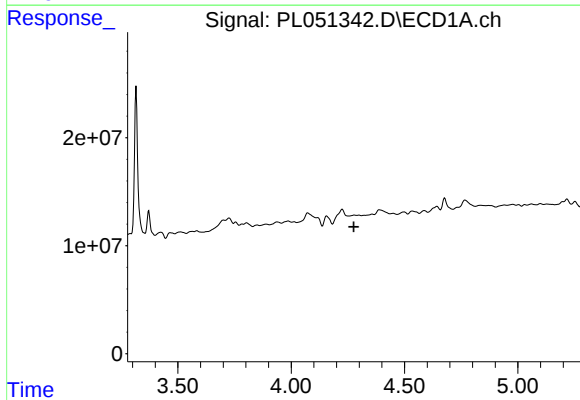


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

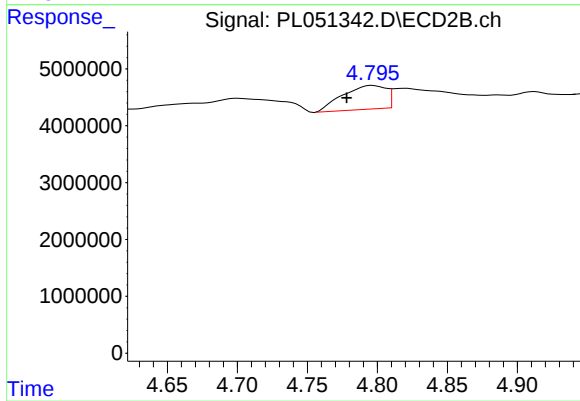

#6 beta-BHC


R.T.: 4.796 min
Delta R.T.: 0.018 min
Response: 9247846
Conc: 5.35 ng/ml

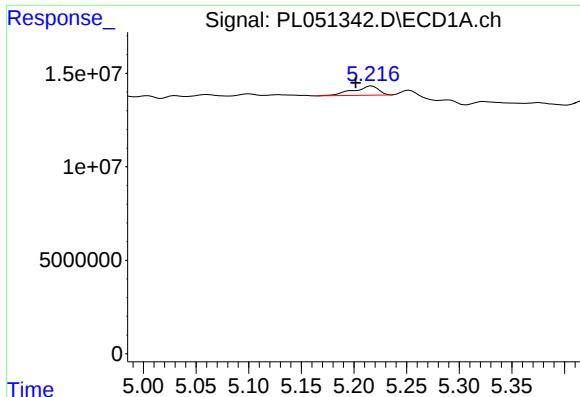

#10 gamma-Chlordane


R.T.: 5.217 min
Delta R.T.: 0.015 min
Response: 8281008
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

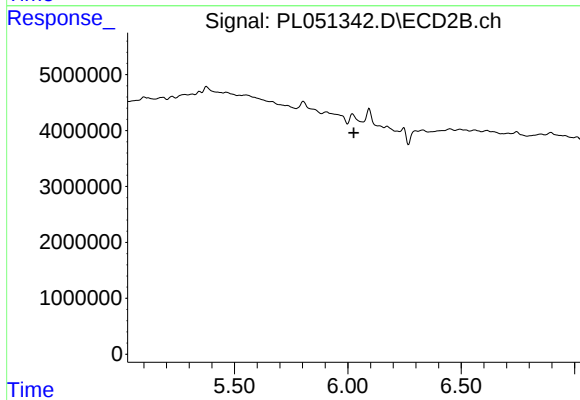


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

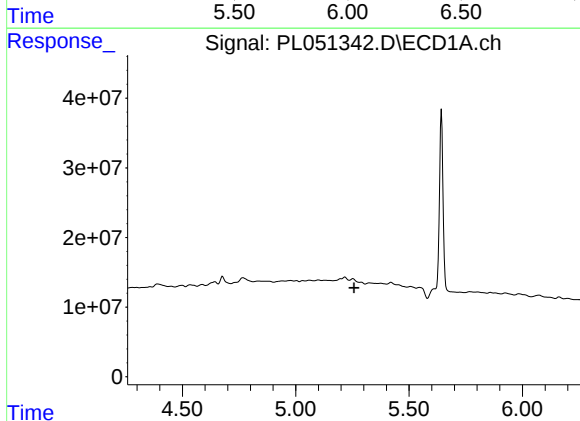


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

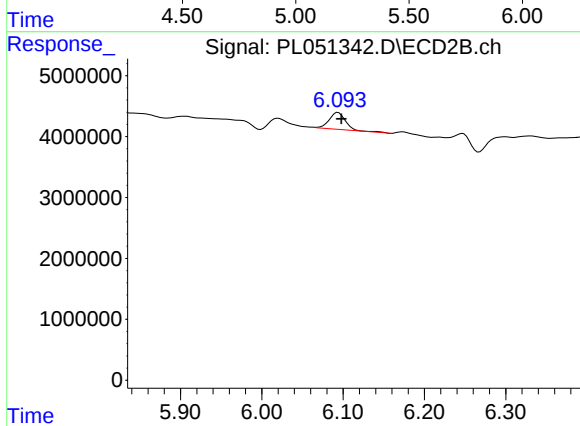

#11 alpha-Chlordane


R.T.: 6.094 min
Delta R.T.: -0.004 min
Response: 3990024
Conc: 1.09 ng/ml

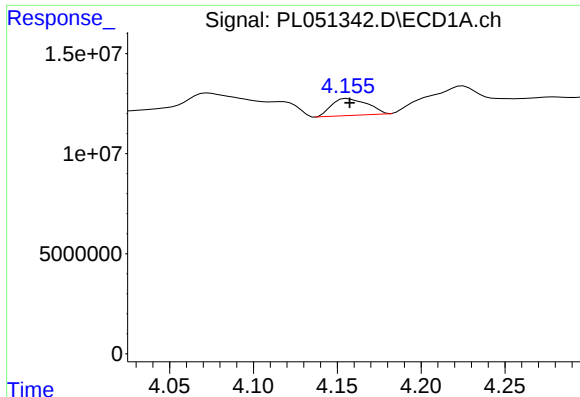

#23 Chlordane-1


R.T.: 4.156 min
Delta R.T.: -0.001 min
Response: 12475732
Conc: 33.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

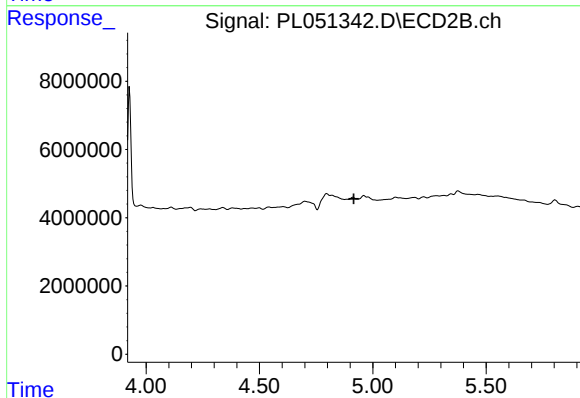


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.916 min
Response: 0
Conc: N.D.

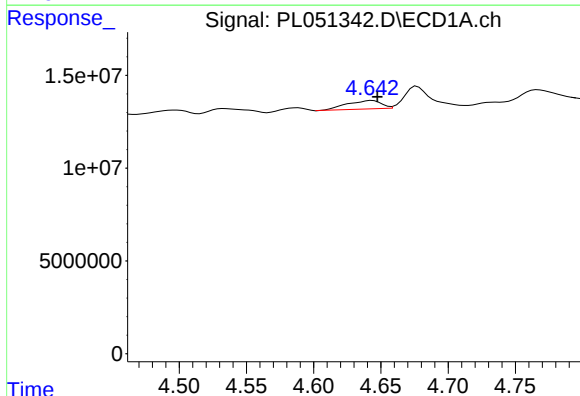


#24 Chlordane-2

R.T.: 4.643 min
Delta R.T.: -0.004 min
Response: 8010662
Conc: 17.90 ng/ml

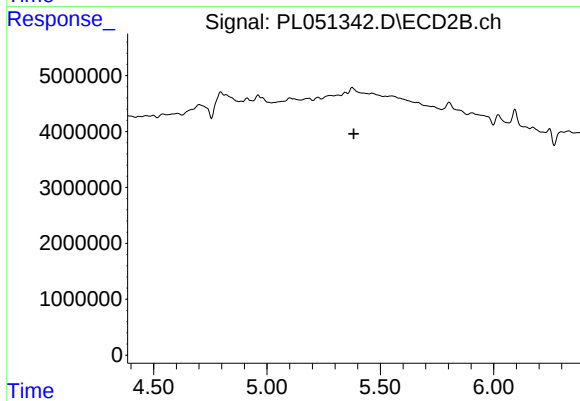

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.383 min
Response: 0
Conc: N.D.

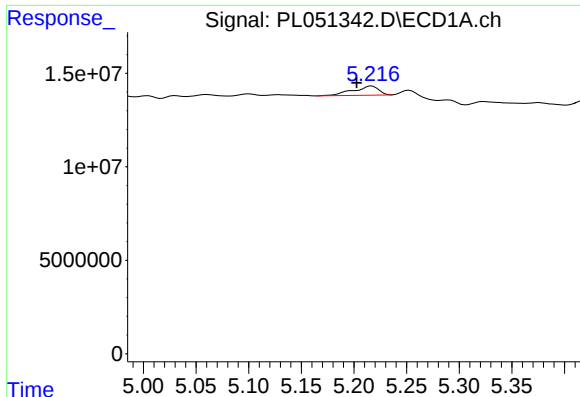

#25 Chlordane-3


R.T.: 5.217 min
Delta R.T.: 0.015 min
Response: 8281008
Conc: 5.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

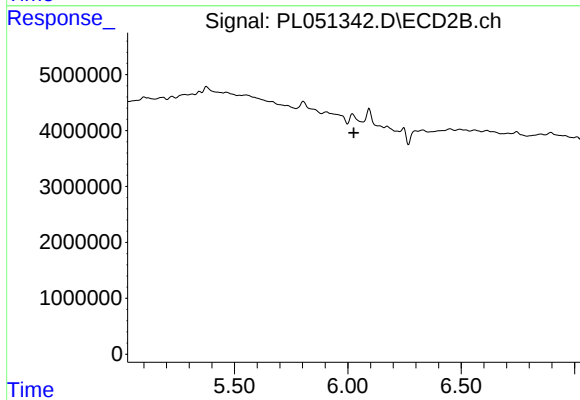


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

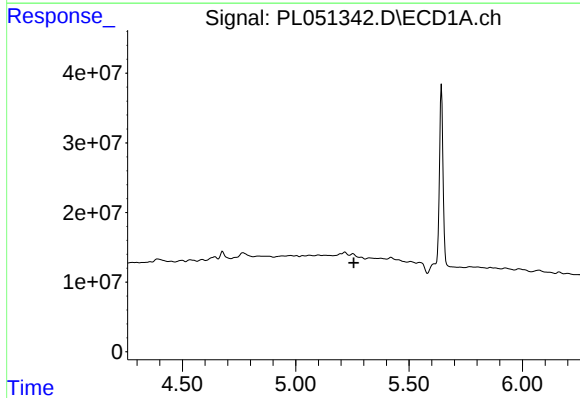


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

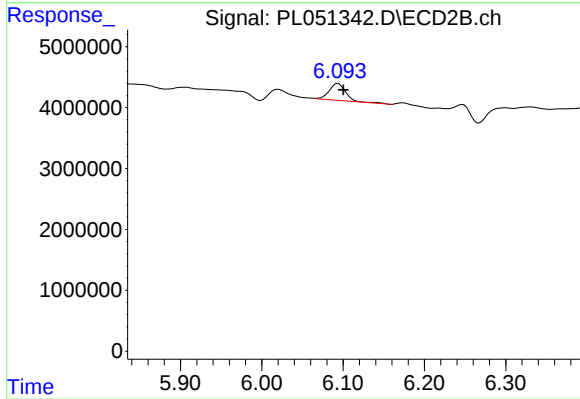

#26 Chlordane-4


R.T.: 6.094 min
Delta R.T.: -0.006 min
Response: 3990024
Conc: 6.87 ng/ml

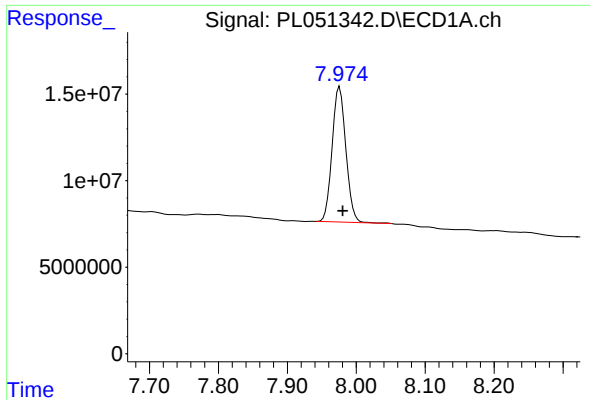

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 108113576
Conc: 10.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-080919-A

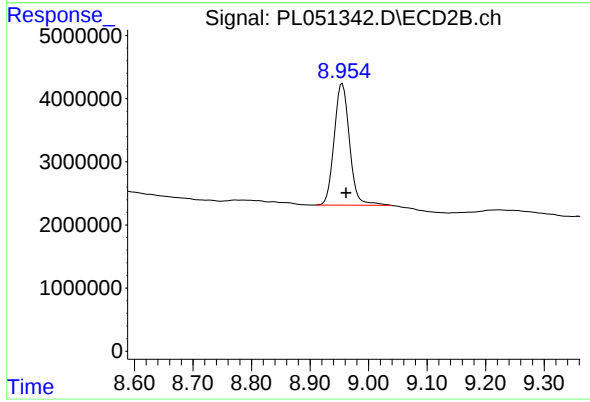

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 35164579
Conc: 12.43 ng/ml