

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 01:59
 Operator : SM\AJ
 Sample : K4294-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RBR-200052

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:56:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	173.5E6	44013352	17.263	15.426
28)	SA Decachlor...	7.976	8.955	83213146	22915797	8.218	8.103
Target Compounds							
2)	A alpha-BHC	3.750	0.000	12567500	0	0.750	N.D. #
5)	MB Aldrin	4.557	0.000	1025277	0	0.066	N.D. #
8)	B Heptachlo...	0.000	5.802	0	3022552	N.D.	0.790 #
10)	B gamma-Chl...	5.197	0.000	40880137	0	2.590	N.D. #
11)	B alpha-Chl...	5.253	0.000	23103558	0	1.514	N.D. #
15)	B Endosulfa...	0.000	6.845	0	961405	N.D.	0.302 #
25)	Chlordane-3	5.197	0.000	40880137	0	29.205	N.D. #
26)	Chlordane-4	5.253	0.000	23103558	0	17.516	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 01:59
Operator : SM\AJ
Sample : K4294-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RBR-200052

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:56:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

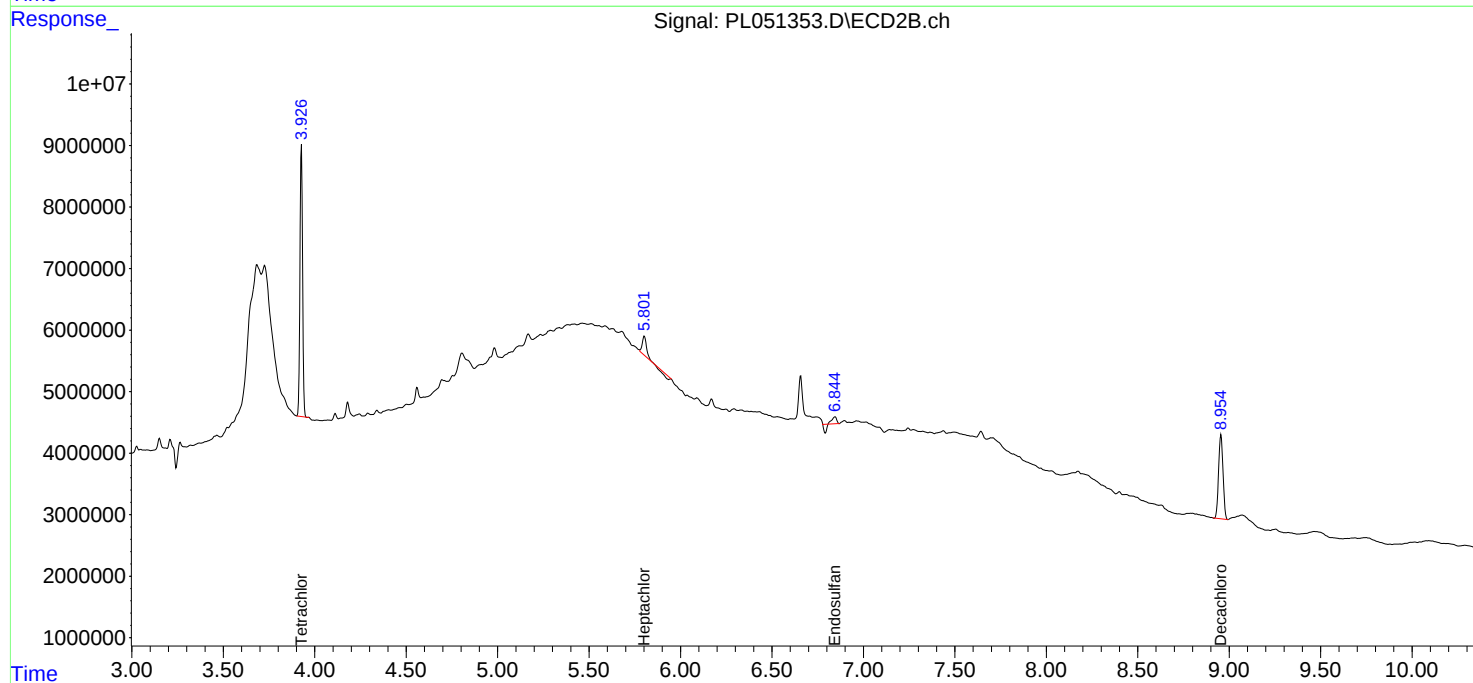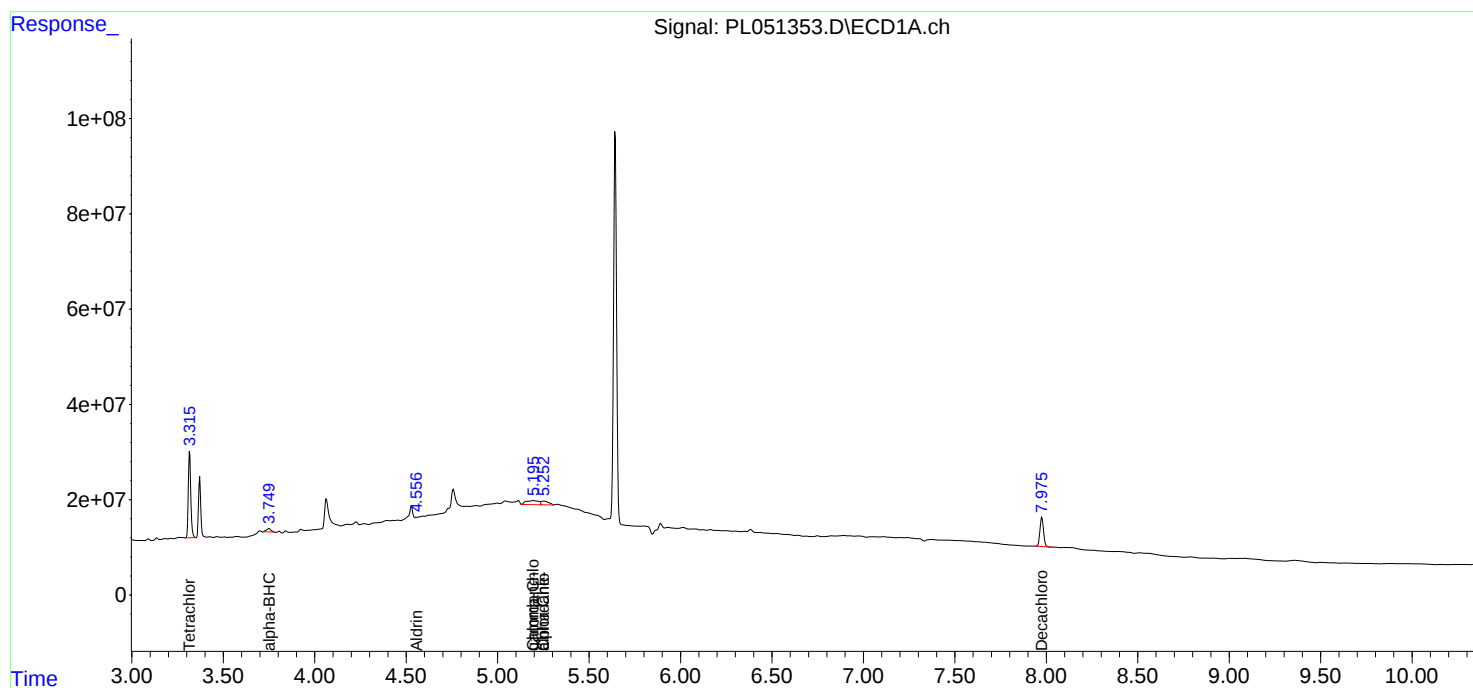


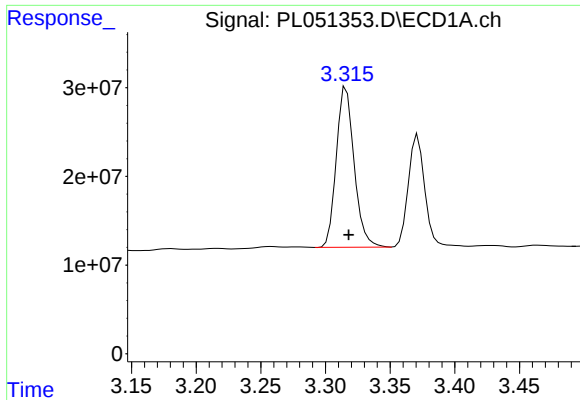

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 173452737
Conc: 17.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

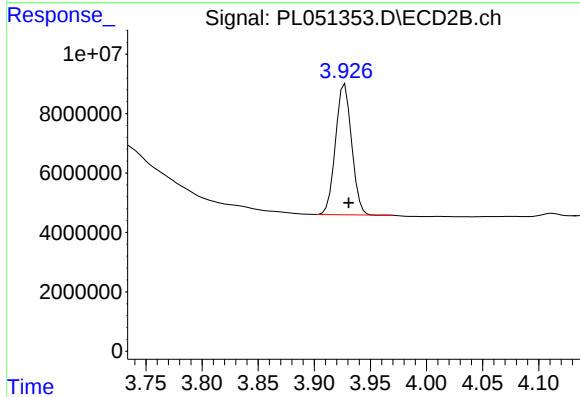


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 44013352
Conc: 15.43 ng/ml

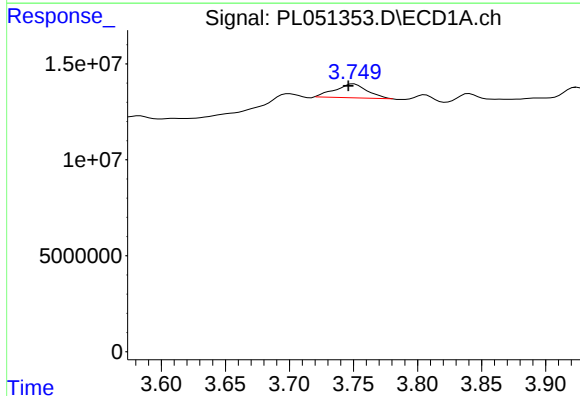


#2 alpha-BHC

R.T.: 3.750 min
Delta R.T.: 0.004 min
Response: 12567500
Conc: 0.75 ng/ml

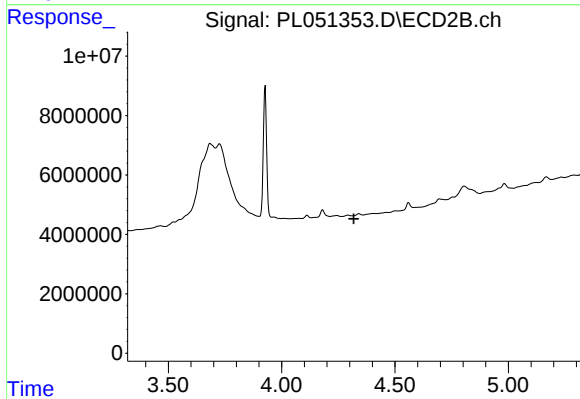

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.319 min
Response: 0
Conc: N.D.

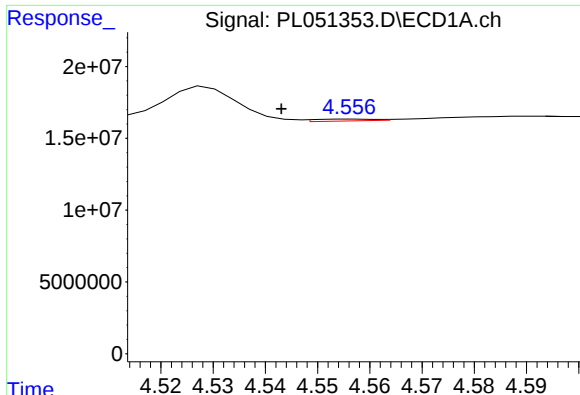

#5 Aldrin


R.T.: 4.557 min
Delta R.T.: 0.014 min
Response: 1025277
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

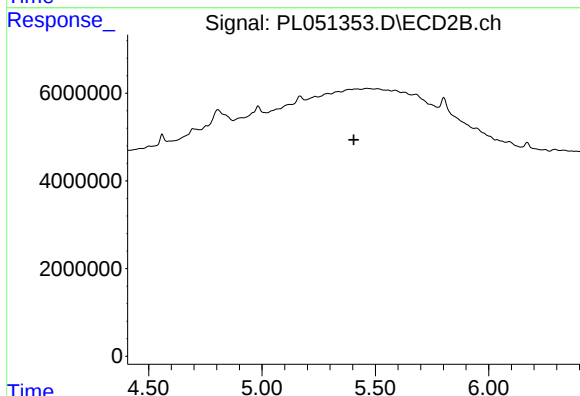


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

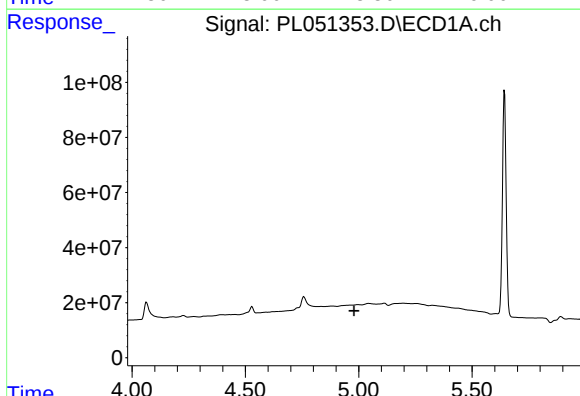


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.979 min
Response: 0
Conc: N.D.

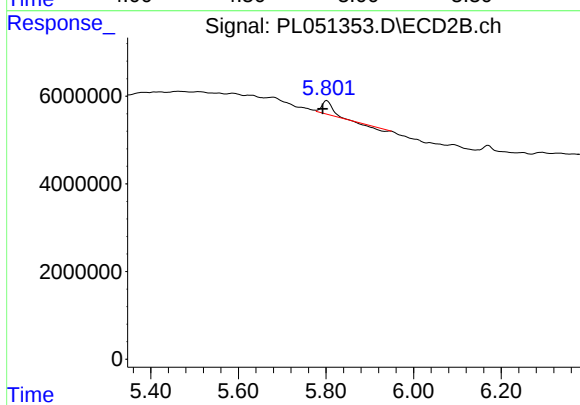

#8 Heptachlor epoxide


R.T.: 5.802 min
Delta R.T.: 0.010 min
Response: 3022552
Conc: 0.79 ng/ml

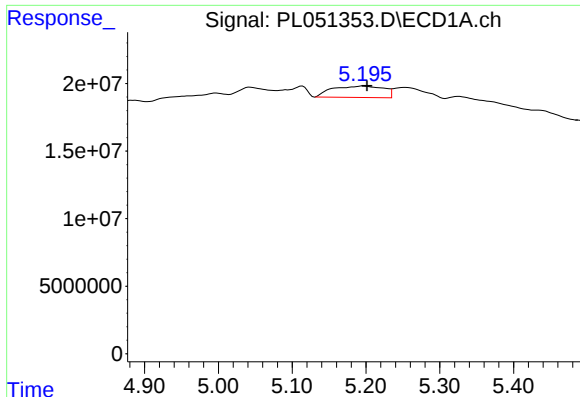

#10 gamma-Chlordane


R.T.: 5.197 min
Delta R.T.: -0.005 min
Response: 40880137
Conc: 2.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

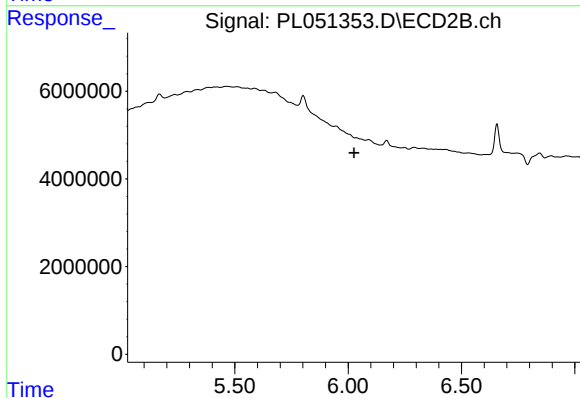


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

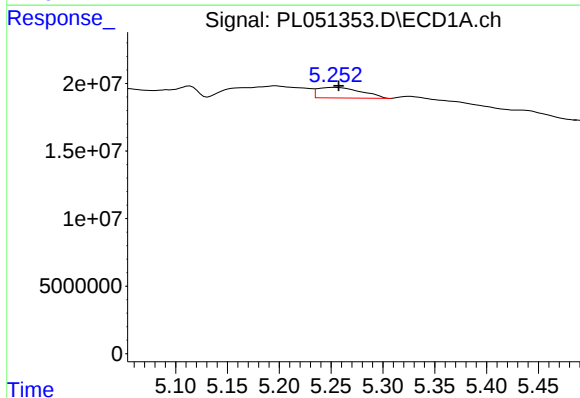


#11 alpha-Chlordane

R.T.: 5.253 min
Delta R.T.: -0.004 min
Response: 23103558
Conc: 1.51 ng/ml

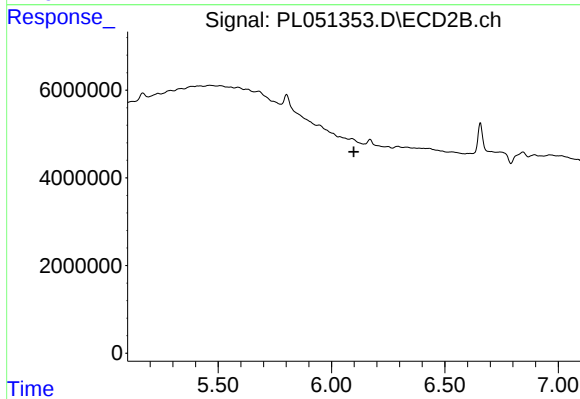

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

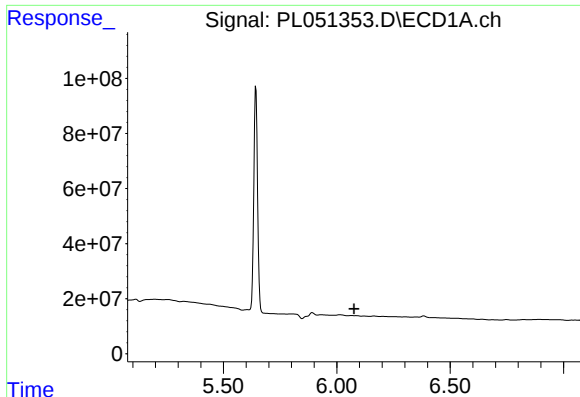

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
RBR-200052

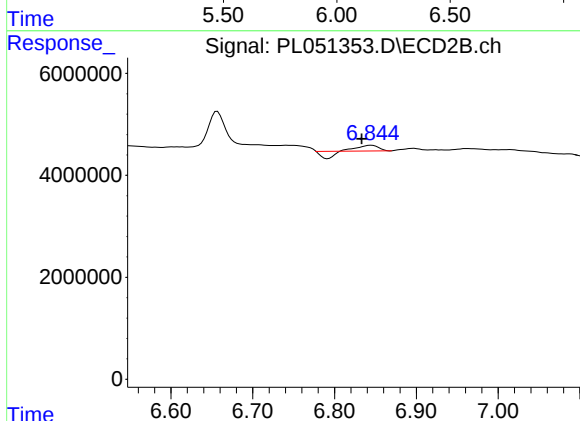


#15 Endosulfan II

R.T.: 6.845 min
Delta R.T.: 0.012 min
Response: 961405
Conc: 0.30 ng/ml

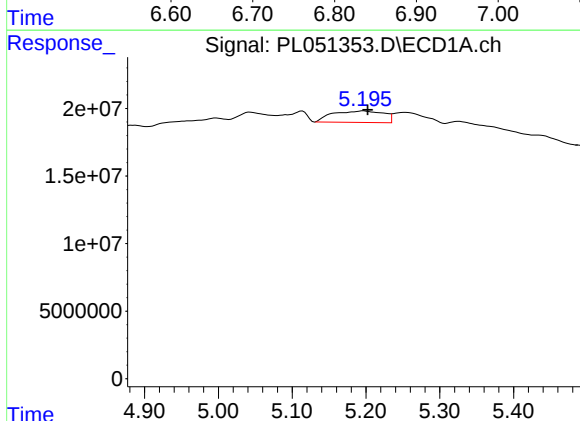


#25 Chlordane-3

R.T.: 5.197 min
Delta R.T.: -0.006 min
Response: 40880137
Conc: 29.20 ng/ml

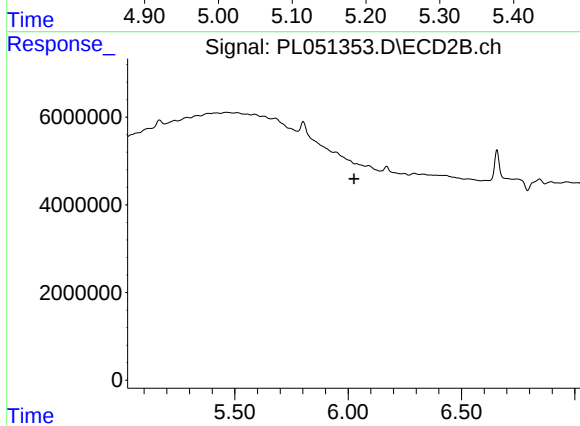

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 6.027 min
Response: 0
Conc: N.D.

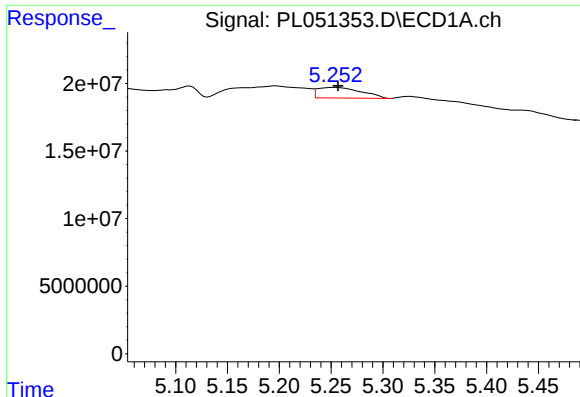

#26 Chlordane-4


R.T.: 5.253 min
Delta R.T.: -0.004 min
Response: 23103558
Conc: 17.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR-200052

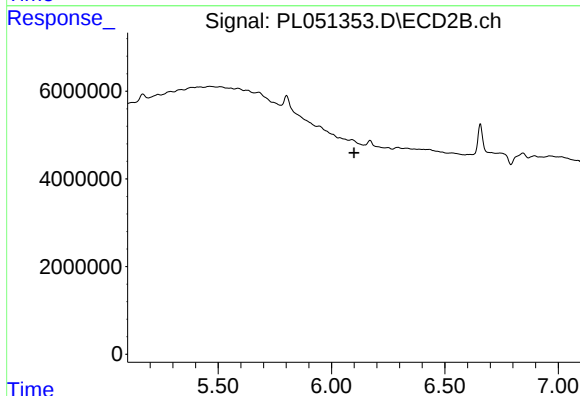


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

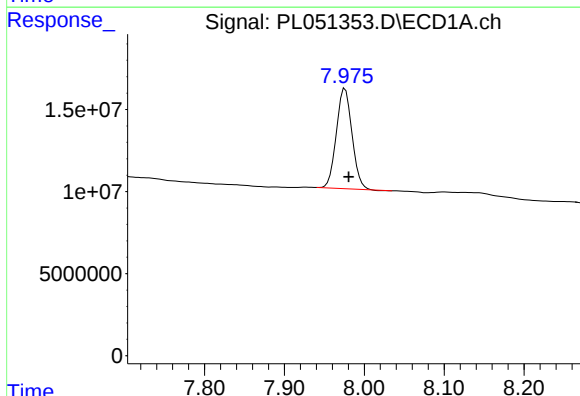

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 83213146
Conc: 8.22 ng/ml

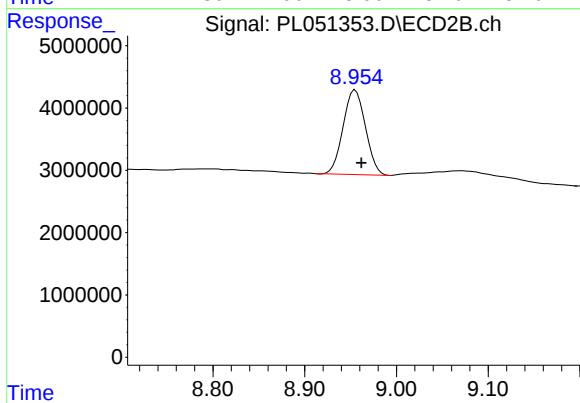

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 22915797
Conc: 8.10 ng/ml