

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 04:21
 Operator : SM\AJ
 Sample : K4239-04
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-034-B233-080519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:58:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	240.3E6	54804888	23.914	19.208
28)	SA Decachlor...	7.977	8.956	132.6E6	36128403	13.098	12.776
Target Compounds							
6)	B beta-BHC	0.000	4.804f	0	2529537	N.D.	1.463 #
8)	B Heptachlo...	0.000	5.804	0	5298144	N.D.	1.385 #
9)	A Endosulfan I	5.338f	0.000	3010219	0	0.207	N.D. #
11)	B alpha-Chl...	5.266	0.000	8068977	0	0.529	N.D. #
13)	MA Dieldrin	5.561	0.000	14340351	0	0.925	N.D. #
16)	A 4,4'-DDD	5.963f	0.000	5011282	0	0.418	N.D. #
26)	Chlordane-4	5.266	0.000	8068977	0	6.118	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 04:21
Operator : SM\AJ
Sample : K4239-04
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:58:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

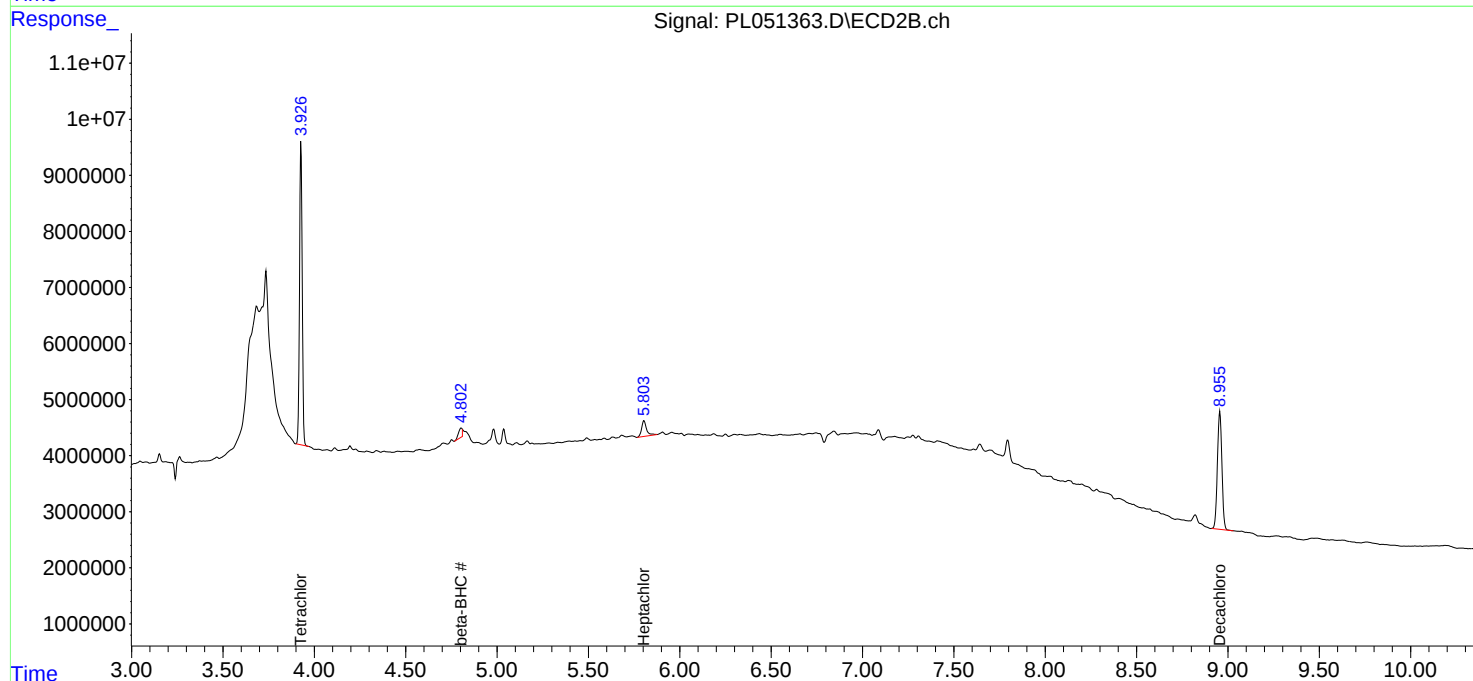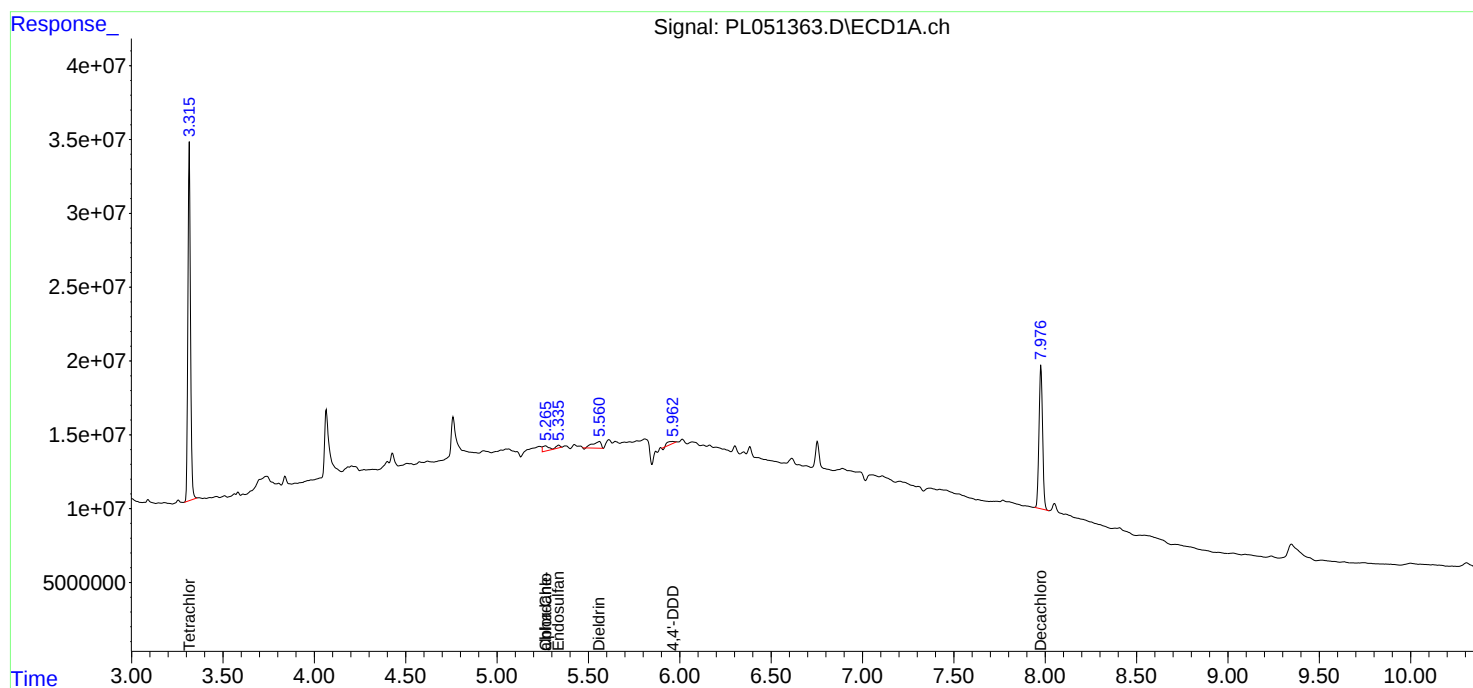


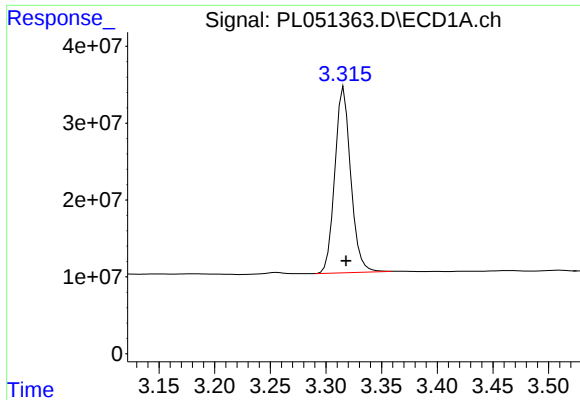

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 240283831
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

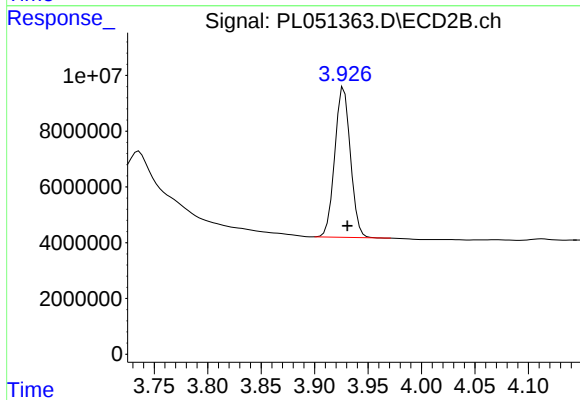


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 54804888
Conc: 19.21 ng/ml

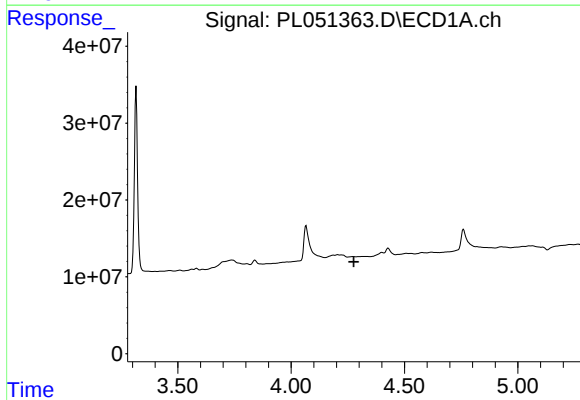


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

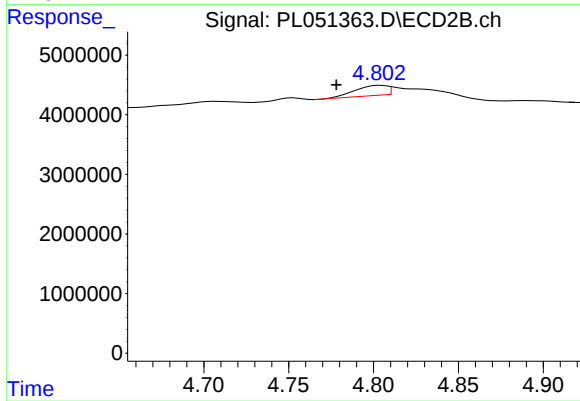

#6 beta-BHC


R.T.: 4.804 min
Delta R.T.: 0.026 min
Response: 2529537
Conc: 1.46 ng/ml

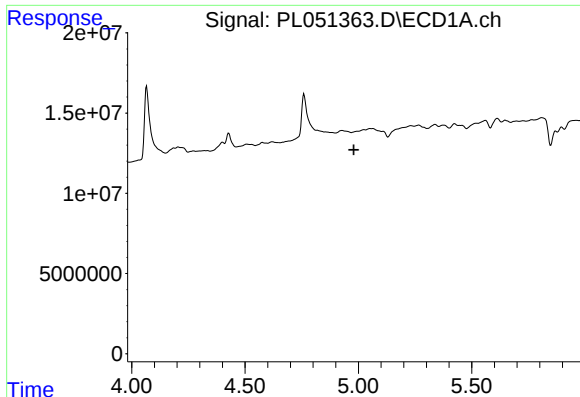

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

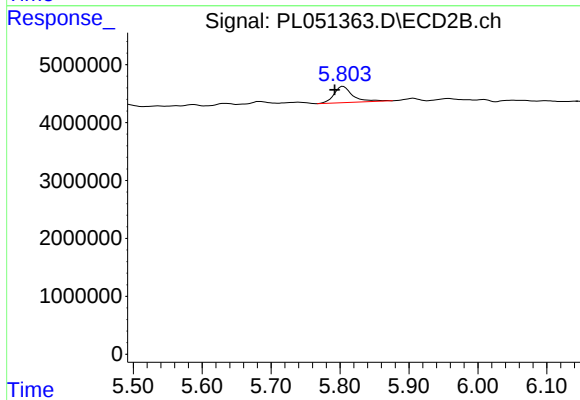


#8 Heptachlor epoxide

R.T.: 5.804 min
Delta R.T.: 0.012 min
Response: 5298144
Conc: 1.39 ng/ml

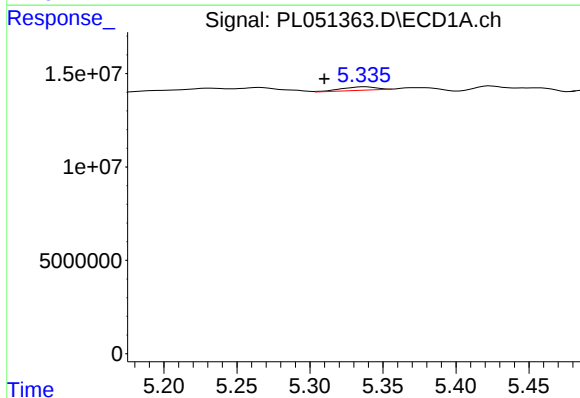


#9 Endosulfan I

R.T.: 5.338 min
Delta R.T.: 0.028 min
Response: 3010219
Conc: 0.21 ng/ml

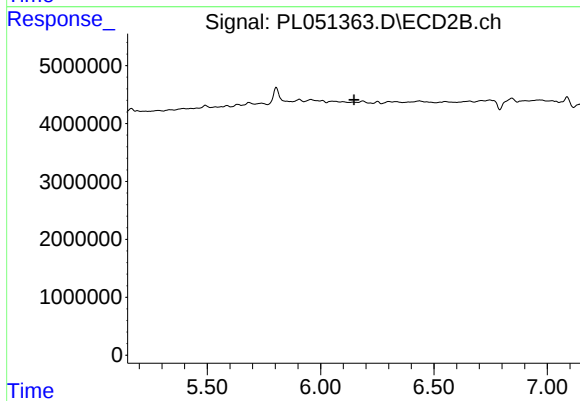

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

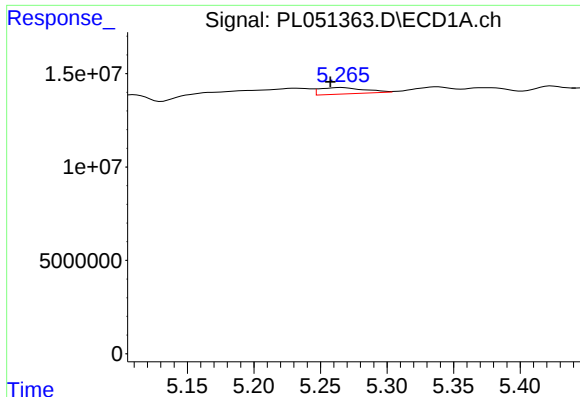

#11 alpha-Chlordane


R.T.: 5.266 min
Delta R.T.: 0.009 min
Response: 8068977
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

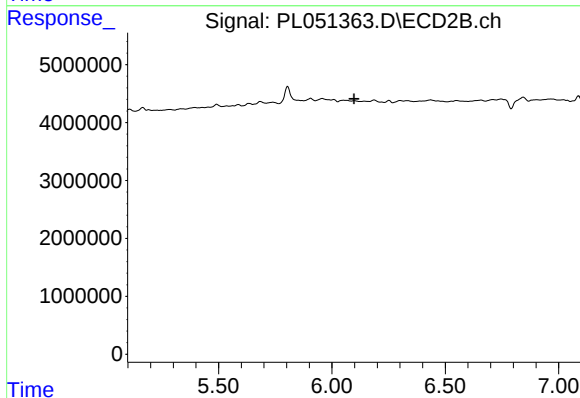


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

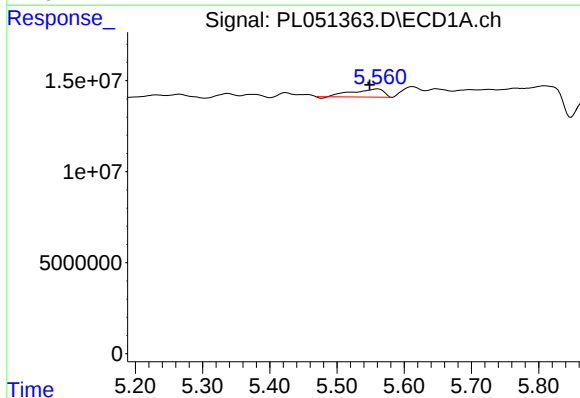


#13 Dieldrin

R.T.: 5.561 min
Delta R.T.: 0.012 min
Response: 14340351
Conc: 0.93 ng/ml

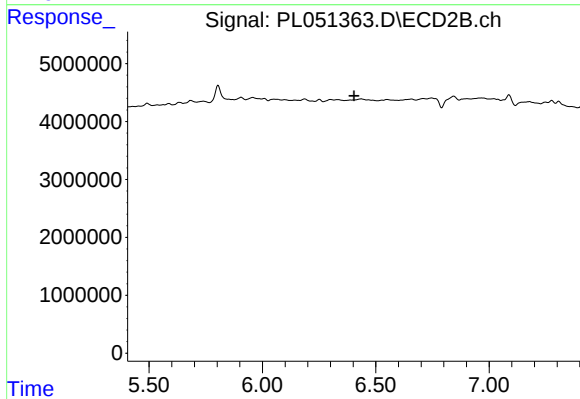

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

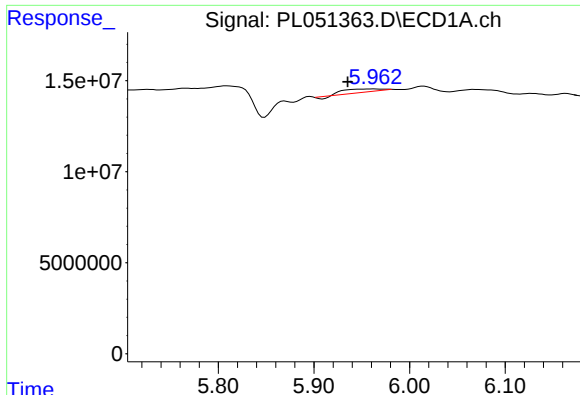

#16 4,4'-DDD


R.T.: 5.963 min
Delta R.T.: 0.027 min
Response: 5011282
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

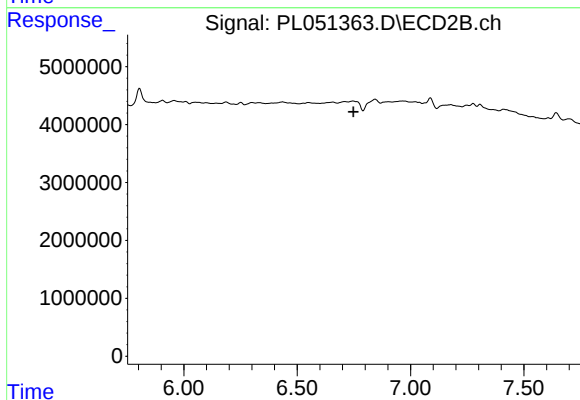


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

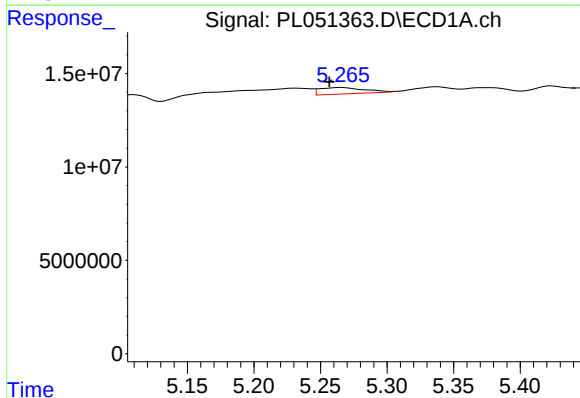


#26 Chlordane-4

R.T.: 5.266 min
Delta R.T.: 0.010 min
Response: 8068977
Conc: 6.12 ng/ml

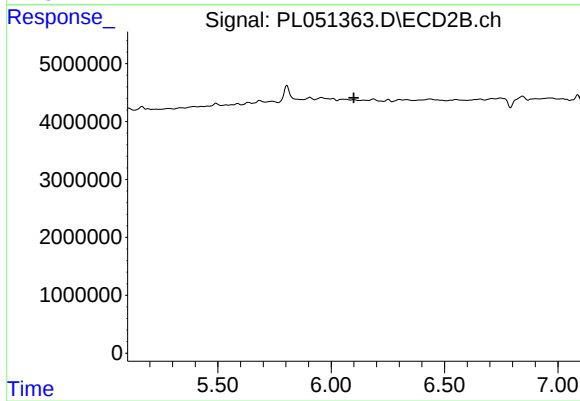

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.100 min
Response: 0
Conc: N.D.

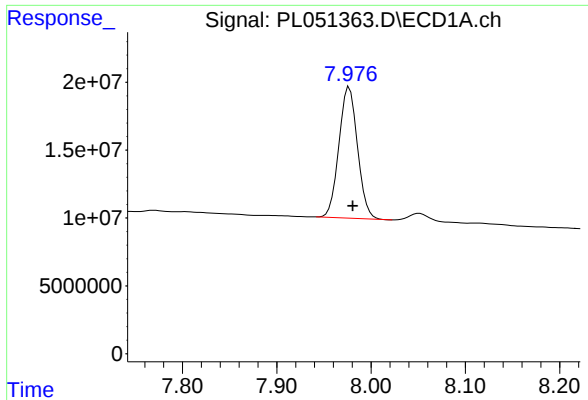

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 132626131
Conc: 13.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-034-B233-080519

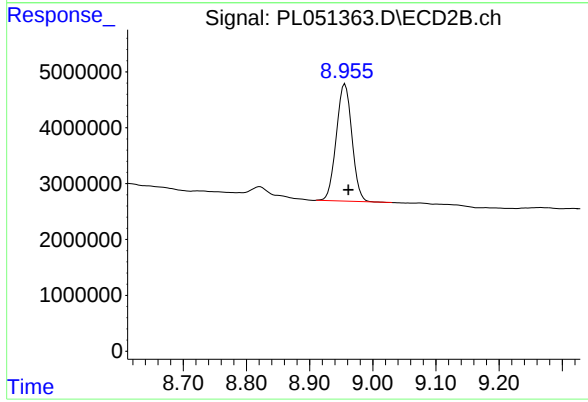

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 36128403
Conc: 12.78 ng/ml