

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 06:00
 Operator : SM\AJ
 Sample : K4239-08
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-013-B209-080519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 06:44:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.927	293.4E6	58180741	29.204	20.391 #
28)	SA Decachlor...	7.976	8.955	136.6E6	37191012	13.491	13.151
Target Compounds							
7)	B delta-BHC	0.000	4.981	0	3336680	N.D.	0.863 #
8)	B Heptachlo...	0.000	5.803	0	5888159	N.D.	1.539 #
9)	A Endosulfan I	5.339f	0.000	3180282	0	0.219	N.D. #
11)	B alpha-Chl...	5.249	0.000	19230713	0	1.261	N.D. #
13)	MA Dieldrin	5.559	0.000	16121421	0	1.040	N.D. #
16)	A 4,4'-DDD	5.963f	0.000	7072373	0	0.590	N.D. #
21)	B Endrin ke...	6.945	0.000	8165924	0	0.597	N.D. #
26)	Chlordane-4	5.249	0.000	19230713	0	14.580	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 06:00
Operator : SM\AJ
Sample : K4239-08
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 06:44:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

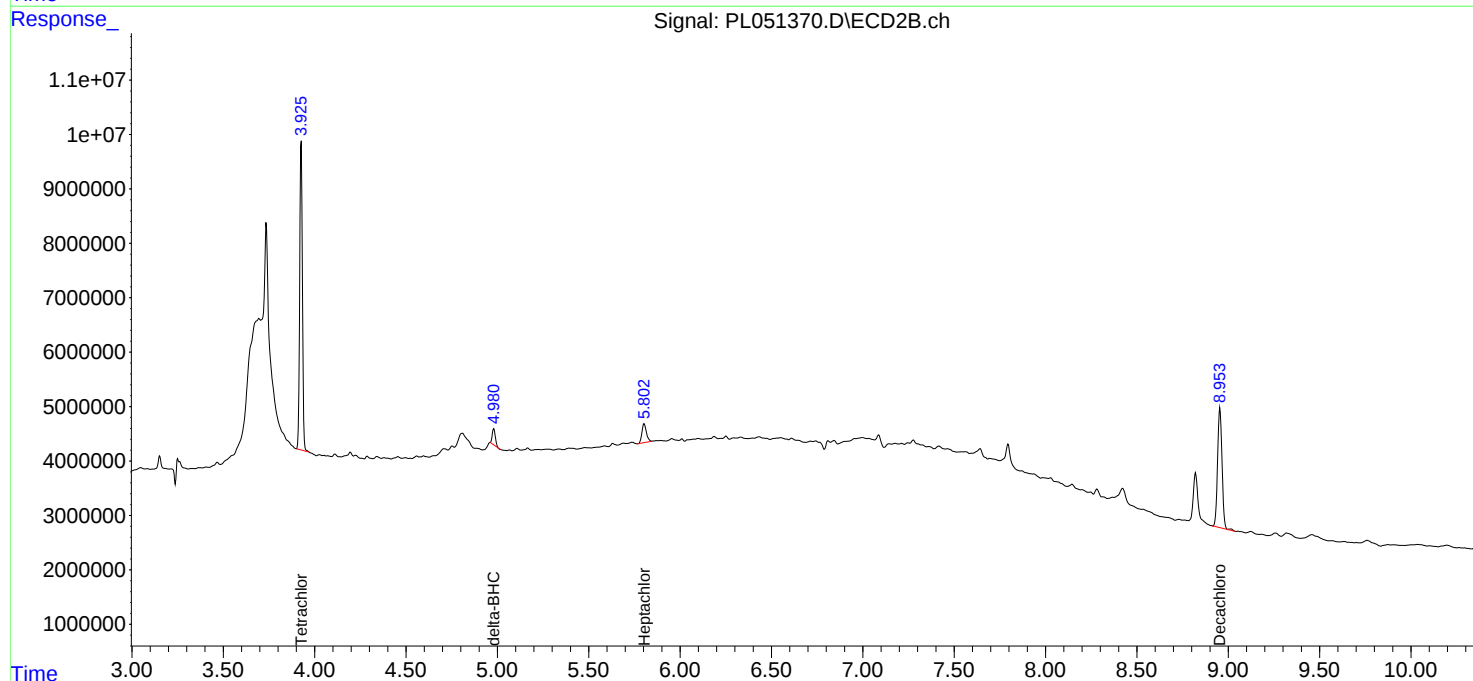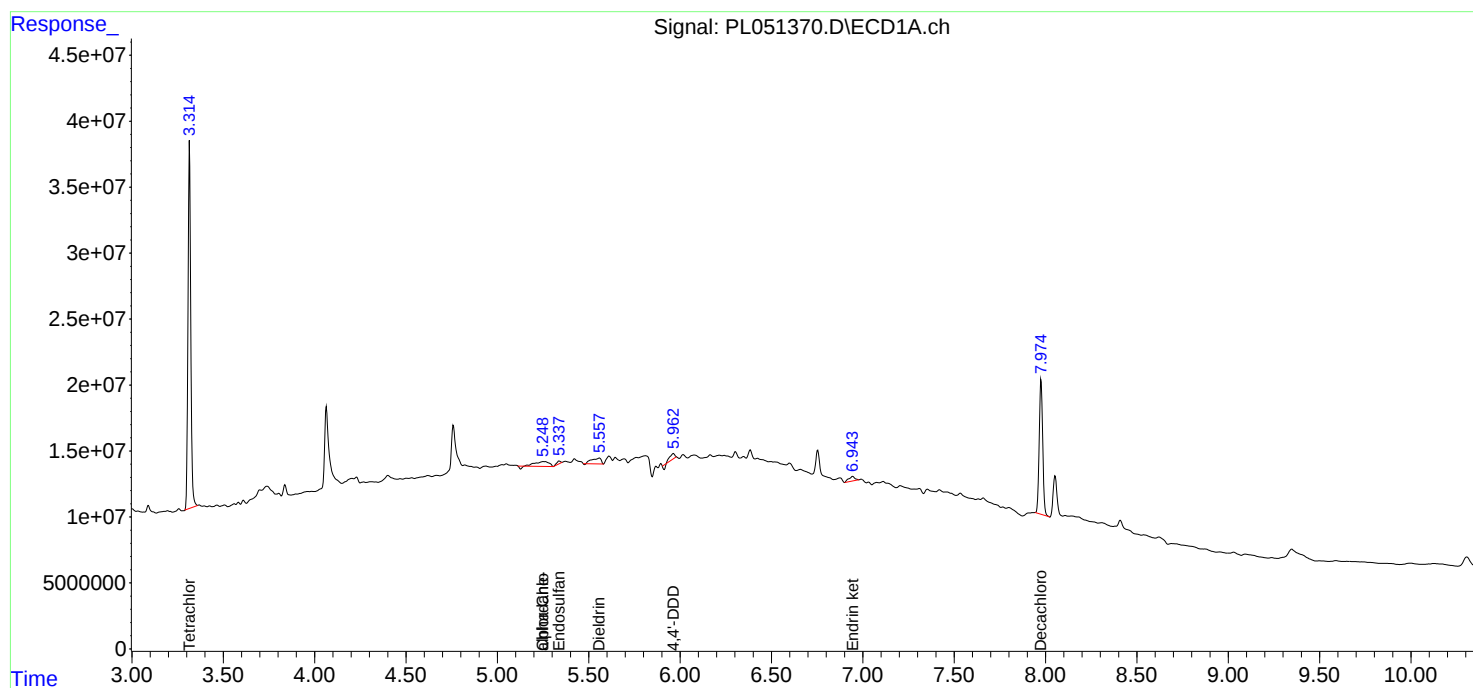


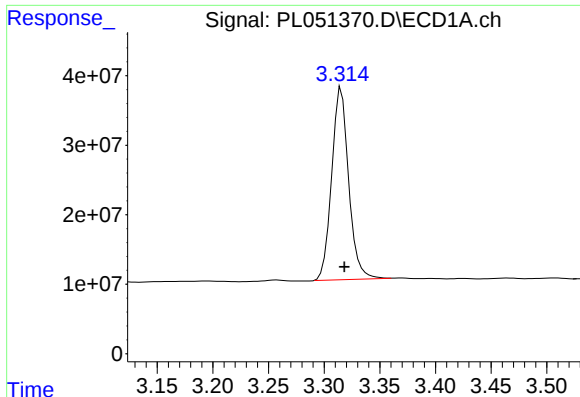

#1 Tetrachloro-m-xylene


R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 293438891
Conc: 29.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

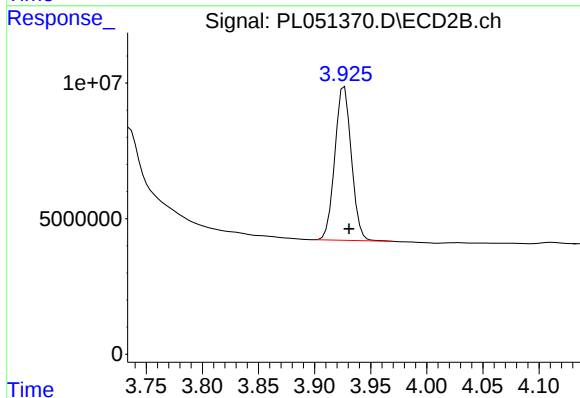


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 58180741
Conc: 20.39 ng/ml

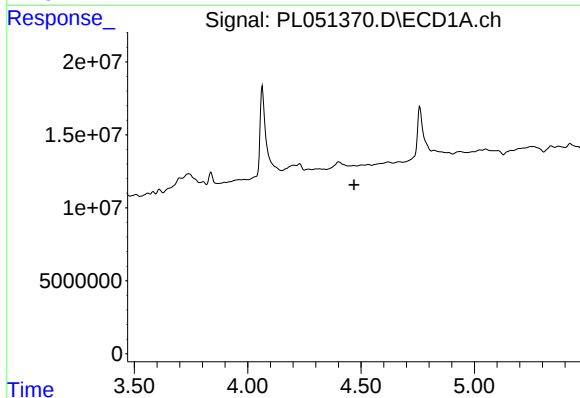


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.469 min
Response: 0
Conc: N.D.

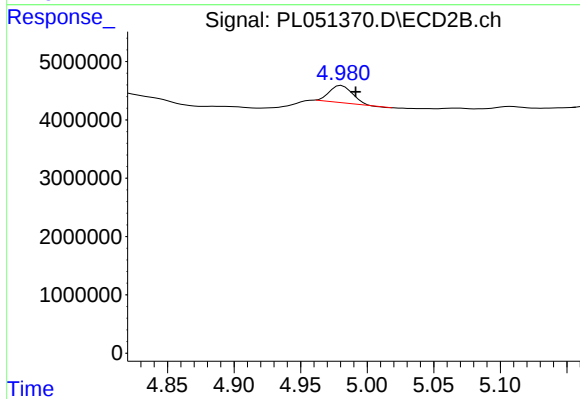

#7 delta-BHC


R.T.: 4.981 min
Delta R.T.: -0.011 min
Response: 3336680
Conc: 0.86 ng/ml

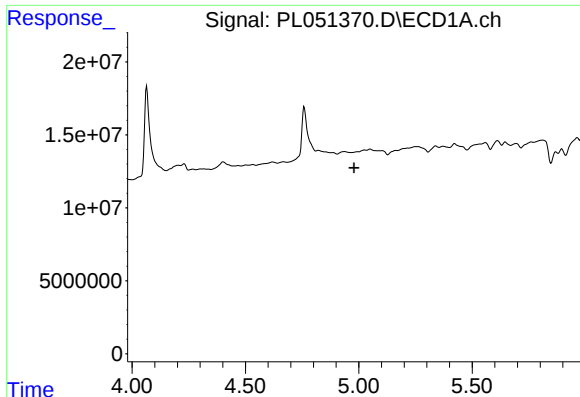

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

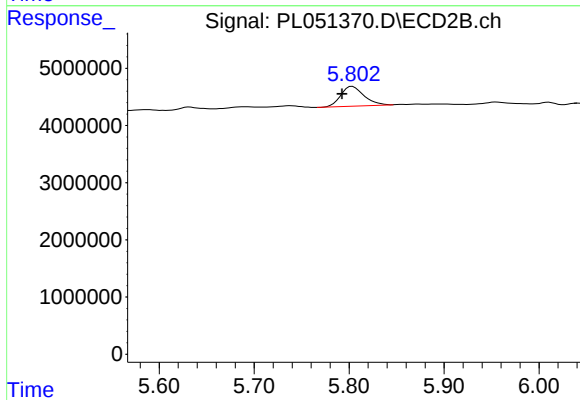


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: 0.011 min
Response: 5888159
Conc: 1.54 ng/ml

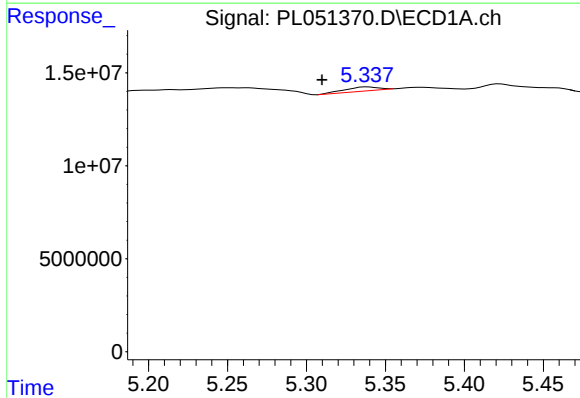


#9 Endosulfan I

R.T.: 5.339 min
Delta R.T.: 0.029 min
Response: 3180282
Conc: 0.22 ng/ml

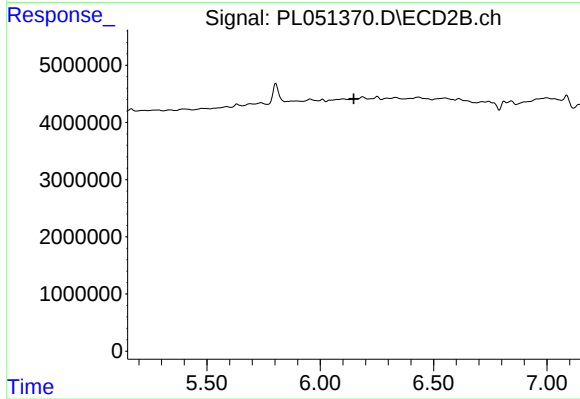

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

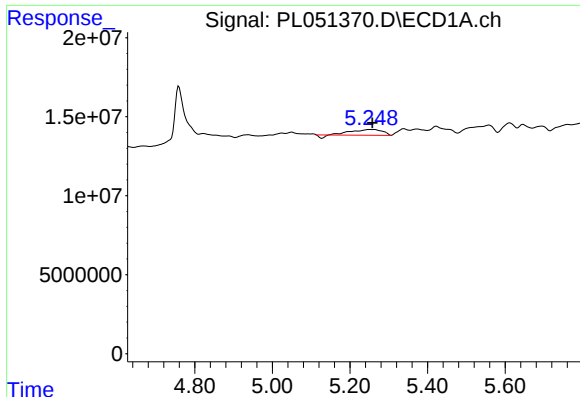

#11 alpha-Chlordane


R.T.: 5.249 min
Delta R.T.: -0.008 min
Response: 19230713
Conc: 1.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

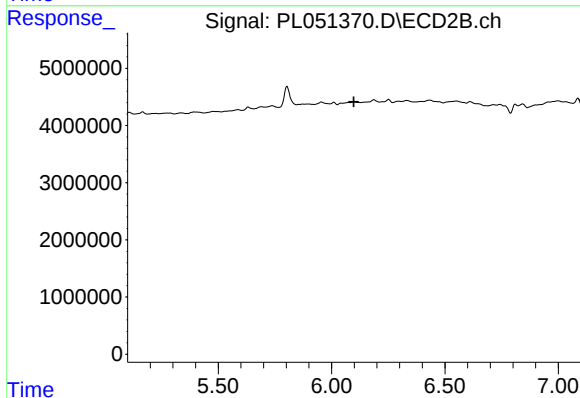


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.098 min
Response: 0
Conc: N.D.

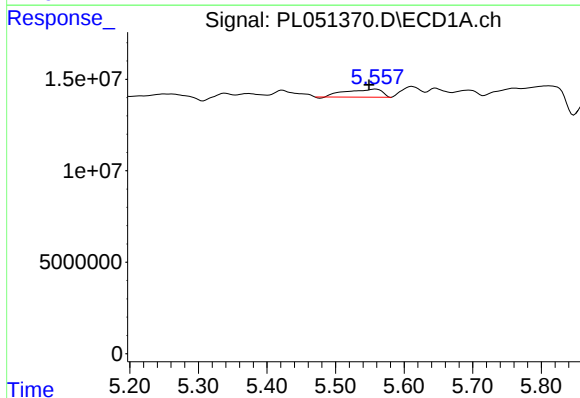


#13 Dieldrin

R.T.: 5.559 min
Delta R.T.: 0.010 min
Response: 16121421
Conc: 1.04 ng/ml

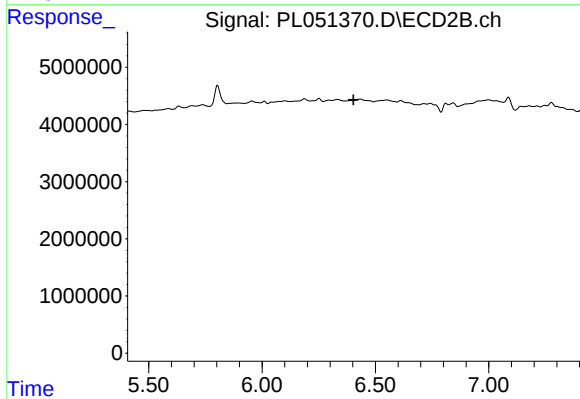

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.404 min
Response: 0
Conc: N.D.

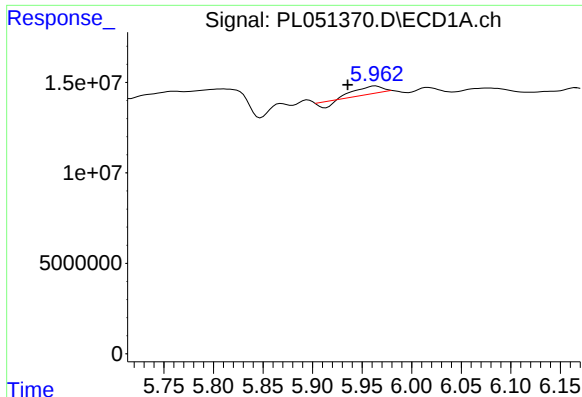

#16 4,4'-DDD


R.T.: 5.963 min
Delta R.T.: 0.028 min
Response: 7072373
Conc: 0.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

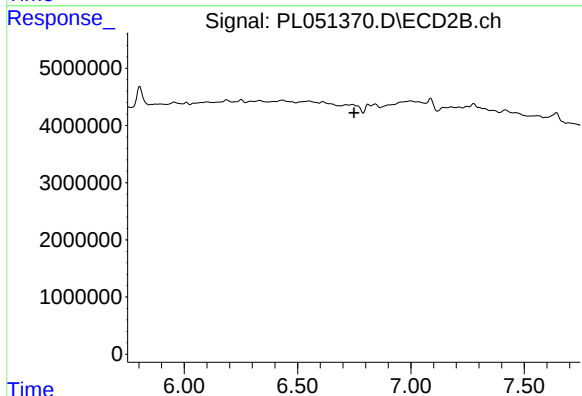


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.749 min
Response: 0
Conc: N.D.

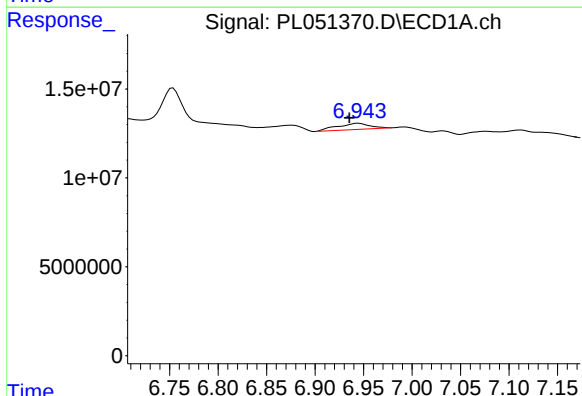


#21 Endrin ketone

R.T.: 6.945 min
Delta R.T.: 0.009 min
Response: 8165924
Conc: 0.60 ng/ml

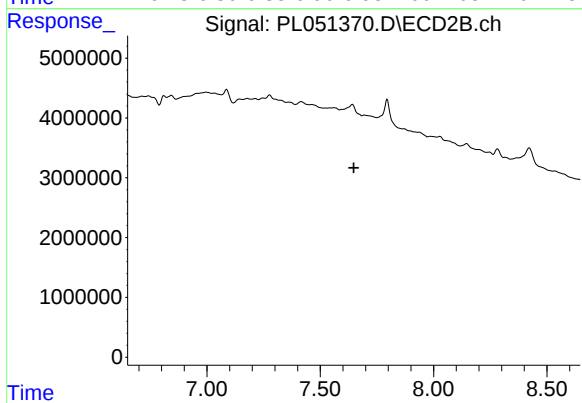

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.648 min
Response: 0
Conc: N.D.

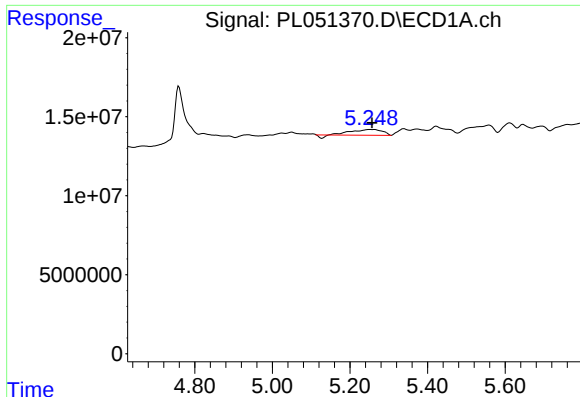

#26 Chlordane-4


R.T.: 5.249 min
Delta R.T.: -0.007 min
Response: 19230713
Conc: 14.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-013-B209-080519

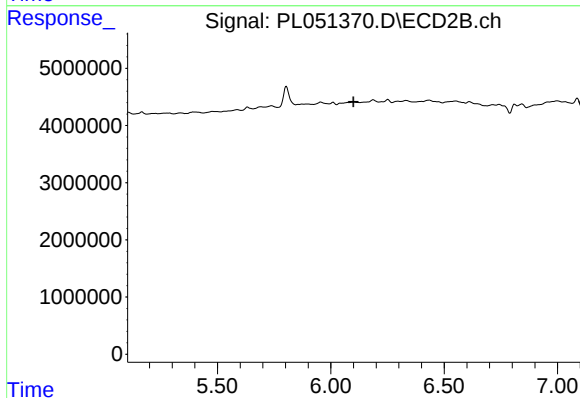


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

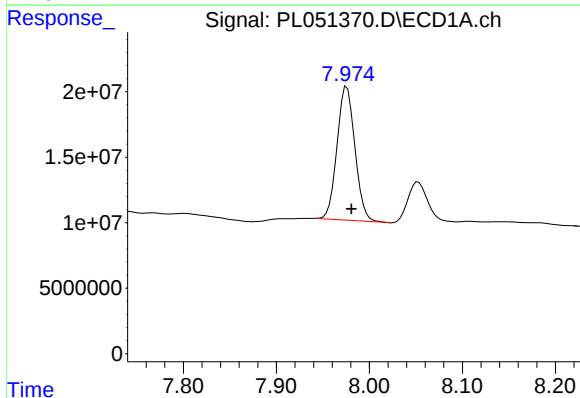

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 136599612
Conc: 13.49 ng/ml

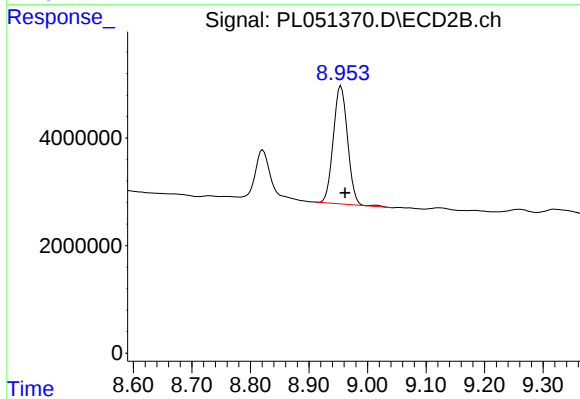

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.007 min
Response: 37191012
Conc: 13.15 ng/ml