

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 00:06
 Operator : SM\AJ
 Sample : K4095-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-04-080919-B

Manual Integrations
 APPROVED

Ankita
 8/14/2019 9:34:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 00:54:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.925	91725789	23689669	9.129m	8.303m
28)	SA Decachlor...	7.977	8.955	89664109	27539575	8.855	9.738
Target Compounds							
10)	B gamma-Chl...	5.191	6.019	13746015	4131082	0.871m	1.118m#
11)	B alpha-Chl...	5.253	6.094	12046618	4972400	0.790m	1.357 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 00:06
Operator : SM\AJ
Sample : K4095-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SU-04-080919-B


Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 00:54:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm



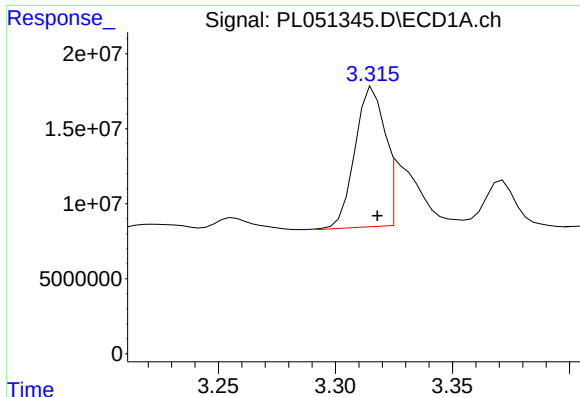


#1 Tetrachloro-m-xylene

R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 91725789
Conc: 9.13 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SU-04-080919-B


Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:05 AM

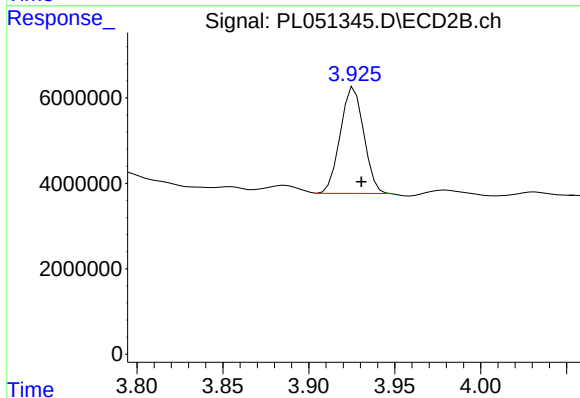


#1 Tetrachloro-m-xylene

R.T.: 3.925 min
Delta R.T.: -0.006 min
Response: 23689669
Conc: 8.30 ng/ml m

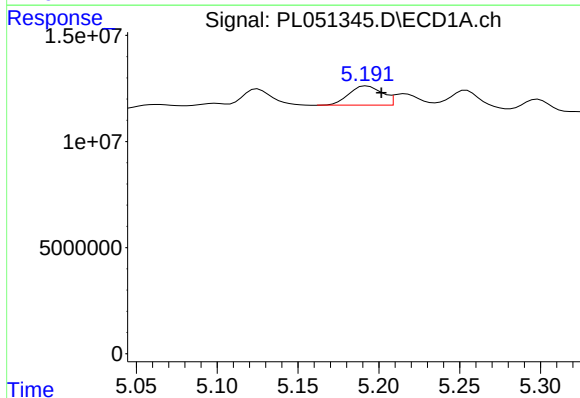


#10 gamma-Chlordane

R.T.: 5.191 min
Delta R.T.: -0.010 min
Response: 13746015
Conc: 0.87 ng/ml m

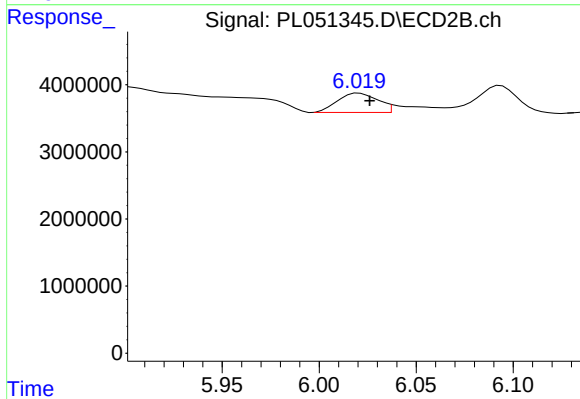

#10 gamma-Chlordane

R.T.: 6.019 min
Delta R.T.: -0.007 min
Response: 4131082
Conc: 1.12 ng/ml m

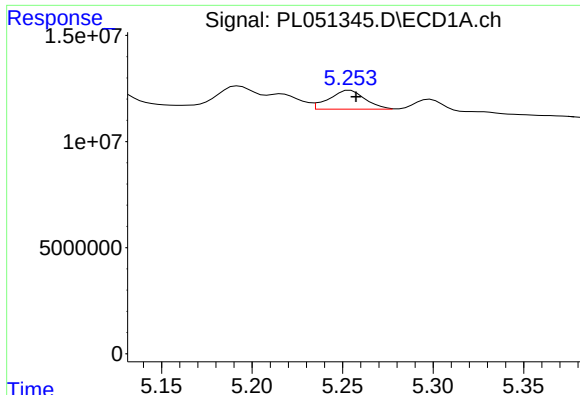


#11 alpha-Chlordane

R.T.: 5.253 min
Delta R.T.: -0.004 min
Response: 12046618
Conc: 0.79 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SU-04-080919-B


Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:05 AM

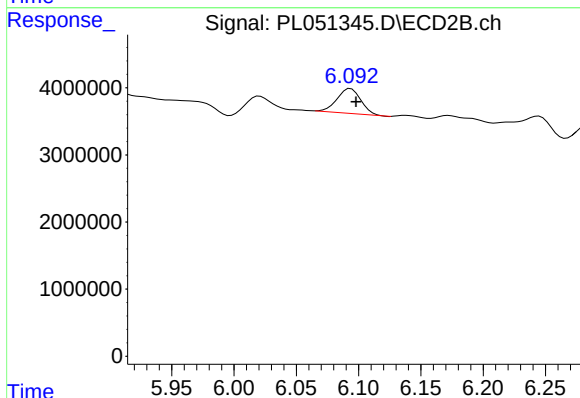


#11 alpha-Chlordane

R.T.: 6.094 min
Delta R.T.: -0.004 min
Response: 4972400
Conc: 1.36 ng/ml

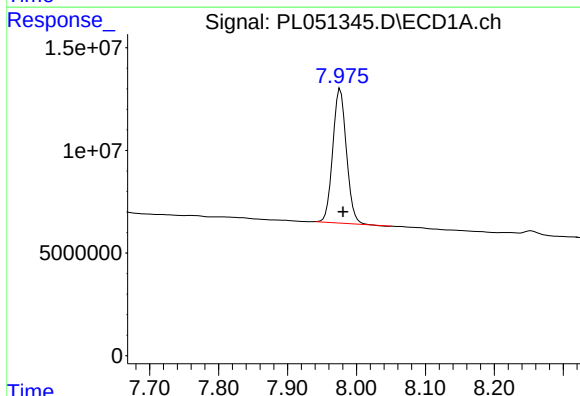

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 89664109
Conc: 8.86 ng/ml

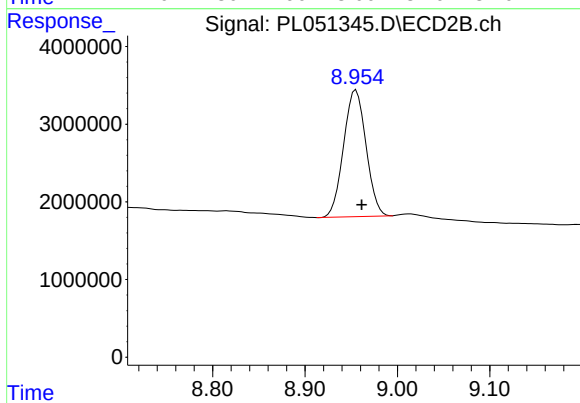

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 27539575
Conc: 9.74 ng/ml