

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
 Data File : PL051375.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 07:11
 Operator : SM\AJ
 Sample : K4239-13
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-034-B231-080519

Manual Integrations
 APPROVED

Ankita
 8/14/2019 9:34:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 07:35:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.315	3.926	150.3E6	33062175	14.955m	11.588m
28)	SA Decachlor...	7.977	8.955	200.3E6	52701877	19.780	18.636
Target Compounds							
17)	MA 4,4'-DDT	6.165	7.040	70890460	15554614	5.724m	5.762

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081219\
Data File : PL051375.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 07:11
Operator : SM\AJ
Sample : K4239-13
Misc :
ALS Vial : 61 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-034-B231-080519


Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 07:35:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

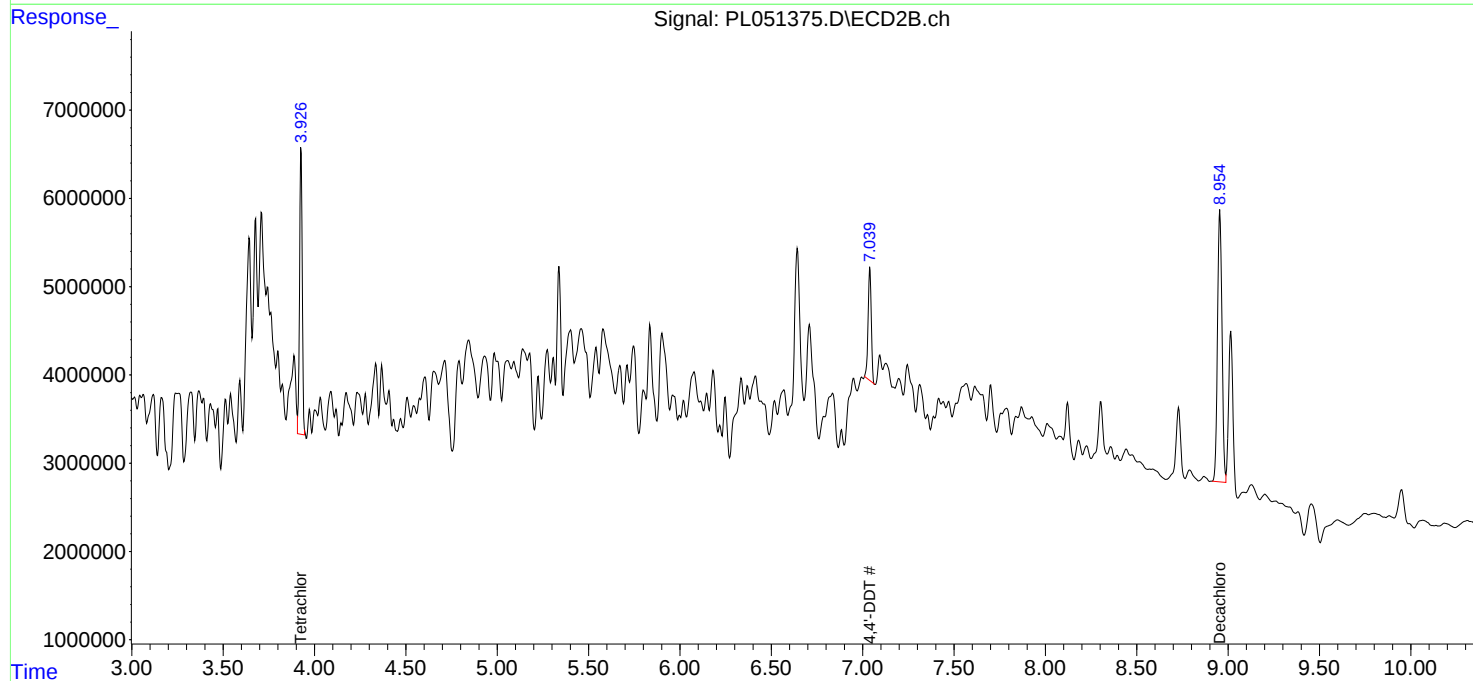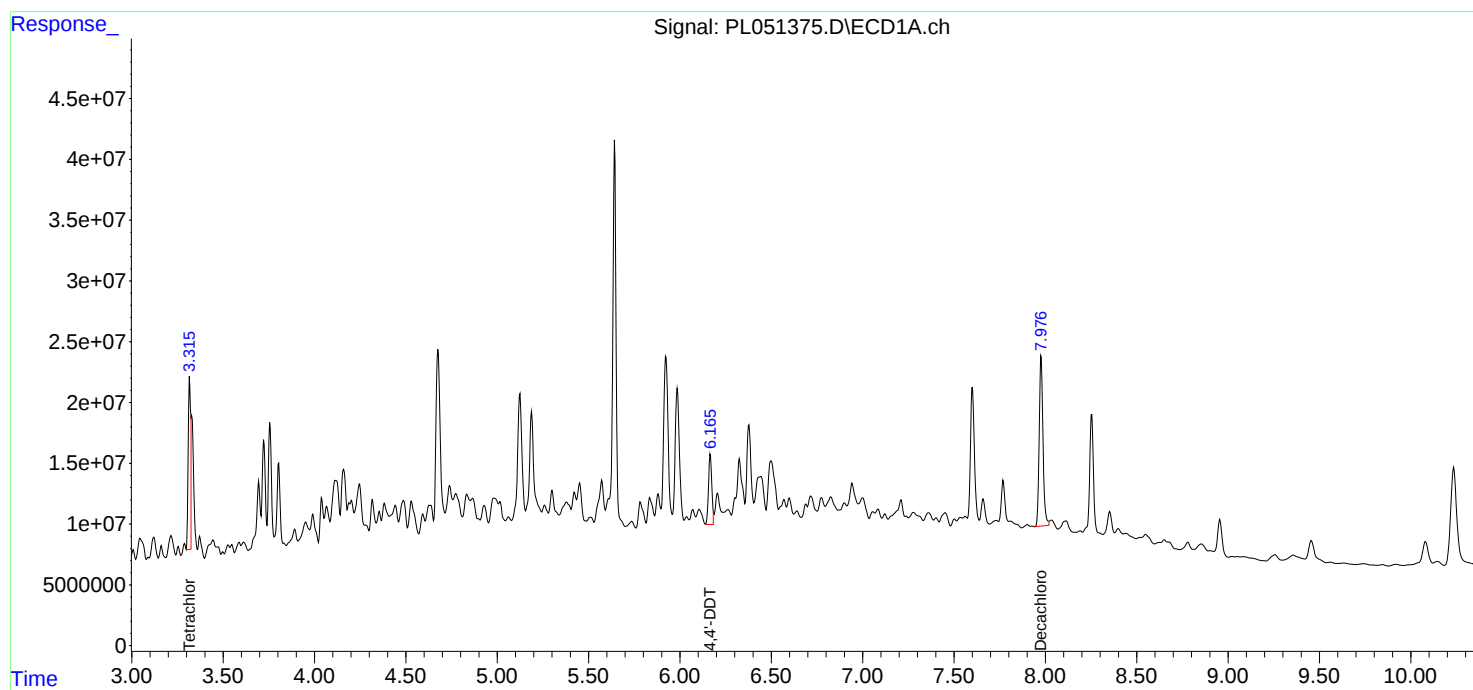

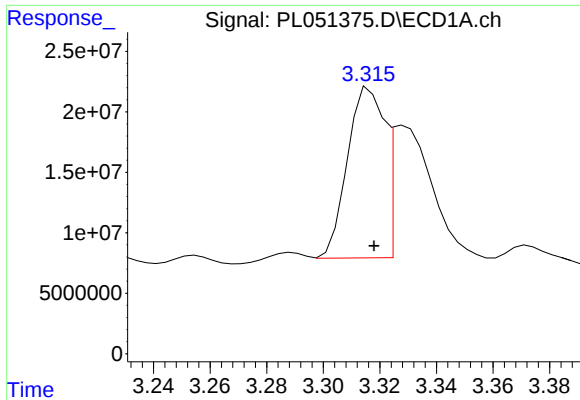


#1 Tetrachloro-m-xylene

R.T.: 3.315 min
Delta R.T.: -0.003 min
Response: 150264229
Conc: 14.95 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PST-034-B231-080519


Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:38 AM

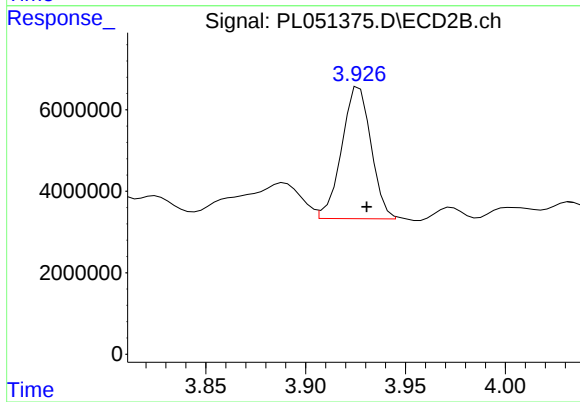


#1 Tetrachloro-m-xylene

R.T.: 3.926 min
Delta R.T.: -0.005 min
Response: 33062175
Conc: 11.59 ng/ml m

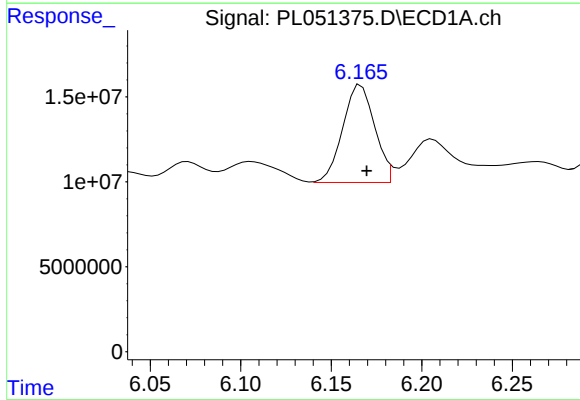


#17 4,4'-DDT

R.T.: 6.165 min
Delta R.T.: -0.005 min
Response: 70890460
Conc: 5.72 ng/ml m

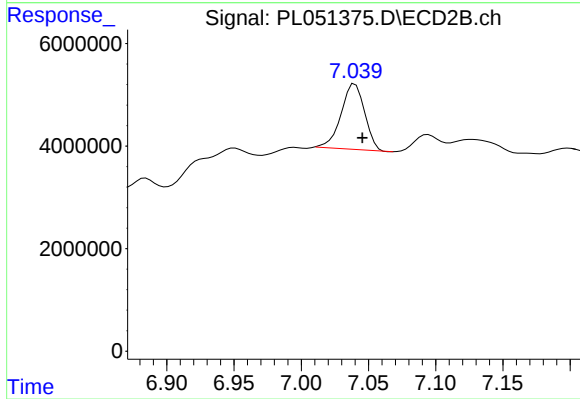

#17 4,4'-DDT

R.T.: 7.040 min
Delta R.T.: -0.006 min
Response: 15554614
Conc: 5.76 ng/ml

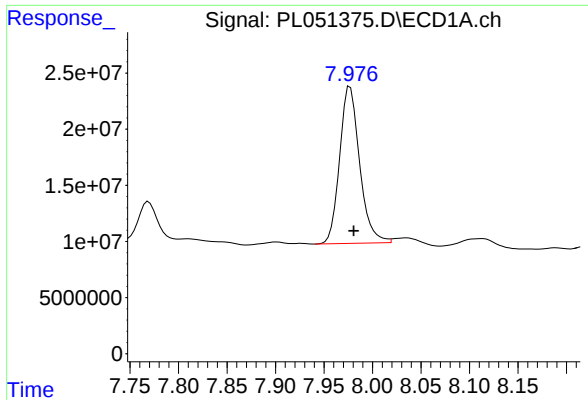


#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 200282663
Conc: 19.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-034-B231-080519

Manual Integrations
APPROVED

Ankita
8/14/2019 9:34:38 AM

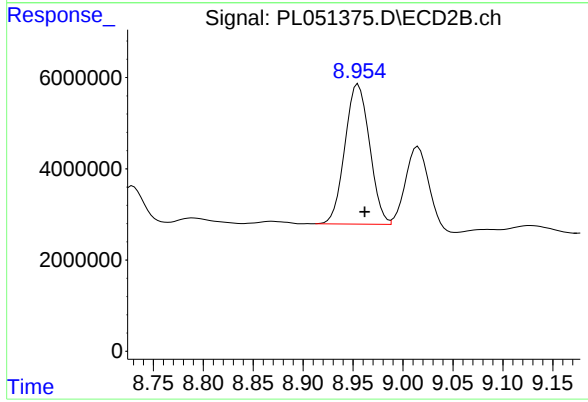

#28 Decachlorobiphenyl

R.T.: 8.955 min
Delta R.T.: -0.006 min
Response: 52701877
Conc: 18.64 ng/ml