

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
 Data File : PL060637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 12:23
 Operator : DD\AJ
 Sample : L3504-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-081120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:12:29 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.011	26891842	33524085	14.345	12.607
28)	SA Decachlor...	8.219	9.098	21015918	23793297	11.514	12.681
Target Compounds							
5)	MB Aldrin	4.714f	0.000	8289158	0	3.787	N.D. #
9)	A Endosulfan I	5.529	6.244	14361685	2037368	7.285	0.719 #
10)	B gamma-Chl...	0.000	6.126	0	14450287	N.D.	4.780 #
11)	B alpha-Chl...	0.000	6.199	0	21379222	N.D.	6.954 #
12)	B 4,4'-DDE	0.000	6.350	0	6625482	N.D.	2.327 #
23)	Chlordane-1	4.332	5.009	7570219	4442666	139.139	42.263 #
25)	Chlordane-3	0.000	6.126	0	14450287	N.D.	39.906 #
26)	Chlordane-4	0.000	6.199	0	21379222	N.D.	49.318 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
Data File : PL060637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 12:23
Operator : DD\AJ
Sample : L3504-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:12:29 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

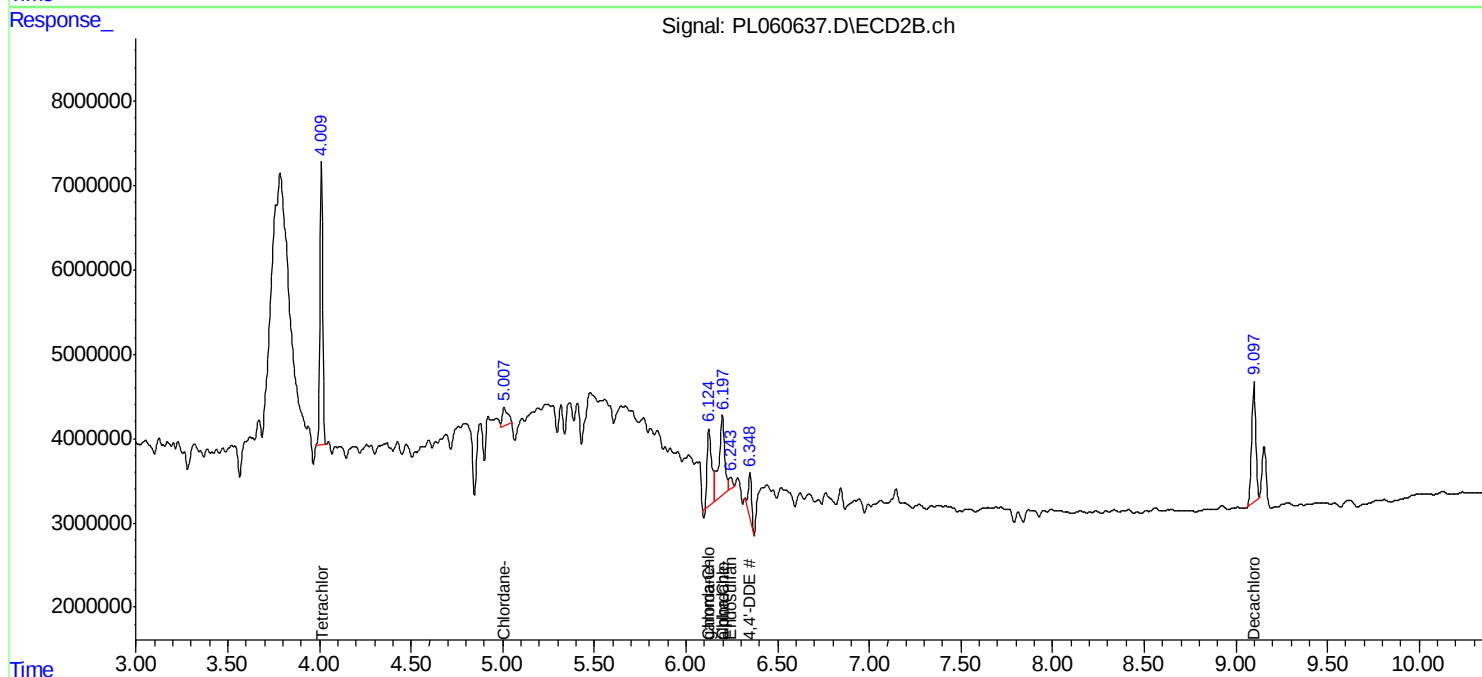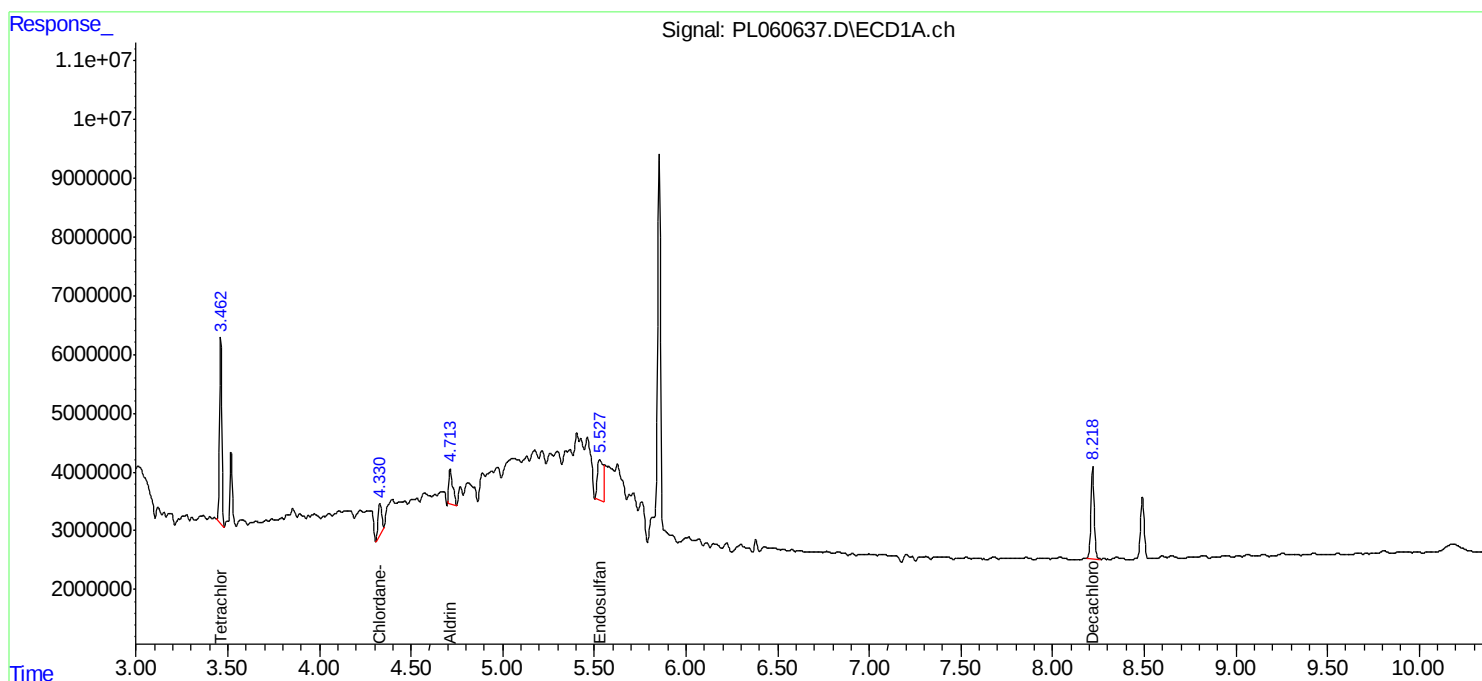


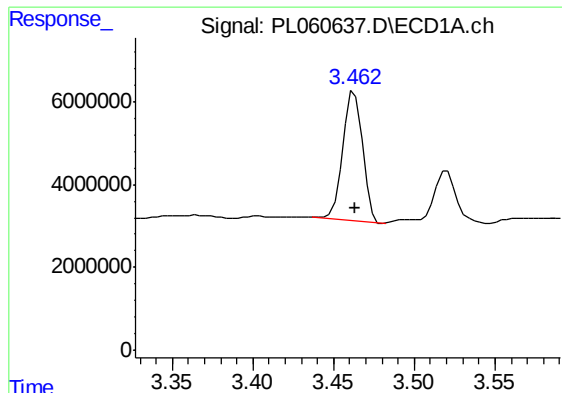

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 26891842
Conc: 14.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

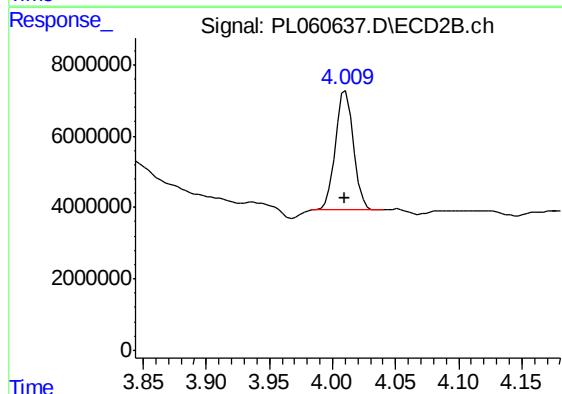


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 33524085
Conc: 12.61 ng/ml

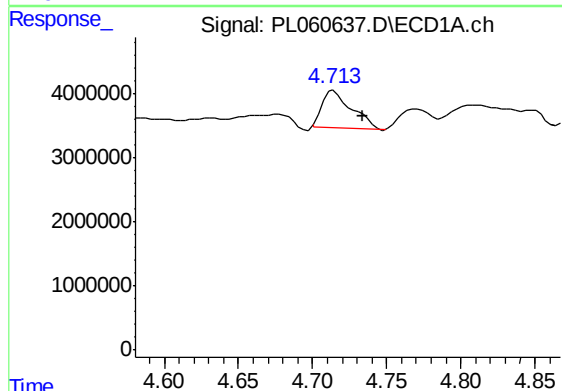


#5 Aldrin

R.T.: 4.714 min
Delta R.T.: -0.020 min
Response: 8289158
Conc: 3.79 ng/ml

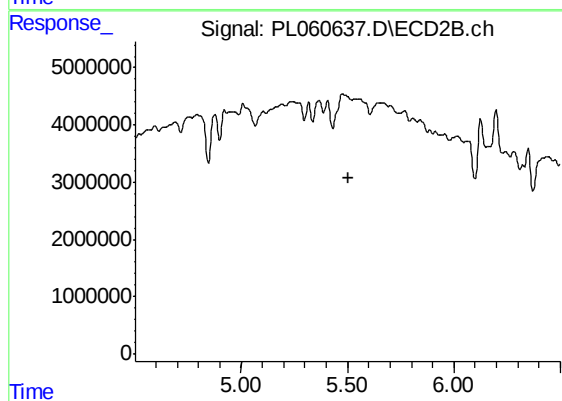

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

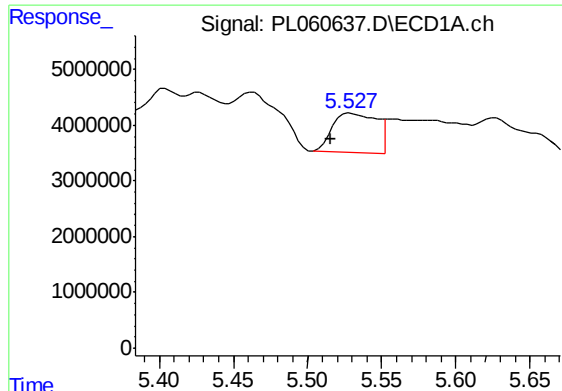

#9 Endosulfan I


R.T.: 5.529 min
Delta R.T.: 0.013 min
Response: 14361685
Conc: 7.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

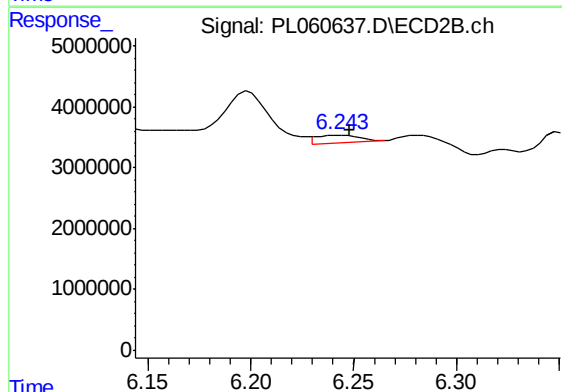


#9 Endosulfan I

R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 2037368
Conc: 0.72 ng/ml

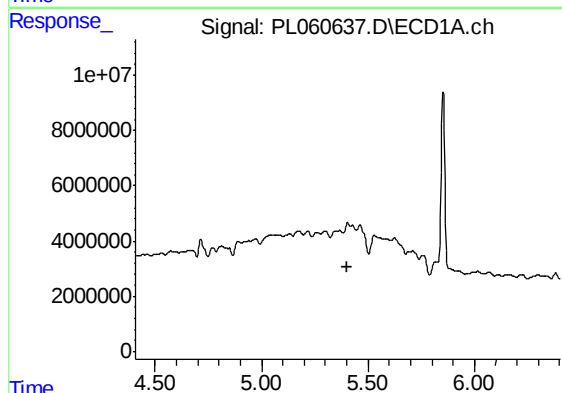


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

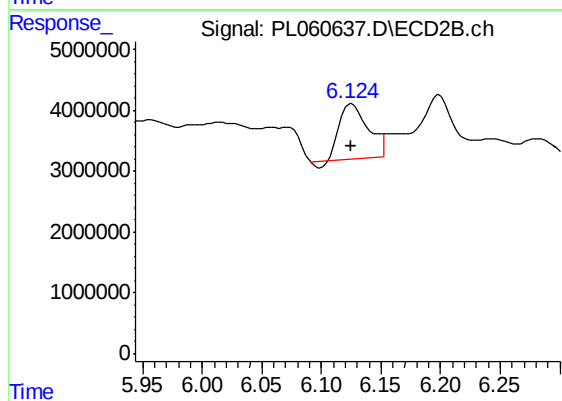

#10 gamma-Chlordane


R.T.: 6.126 min
Delta R.T.: 0.001 min
Response: 14450287
Conc: 4.78 ng/ml

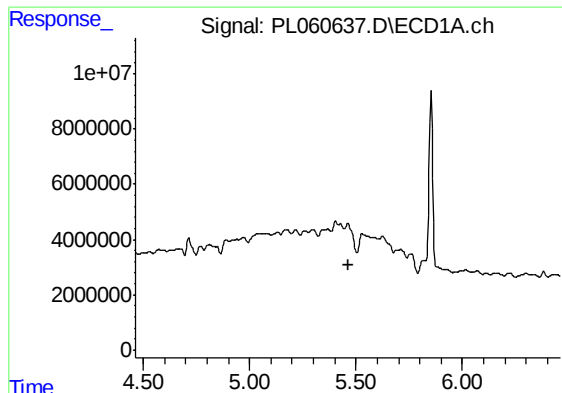

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

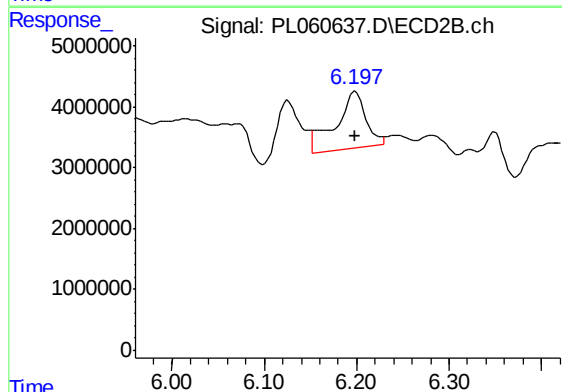


#11 alpha-Chlordane

R.T.: 6.199 min
Delta R.T.: 0.001 min
Response: 21379222
Conc: 6.95 ng/ml

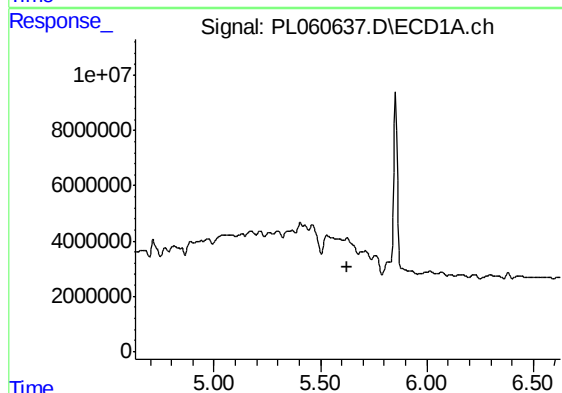


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.628 min
Response: 0
Conc: N.D.

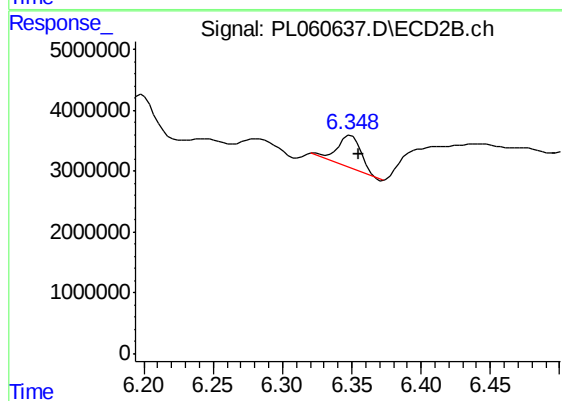

#12 4,4'-DDE


R.T.: 6.350 min
Delta R.T.: -0.006 min
Response: 6625482
Conc: 2.33 ng/ml

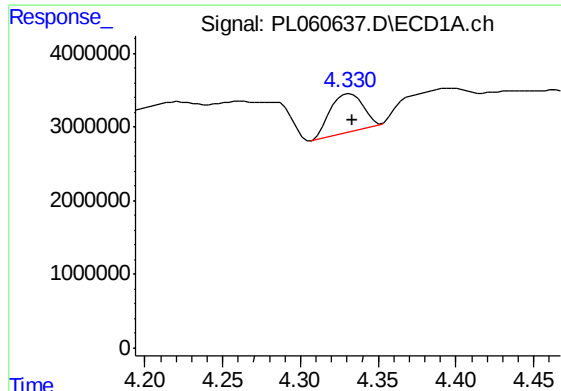

#23 Chlordane-1


R.T.: 4.332 min
Delta R.T.: -0.002 min
Response: 7570219
Conc: 139.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

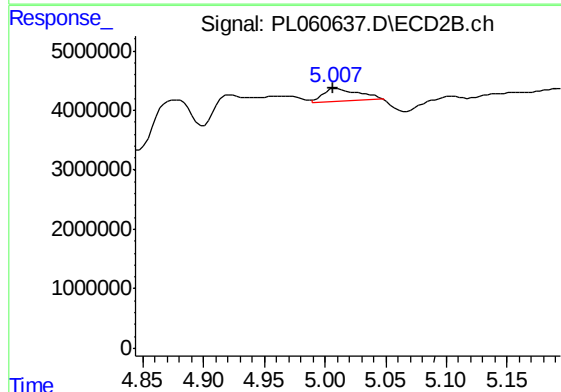


#23 Chlordane-1

R.T.: 5.009 min
Delta R.T.: 0.002 min
Response: 4442666
Conc: 42.26 ng/ml

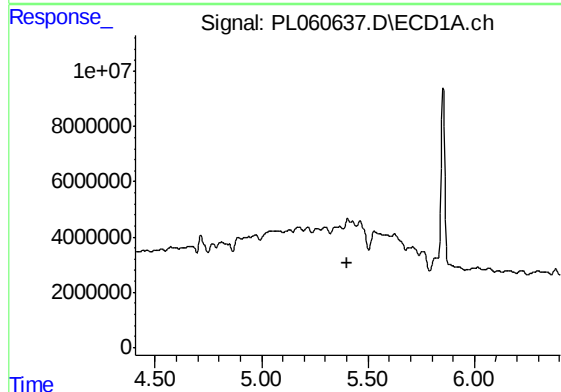


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.404 min
Response: 0
Conc: N.D.

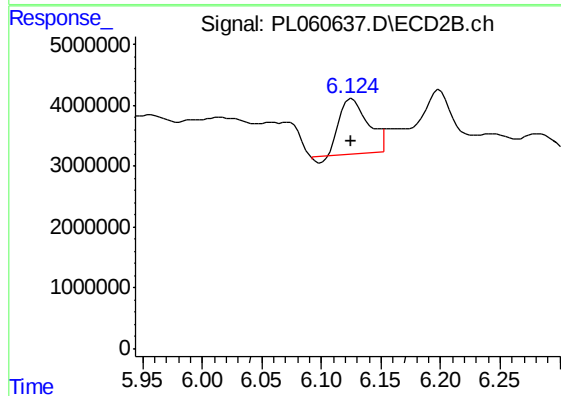

#25 Chlordane-3


R.T.: 6.126 min
Delta R.T.: 0.000 min
Response: 14450287
Conc: 39.91 ng/ml

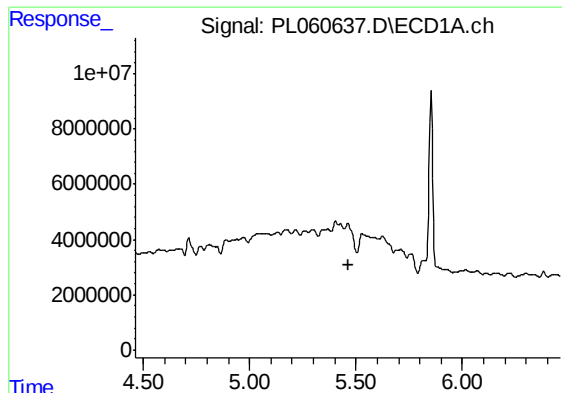

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-081120

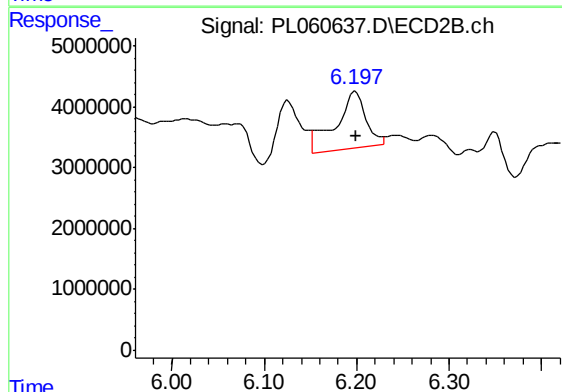


#26 Chlordane-4

R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 21379222
Conc: 49.32 ng/ml

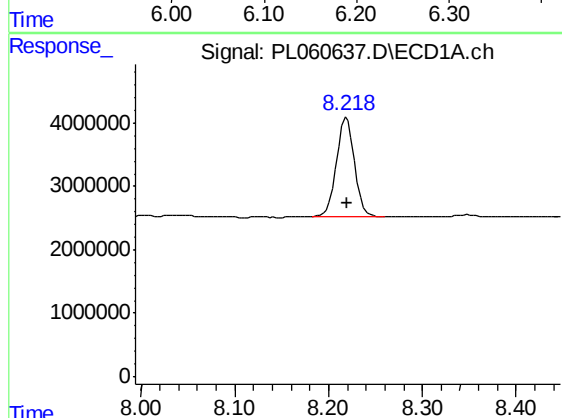

#28 Decachlorobiphenyl

R.T.: 8.219 min
Delta R.T.: -0.001 min
Response: 21015918
Conc: 11.51 ng/ml

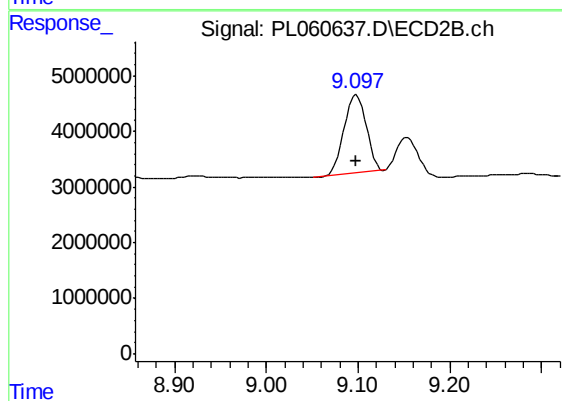

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 23793297
Conc: 12.68 ng/ml