

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
 Data File : PL060638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 12:37
 Operator : DD\AJ
 Sample : L3508-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-081120

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:12:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.011	25888727	29771071	13.809	11.196
28)	SA Decachlor...	8.220	9.098	19422231	19749693	10.641	10.526
Target Compounds							
3)	MA gamma-BHC...	0.000	4.691	0	10785406	N.D.	2.810 #
6)	B beta-BHC	0.000	4.869	0	9268817	N.D.	5.786 #
9)	A Endosulfan I	5.532f	0.000	10916554	0	5.538	N.D. #
10)	B gamma-Chl...	0.000	6.129	0	737290	N.D.	0.244 #
21)	B Endrin ke...	0.000	7.735f	0	16308546	N.D.	6.692 #
23)	Chlordane-1	4.330	5.029f	7244854	9217752	133.159	87.689 #
24)	Chlordane-2	4.849	0.000	7474503	0	117.977	N.D. #
25)	Chlordane-3	0.000	6.129	0	737290	N.D.	2.036 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
Data File : PL060638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 12:37
Operator : DD\AJ
Sample : L3508-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:12:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

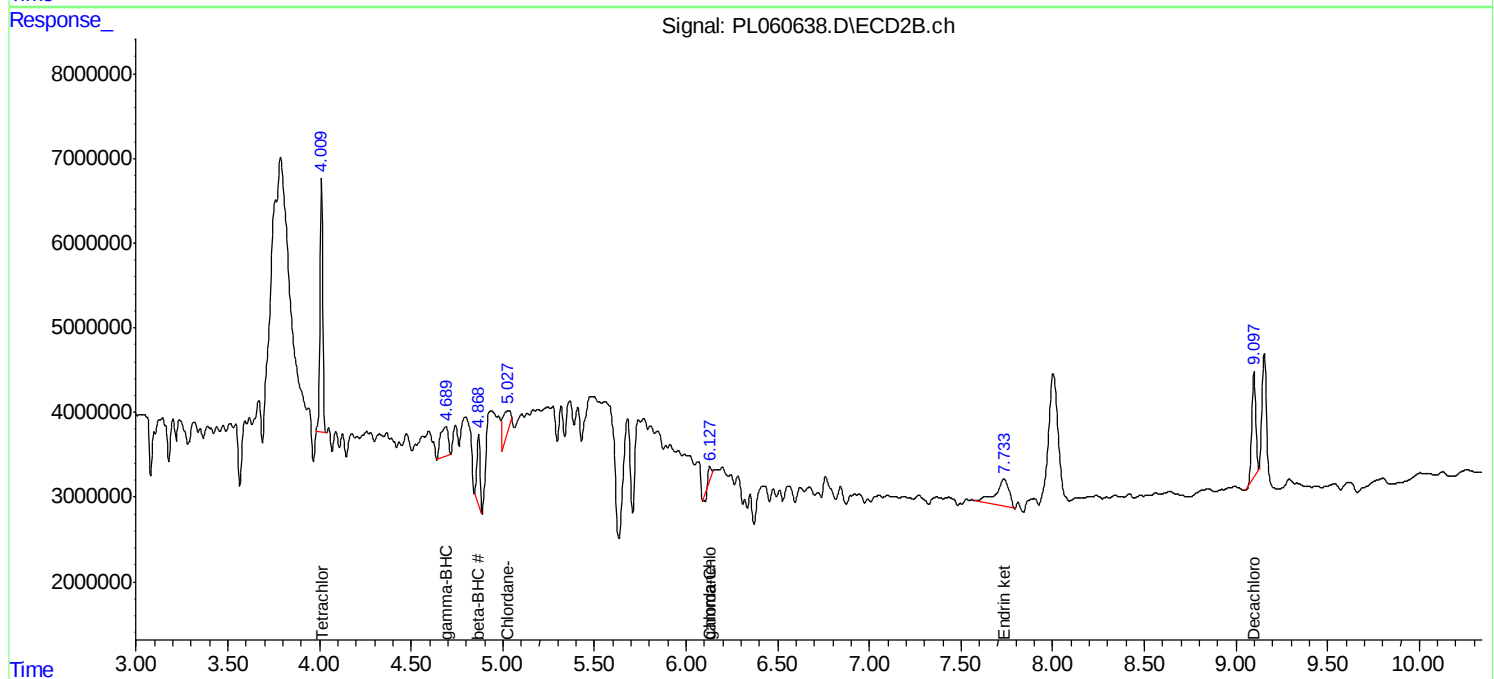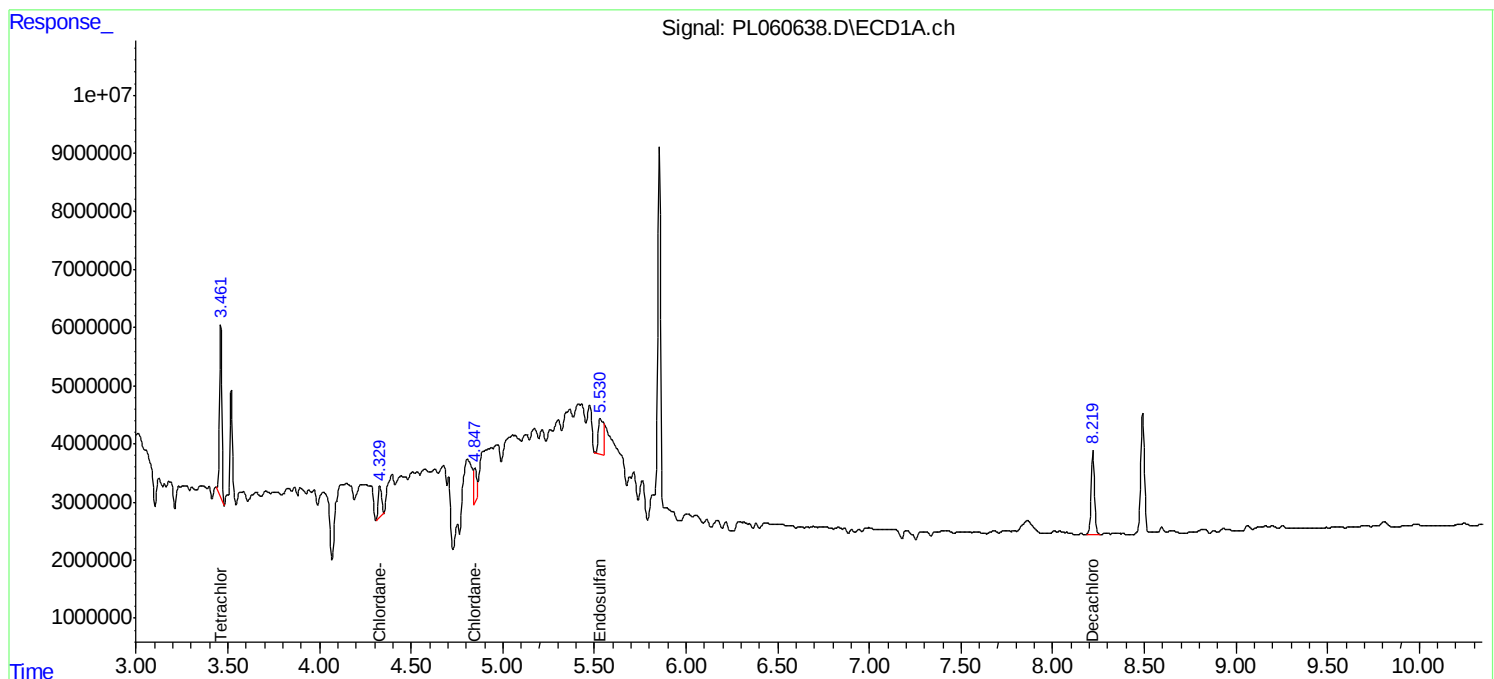


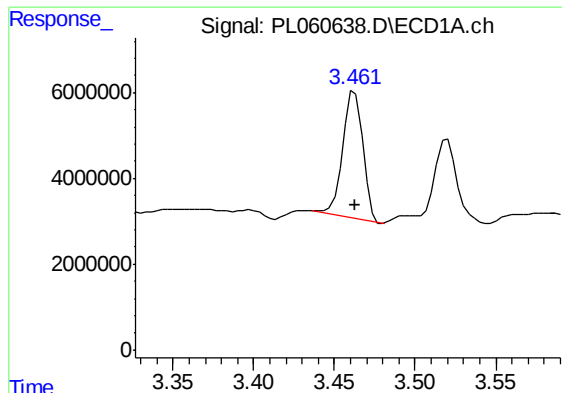

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 25888727
Conc: 13.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

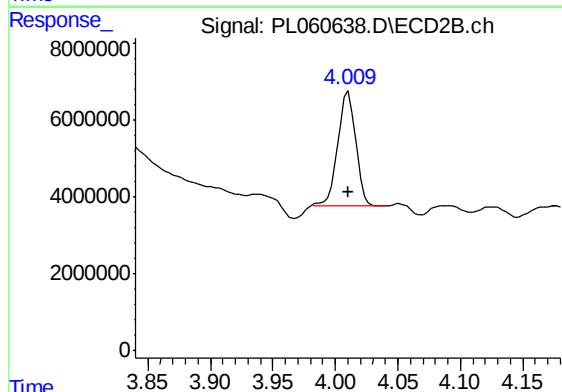


#1 Tetrachloro-m-xylene

R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 29771071
Conc: 11.20 ng/ml

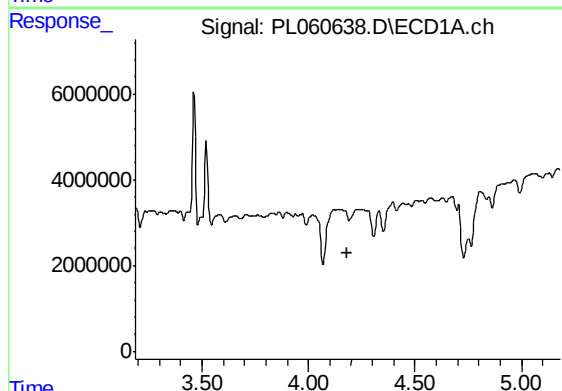


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.184 min
Response: 0
Conc: N.D.

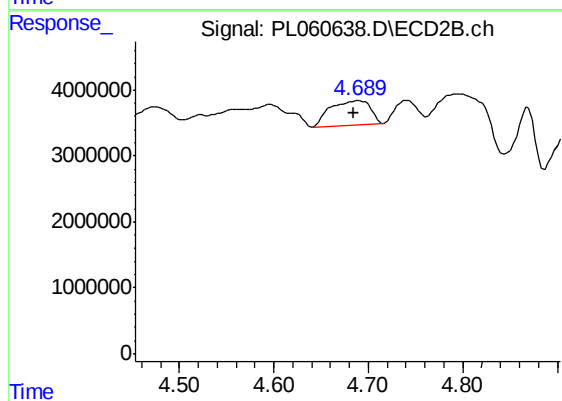

#3 gamma-BHC (Lindane)


R.T.: 4.691 min
Delta R.T.: 0.005 min
Response: 10785406
Conc: 2.81 ng/ml

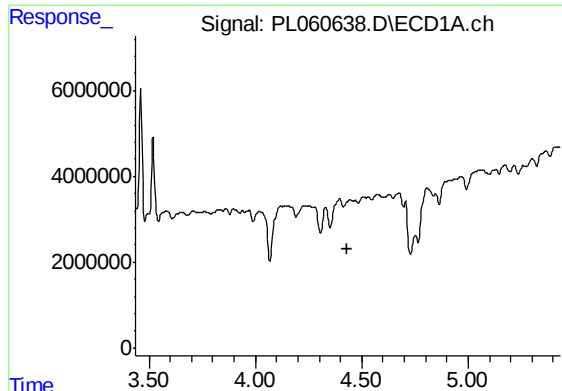

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

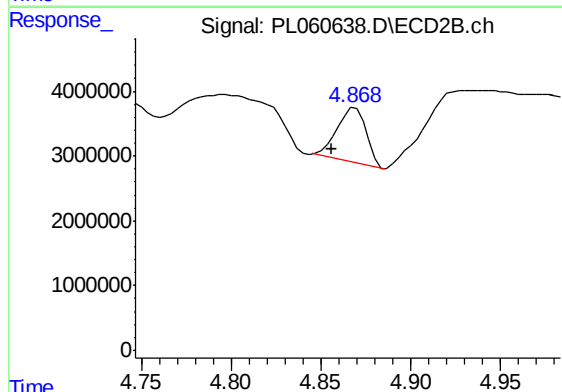


#6 beta-BHC

R.T.: 4.869 min
Delta R.T.: 0.013 min
Response: 9268817
Conc: 5.79 ng/ml

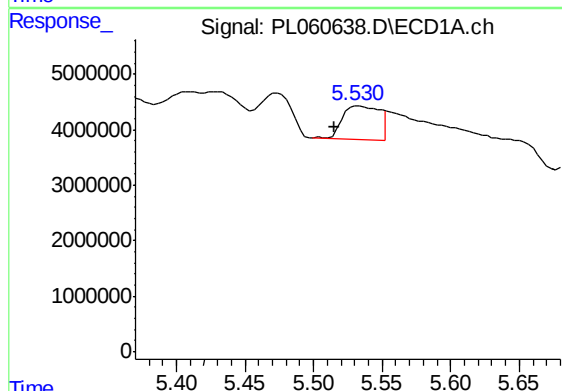


#9 Endosulfan I

R.T.: 5.532 min
Delta R.T.: 0.016 min
Response: 10916554
Conc: 5.54 ng/ml

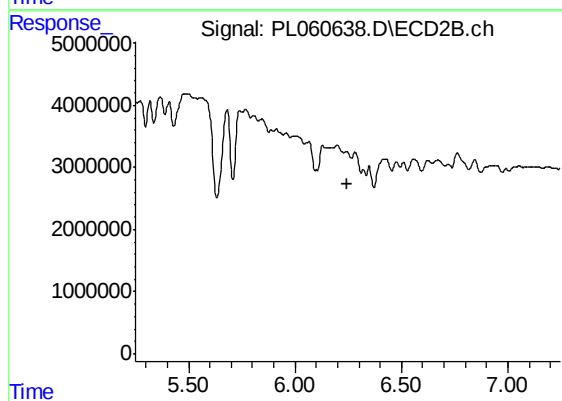

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

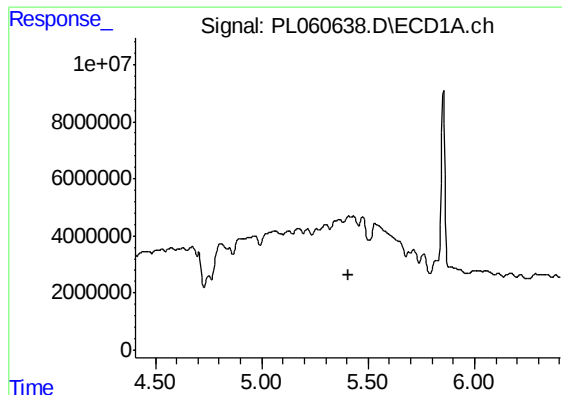

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

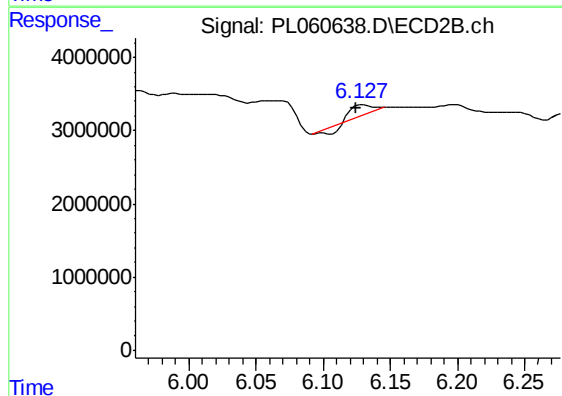


#10 gamma-Chlordane

R.T.: 6.129 min
Delta R.T.: 0.005 min
Response: 737290
Conc: 0.24 ng/ml

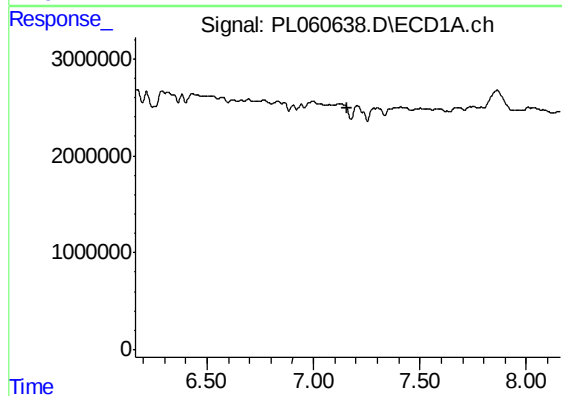


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

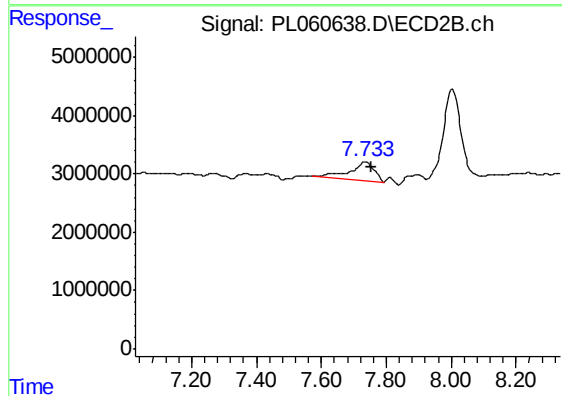

#21 Endrin ketone


R.T.: 7.735 min
Delta R.T.: -0.019 min
Response: 16308546
Conc: 6.69 ng/ml

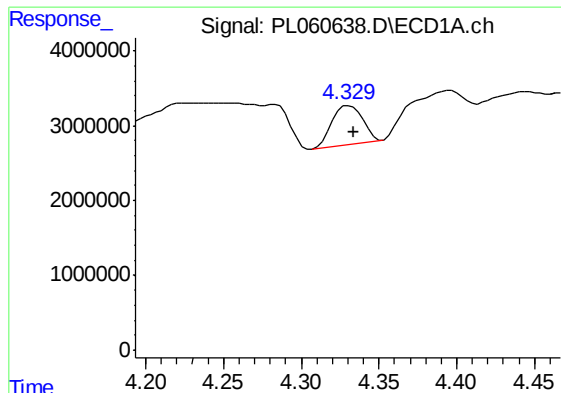

#23 Chlordane-1


R.T.: 4.330 min
Delta R.T.: -0.003 min
Response: 7244854
Conc: 133.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

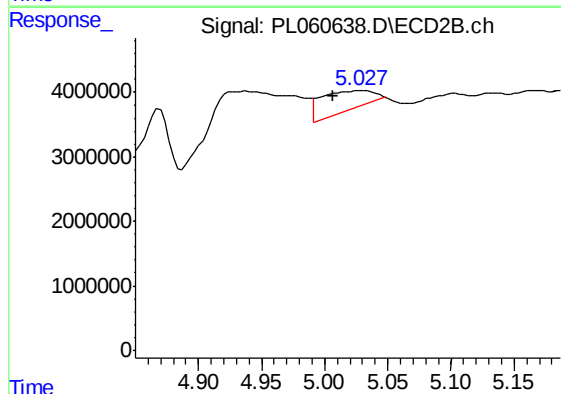


#23 Chlordane-1

R.T.: 5.029 min
Delta R.T.: 0.022 min
Response: 9217752
Conc: 87.69 ng/ml

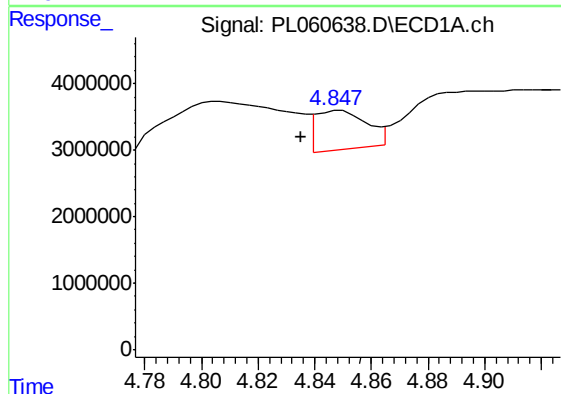


#24 Chlordane-2

R.T.: 4.849 min
Delta R.T.: 0.014 min
Response: 7474503
Conc: 117.98 ng/ml

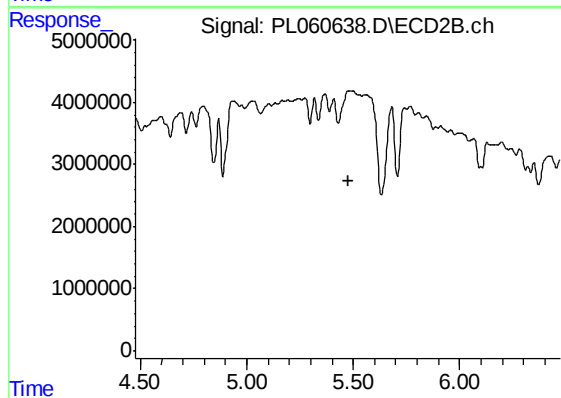

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.476 min
Response: 0
Conc: N.D.

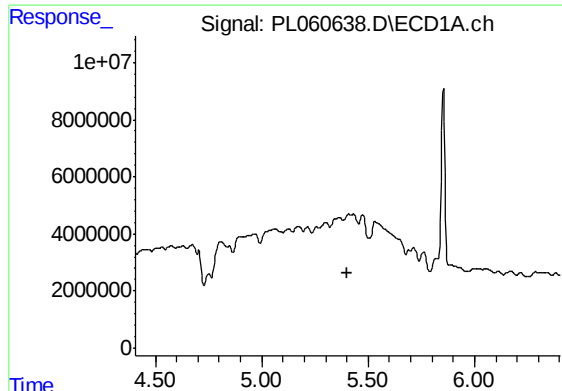

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TR-05-081120

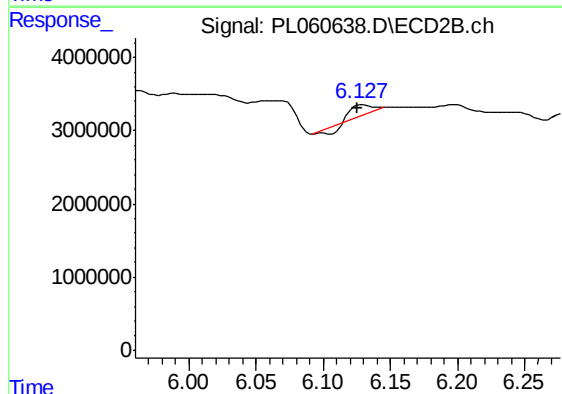


#25 Chlordane-3

R.T.: 6.129 min
Delta R.T.: 0.004 min
Response: 737290
Conc: 2.04 ng/ml

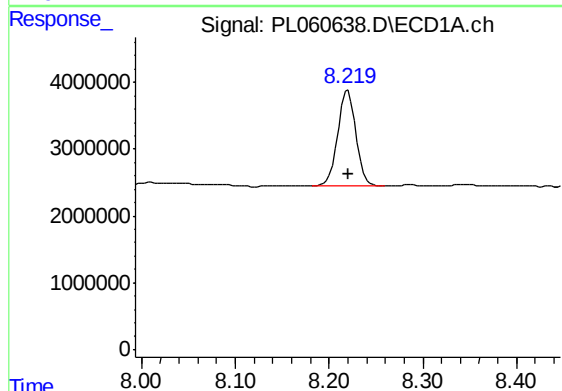

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 1942231
Conc: 10.64 ng/ml

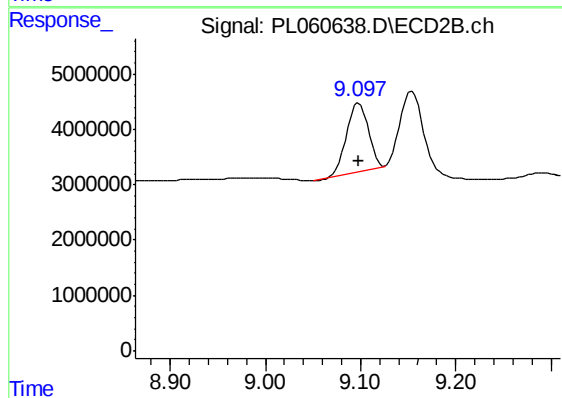

#28 Decachlorobiphenyl

R.T.: 9.098 min
Delta R.T.: 0.000 min
Response: 19749693
Conc: 10.53 ng/ml