

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
 Data File : PL060650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2020 16:58
 Operator : DD\AJ
 Sample : L3508-07
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:44:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 11 01:39:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.463	4.010	26838656	31914682	14.316	12.002
28)	SA Decachlor...	8.220	9.097	21755935	23020649	11.919	12.270
Target Compounds							
3)	MA gamma-BHC...	0.000	4.690	0	12870564	N.D.	3.353 #
6)	B beta-BHC	0.000	4.869	0	2323094	N.D.	1.450 #
9)	A Endosulfan I	0.000	6.244	0	9732208	N.D.	3.436 #
10)	B gamma-Chl...	0.000	6.130	0	8168360	N.D.	2.702 #
11)	B alpha-Chl...	0.000	6.196	0	27870967	N.D.	9.066 #
15)	B Endosulfa...	0.000	6.944	0	9649746	N.D.	3.699 #
16)	A 4,4'-DDD	0.000	6.844	0	4150719	N.D.	1.809 #
23)	Chlordane-1	4.331	5.028f	-2295	7692287	N.D.	73.177
24)	Chlordane-2	4.848	0.000	6247125	0	98.604	N.D. #
25)	Chlordane-3	0.000	6.130	0	8168360	N.D.	22.558 #
26)	Chlordane-4	0.000	6.196	0	27870967	N.D.	64.293 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081220\
Data File : PL060650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2020 16:58
Operator : DD\AJ
Sample : L3508-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:44:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081020.M
Quant Title : GC Extractables
QLast Update : Tue Aug 11 01:39:18 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

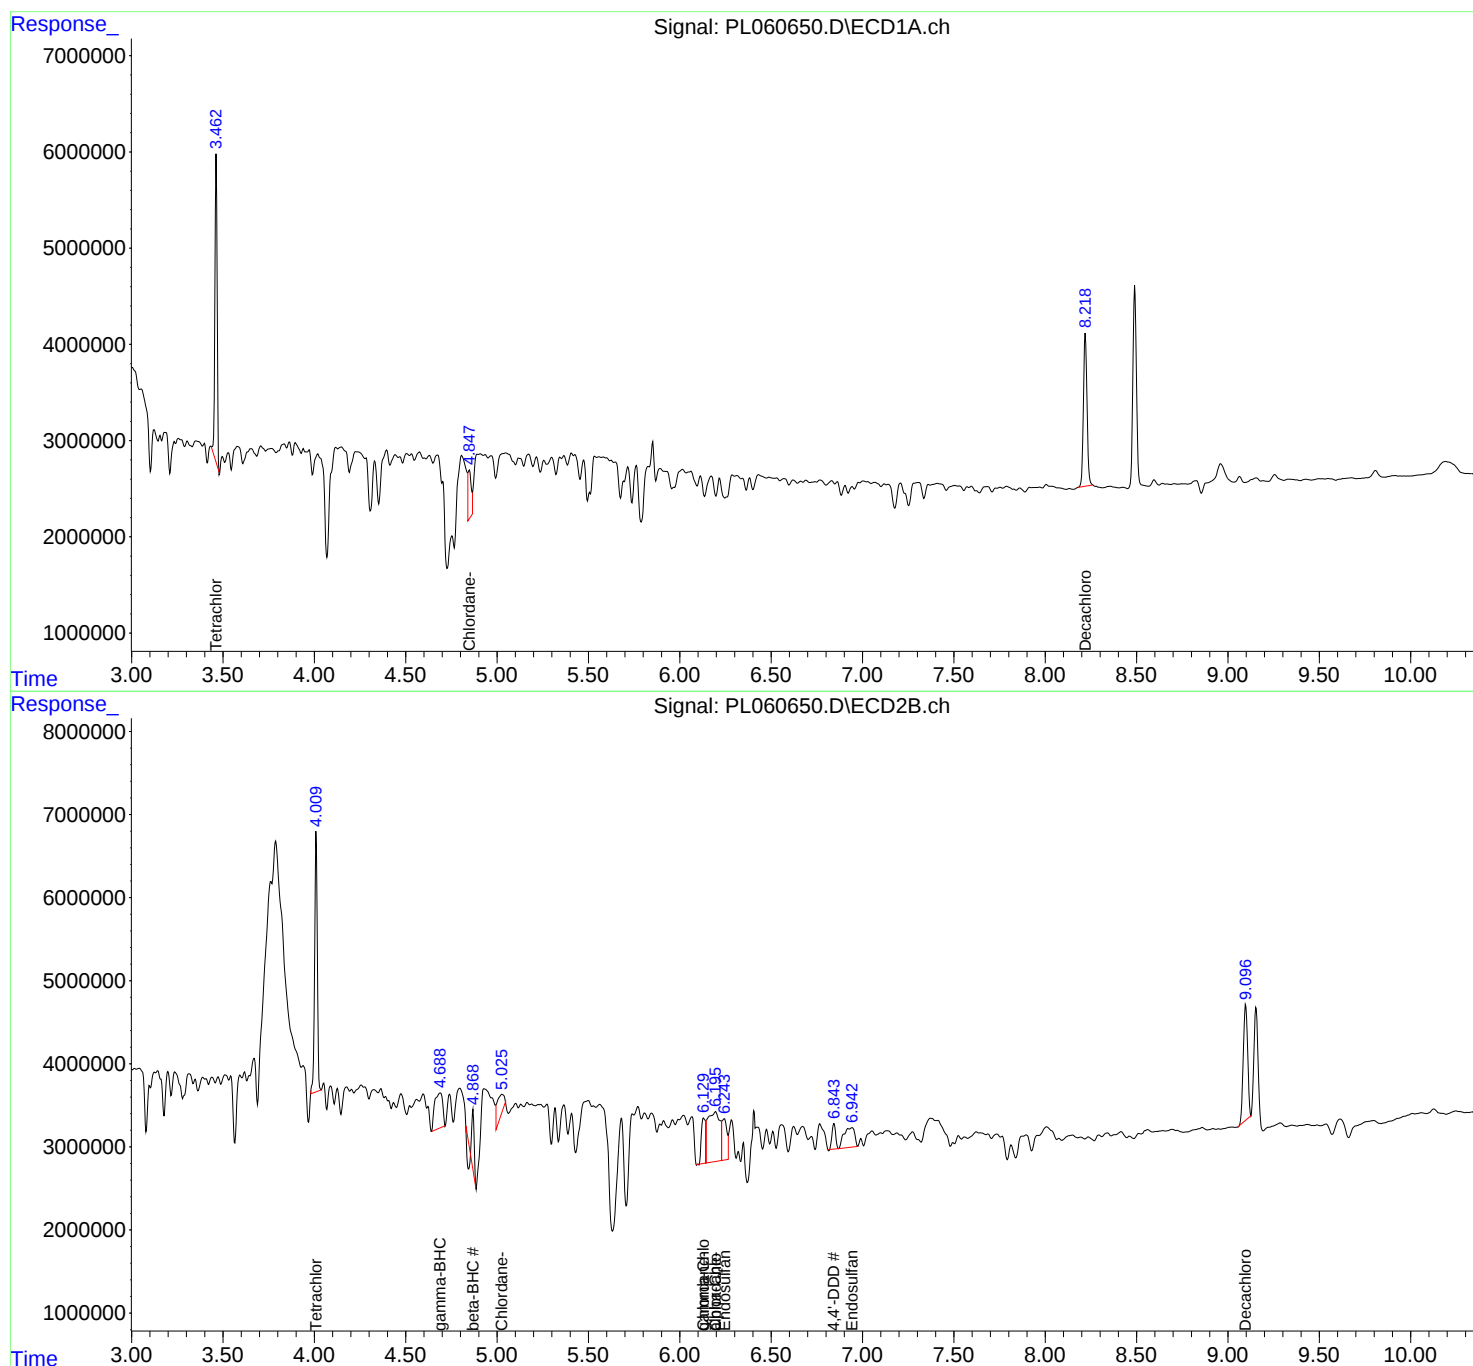


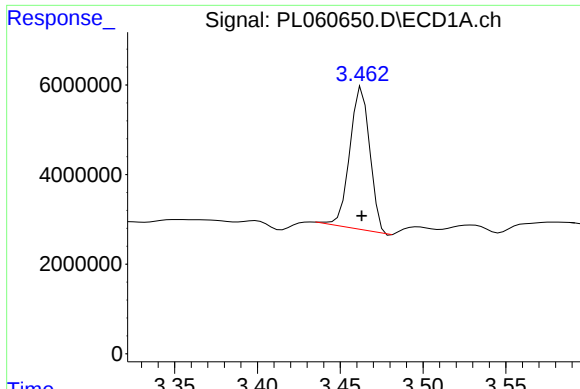

#1 Tetrachloro-m-xylene


R.T.: 3.463 min
Delta R.T.: 0.000 min
Response: 26838656
Conc: 14.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

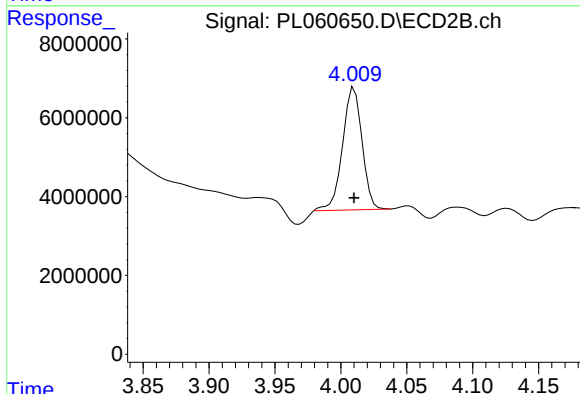


#1 Tetrachloro-m-xylene

R.T.: 4.010 min
Delta R.T.: 0.000 min
Response: 31914682
Conc: 12.00 ng/ml

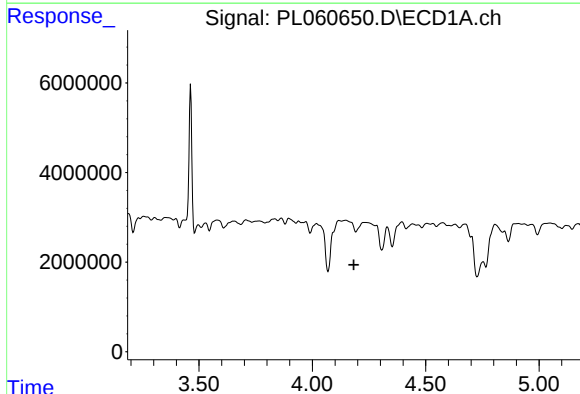


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.184 min
Response: 0
Conc: N.D.

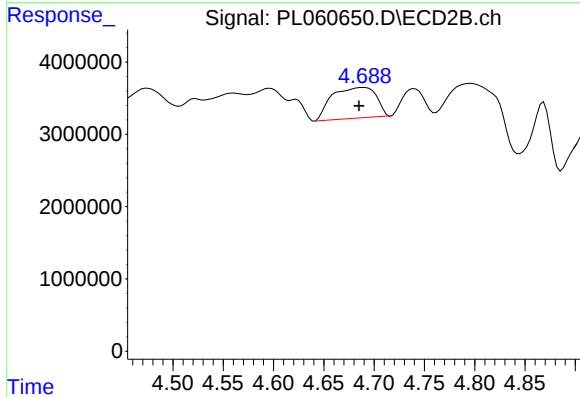

#3 gamma-BHC (Lindane)


R.T.: 4.690 min
Delta R.T.: 0.004 min
Response: 12870564
Conc: 3.35 ng/ml

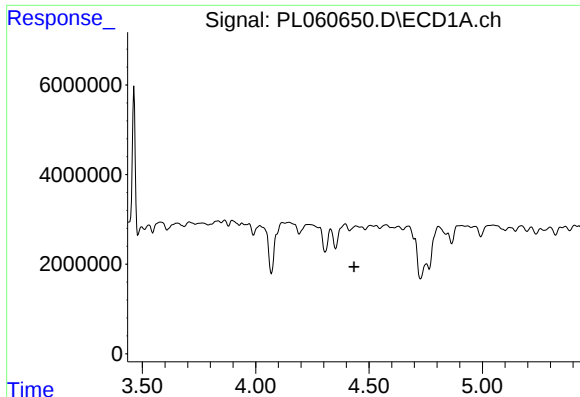

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.434 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

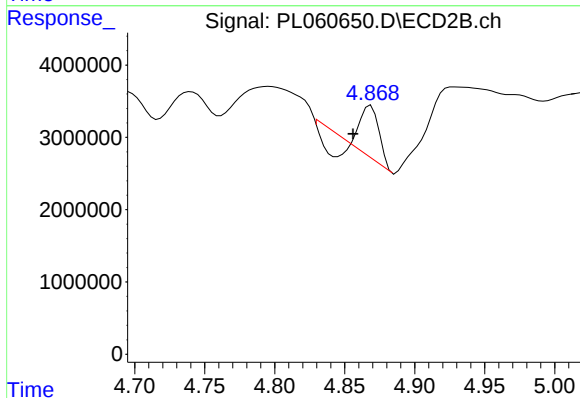


#6 beta-BHC

R.T.: 4.869 min
Delta R.T.: 0.013 min
Response: 2323094
Conc: 1.45 ng/ml

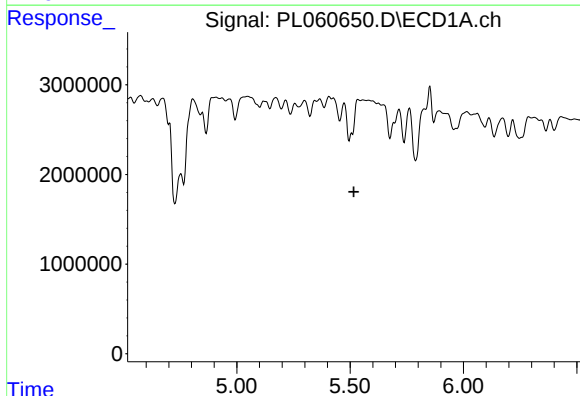


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.516 min
Response: 0
Conc: N.D.

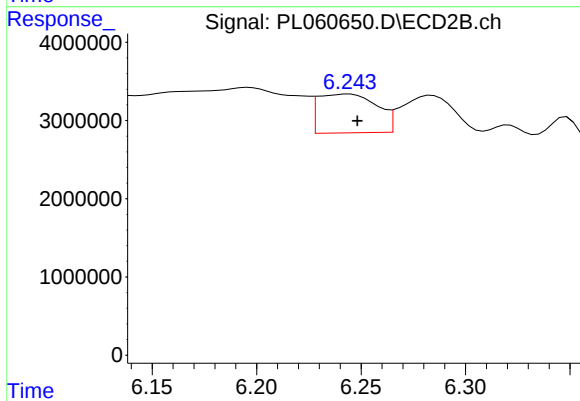

#9 Endosulfan I


R.T.: 6.244 min
Delta R.T.: -0.004 min
Response: 9732208
Conc: 3.44 ng/ml

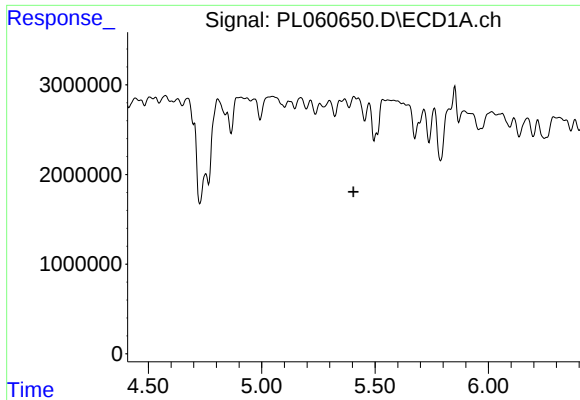

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

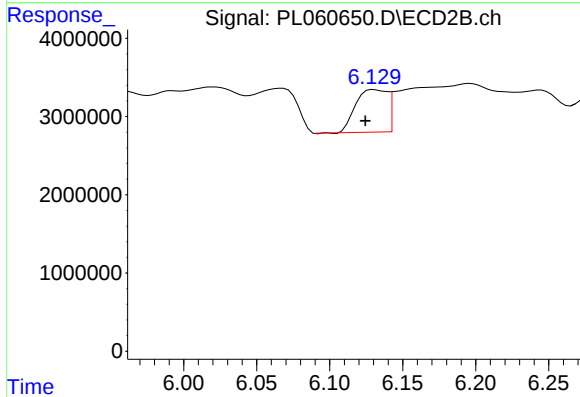


#10 gamma-Chlordane

R.T.: 6.130 min
Delta R.T.: 0.006 min
Response: 8168360
Conc: 2.70 ng/ml

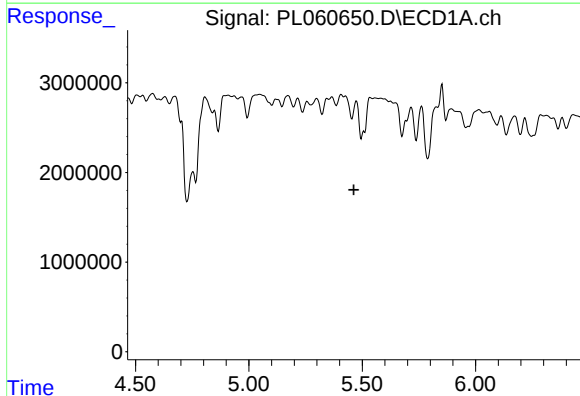


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

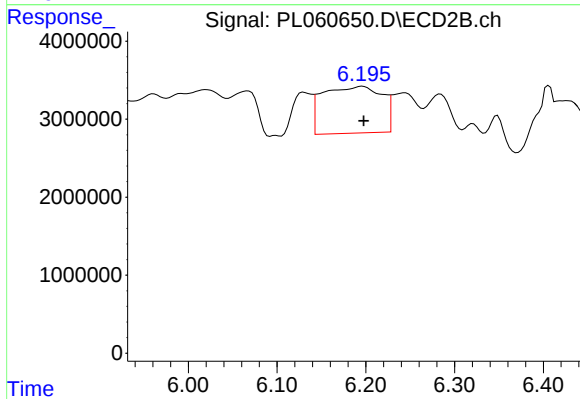

#11 alpha-Chlordane


R.T.: 6.196 min
Delta R.T.: -0.001 min
Response: 27870967
Conc: 9.07 ng/ml

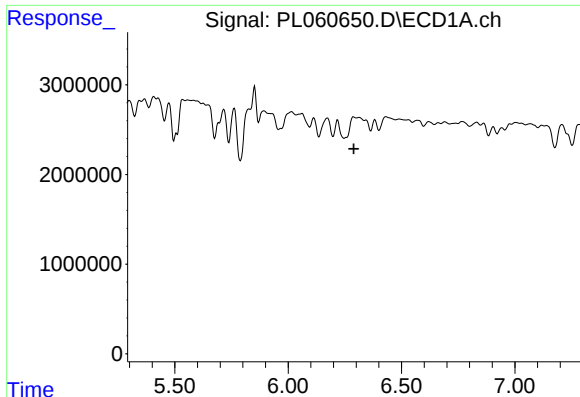

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

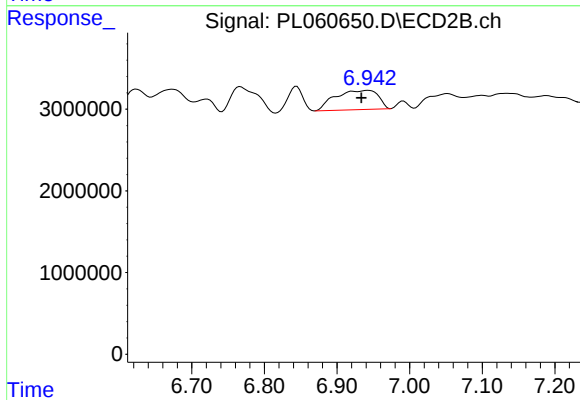


#15 Endosulfan II

R.T.: 6.944 min
Delta R.T.: 0.010 min
Response: 9649746
Conc: 3.70 ng/ml

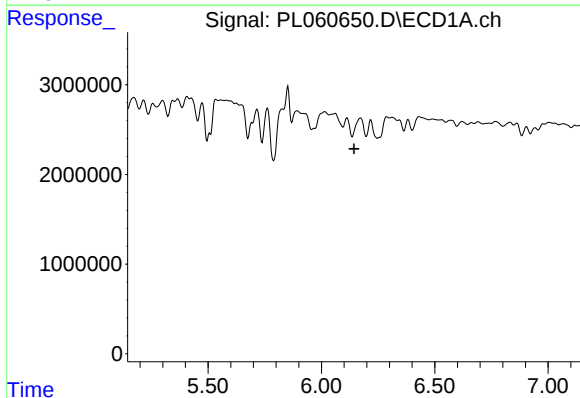


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.144 min
Response: 0
Conc: N.D.

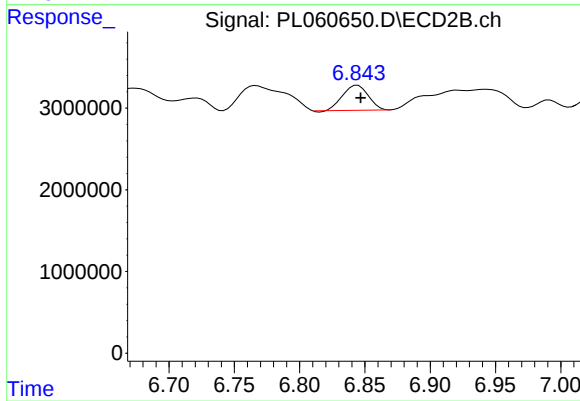

#16 4,4'-DDD


R.T.: 6.844 min
Delta R.T.: -0.002 min
Response: 4150719
Conc: 1.81 ng/ml

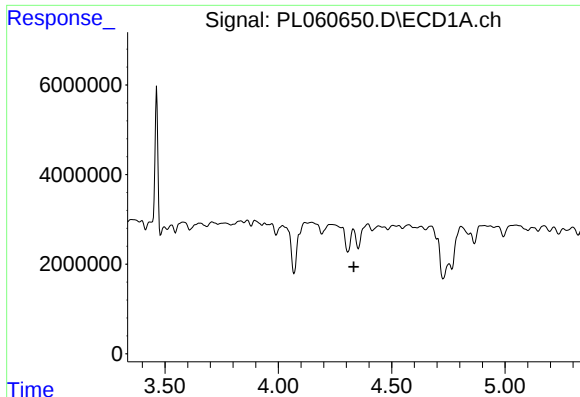

#23 Chlordane-1


R.T.: 4.331 min
Delta R.T.: -0.003 min
Response: -2295
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

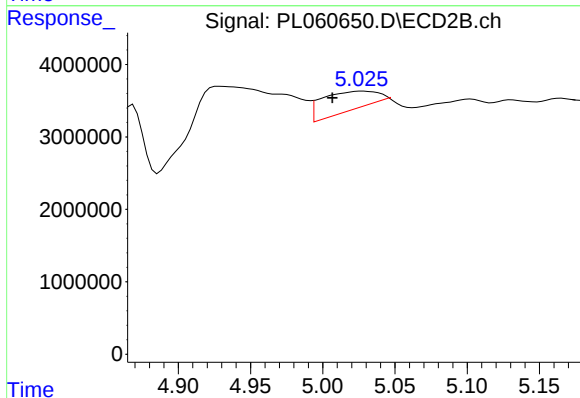


#23 Chlordane-1

R.T.: 5.028 min
Delta R.T.: 0.021 min
Response: 7692287
Conc: 73.18 ng/ml

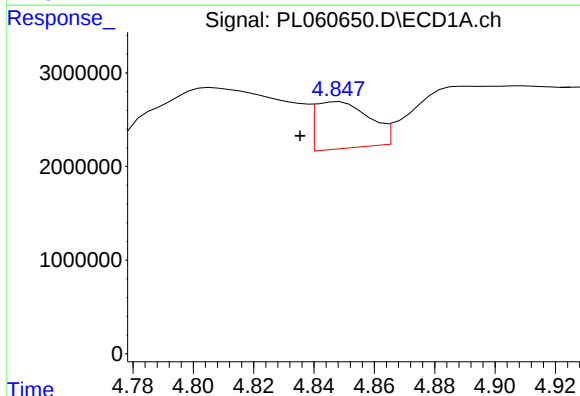


#24 Chlordane-2

R.T.: 4.848 min
Delta R.T.: 0.013 min
Response: 6247125
Conc: 98.60 ng/ml

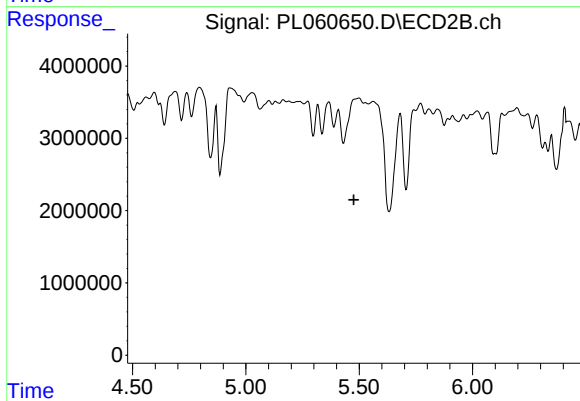

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.476 min
Response: 0
Conc: N.D.

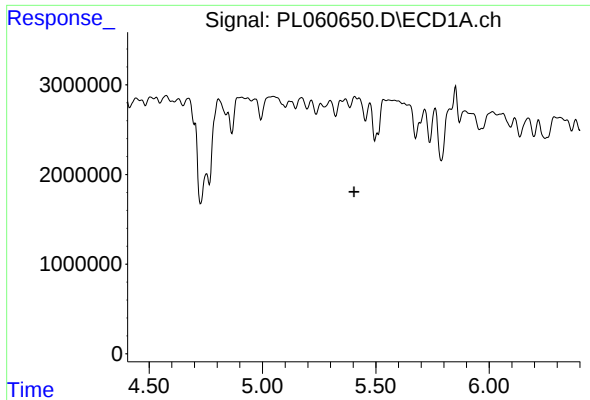

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

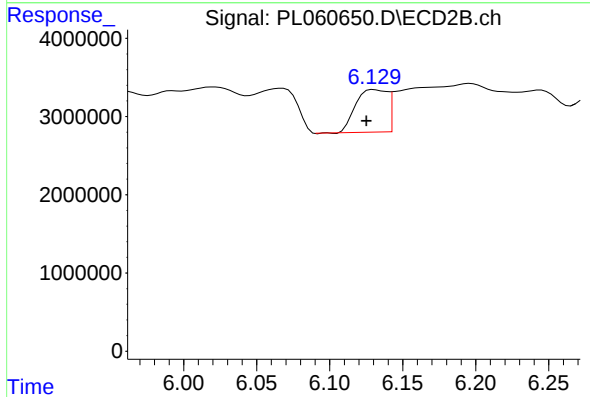


#25 Chlordane-3

R.T.: 6.130 min
Delta R.T.: 0.005 min
Response: 8168360
Conc: 22.56 ng/ml

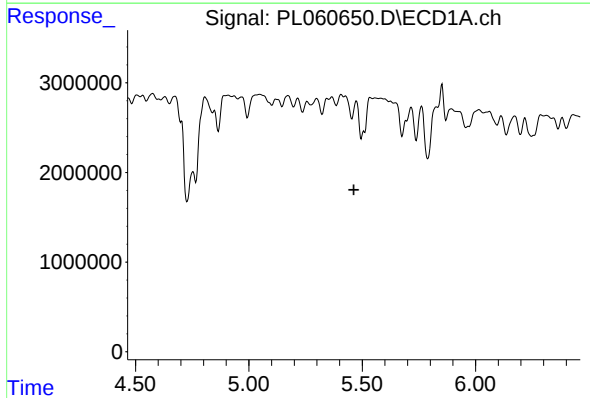


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.463 min
Response: 0
Conc: N.D.

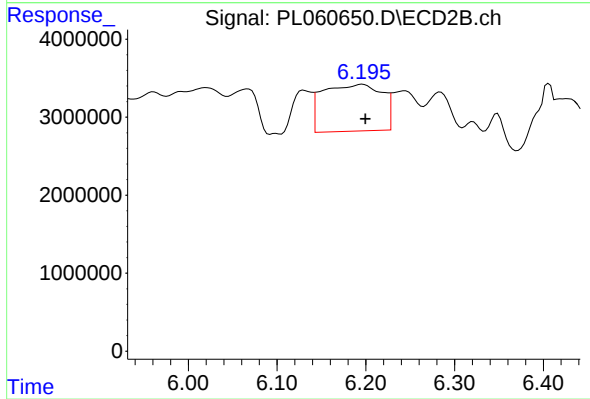

#26 Chlordane-4


R.T.: 6.196 min
Delta R.T.: -0.003 min
Response: 27870967
Conc: 64.29 ng/ml

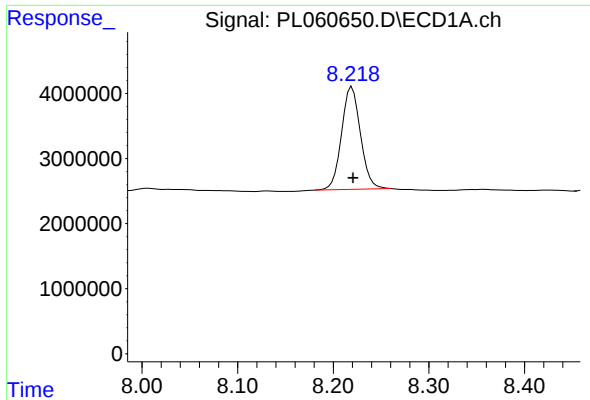

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: 0.000 min
Response: 21755935
Conc: 11.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

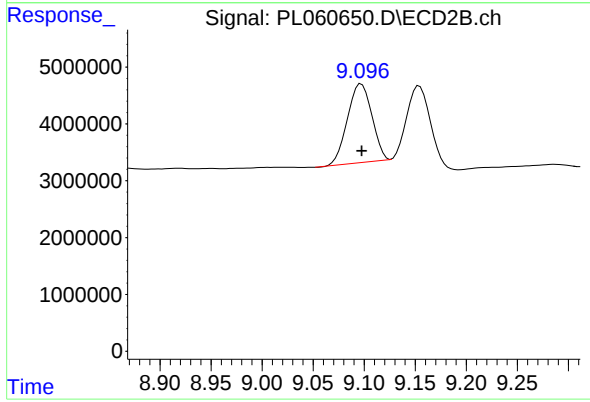

#28 Decachlorobiphenyl

R.T.: 9.097 min
Delta R.T.: 0.000 min
Response: 23020649
Conc: 12.27 ng/ml