

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081221\
 Data File : PL068932.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 09:24
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:17:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) MB Aldrin	0.000	7.575	0	132115	N.D.	0.109 #
8) B Heptachlo...	0.000	8.039	0	10639127	N.D.	9.203 #
13) MA Dieldrin	7.774	0.000	1195145	0	2.310	N.D. #
14) MA Endrin	8.082f	0.000	3807571	0	7.901	N.D. #
15) B Endosulfa...	0.000	9.215	0	375495	N.D.	0.409 #
17) MA 4,4'-DDT	0.000	9.434	0	1264952	N.D.	1.337 #
18) B Endrin al...	0.000	9.338	0	800351	N.D.	1.142 #
19) B Endosulfa...	0.000	9.572	0	150290	N.D.	0.165 #
22) Mirex	0.000	10.568f	0	279183	N.D.	0.353 #
23) Chlordane-1	0.000	6.976f	0	424445	N.D.	10.065 #
24) Chlordane-2	0.000	7.575f	0	132115	N.D.	3.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081221\
Data File : PL068932.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 09:24
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:17:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

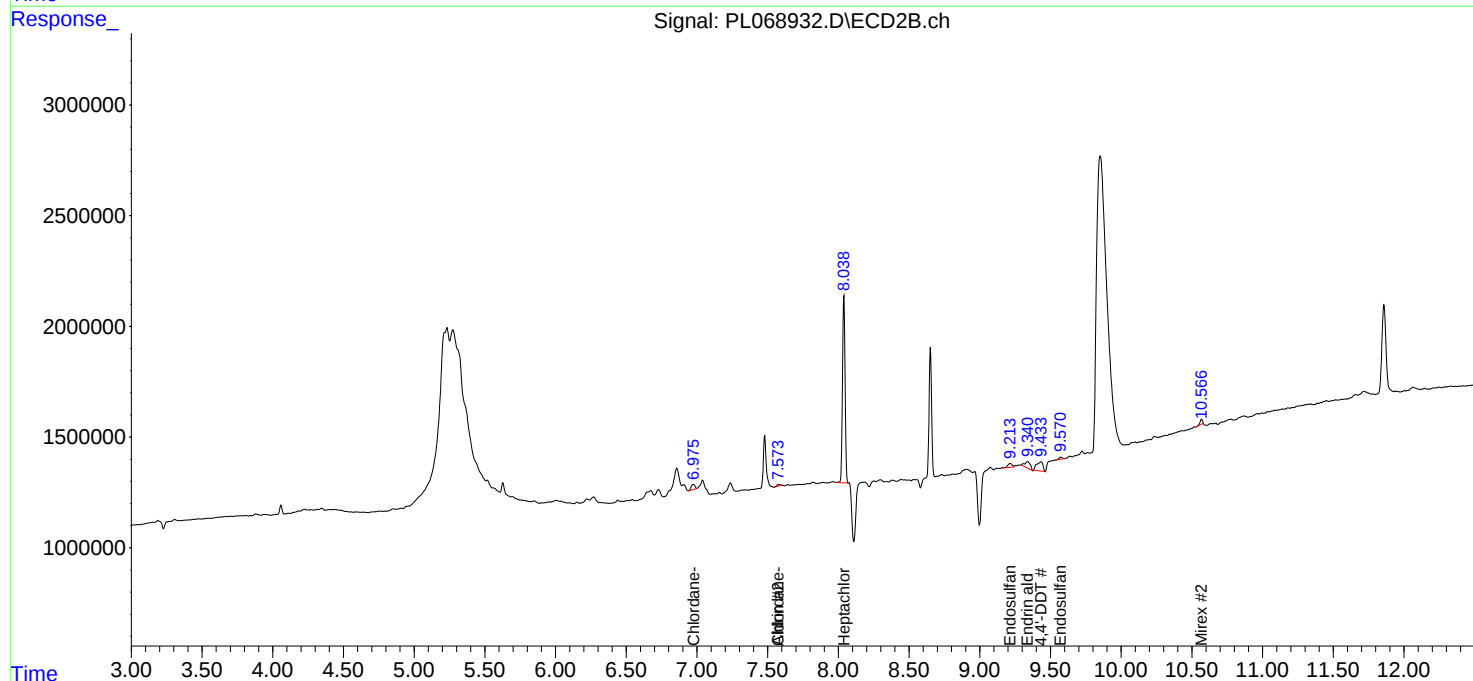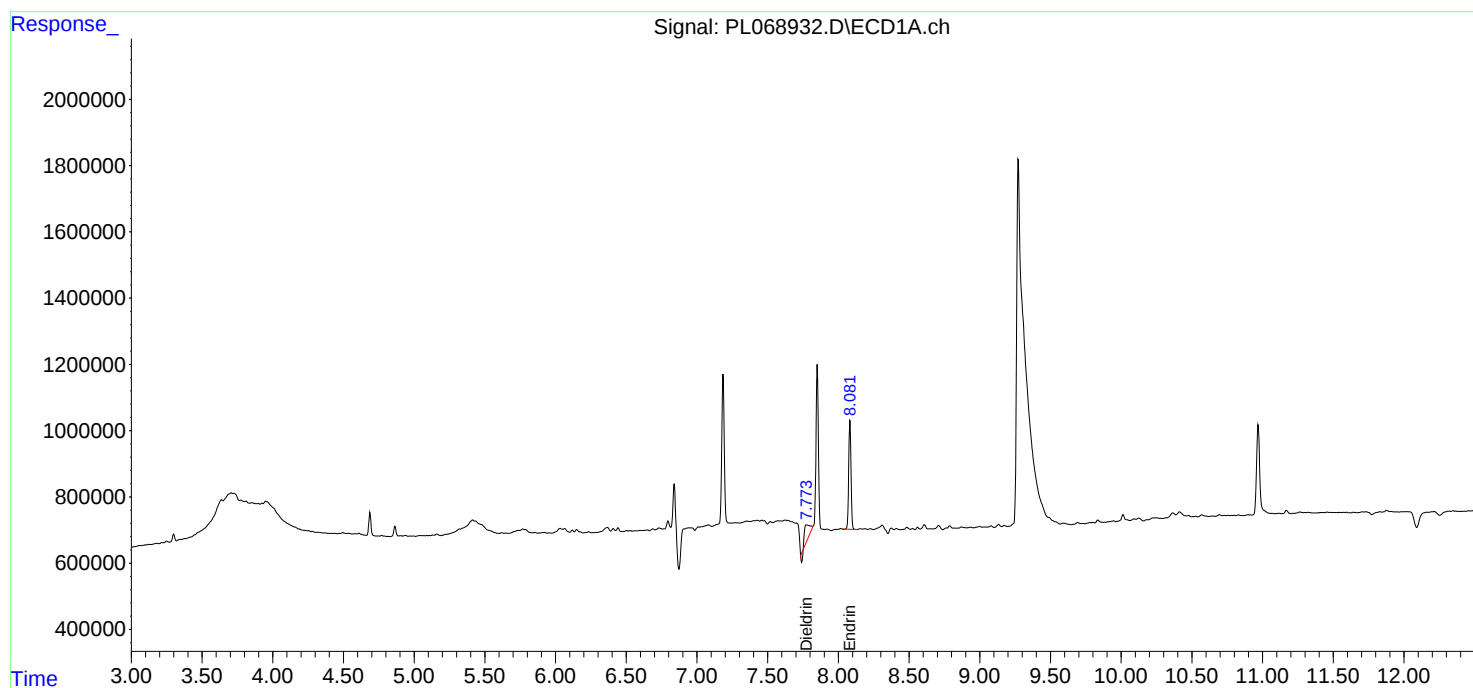


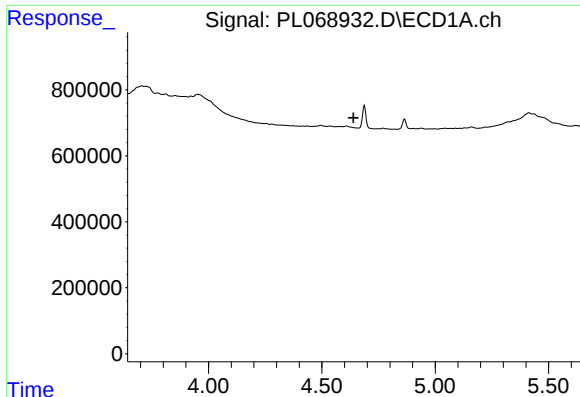

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.640 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

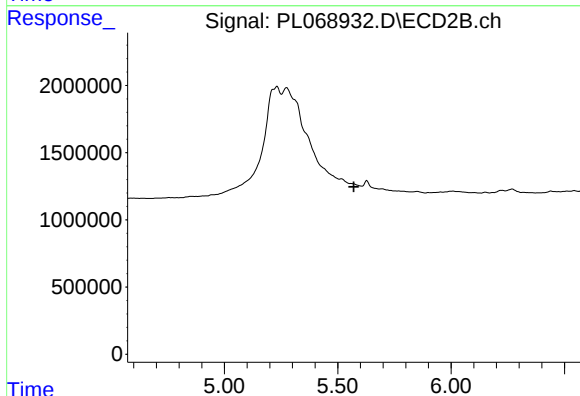


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.571 min
Response: 0
Conc: N.D.

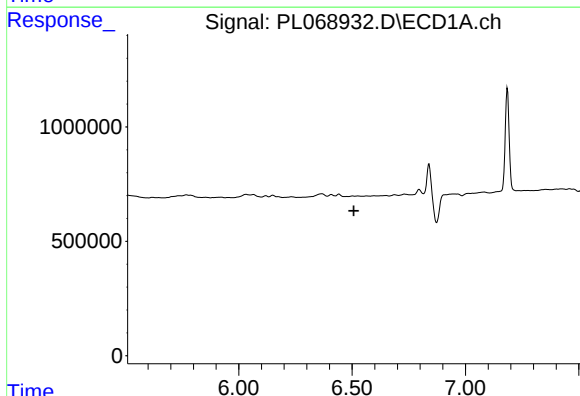


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.507 min
Response: 0
Conc: N.D.

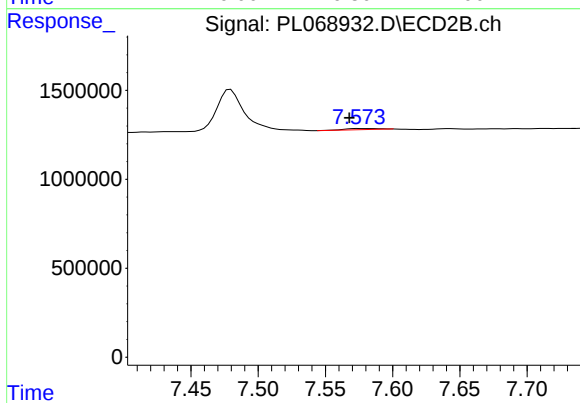

#5 Aldrin


R.T.: 7.575 min
Delta R.T.: 0.007 min
Response: 132115
Conc: 0.11 ng/ml

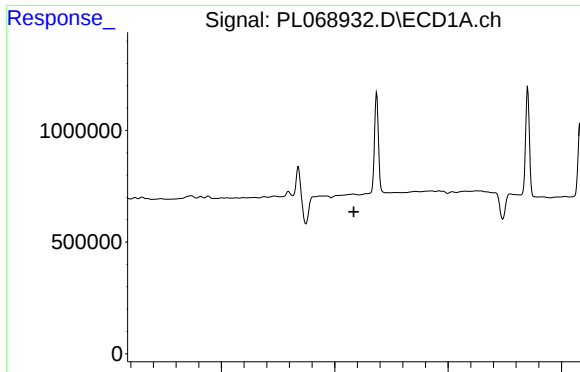

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

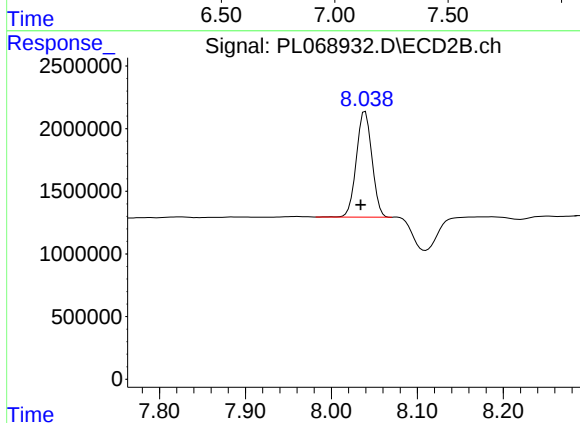


#8 Heptachlor epoxide

R.T.: 8.039 min
Delta R.T.: 0.005 min
Response: 10639127
Conc: 9.20 ng/ml

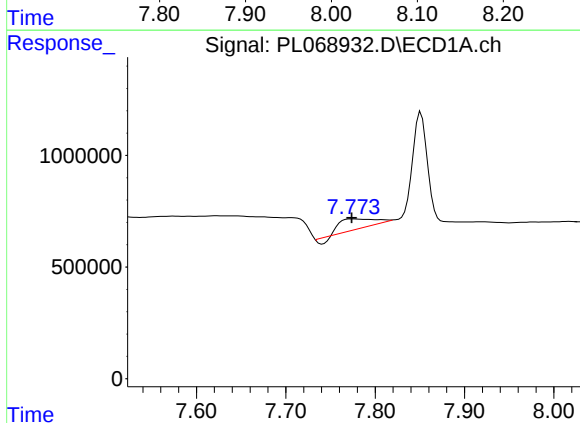


#13 Dieldrin

R.T.: 7.774 min
Delta R.T.: 0.000 min
Response: 1195145
Conc: 2.31 ng/ml

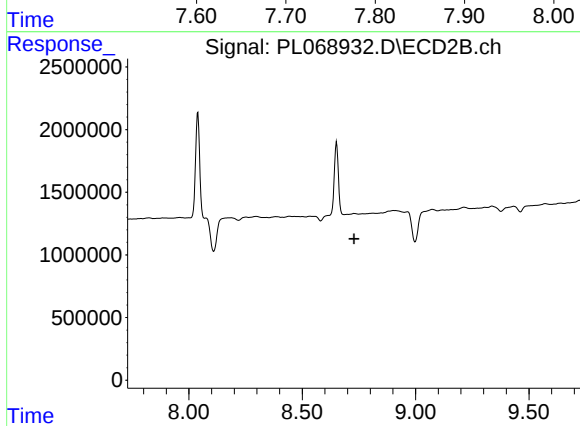

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.729 min
Response: 0
Conc: N.D.

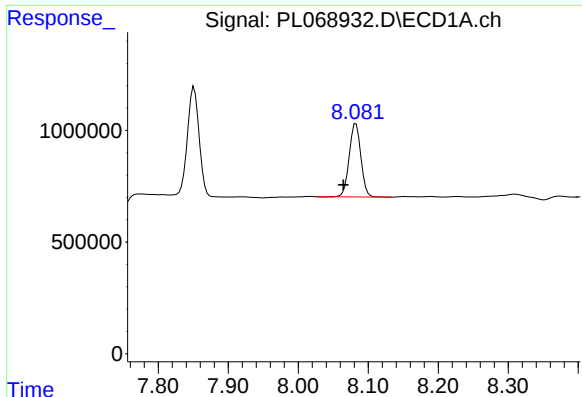

#14 Endrin


R.T.: 8.082 min
Delta R.T.: 0.018 min
Response: 3807571
Conc: 7.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

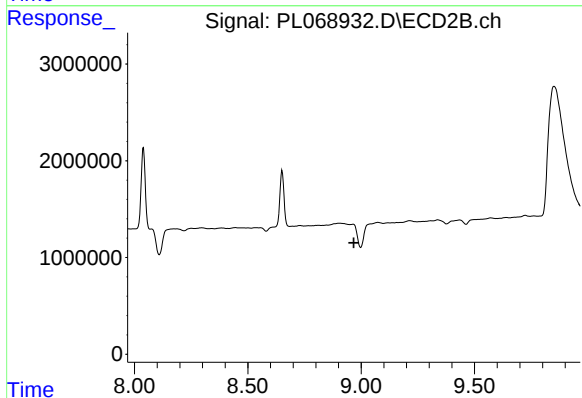


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.968 min
Response: 0
Conc: N.D.

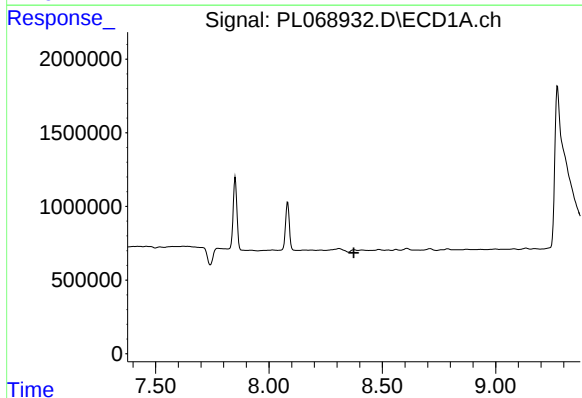


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.375 min
Response: 0
Conc: N.D.

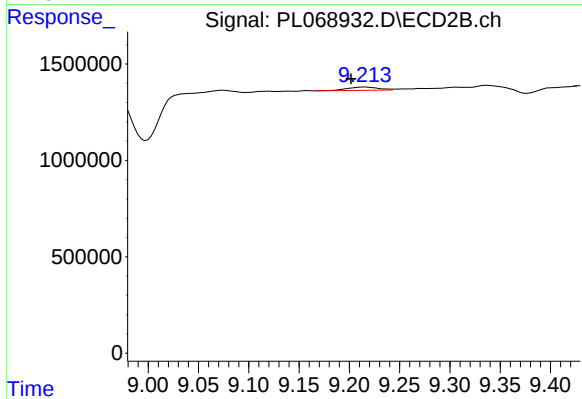

#15 Endosulfan II


R.T.: 9.215 min
Delta R.T.: 0.013 min
Response: 375495
Conc: 0.41 ng/ml

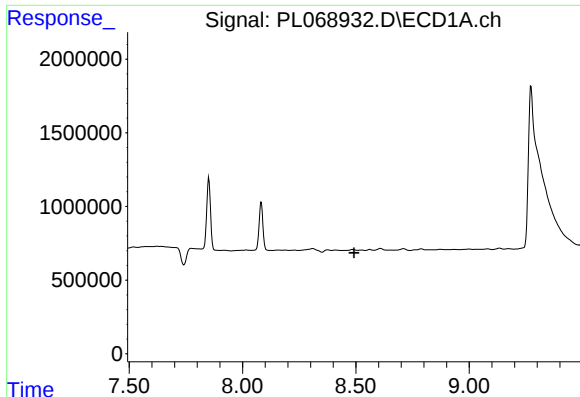

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

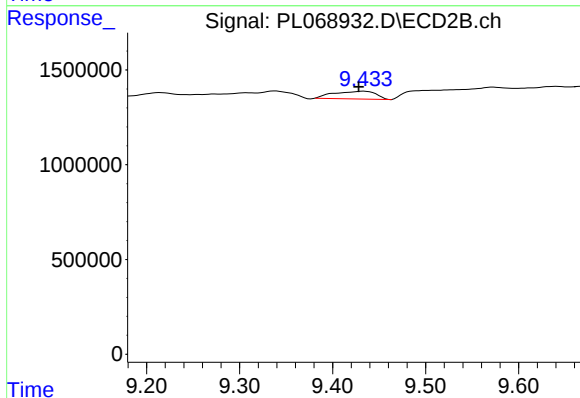


#17 4,4'-DDT

R.T.: 9.434 min
Delta R.T.: 0.005 min
Response: 1264952
Conc: 1.34 ng/ml

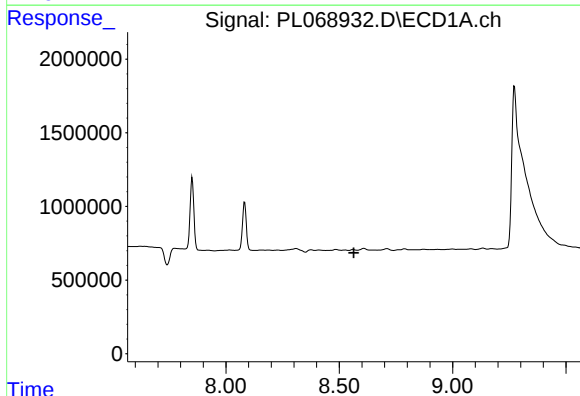


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.564 min
Response: 0
Conc: N.D.

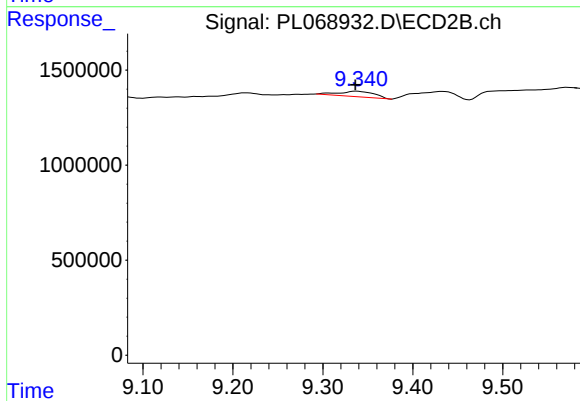

#18 Endrin aldehyde


R.T.: 9.338 min
Delta R.T.: 0.002 min
Response: 800351
Conc: 1.14 ng/ml

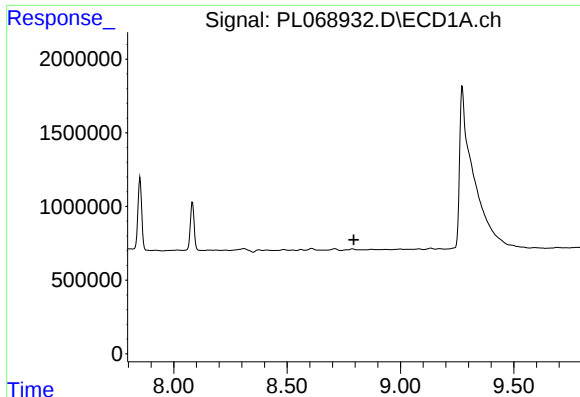

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

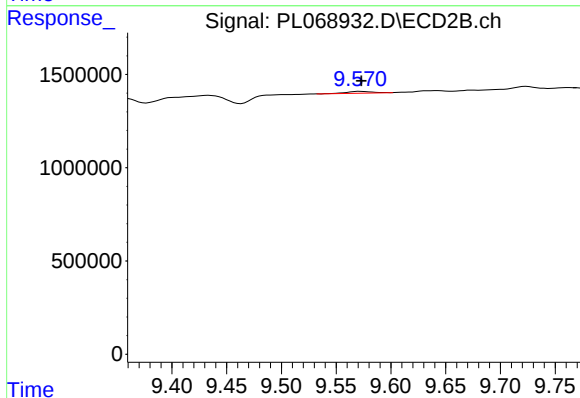


#19 Endosulfan Sulfate

R.T.: 9.572 min
Delta R.T.: -0.001 min
Response: 150290
Conc: 0.16 ng/ml

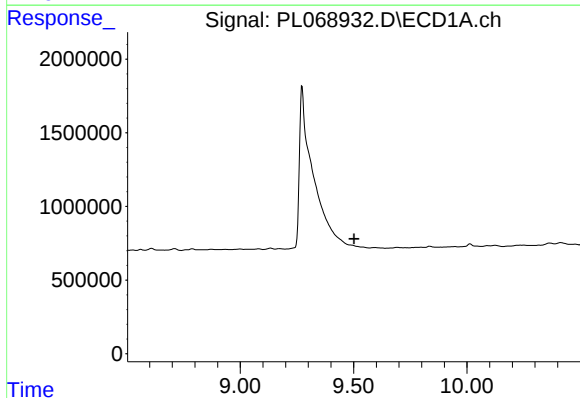


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

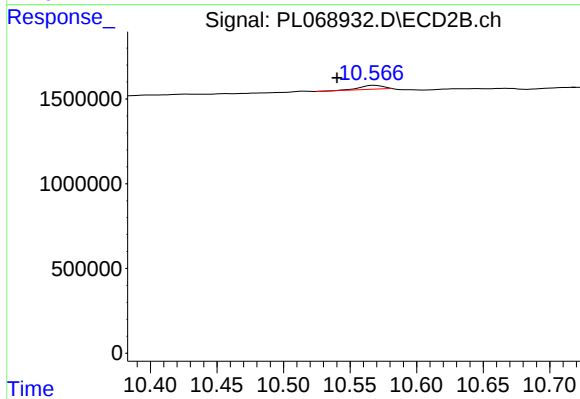

#22 Mirex


R.T.: 10.568 min
Delta R.T.: 0.028 min
Response: 279183
Conc: 0.35 ng/ml

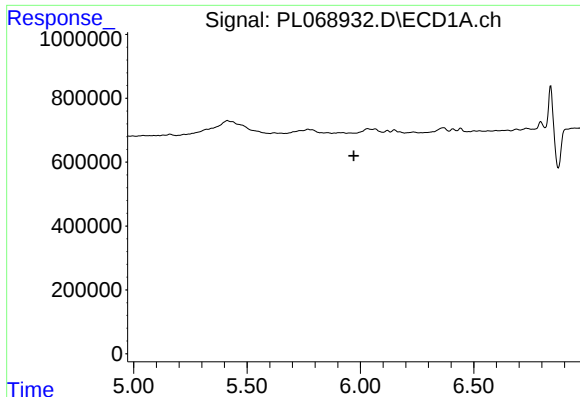

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

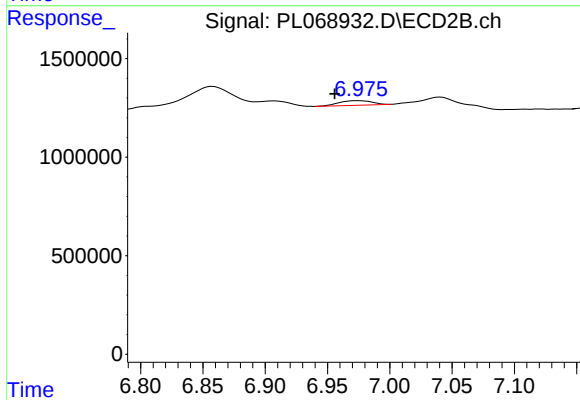


#23 Chlordane-1

R.T.: 6.976 min
Delta R.T.: 0.020 min
Response: 424445
Conc: 10.07 ng/ml

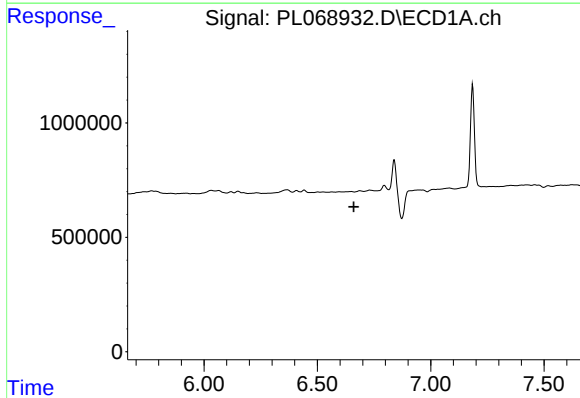


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.661 min
Response: 0
Conc: N.D.

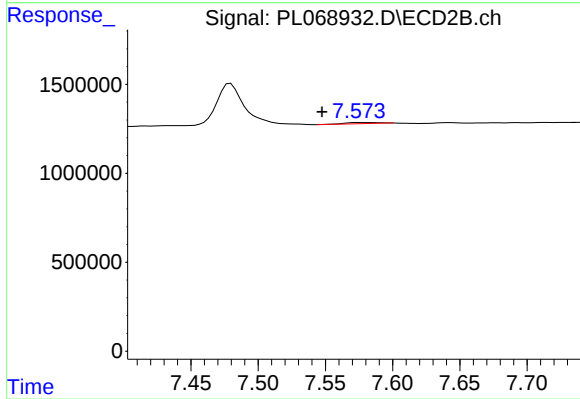

#24 Chlordane-2


R.T.: 7.575 min
Delta R.T.: 0.028 min
Response: 132115
Conc: 3.05 ng/ml

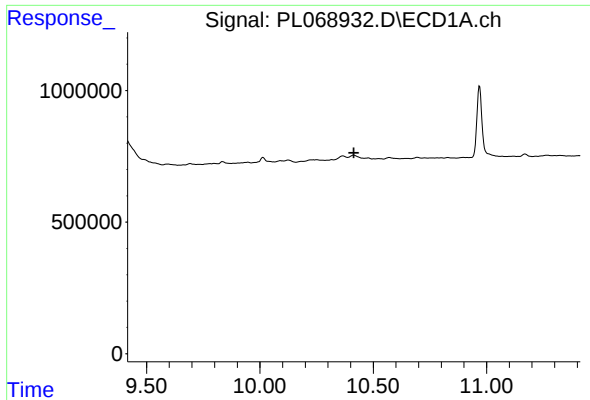

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

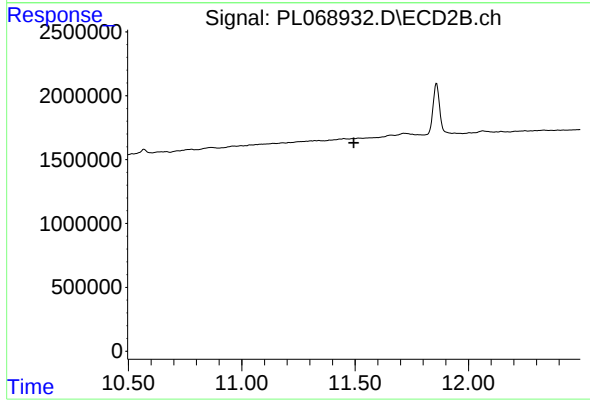

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.495 min
Response: 0
Conc: N.D.