

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081221\
 Data File : PL068948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 20:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:22:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 06 03:02:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.568	9100443	25175611	22.001	24.795
28)	SA Decachlor...	10.402	11.487	12992333	22640942	22.607	23.335
Target Compounds							
2)	A alpha-BHC	5.363f	0.000	1352742	0	2.446	N.D. #
4)	MA Heptachlor	6.151f	7.227f	385666	848559	0.657	0.632
6)	B beta-BHC	6.151	0.000	385666	0	1.368	N.D. #
8)	B Heptachlo...	0.000	8.035	0	2978178	N.D.	2.576 #
14)	MA Endrin	8.078	0.000	1104200	0	2.291	N.D. #
15)	B Endosulfa...	0.000	9.214	0	435545	N.D.	0.475 #
17)	MA 4,4'-DDT	0.000	9.435	0	578748	N.D.	0.612 #
22)	Mirex	0.000	10.561f	0	316748	N.D.	0.400 #
23)	Chlordane-1	0.000	6.965	0	878427	N.D.	20.831 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081221\
Data File : PL068948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 20:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:22:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080521.M
Quant Title : GC Extractables
QLast Update : Fri Aug 06 03:02:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

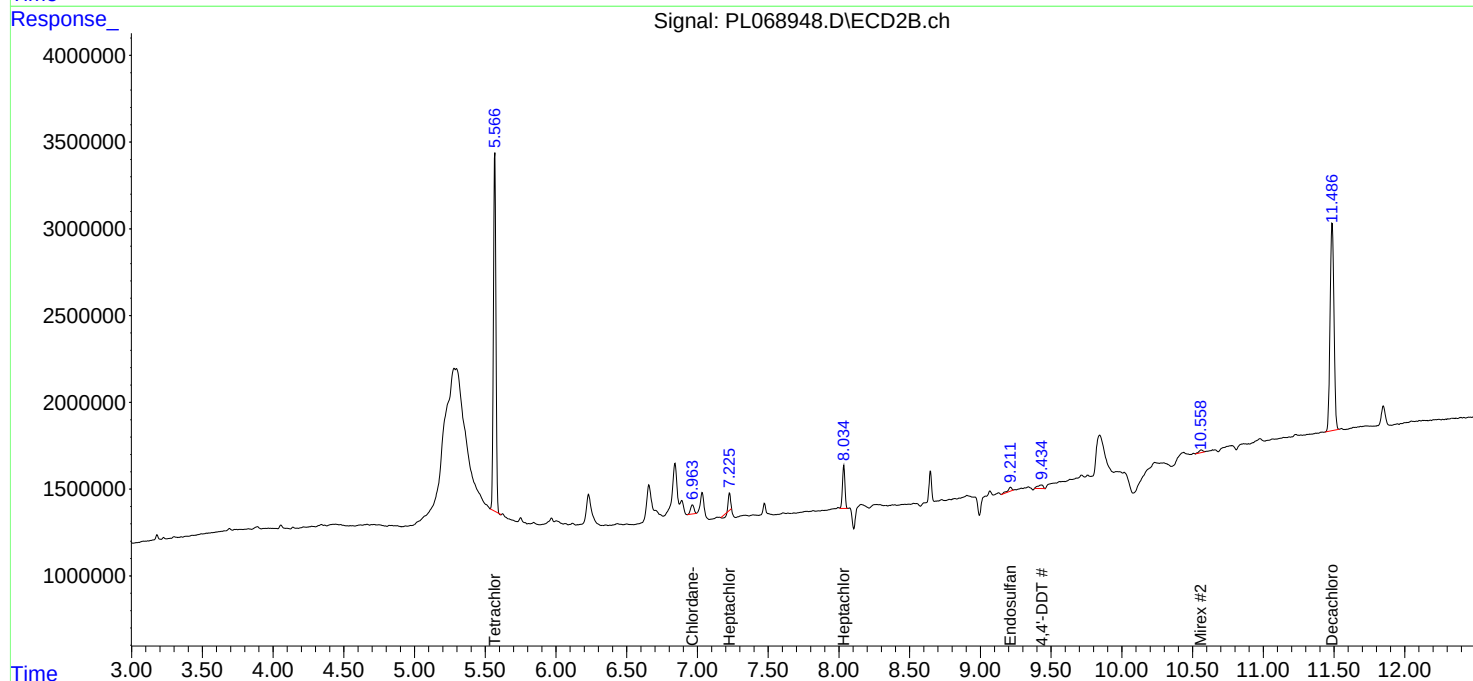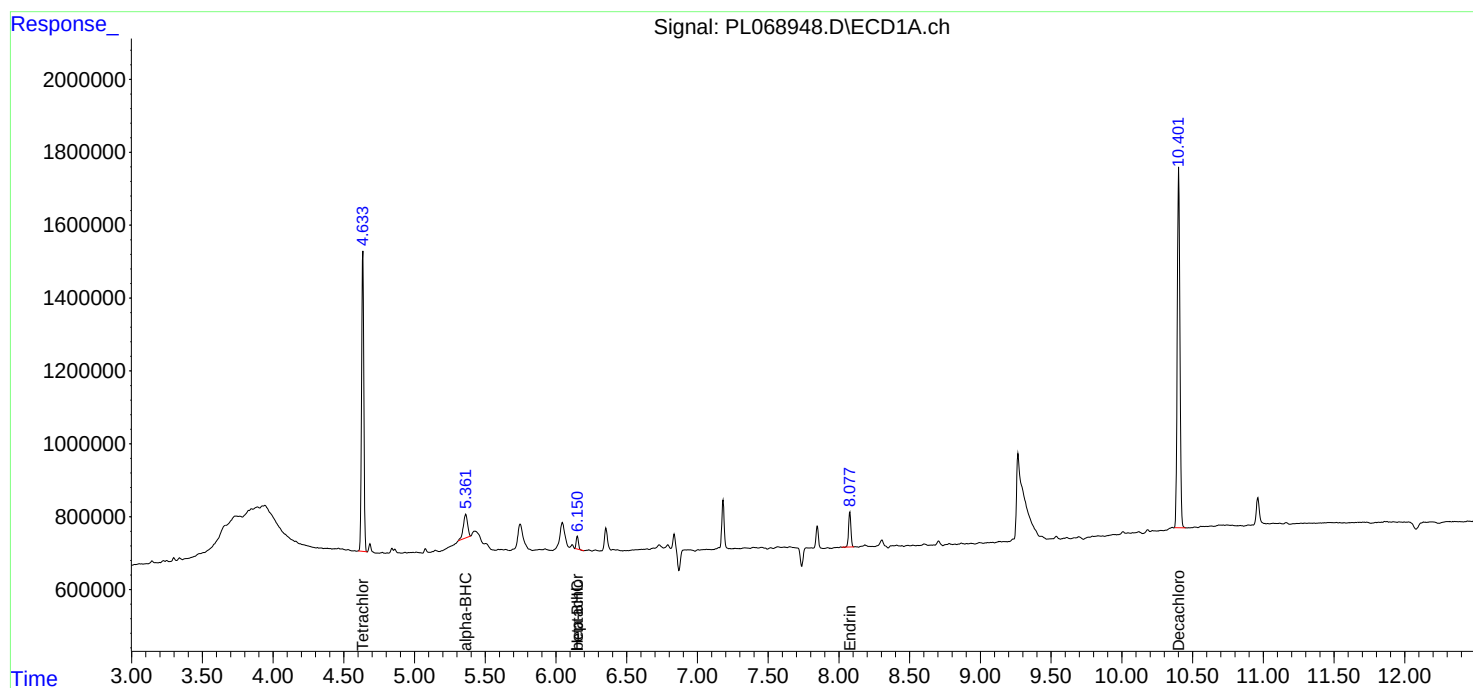


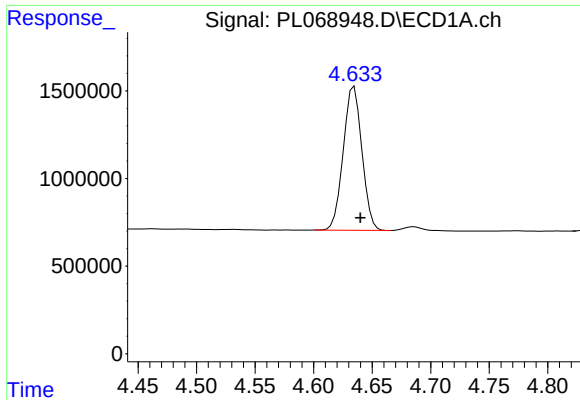

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.005 min
Response: 9100443
Conc: 22.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

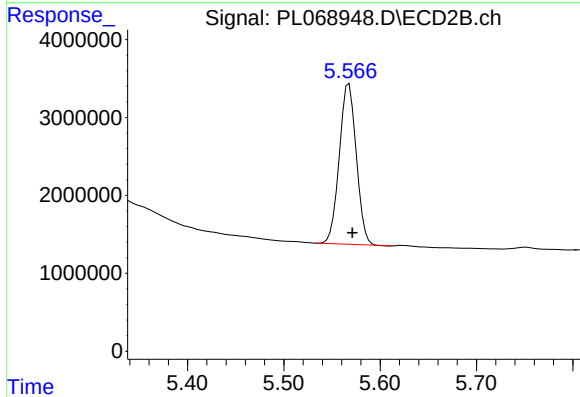


#1 Tetrachloro-m-xylene

R.T.: 5.568 min
Delta R.T.: -0.003 min
Response: 25175611
Conc: 24.80 ng/ml

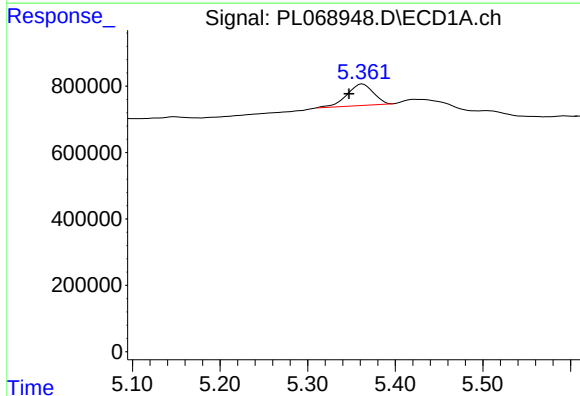


#2 alpha-BHC

R.T.: 5.363 min
Delta R.T.: 0.016 min
Response: 1352742
Conc: 2.45 ng/ml

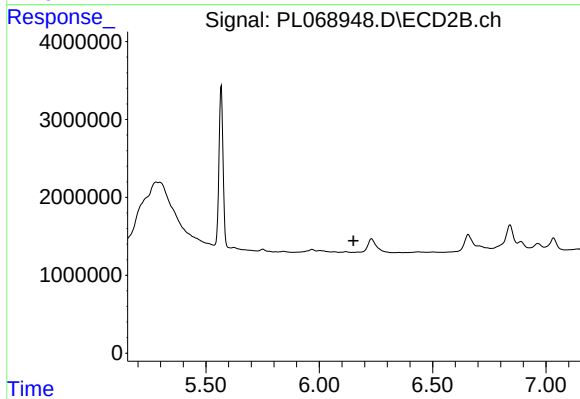

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

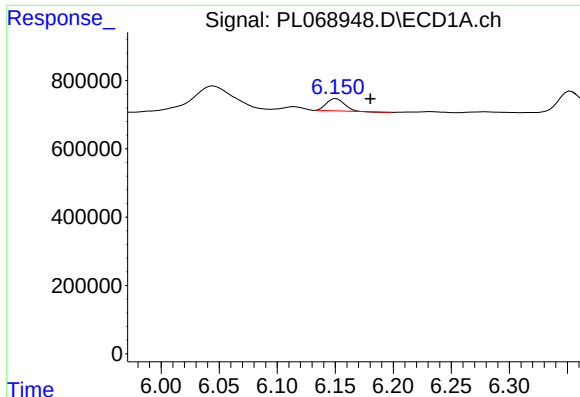

#4 Heptachlor


R.T.: 6.151 min
Delta R.T.: -0.029 min
Response: 385666
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

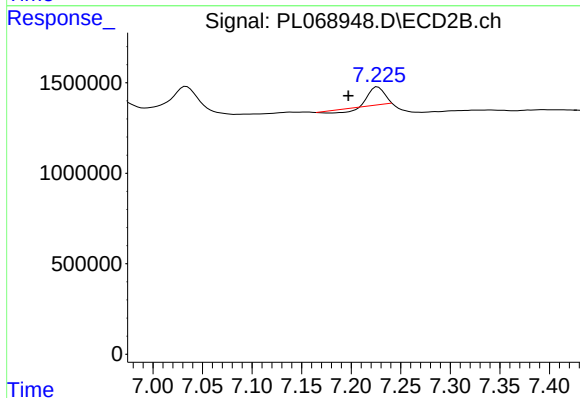


#4 Heptachlor

R.T.: 7.227 min
Delta R.T.: 0.030 min
Response: 848559
Conc: 0.63 ng/ml

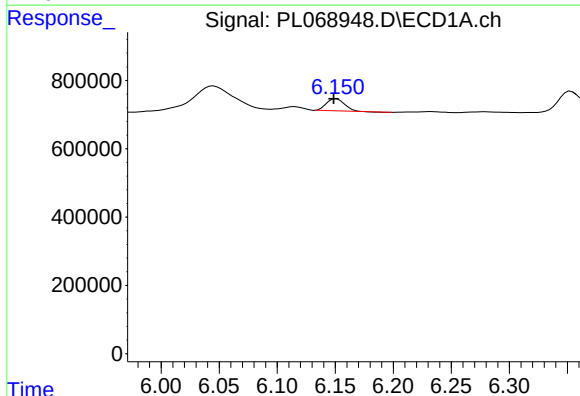


#6 beta-BHC

R.T.: 6.151 min
Delta R.T.: 0.002 min
Response: 385666
Conc: 1.37 ng/ml

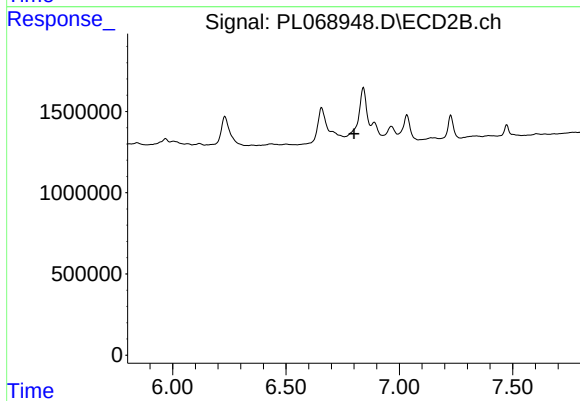

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.800 min
Response: 0
Conc: N.D.

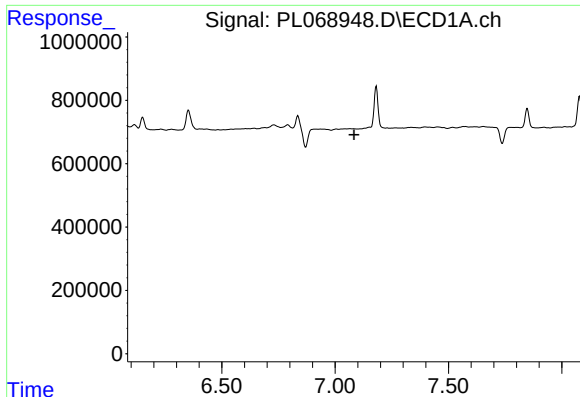

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.084 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

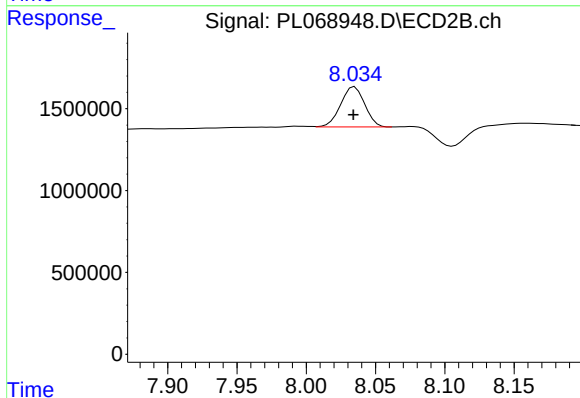


#8 Heptachlor epoxide

R.T.: 8.035 min
Delta R.T.: 0.000 min
Response: 2978178
Conc: 2.58 ng/ml

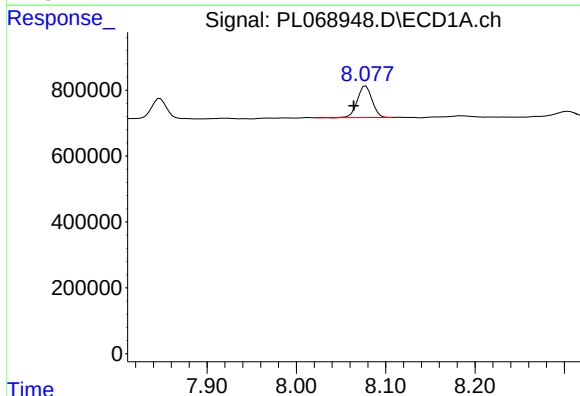


#14 Endrin

R.T.: 8.078 min
Delta R.T.: 0.013 min
Response: 1104200
Conc: 2.29 ng/ml

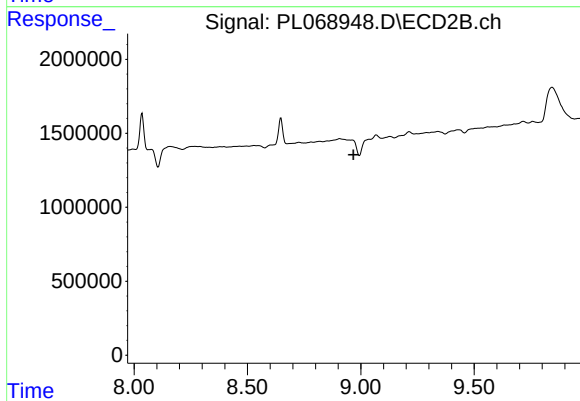

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.968 min
Response: 0
Conc: N.D.

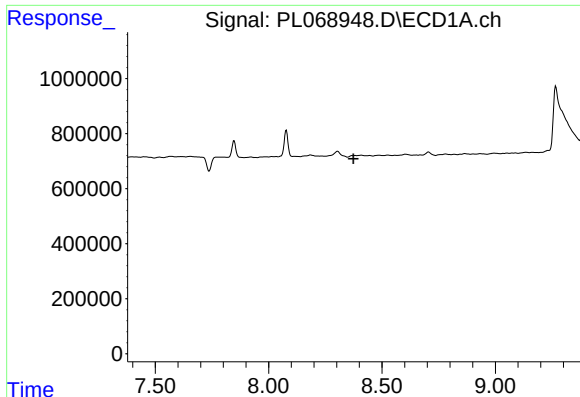

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.375 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

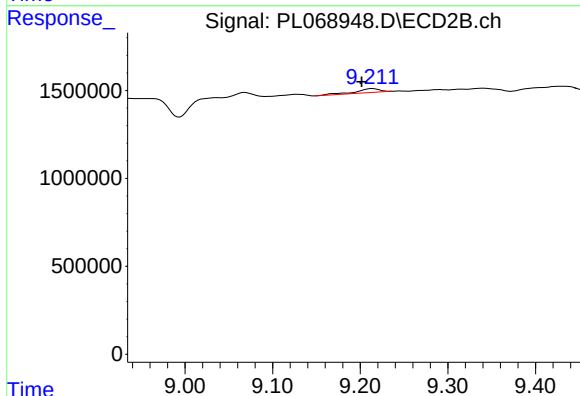


#15 Endosulfan II

R.T.: 9.214 min
Delta R.T.: 0.012 min
Response: 435545
Conc: 0.47 ng/ml

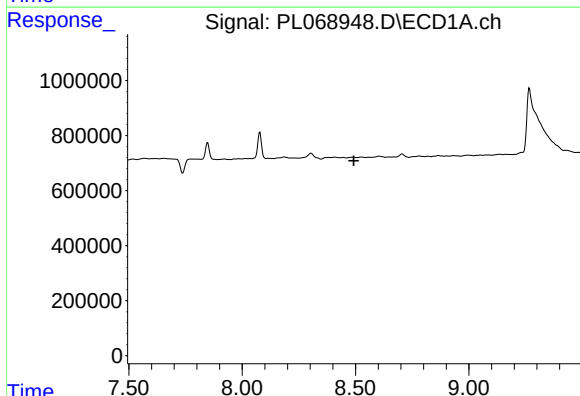


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.492 min
Response: 0
Conc: N.D.

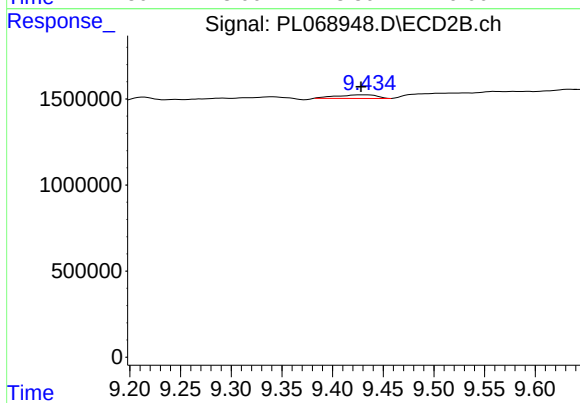

#17 4,4'-DDT


R.T.: 9.435 min
Delta R.T.: 0.007 min
Response: 578748
Conc: 0.61 ng/ml

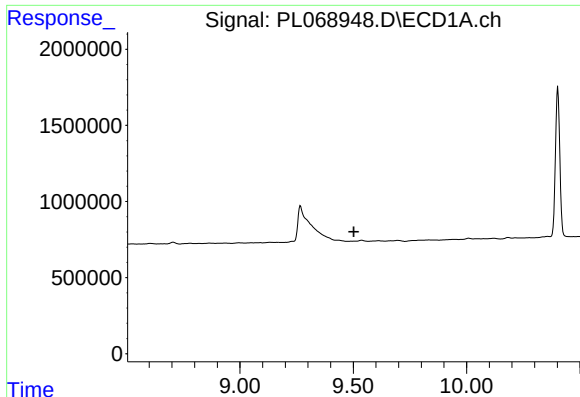

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

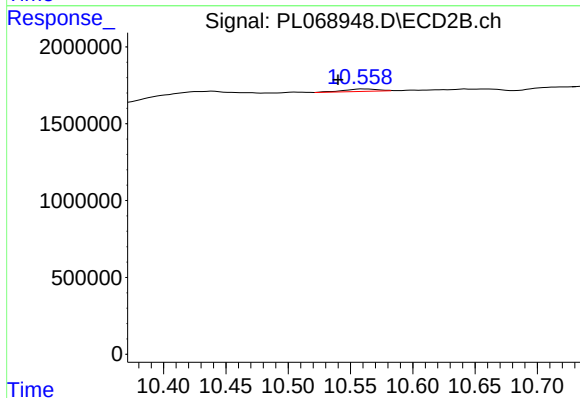


#22 Mirex

R.T.: 10.561 min
Delta R.T.: 0.021 min
Response: 316748
Conc: 0.40 ng/ml

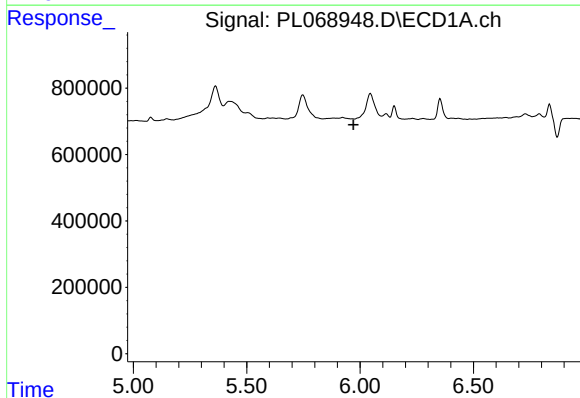


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.971 min
Response: 0
Conc: N.D.

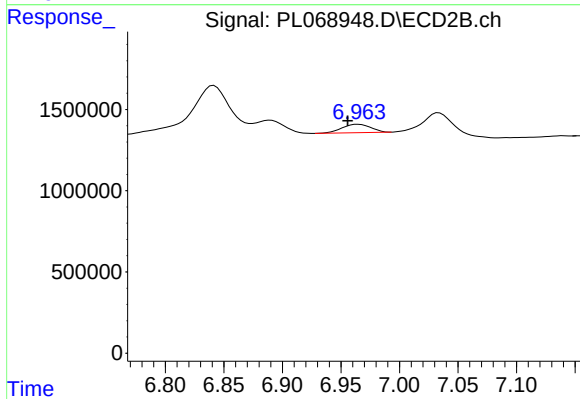

#23 Chlordane-1


R.T.: 6.965 min
Delta R.T.: 0.009 min
Response: 878427
Conc: 20.83 ng/ml

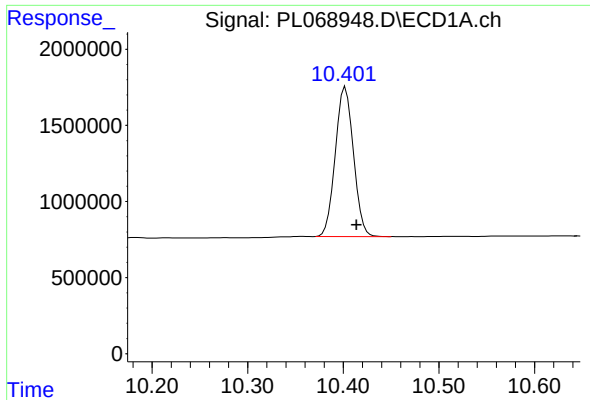

#28 Decachlorobiphenyl

R.T.: 10.402 min
Delta R.T.: -0.011 min
Response: 12992333
Conc: 22.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

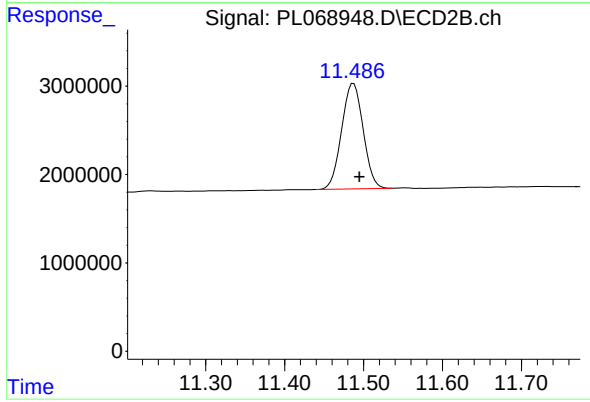

#28 Decachlorobiphenyl

R.T.: 11.487 min
Delta R.T.: -0.007 min
Response: 22640942
Conc: 23.34 ng/ml