

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
 Data File : PL077064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 18:00
 Operator : AR\AJ
 Sample : N4188-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 22:28:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.637	6752231	17948967	6.886	6.270
28)	SA Decachlor...	8.911	7.743	7131987	18495326	9.447	8.216
Target Compounds							
3)	MA gamma-BHC...	4.247f	0.000	27146	0	0.021	N.D. #
10)	B gamma-Chl...	0.000	4.836f	0	2022421	N.D.	0.664 #
11)	B alpha-Chl...	5.905	0.000	513856	0	0.515	N.D. #
15)	B Endosulfa...	6.713f	0.000	145322	0	0.169	N.D. #
25)	Chlordane-3	0.000	4.836f	0	2022421	N.D.	6.388 #
26)	Chlordane-4	5.905	0.000	513856	0	2.911	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
Data File : PL077064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 18:00
Operator : AR\AJ
Sample : N4188-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 22:28:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

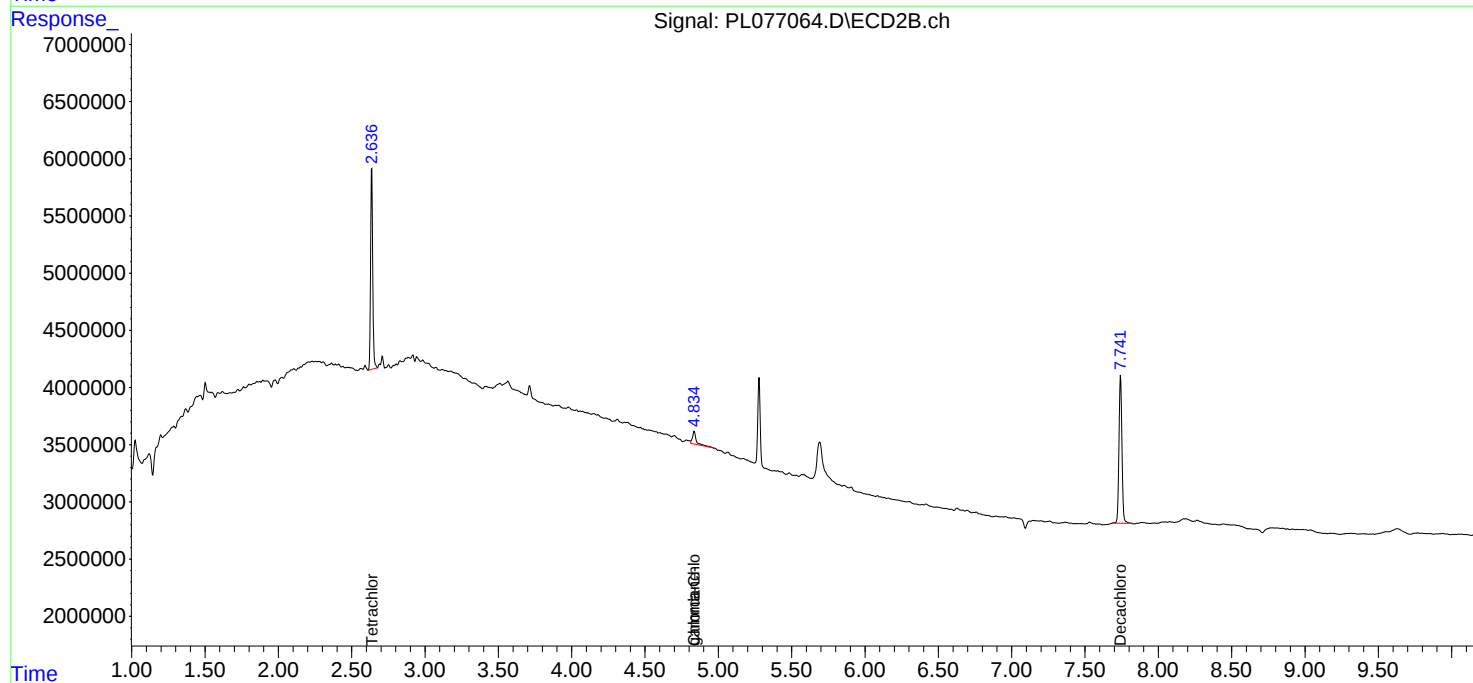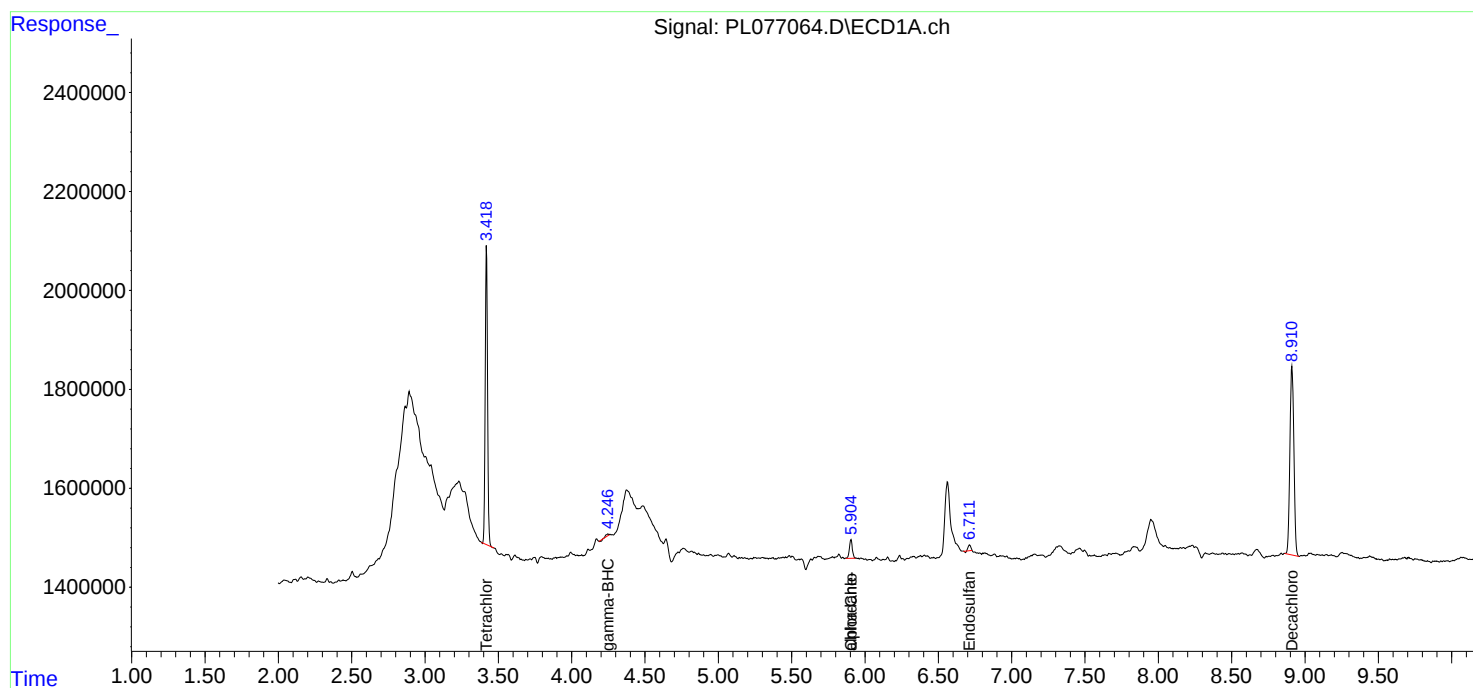


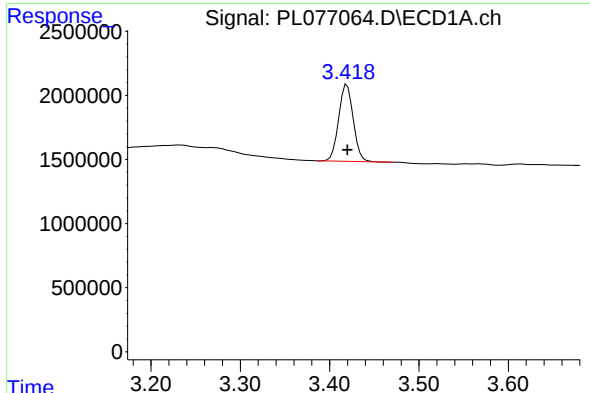

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 6752231
Conc: 6.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

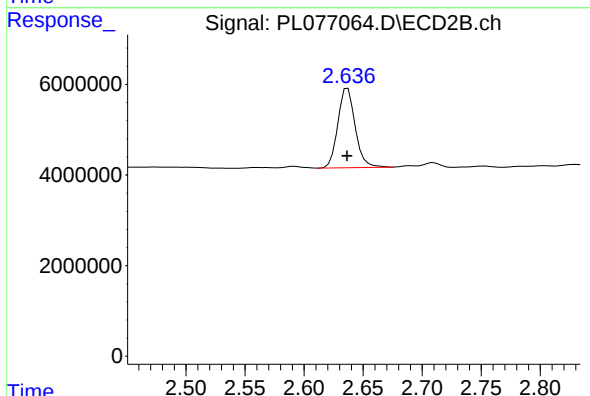


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 17948967
Conc: 6.27 ng/ml

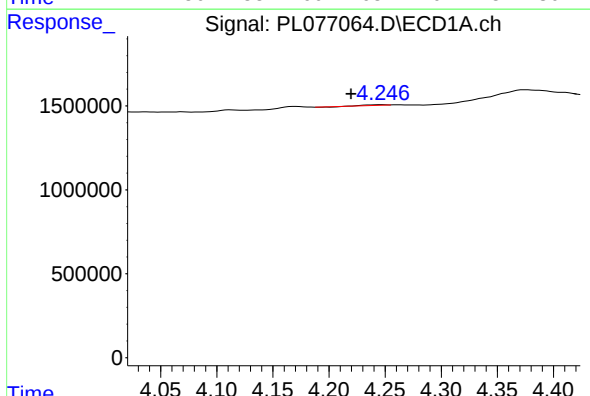


#3 gamma-BHC (Lindane)

R.T.: 4.247 min
Delta R.T.: 0.028 min
Response: 27146
Conc: 0.02 ng/ml

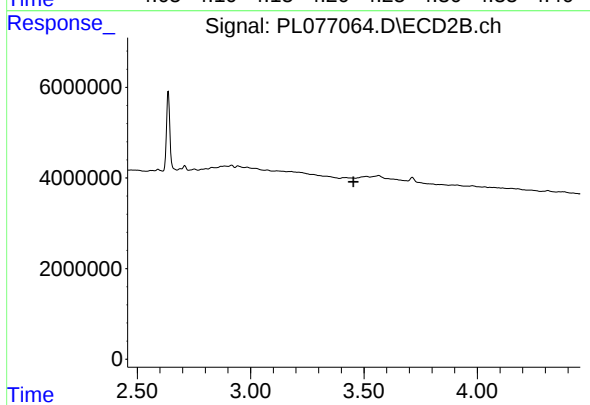

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 3.454 min
Response: 0
Conc: N.D.

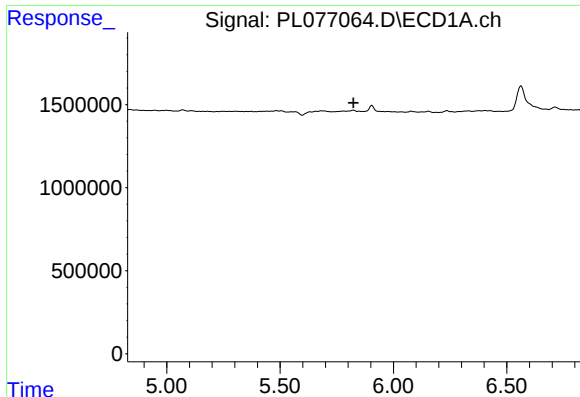

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

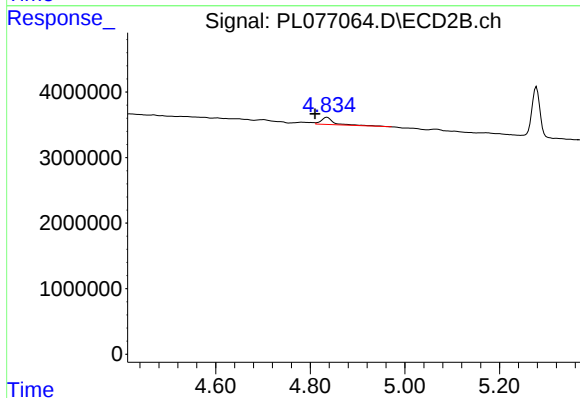


#10 gamma-Chlordane

R.T.: 4.836 min
Delta R.T.: 0.025 min
Response: 2022421
Conc: 0.66 ng/ml

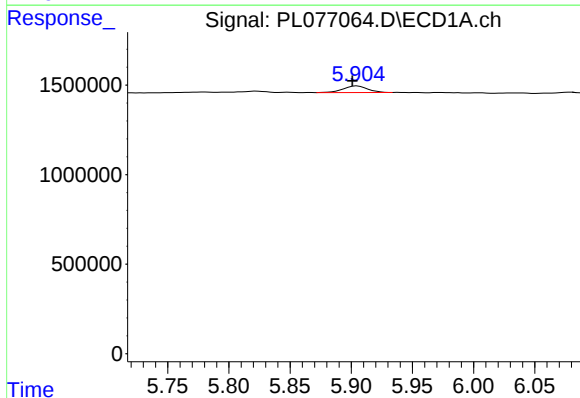


#11 alpha-Chlordane

R.T.: 5.905 min
Delta R.T.: 0.004 min
Response: 513856
Conc: 0.51 ng/ml

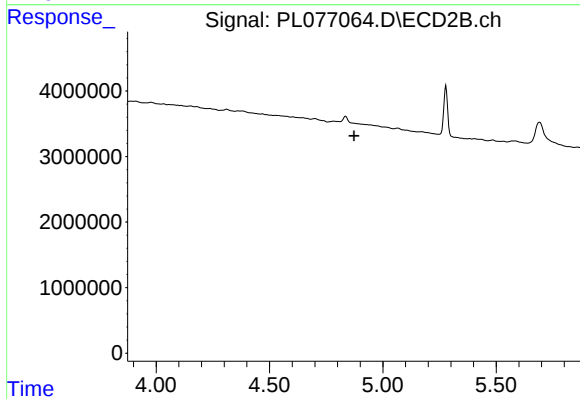

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.873 min
Response: 0
Conc: N.D.

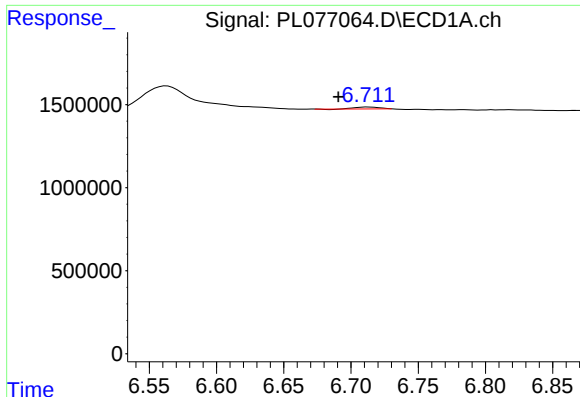

#15 Endosulfan II


R.T.: 6.713 min
Delta R.T.: 0.022 min
Response: 145322
Conc: 0.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

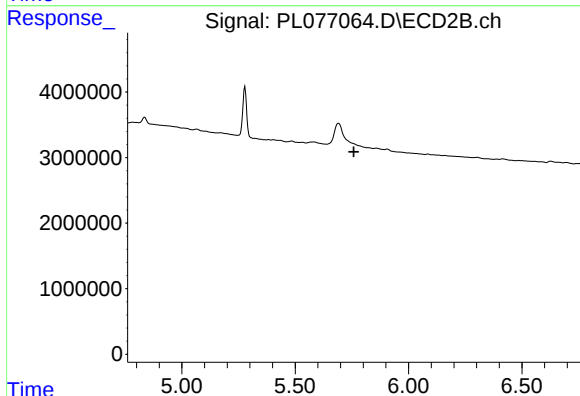


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.759 min
Response: 0
Conc: N.D.

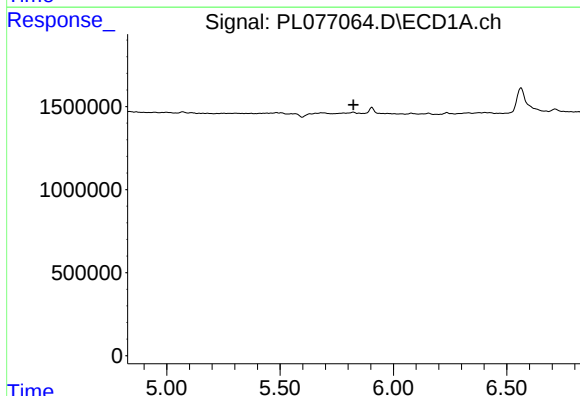


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.824 min
Response: 0
Conc: N.D.

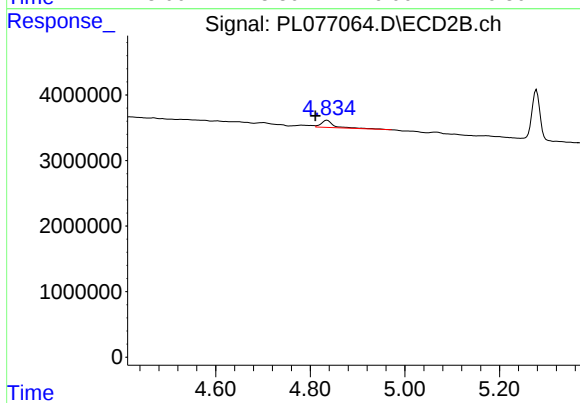

#25 Chlordane-3


R.T.: 4.836 min
Delta R.T.: 0.024 min
Response: 2022421
Conc: 6.39 ng/ml

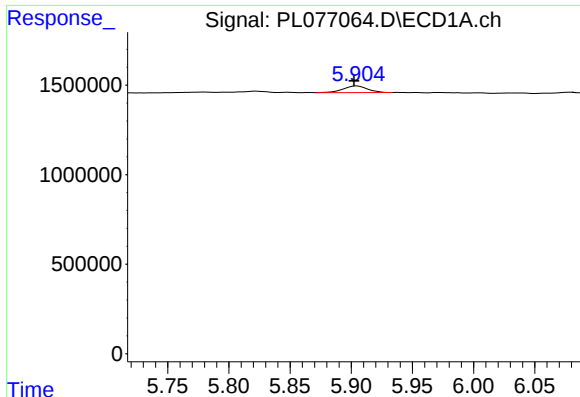

#26 Chlordane-4


R.T.: 5.905 min
Delta R.T.: 0.003 min
Response: 513856
Conc: 2.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

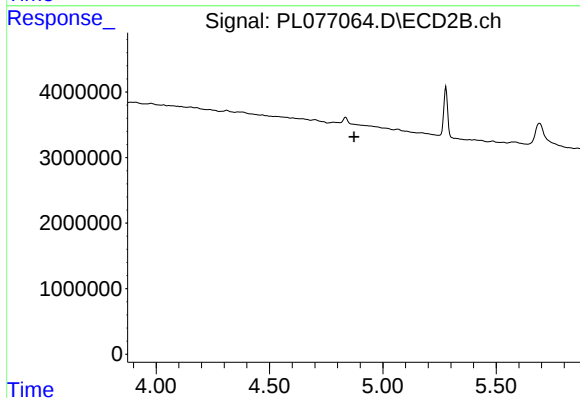


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.873 min
Response: 0
Conc: N.D.

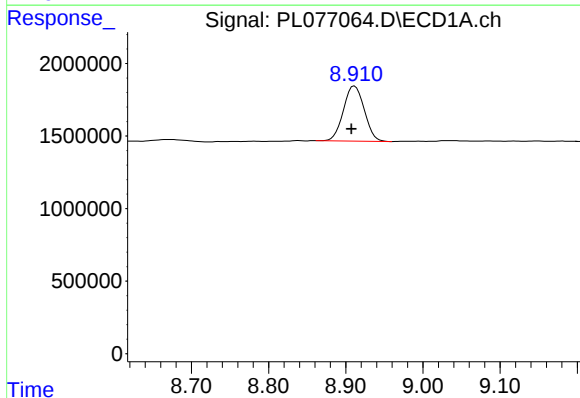

#28 Decachlorobiphenyl

R.T.: 8.911 min
Delta R.T.: 0.004 min
Response: 7131987
Conc: 9.45 ng/ml

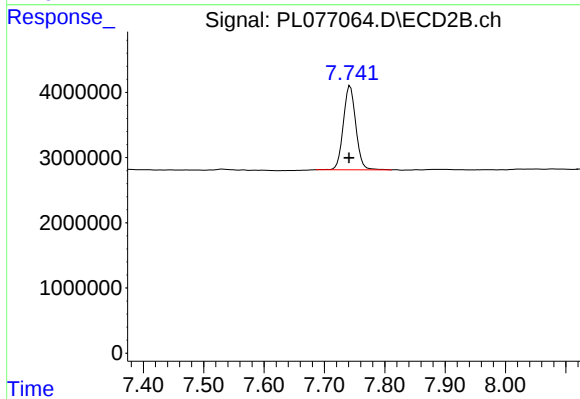

#28 Decachlorobiphenyl

R.T.: 7.743 min
Delta R.T.: 0.002 min
Response: 18495326
Conc: 8.22 ng/ml