

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
 Data File : PL077079.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 21:28
 Operator : AR\AJ
 Sample : N4154-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 22:31:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.419	2.636	13882275	38033064	14.158	13.286
28)	SA Decachlor...	8.907	7.739	10389073	27613204	13.761	12.266
Target Compounds							
2)	A alpha-BHC	0.000	3.118	0	297701	N.D.	0.070 #
11)	B alpha-Chl...	0.000	4.879	0	459299	N.D.	0.154 #
13)	MA Dieldrin	6.234	0.000	128501	0	0.132	N.D. #
15)	B Endosulfa...	6.710f	0.000	260891	0	0.304	N.D. #
26)	Chlordane-4	0.000	4.879	0	459299	N.D.	1.395 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
Data File : PL077079.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 21:28
Operator : AR\AJ
Sample : N4154-03
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 22:31:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

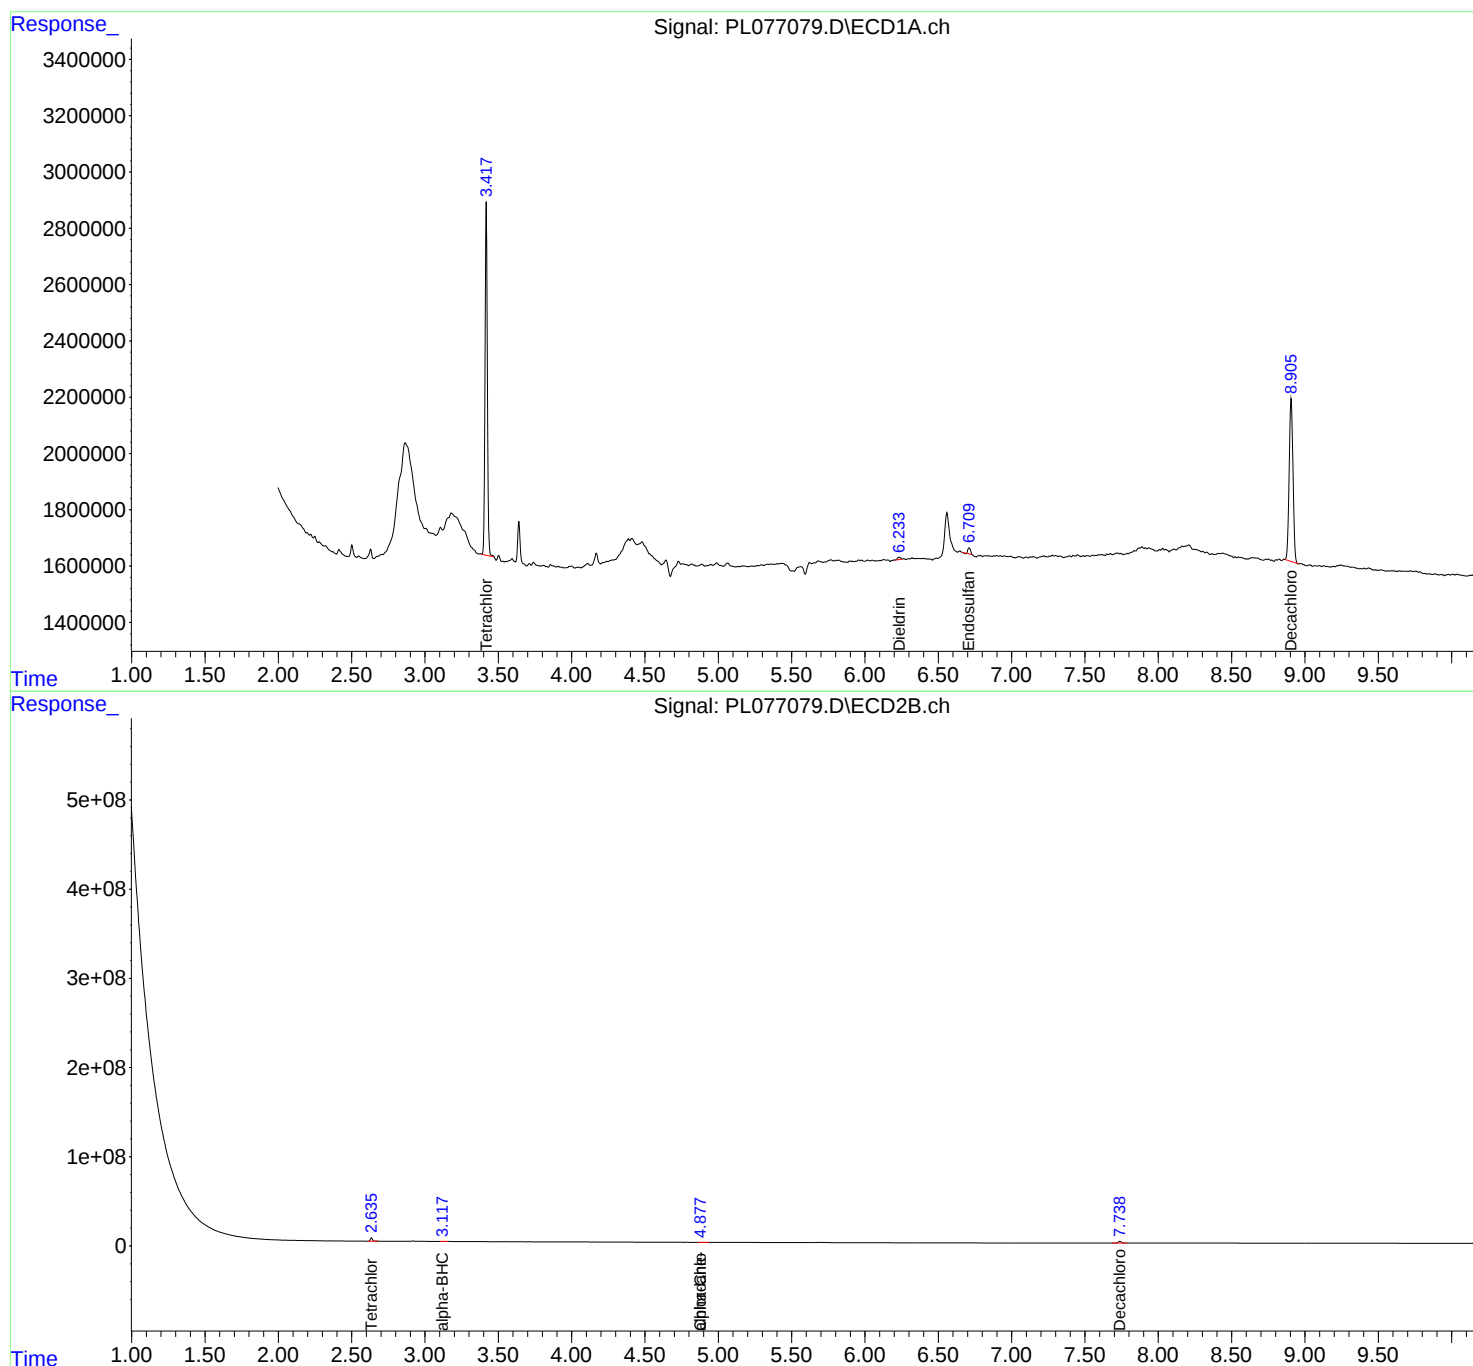


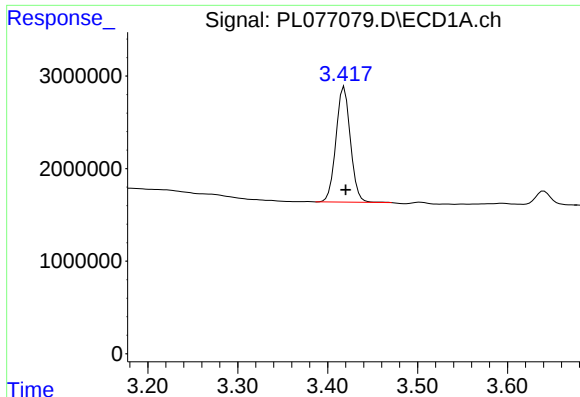

#1 Tetrachloro-m-xylene


R.T.: 3.419 min
Delta R.T.: -0.001 min
Response: 13882275
Conc: 14.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

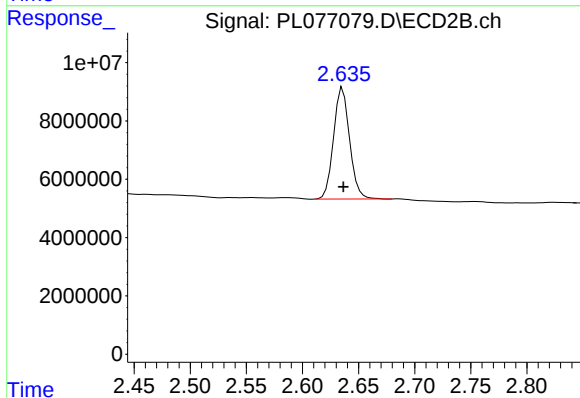


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 38033064
Conc: 13.29 ng/ml

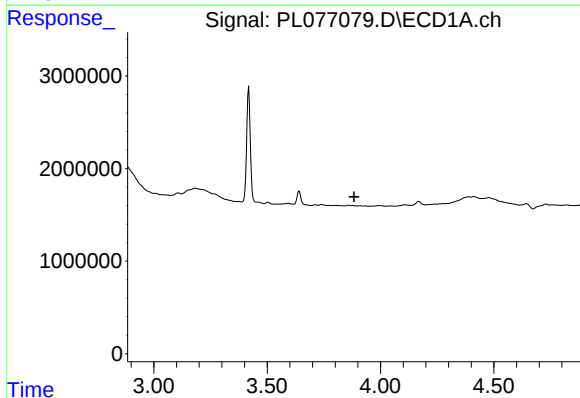


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.884 min
Response: 0
Conc: N.D.

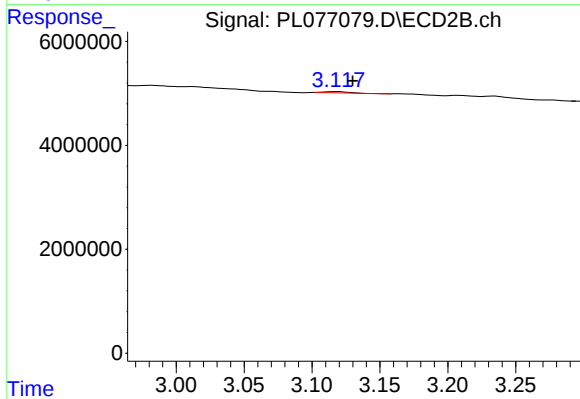

#2 alpha-BHC


R.T.: 3.118 min
Delta R.T.: -0.012 min
Response: 297701
Conc: 0.07 ng/ml

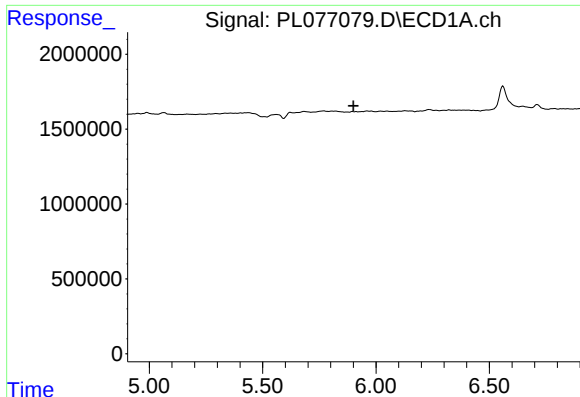

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

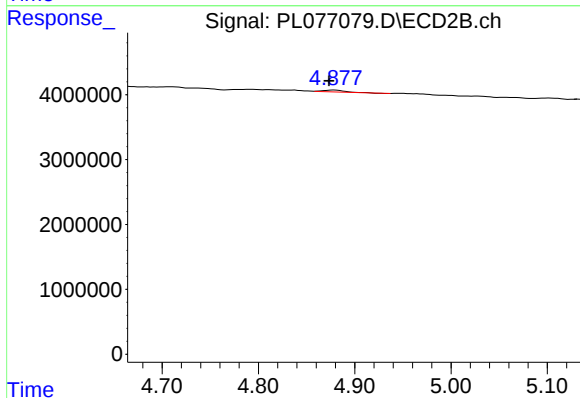


#11 alpha-Chlordane

R.T.: 4.879 min
Delta R.T.: 0.005 min
Response: 459299
Conc: 0.15 ng/ml

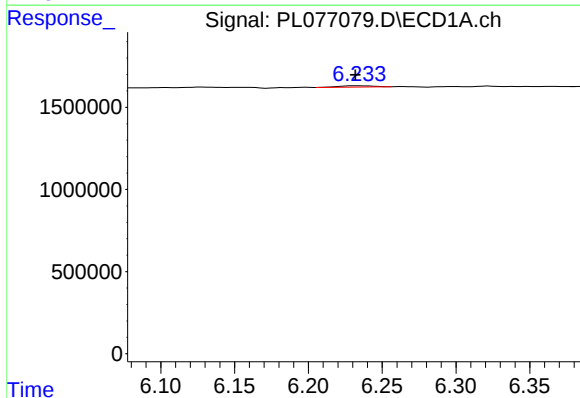


#13 Dieldrin

R.T.: 6.234 min
Delta R.T.: 0.002 min
Response: 128501
Conc: 0.13 ng/ml

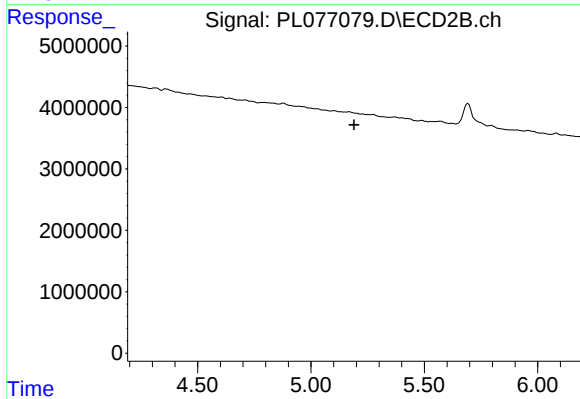

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.190 min
Response: 0
Conc: N.D.

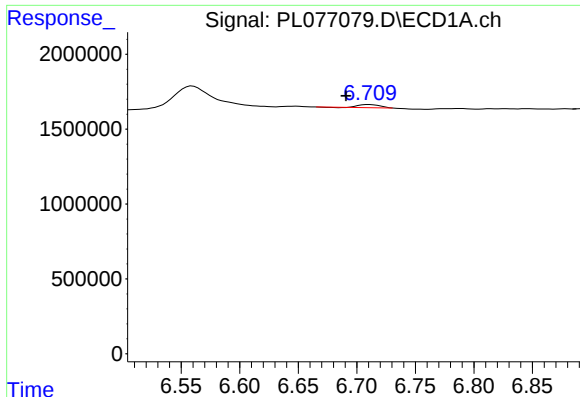

#15 Endosulfan II


R.T.: 6.710 min
Delta R.T.: 0.020 min
Response: 260891
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

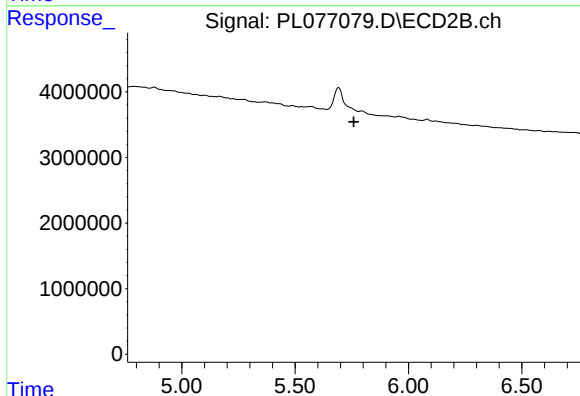


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.759 min
Response: 0
Conc: N.D.

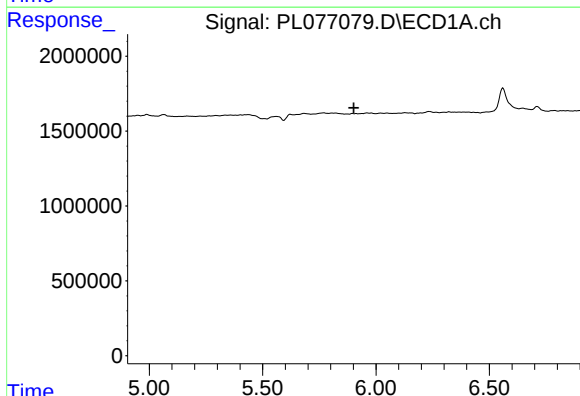


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.902 min
Response: 0
Conc: N.D.

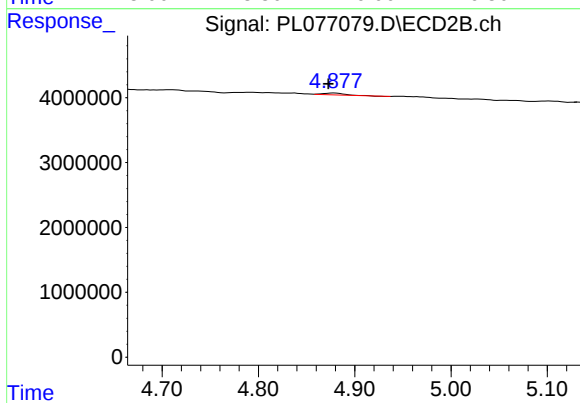

#26 Chlordane-4


R.T.: 4.879 min
Delta R.T.: 0.006 min
Response: 459299
Conc: 1.39 ng/ml

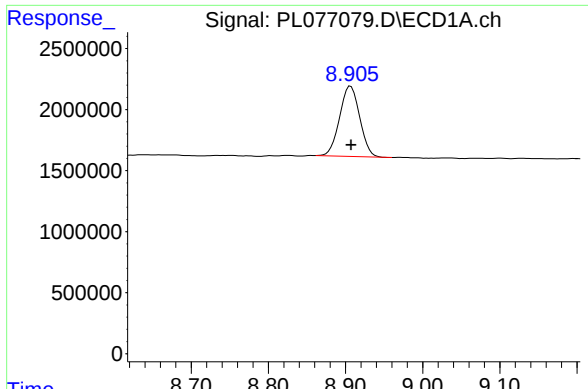

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 10389073
Conc: 13.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

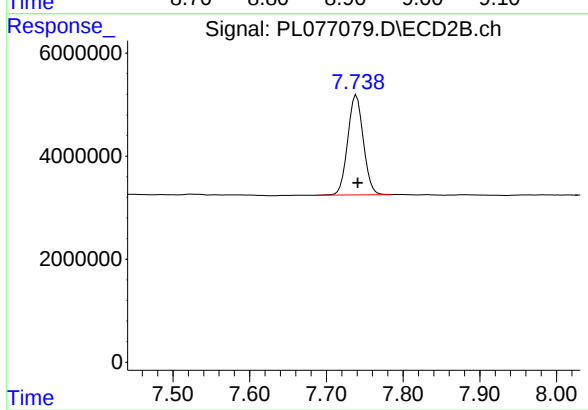

#28 Decachlorobiphenyl

R.T.: 7.739 min
Delta R.T.: -0.002 min
Response: 27613204
Conc: 12.27 ng/ml