

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
 Data File : PL077056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 16:09
 Operator : AR\AJ
 Sample : N4140-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 22:25:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	2.637	7007791	19352934	7.147	6.761
28)	SA Decachlor...	8.913	7.744	6759988	16972592	8.954	7.539
Target Compounds							
12)	B 4,4'-DDE	6.082	5.069	21860207	64643090	25.053	22.404
16)	A 4,4'-DDD	6.606	5.621	4004659	8161886	5.257	3.622 #
17)	MA 4,4'-DDT	6.917	5.867	1728302	4711107	2.249	2.078



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
Data File : PL077056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 16:09
Operator : AR\AJ
Sample : N4140-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 22:25:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

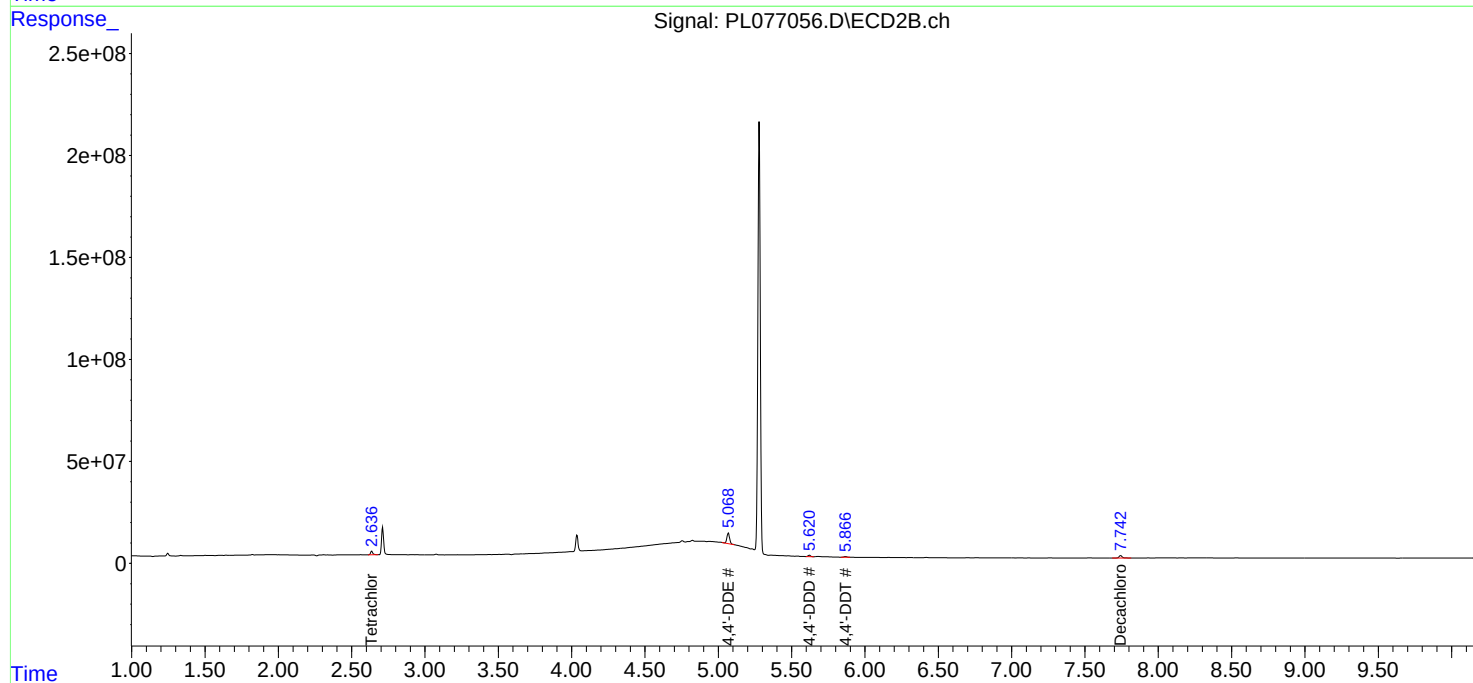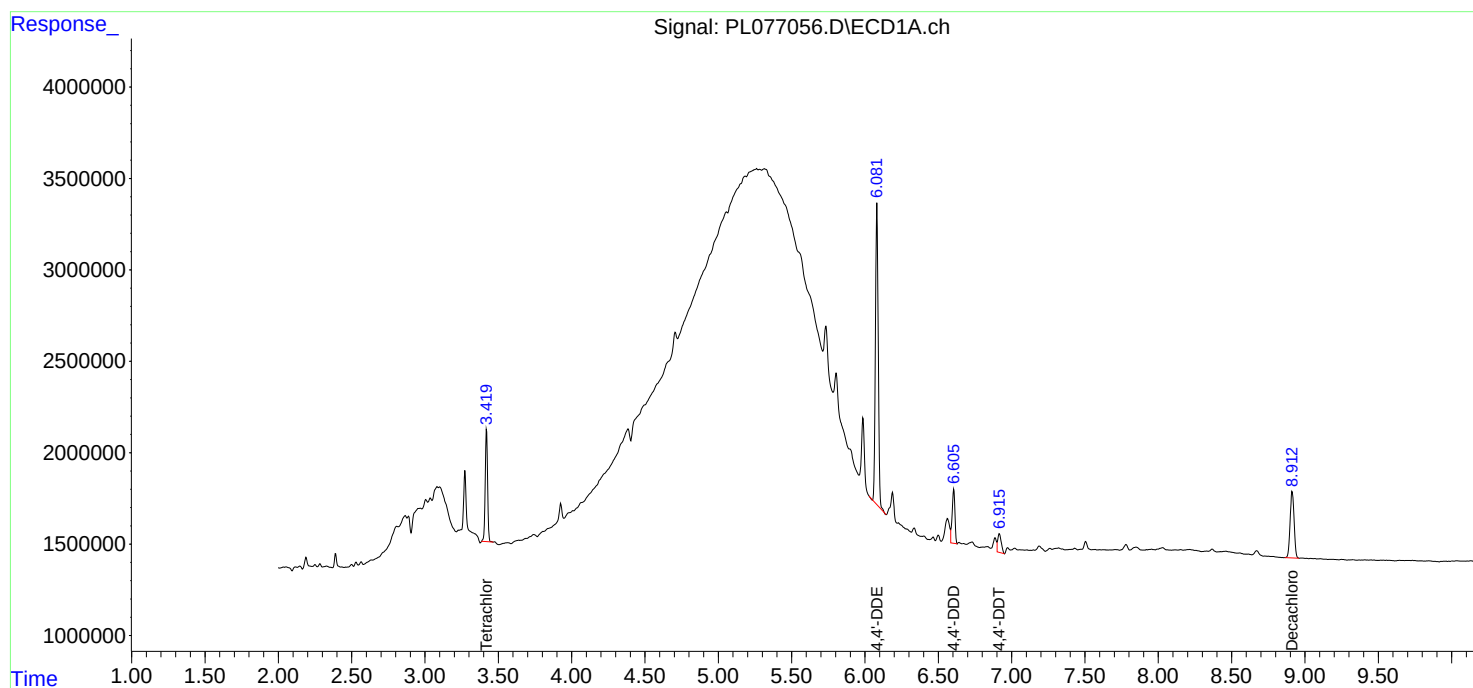


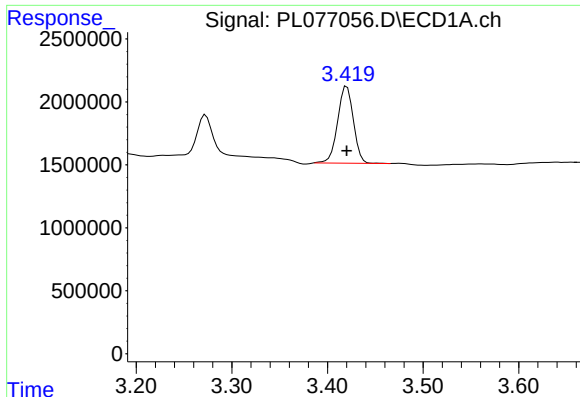

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 7007791
Conc: 7.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

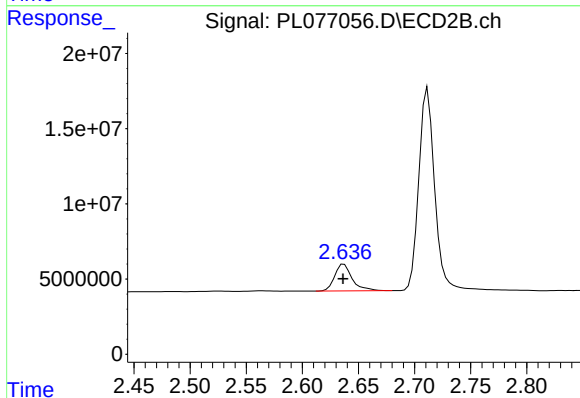


#1 Tetrachloro-m-xylene

R.T.: 2.637 min
Delta R.T.: 0.000 min
Response: 19352934
Conc: 6.76 ng/ml

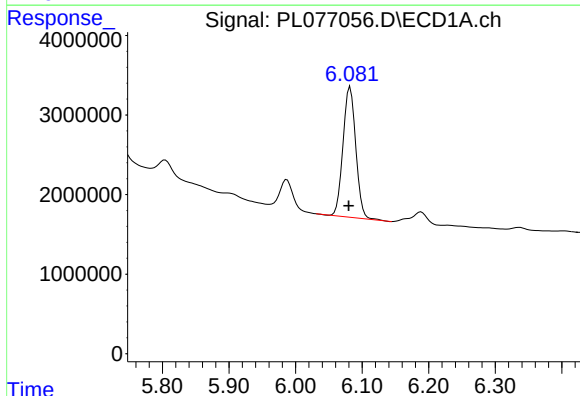


#12 4,4'-DDE

R.T.: 6.082 min
Delta R.T.: 0.002 min
Response: 21860207
Conc: 25.05 ng/ml

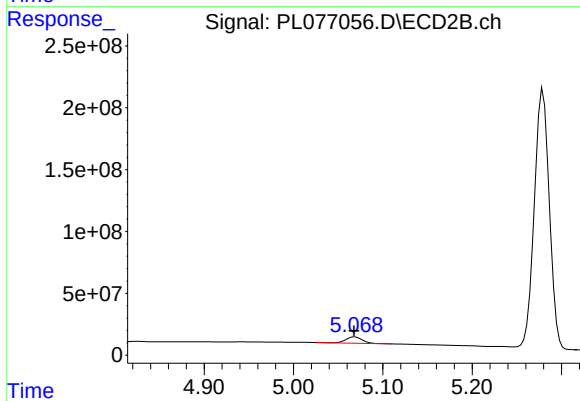

#12 4,4'-DDE


R.T.: 5.069 min
Delta R.T.: 0.001 min
Response: 64643090
Conc: 22.40 ng/ml

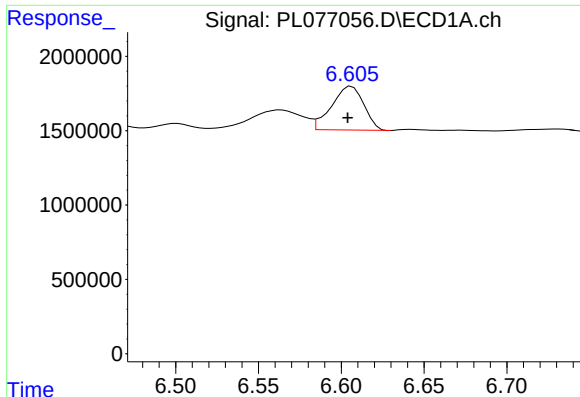

#16 4,4'-DDD


R.T.: 6.606 min
Delta R.T.: 0.002 min
Response: 4004659
Conc: 5.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

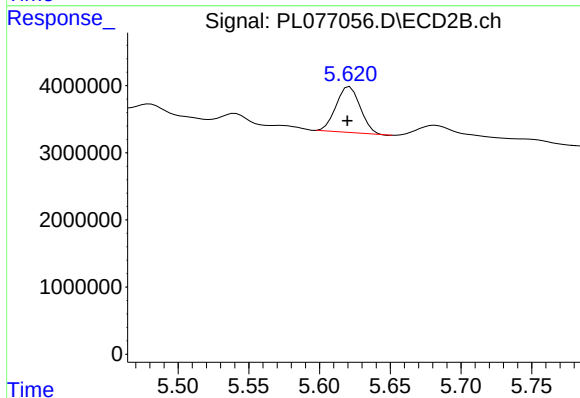


#16 4,4'-DDD

R.T.: 5.621 min
Delta R.T.: 0.002 min
Response: 8161886
Conc: 3.62 ng/ml

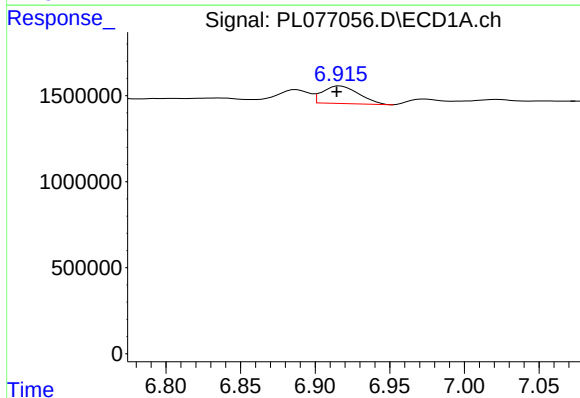


#17 4,4'-DDT

R.T.: 6.917 min
Delta R.T.: 0.002 min
Response: 1728302
Conc: 2.25 ng/ml

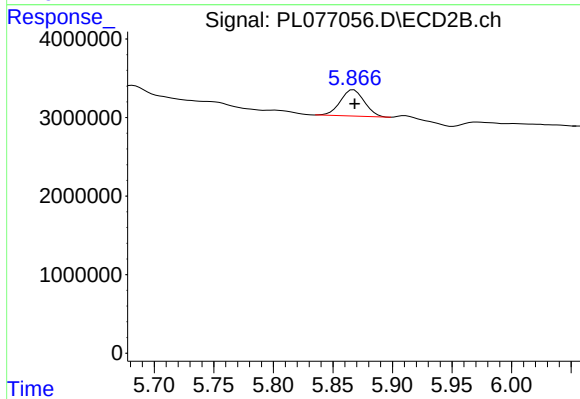

#17 4,4'-DDT


R.T.: 5.867 min
Delta R.T.: -0.001 min
Response: 4711107
Conc: 2.08 ng/ml

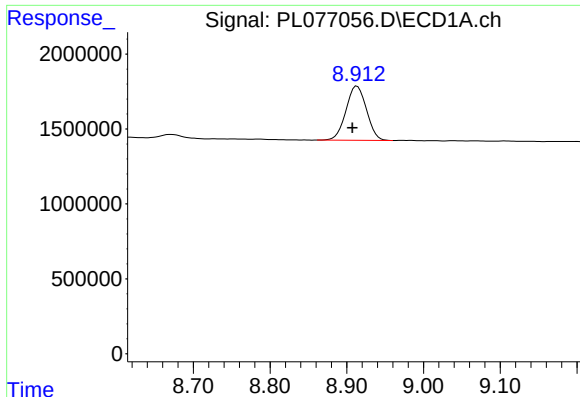

#28 Decachlorobiphenyl

R.T.: 8.913 min
Delta R.T.: 0.006 min
Response: 6759988
Conc: 8.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

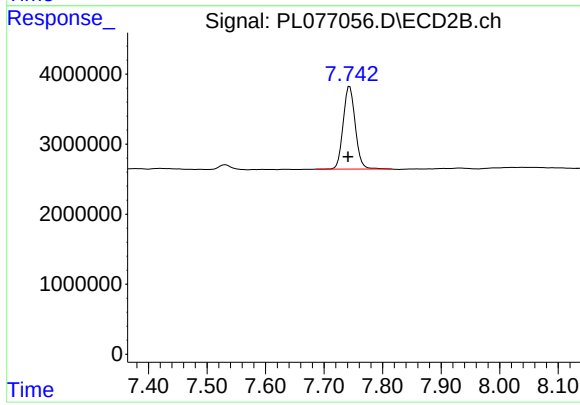

#28 Decachlorobiphenyl

R.T.: 7.744 min
Delta R.T.: 0.003 min
Response: 16972592
Conc: 7.54 ng/ml