

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
 Data File : PL077072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 19:51
 Operator : AR\AJ
 Sample : N4140-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 22:30:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 09 09:13:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.418	2.636	6987278	20795830	7.126	7.265
28)	SA Decachlor...	8.907	7.740	6579913	17259294	8.716	7.667
Target Compounds							
12)	B 4,4'-DDE	6.078	5.066	22142953	63992593	25.377	22.179
16)	A 4,4'-DDD	6.602	5.618	4188797	8921799	5.498	3.959 #
17)	MA 4,4'-DDT	6.915	5.865	1857353	5168531	2.417	2.280



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081222\
Data File : PL077072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 19:51
Operator : AR\AJ
Sample : N4140-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 22:30:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080822.M
Quant Title : GC Extractables
QLast Update : Tue Aug 09 09:13:15 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

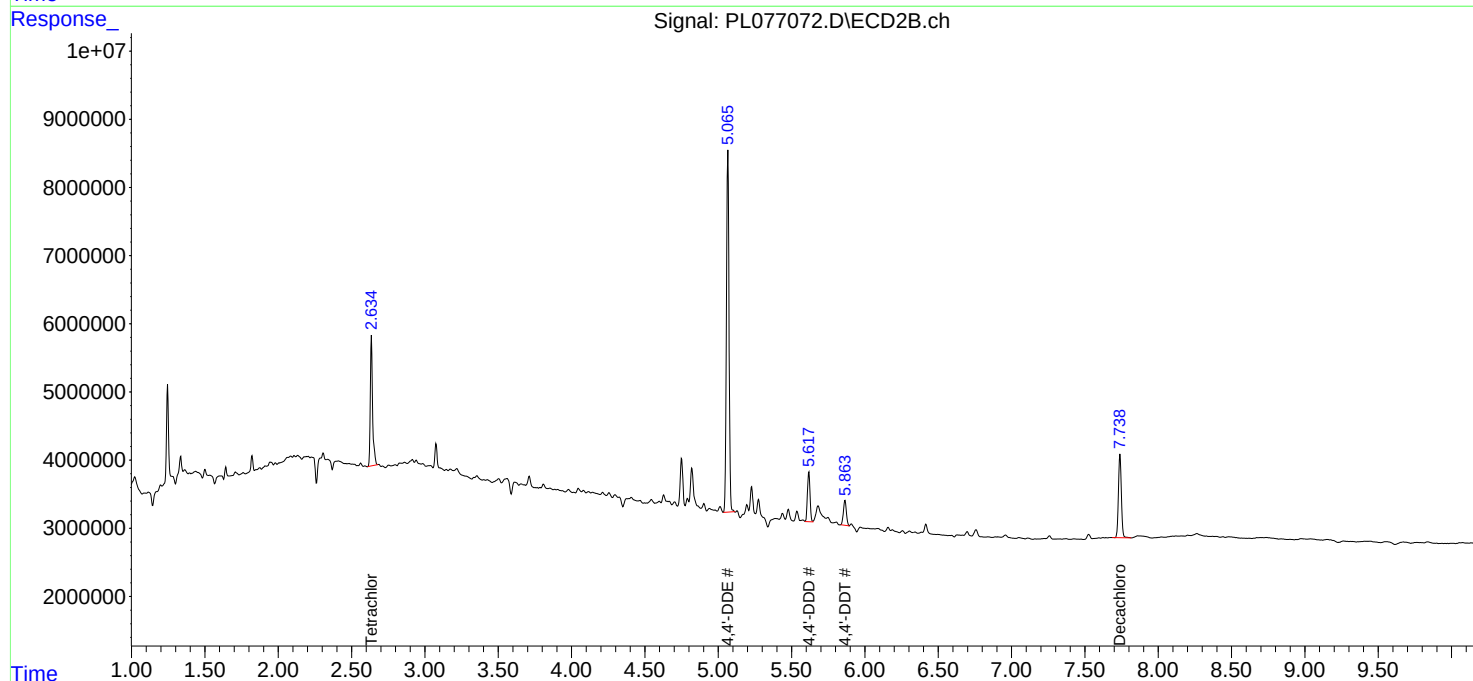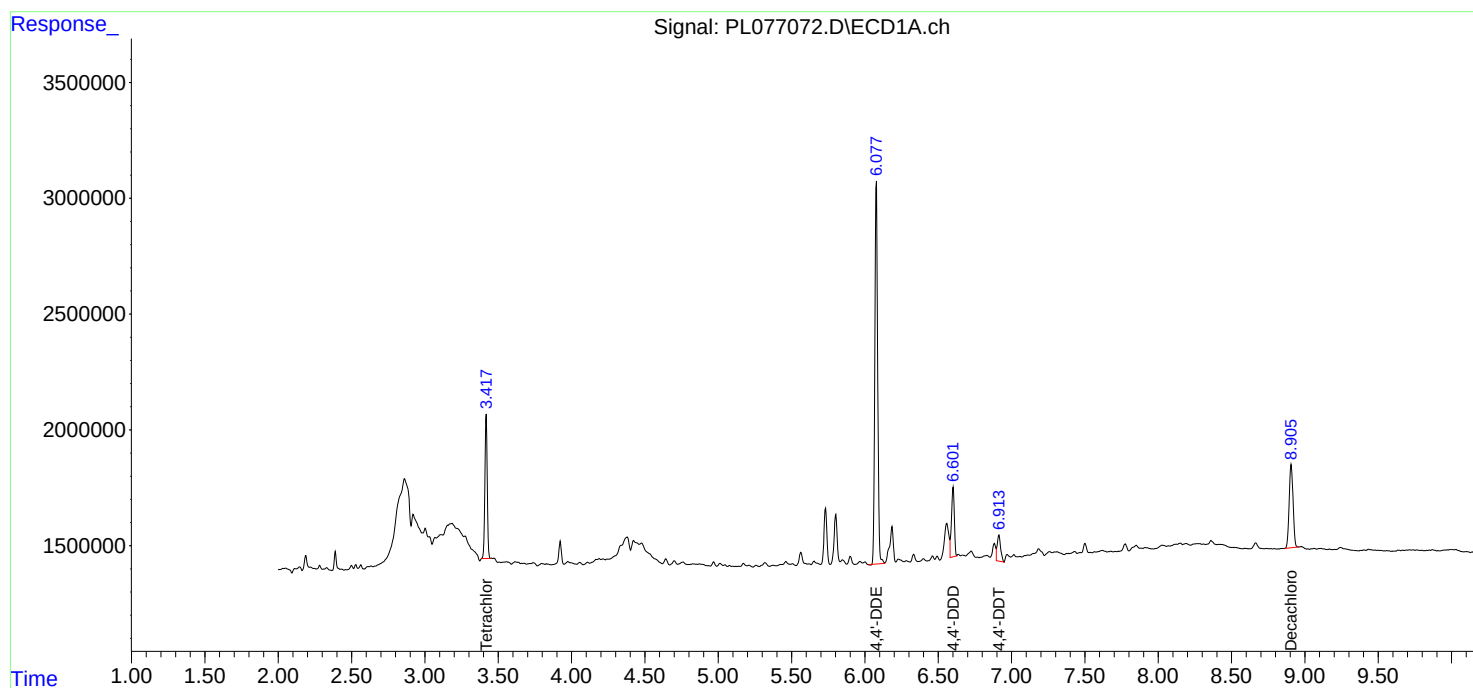


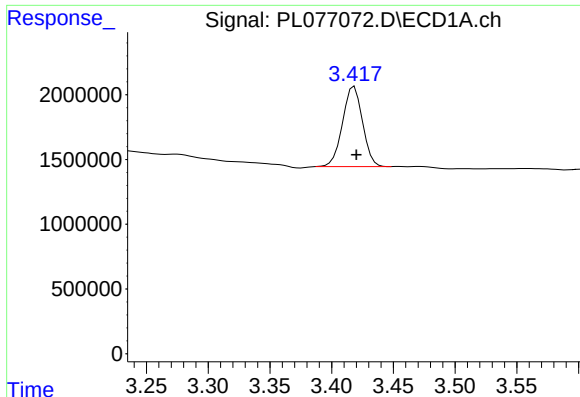

#1 Tetrachloro-m-xylene


R.T.: 3.418 min
Delta R.T.: -0.002 min
Response: 6987278
Conc: 7.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

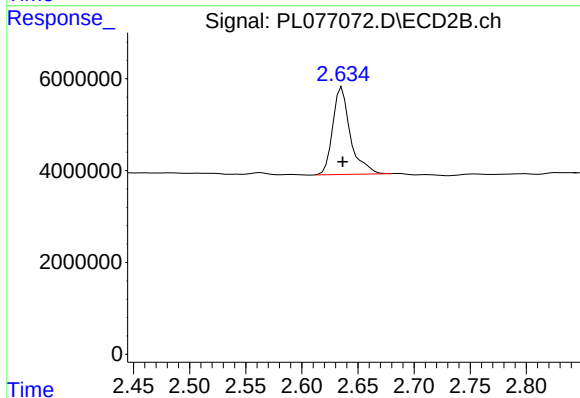


#1 Tetrachloro-m-xylene

R.T.: 2.636 min
Delta R.T.: 0.000 min
Response: 20795830
Conc: 7.26 ng/ml

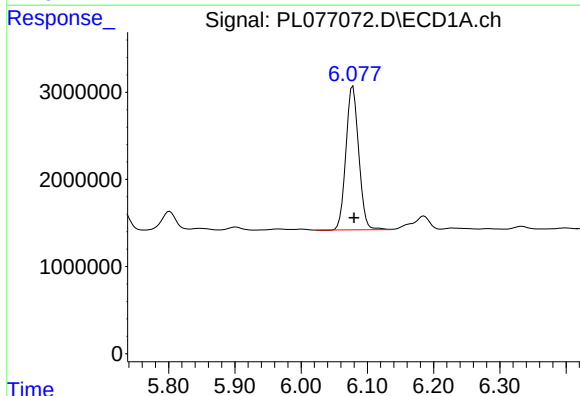


#12 4,4'-DDE

R.T.: 6.078 min
Delta R.T.: -0.002 min
Response: 22142953
Conc: 25.38 ng/ml

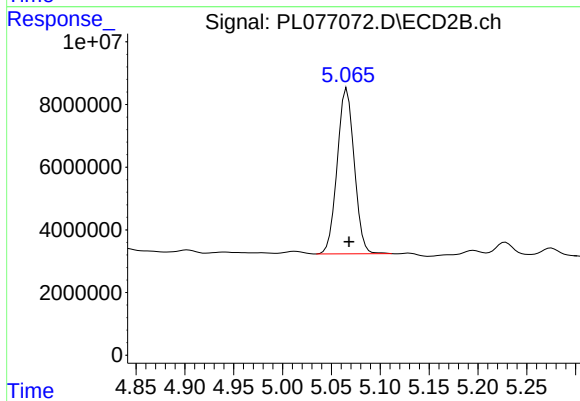

#12 4,4'-DDE


R.T.: 5.066 min
Delta R.T.: -0.002 min
Response: 63992593
Conc: 22.18 ng/ml

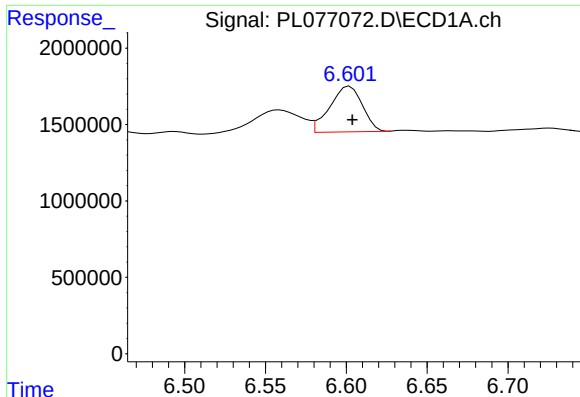

#16 4,4'-DDD


R.T.: 6.602 min
Delta R.T.: -0.002 min
Response: 4188797
Conc: 5.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

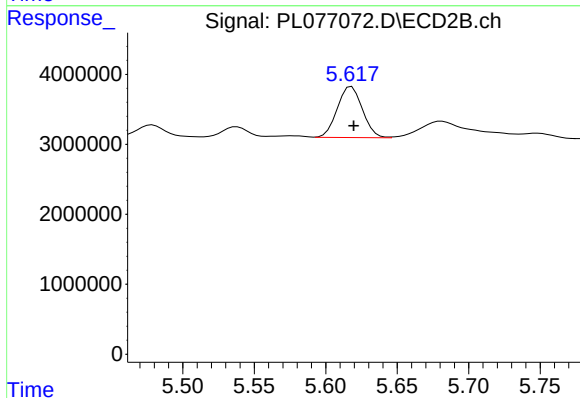


#16 4,4'-DDD

R.T.: 5.618 min
Delta R.T.: -0.002 min
Response: 8921799
Conc: 3.96 ng/ml

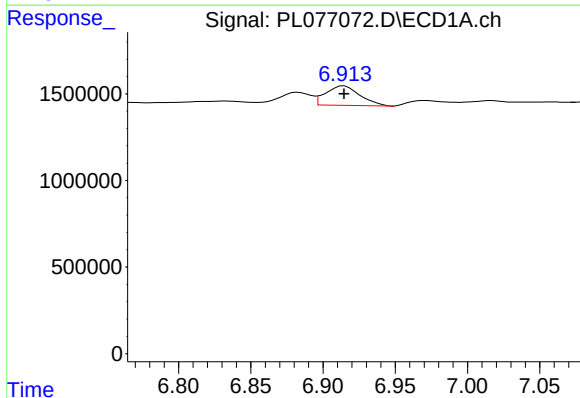


#17 4,4'-DDT

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 1857353
Conc: 2.42 ng/ml

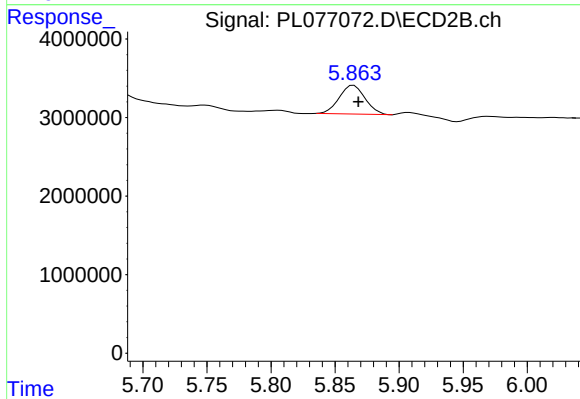

#17 4,4'-DDT


R.T.: 5.865 min
Delta R.T.: -0.004 min
Response: 5168531
Conc: 2.28 ng/ml

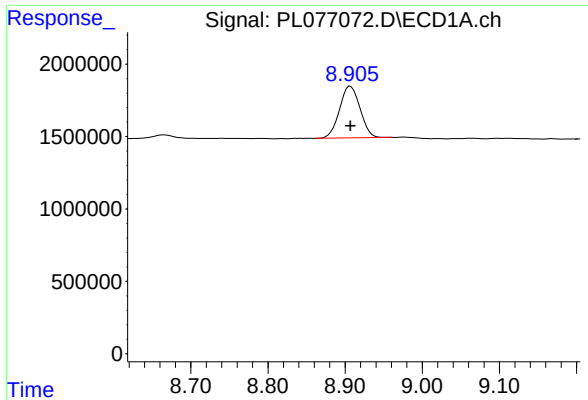

#28 Decachlorobiphenyl

R.T.: 8.907 min
Delta R.T.: 0.000 min
Response: 6579913
Conc: 8.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
LINDEN-MR-B1B-SP

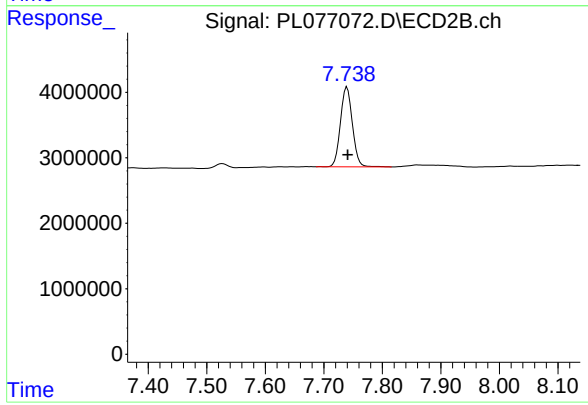

#28 Decachlorobiphenyl

R.T.: 7.740 min
Delta R.T.: -0.001 min
Response: 17259294
Conc: 7.67 ng/ml