

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081224\
 Data File : PL090988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 11:33
 Operator : AR\AJ
 Sample : P3476-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MUL06

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/13/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:11:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 06 10:55:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.544	2.770	20428689	439.1E6	10.551m	254.000m#
28) SA Decachlor...	9.064	7.929	17683743	17396012	12.308m	10.422m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081224\
Data File : PL090988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 11:33
Operator : AR\AJ
Sample : P3476-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
MUL06


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/13/2024
Supervised By : Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:11:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL080524.M
Quant Title : GC Extractables
QLast Update : Tue Aug 06 10:55:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

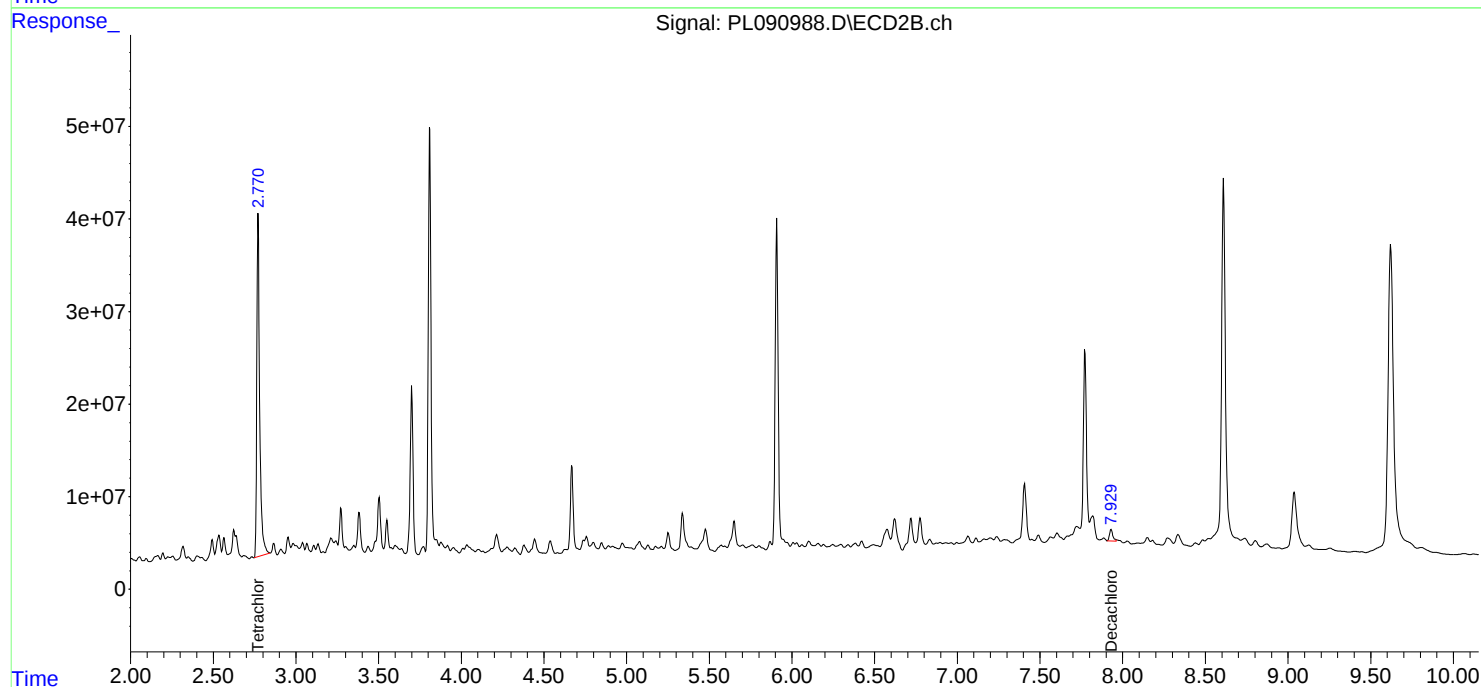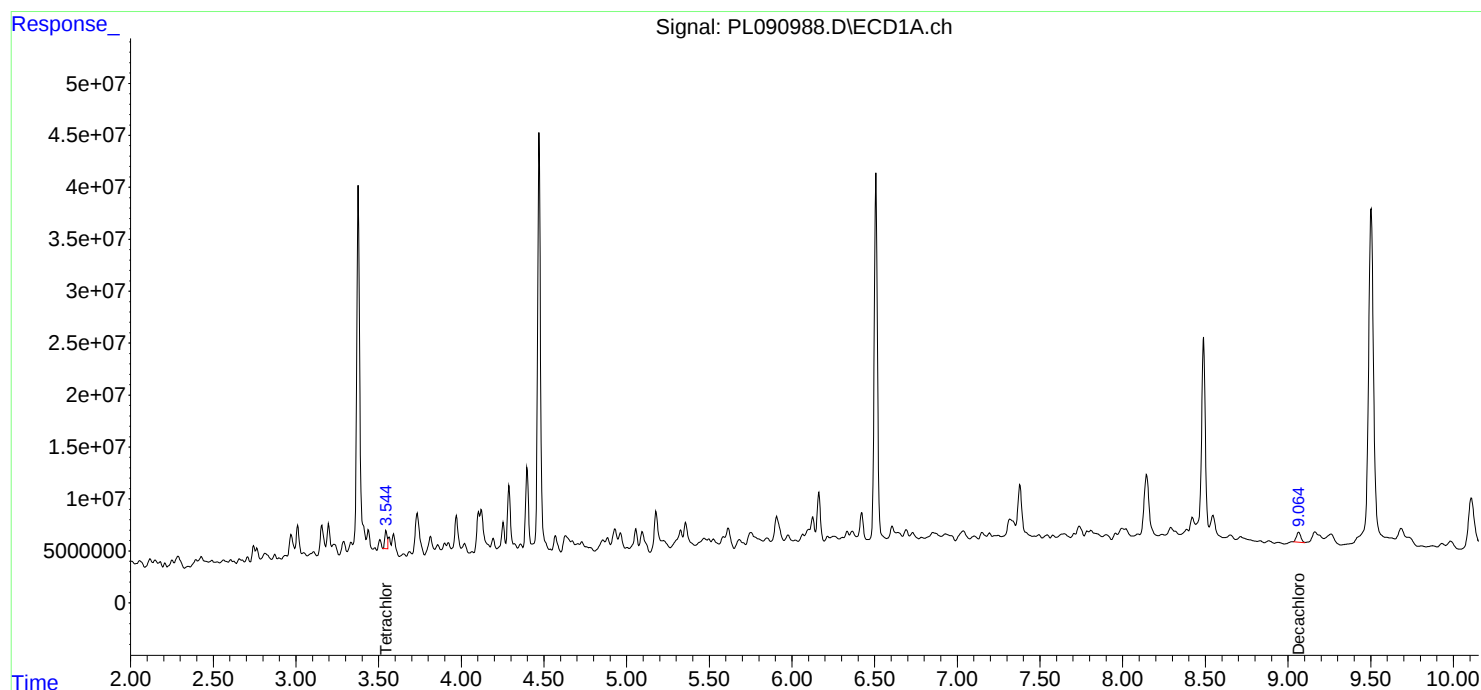

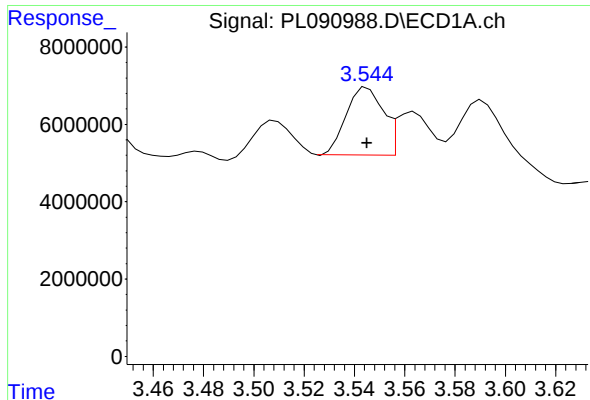


#1 Tetrachloro-m-xylene

R.T.: 3.544 min
Delta R.T.: -0.001 min
Response: 20428689
Conc: 10.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
MUL06


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/13/2024
Supervised By :Ankita Jodhani 08/14/2024

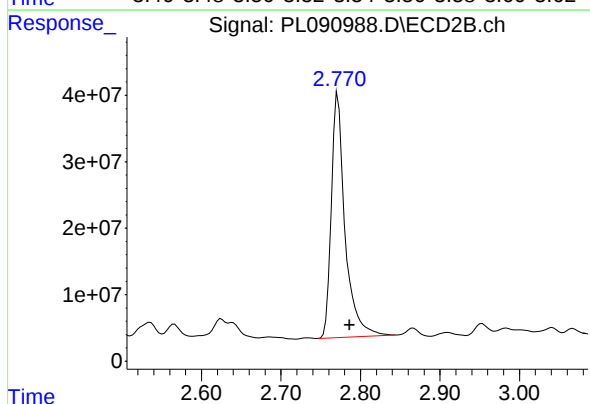


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.017 min
Response: 439117456
Conc: 254.00 ng/ml m

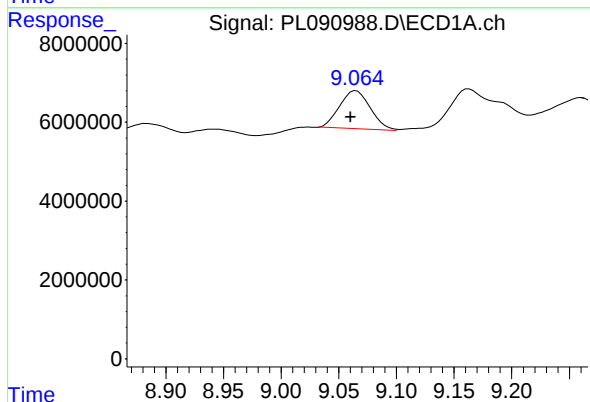

#28 Decachlorobiphenyl

R.T.: 9.064 min
Delta R.T.: 0.003 min
Response: 17683743
Conc: 12.31 ng/ml m

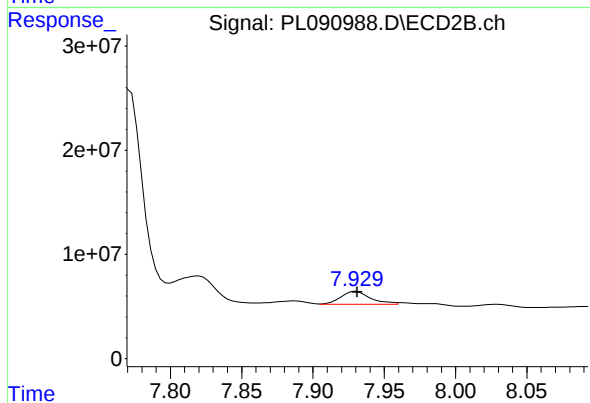

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: -0.002 min
Response: 17396012
Conc: 10.42 ng/ml m