

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
 Data File : PL096758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 19:25
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA3301

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:51:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 13 05:49:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.825	59923278	91505978	20.000	20.000
27)	SA Decachlor...	9.006	7.988	89536867	178.4E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.978	3.331	91591671	137.0E6	20.000	20.000
3)	MA gamma-BHC...	4.306	3.663	86742749	128.1E6	20.000	20.000
4)	MA Heptachlor	4.897	4.011	87040256	128.4E6	20.000	20.000
9)	A Endosulfan I	6.038	5.167	67489993	102.3E6	20.000	20.000
13)	MA Dieldrin	6.310	5.432	144.1E6	232.9E6	40.000	40.000
14)	MA Endrin	6.536	5.706	113.1E6	201.1E6	40.000	40.000
16)	A 4,4'-DDD	6.669	5.853	97923219	184.6E6	40.000	40.000
17)	MA 4,4'-DDT	6.983	6.106	94005749	182.3E6	40.000	40.000
20)	A Methoxychlor	7.456	6.678	259.5E6	497.7E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
Data File : PL096758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 19:25
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:51:35 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 13 05:49:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

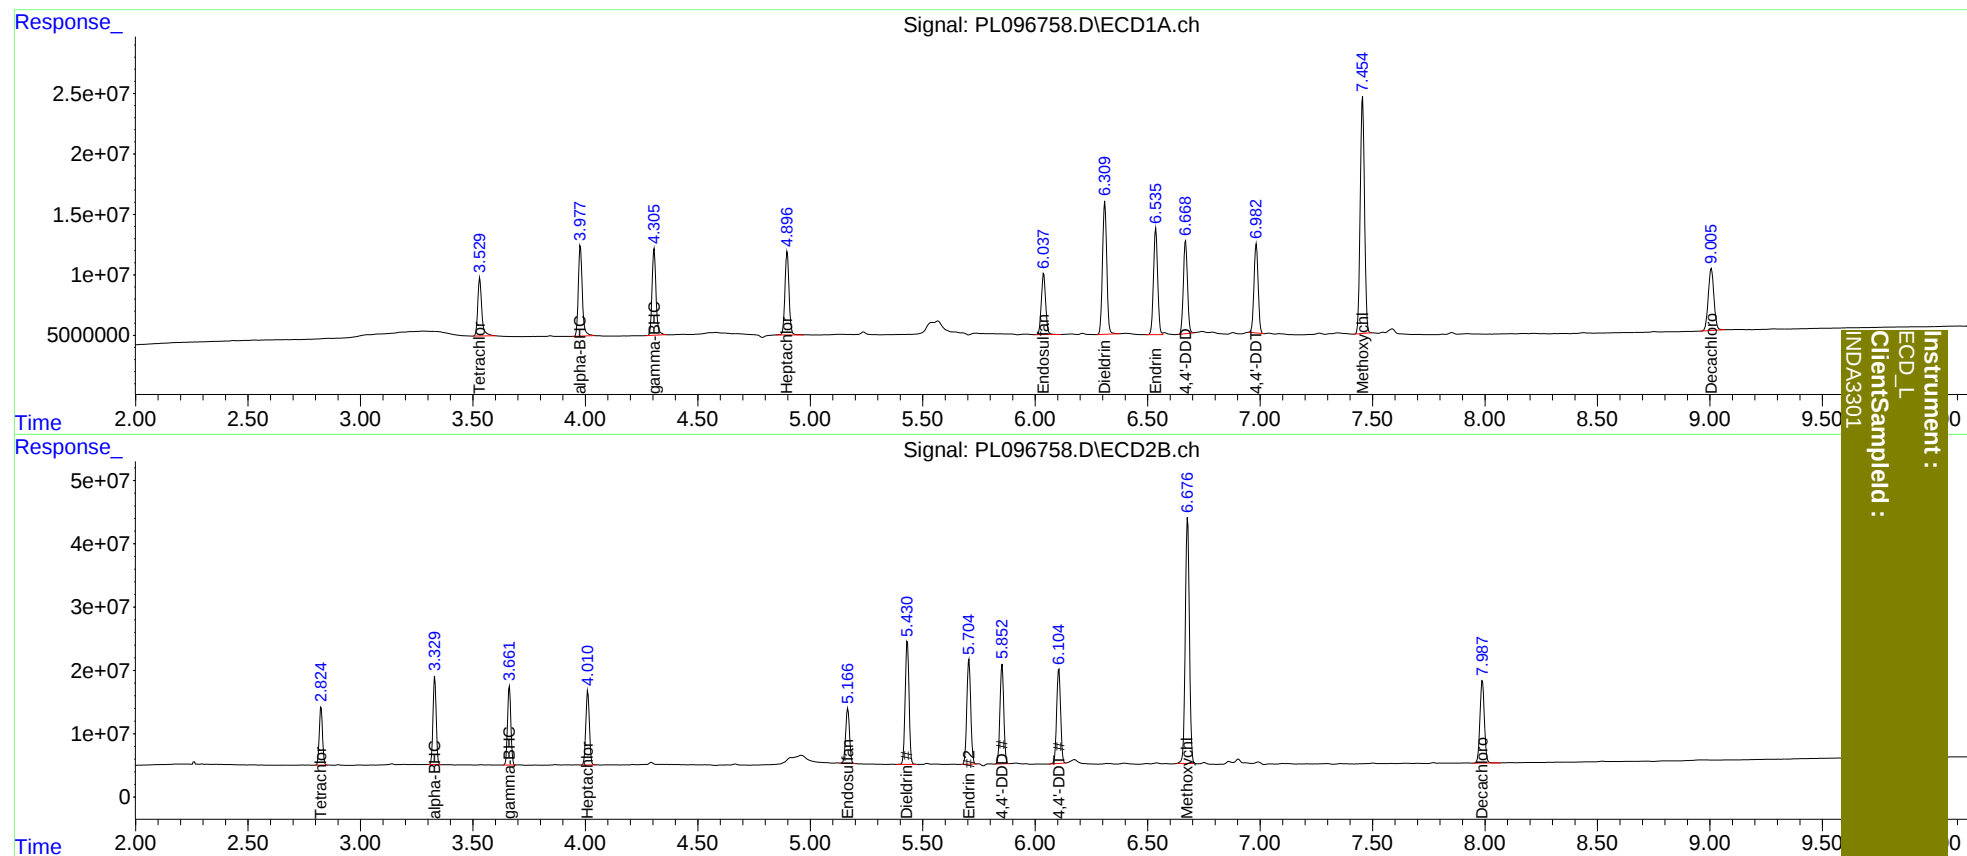


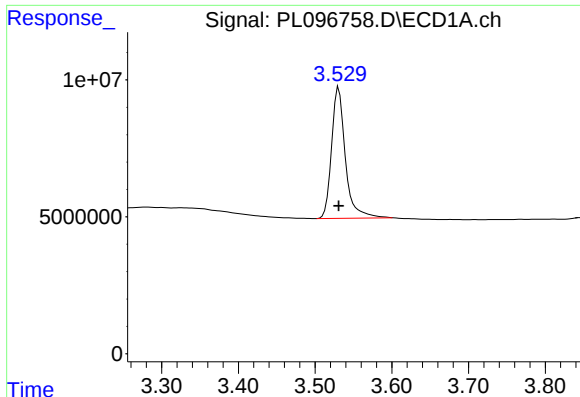

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 59923278
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

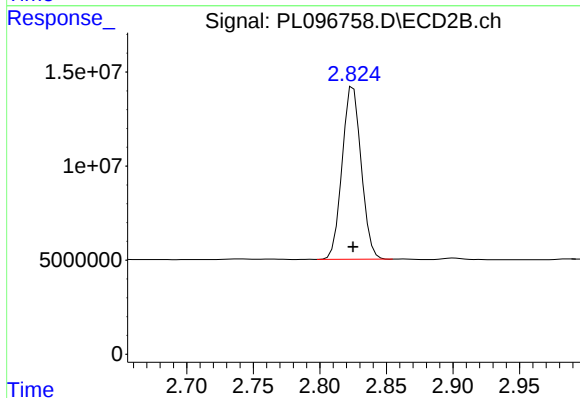


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.000 min
Response: 91505978
Conc: 20.00 ng/ml

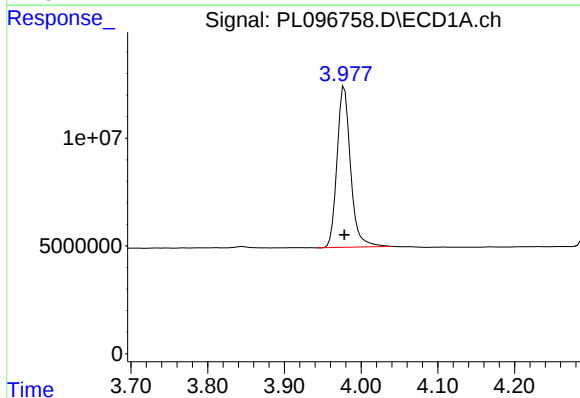


#2 alpha-BHC

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 91591671
Conc: 20.00 ng/ml

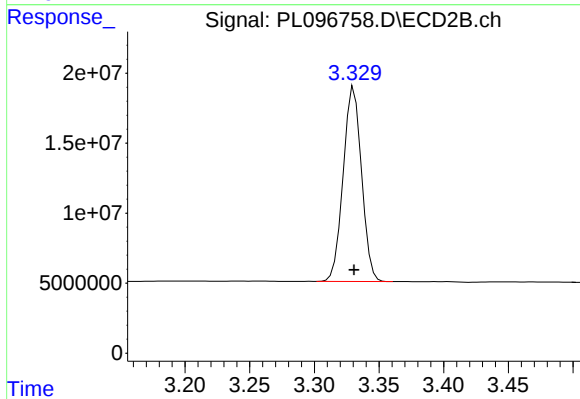

#2 alpha-BHC


R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 137000485
Conc: 20.00 ng/ml

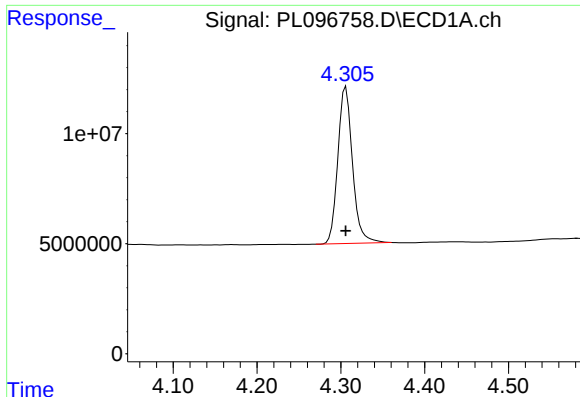

#3 gamma-BHC (Lindane)


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 86742749
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

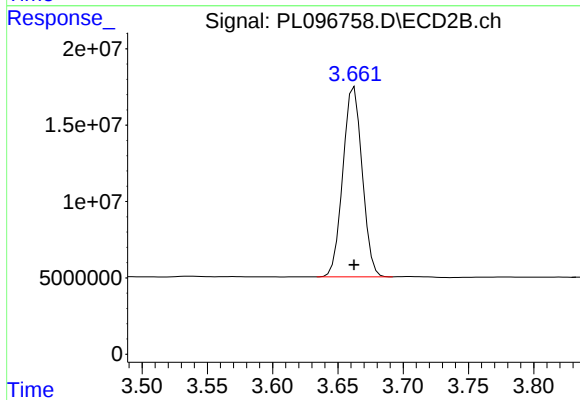


#3 gamma-BHC (Lindane)

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 128062529
Conc: 20.00 ng/ml

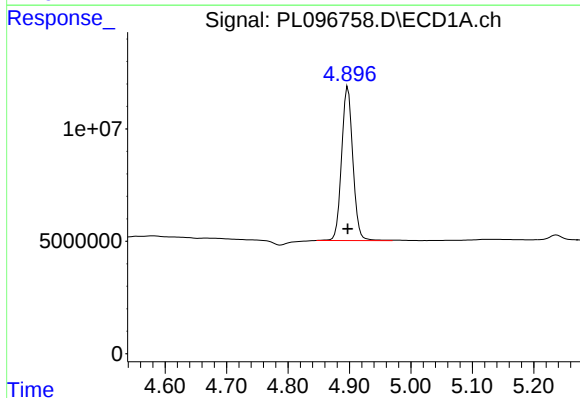


#4 Heptachlor

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 87040256
Conc: 20.00 ng/ml

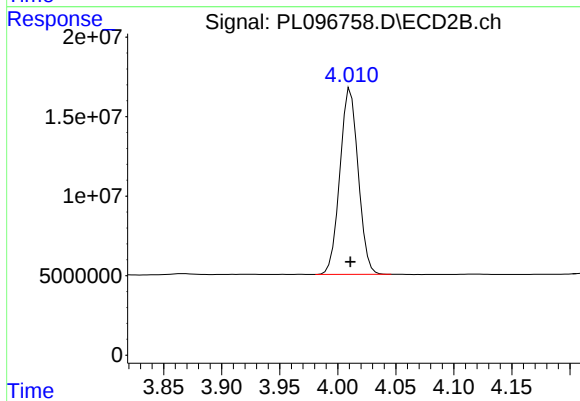

#4 Heptachlor


R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 128427195
Conc: 20.00 ng/ml

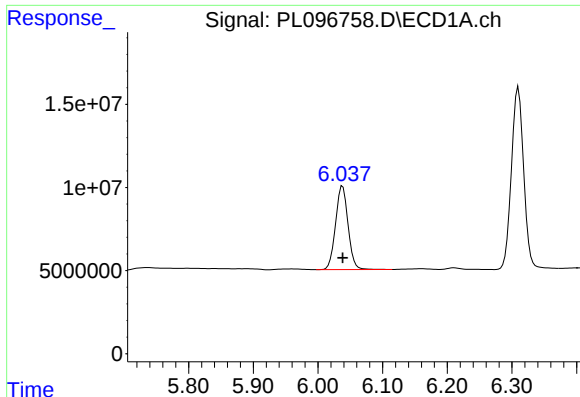

#9 Endosulfan I


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 67489993
Conc: 20.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

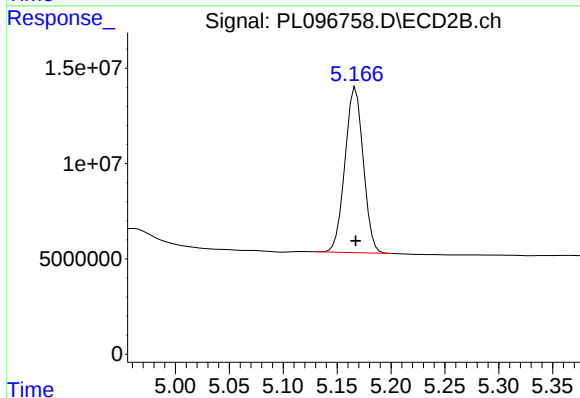


#9 Endosulfan I

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 102313248
Conc: 20.00 ng/ml

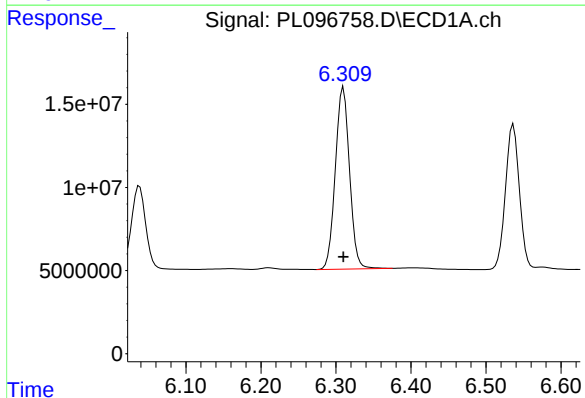


#13 Dieldrin

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 144079266
Conc: 40.00 ng/ml

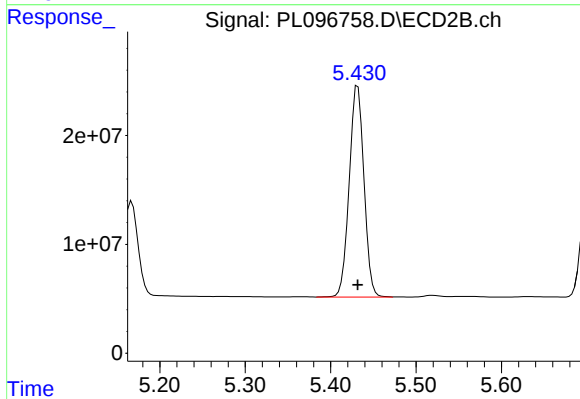

#13 Dieldrin


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 232871519
Conc: 40.00 ng/ml

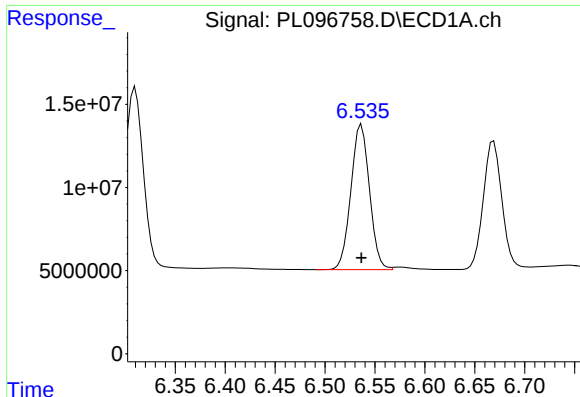

#14 Endrin


R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 113130053
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

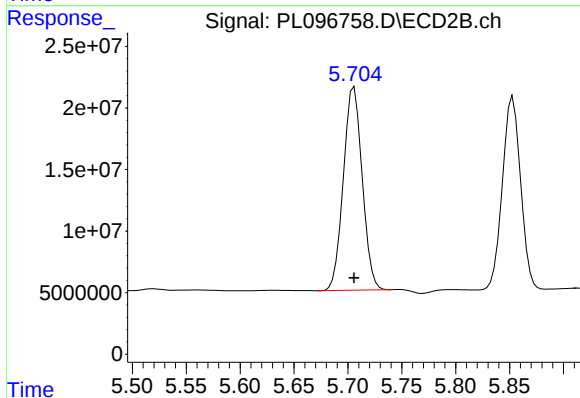


#14 Endrin

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 201057032
Conc: 40.00 ng/ml

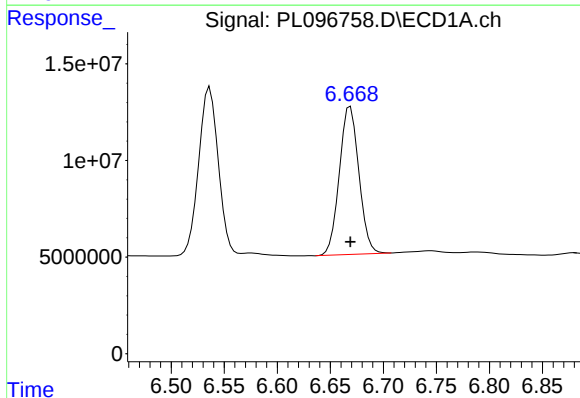


#16 4,4'-DDD

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 97923219
Conc: 40.00 ng/ml

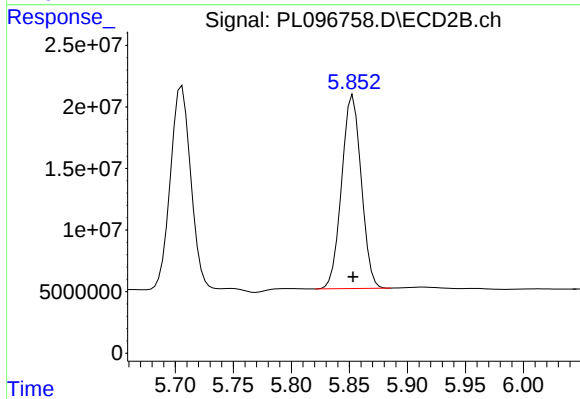

#16 4,4'-DDD


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 184626222
Conc: 40.00 ng/ml

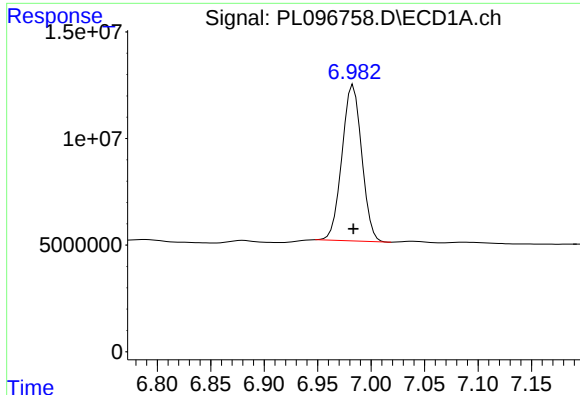

#17 4,4'-DDT


R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 94005749
Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

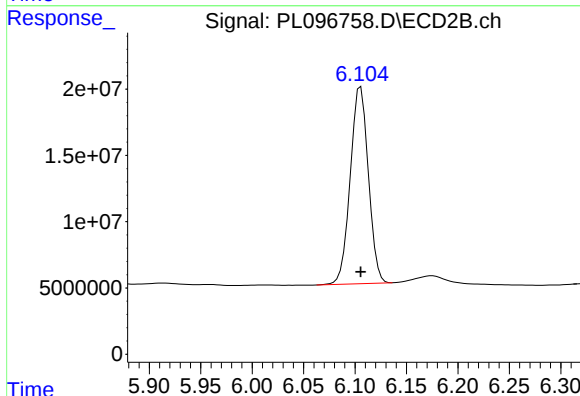


#17 4,4'-DDT

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 182341043
Conc: 40.00 ng/ml

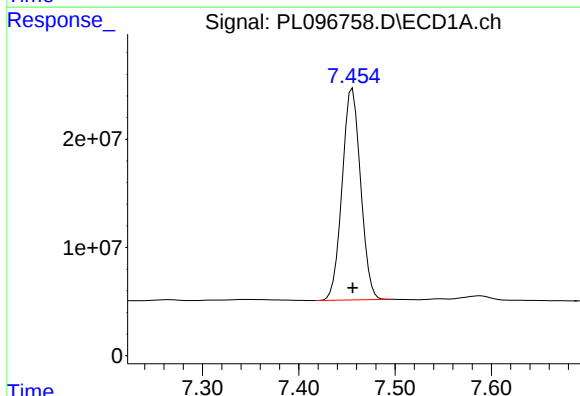


#20 Methoxychlor

R.T.: 7.456 min
Delta R.T.: 0.000 min
Response: 259455519
Conc: 200.00 ng/ml

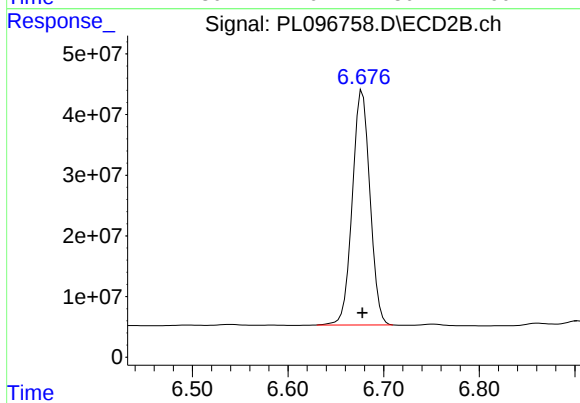

#20 Methoxychlor

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 497665621
Conc: 200.00 ng/ml

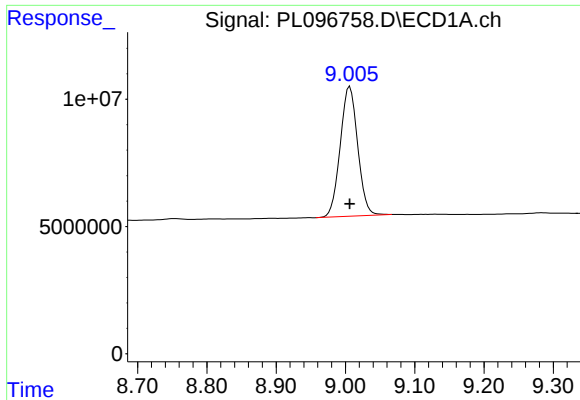

#27 Decachlorobiphenyl


R.T.: 9.006 min

Delta R.T.: 0.000 min

Response: 89536867

Conc: 40.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA3301

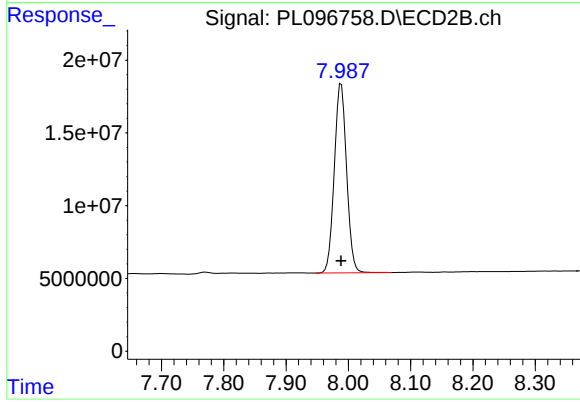

#27 Decachlorobiphenyl

R.T.: 7.988 min

Delta R.T.: 0.000 min

Response: 178424885

Conc: 40.00 ng/ml