

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
 Data File : PL096760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 19:52
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA4303

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:51:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 13 05:49:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.825	119.8E6	182.9E6	39.987	39.967
27)	SA Decachlor...	9.007	7.988	175.4E6	346.4E6	78.358	77.666
Target Compounds							
2)	A alpha-BHC	3.978	3.331	191.9E6	288.6E6	41.893	42.127
3)	MA gamma-BHC...	4.306	3.663	179.2E6	266.3E6	41.323	41.583
4)	MA Heptachlor	4.898	4.011	178.0E6	261.8E6	40.908	40.773
9)	A Endosulfan I	6.039	5.167	136.2E6	208.1E6	40.354	40.676
13)	MA Dieldrin	6.310	5.432	300.1E6	476.1E6	83.326	81.772
14)	MA Endrin	6.537	5.706	235.5E6	412.2E6	83.272	82.004
16)	A 4,4'-DDD	6.669	5.853	202.2E6	381.2E6	82.596	82.579
17)	MA 4,4'-DDT	6.984	6.106	197.9E6	379.8E6	84.220	83.312
20)	A Methoxychlor	7.456	6.678	525.0E6	949.2E6	404.666	381.465


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
Data File : PL096760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 19:52
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:51:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 13 05:49:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

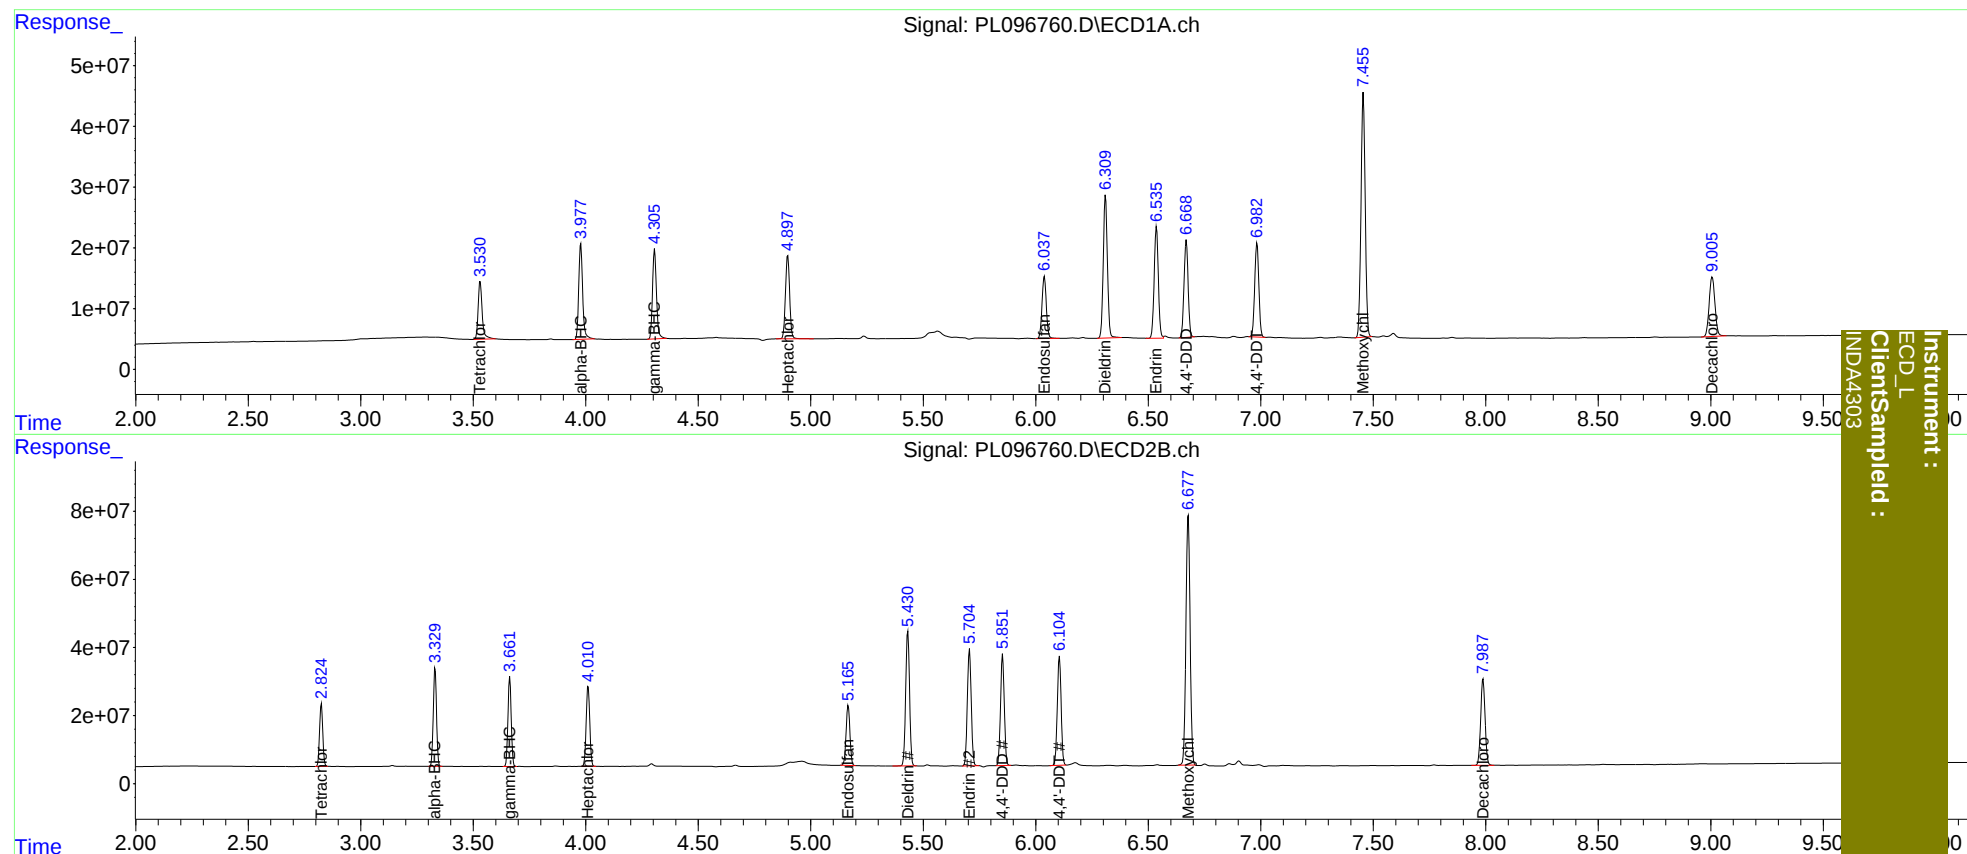


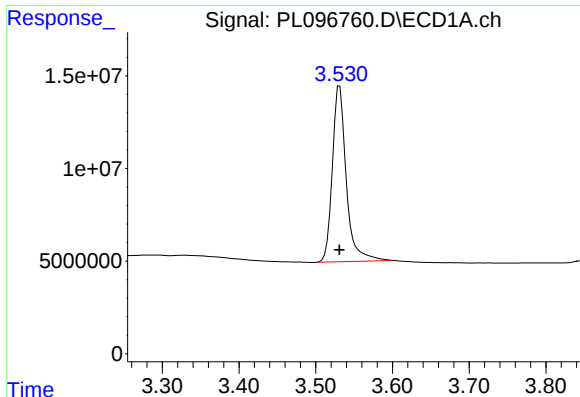

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 119807987
Conc: 39.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

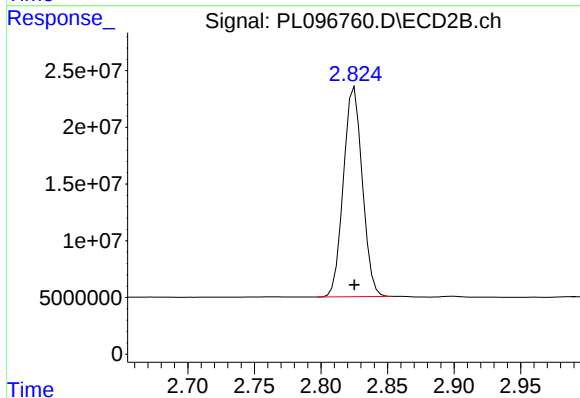


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.000 min
Response: 182859357
Conc: 39.97 ng/ml

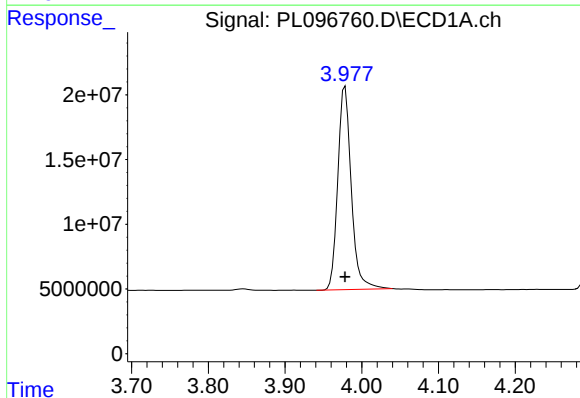


#2 alpha-BHC

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 191853421
Conc: 41.89 ng/ml

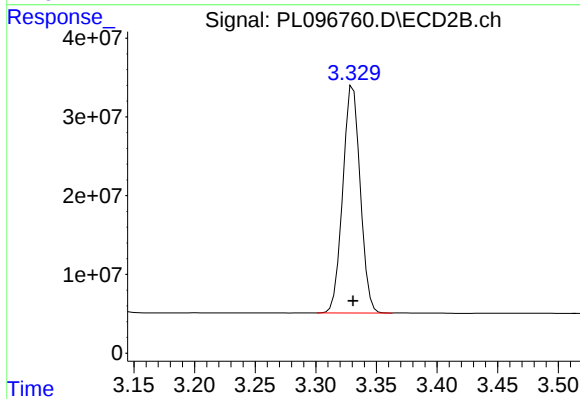

#2 alpha-BHC


R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 288571311
Conc: 42.13 ng/ml

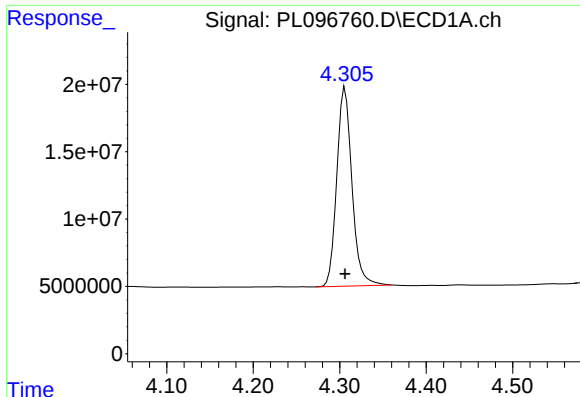

#3 gamma-BHC (Lindane)


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 179221504
Conc: 41.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

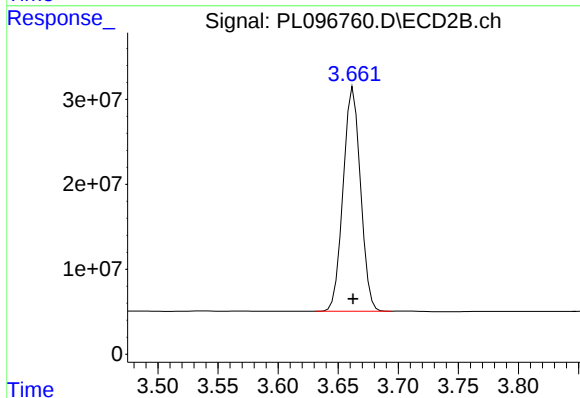


#3 gamma-BHC (Lindane)

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 266259660
Conc: 41.58 ng/ml

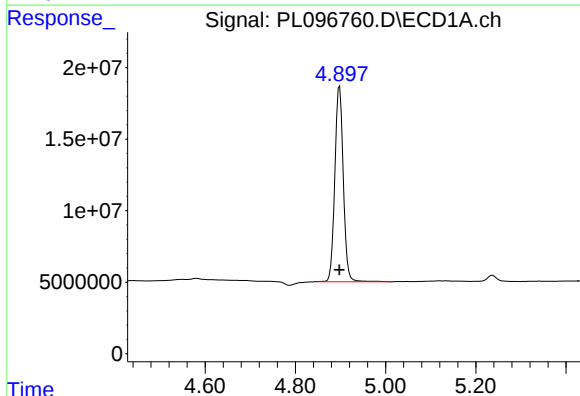


#4 Heptachlor

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 178032576
Conc: 40.91 ng/ml

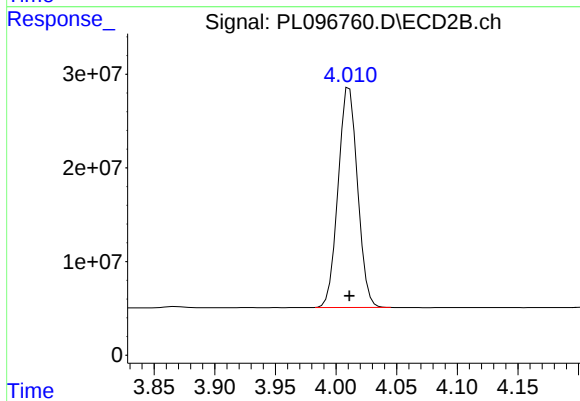

#4 Heptachlor


R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 261817106
Conc: 40.77 ng/ml

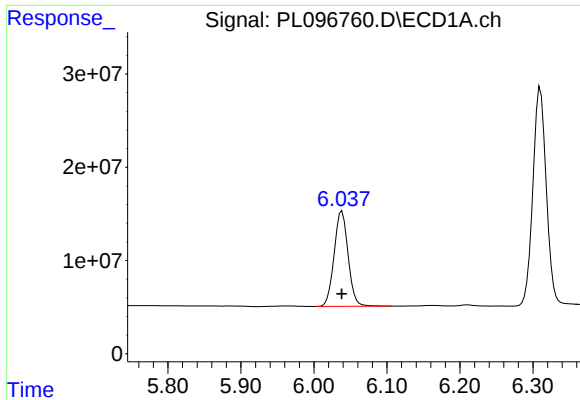

#9 Endosulfan I


R.T.: 6.039 min
Delta R.T.: 0.000 min
Response: 136174714
Conc: 40.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

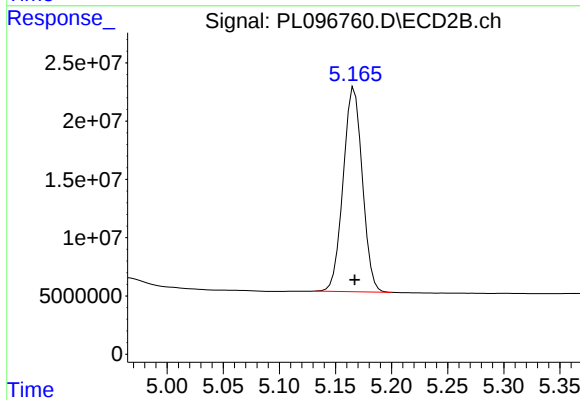


#9 Endosulfan I

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 208085809
Conc: 40.68 ng/ml

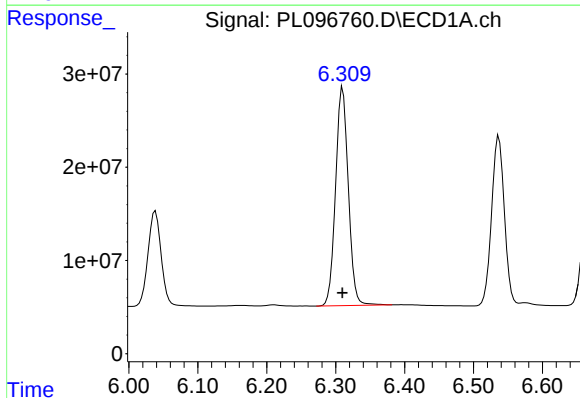


#13 Dieldrin

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 300137724
Conc: 83.33 ng/ml

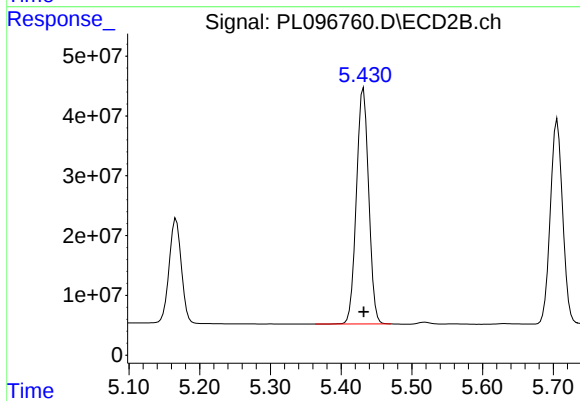

#13 Dieldrin


R.T.: 5.432 min
Delta R.T.: 0.000 min
Response: 476059396
Conc: 81.77 ng/ml

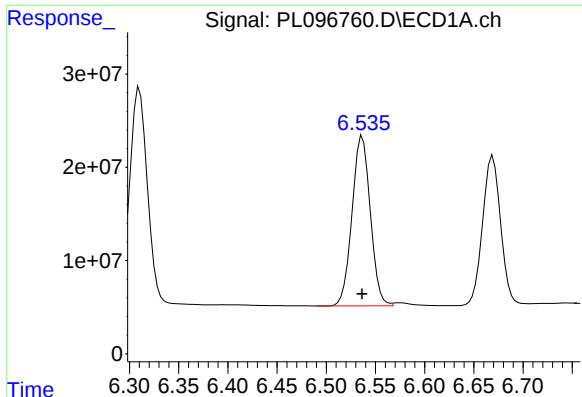

#14 Endrin


R.T.: 6.537 min
Delta R.T.: 0.000 min
Response: 235514301
Conc: 83.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

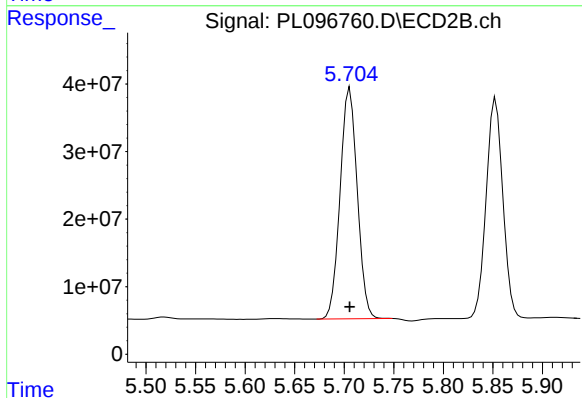


#14 Endrin

R.T.: 5.706 min
Delta R.T.: 0.000 min
Response: 412184986
Conc: 82.00 ng/ml

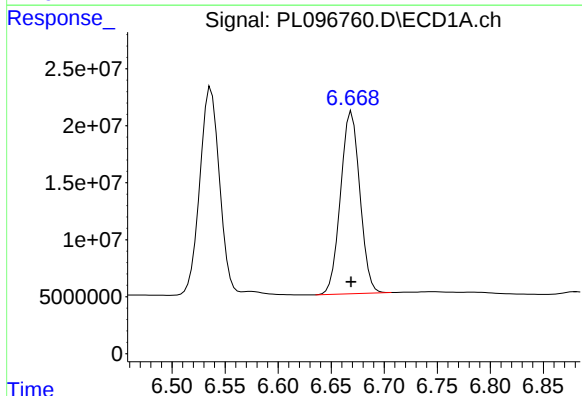


#16 4,4'-DDD

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 202202016
Conc: 82.60 ng/ml

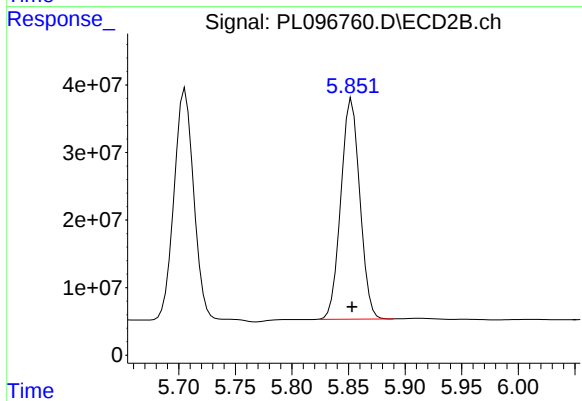

#16 4,4'-DDD


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 381156996
Conc: 82.58 ng/ml

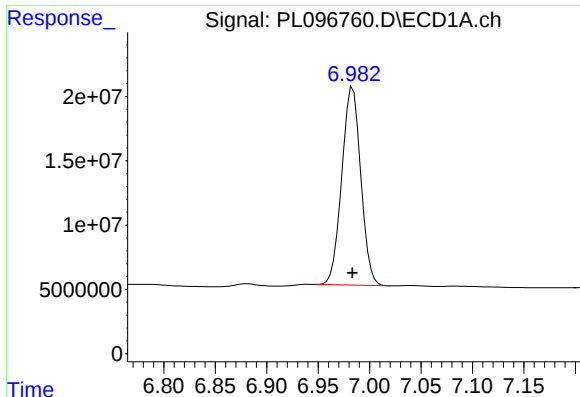

#17 4,4'-DDT


R.T.: 6.984 min
Delta R.T.: 0.000 min
Response: 197929134
Conc: 84.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

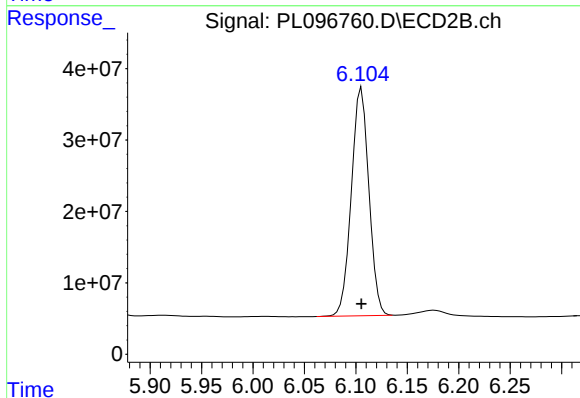


#17 4,4'-DDT

R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 379778846
Conc: 83.31 ng/ml

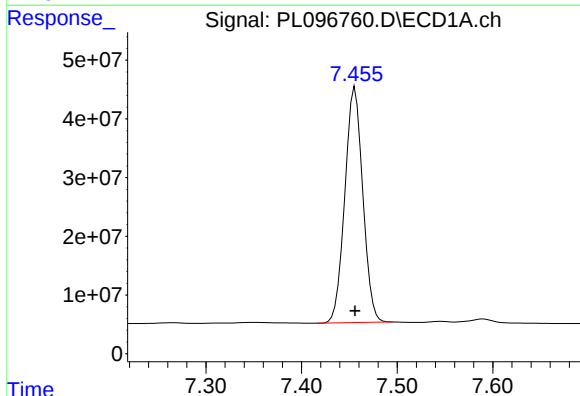


#20 Methoxychlor

R.T.: 7.456 min
Delta R.T.: 0.000 min
Response: 524964031
Conc: 404.67 ng/ml

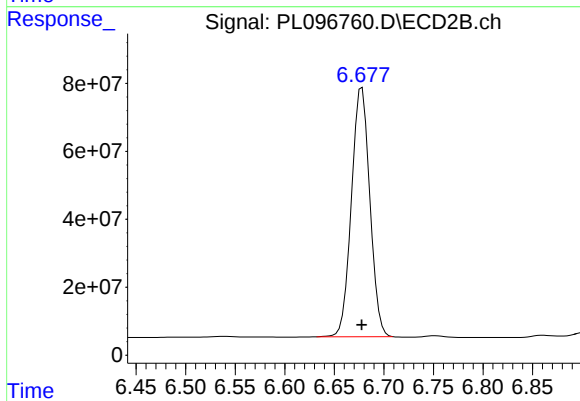

#20 Methoxychlor


R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 949209565
Conc: 381.46 ng/ml

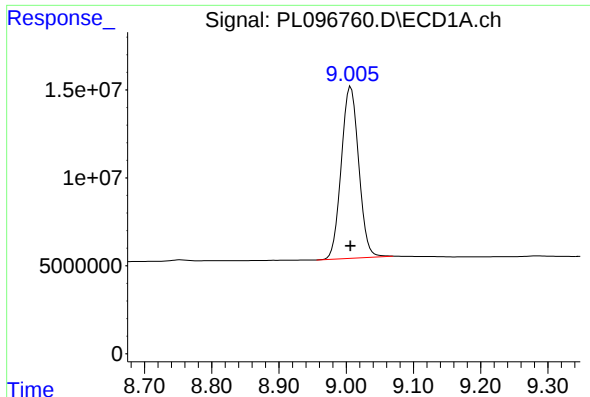

#27 Decachlorobiphenyl

R.T.: 9.007 min
Delta R.T.: 0.000 min
Response: 175397539
Conc: 78.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA4303

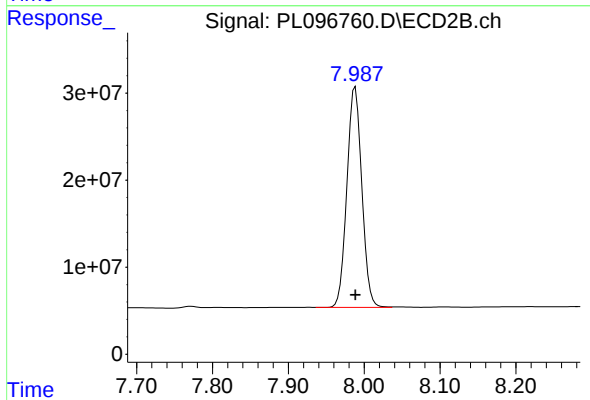

#27 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 346436764
Conc: 77.67 ng/ml