

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
 Data File : PL096762.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 20:19
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 INDA5305

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 05:52:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 13 05:49:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.825	247.4E6	379.0E6	82.563	82.839
27)	SA Decachlor...	9.005	7.988	352.0E6	693.3E6	157.250	155.434
Target Compounds							
2)	A alpha-BHC	3.978	3.331	416.0E6	620.3E6	90.837	90.548
3)	MA gamma-BHC...	4.306	3.662	382.2E6	567.3E6	88.121	88.600
4)	MA Heptachlor	4.897	4.011	374.0E6	550.0E6	85.945	85.659
9)	A Endosulfan I	6.038	5.166	285.2E6	431.8E6	84.516	84.400
13)	MA Dieldrin	6.310	5.431	643.2E6	990.0E6	178.565	170.045
14)	MA Endrin	6.536	5.705	499.4E6	856.0E6	176.592	170.297
16)	A 4,4'-DDD	6.669	5.853	432.1E6	801.1E6	176.524	173.561
17)	MA 4,4'-DDT	6.983	6.105	424.8E6	803.5E6	180.753	176.264
20)	A Methoxychlor	7.455	6.677	1077.1E6	1817.3E6	830.306	730.342


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081225\
Data File : PL096762.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 20:19
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 05:52:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081225CLP.M
Quant Title : GC Extractables
QLast Update : Wed Aug 13 05:49:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

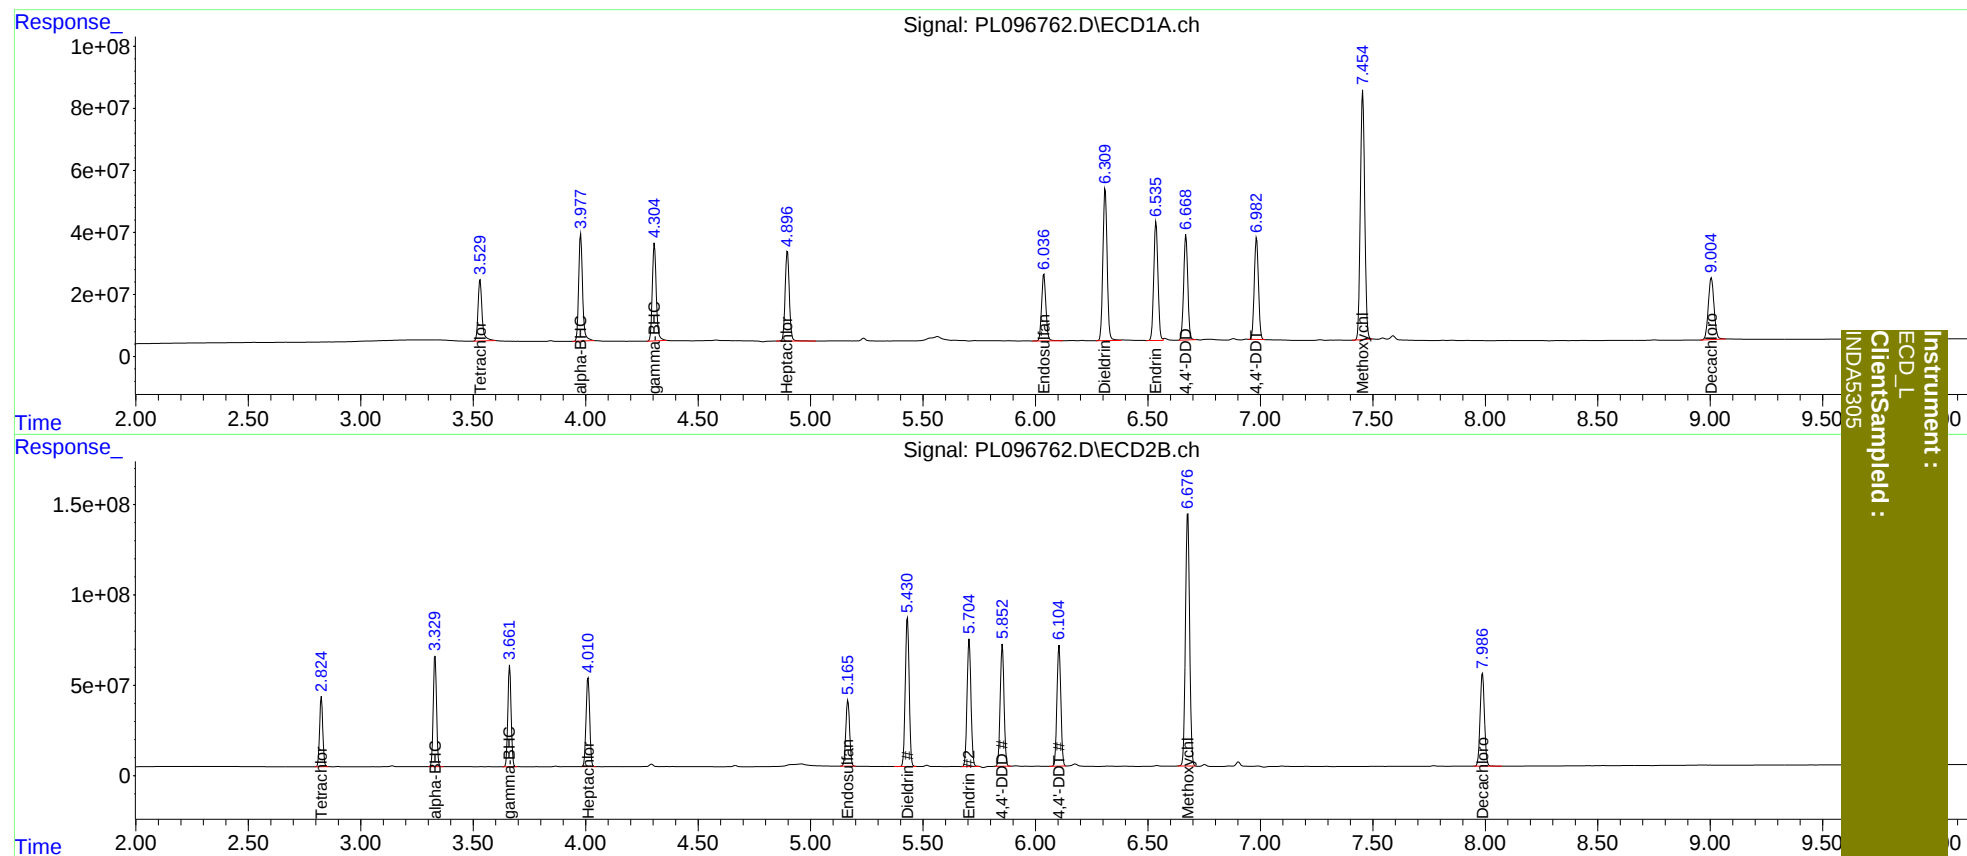


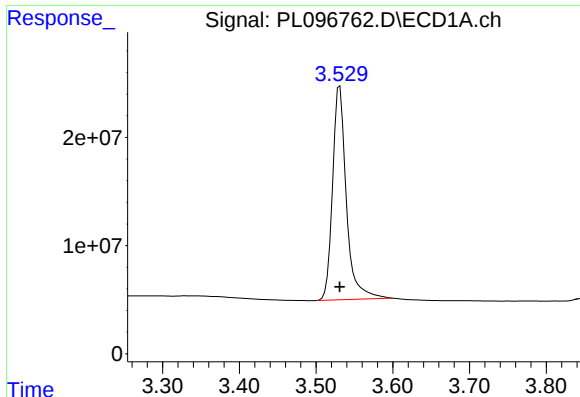

#1 Tetrachloro-m-xylene


R.T.: 3.531 min
Delta R.T.: 0.000 min
Response: 247372194
Conc: 82.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

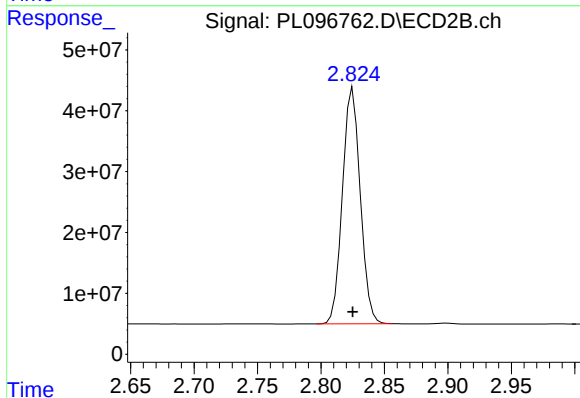


#1 Tetrachloro-m-xylene

R.T.: 2.825 min
Delta R.T.: 0.000 min
Response: 379011031
Conc: 82.84 ng/ml

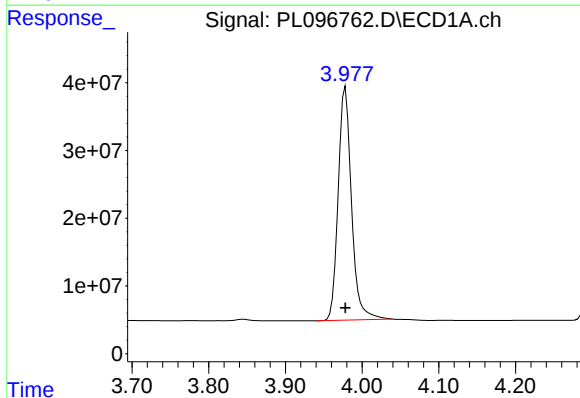


#2 alpha-BHC

R.T.: 3.978 min
Delta R.T.: 0.000 min
Response: 415996689
Conc: 90.84 ng/ml

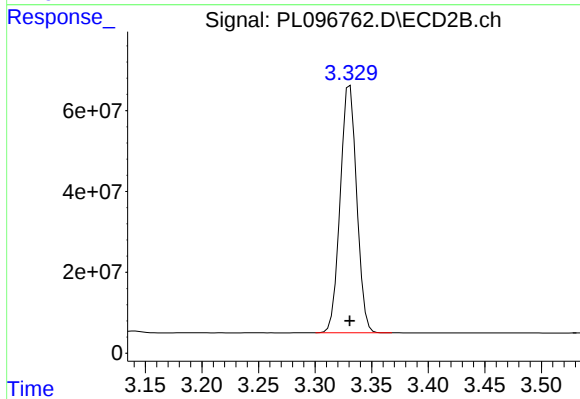

#2 alpha-BHC


R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 620255688
Conc: 90.55 ng/ml

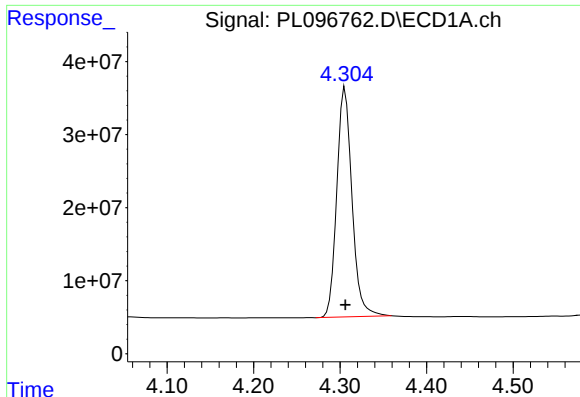

#3 gamma-BHC (Lindane)


R.T.: 4.306 min
Delta R.T.: 0.000 min
Response: 382194810
Conc: 88.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

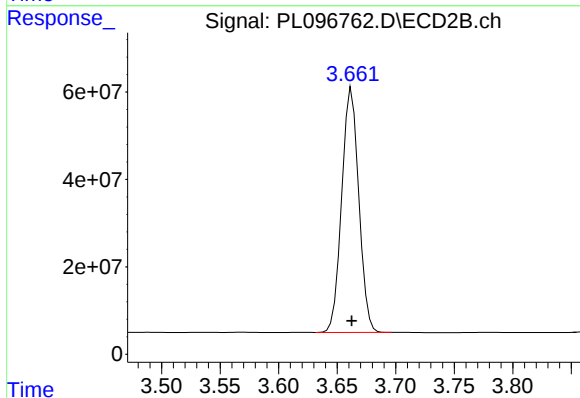


#3 gamma-BHC (Lindane)

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 567314789
Conc: 88.60 ng/ml

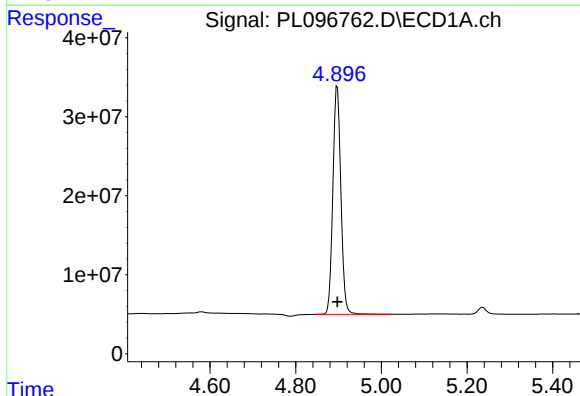


#4 Heptachlor

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 374035768
Conc: 85.95 ng/ml

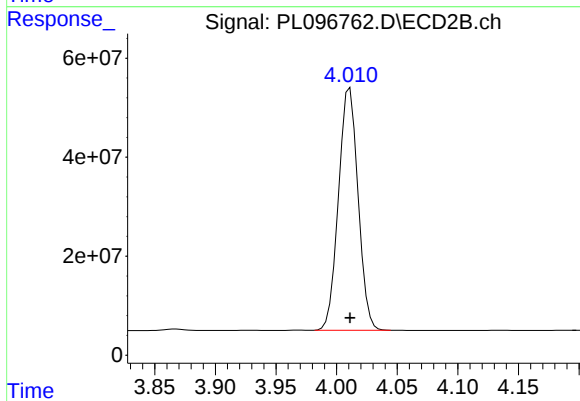

#4 Heptachlor


R.T.: 4.011 min
Delta R.T.: 0.000 min
Response: 550044086
Conc: 85.66 ng/ml

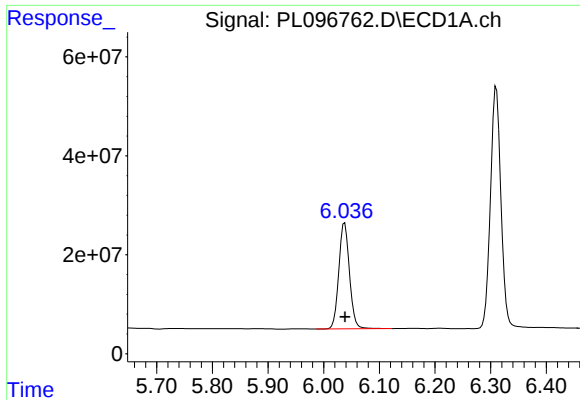

#9 Endosulfan I


R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 285199107
Conc: 84.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

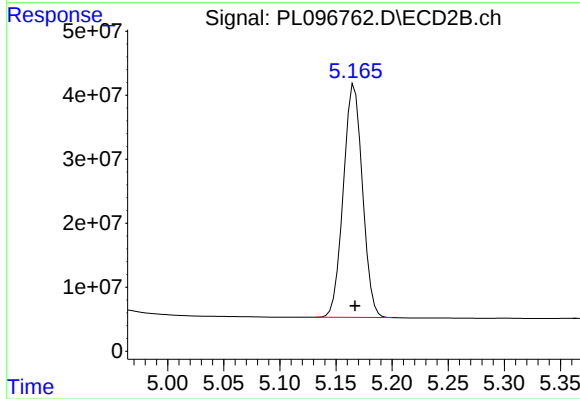


#9 Endosulfan I

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 431760502
Conc: 84.40 ng/ml

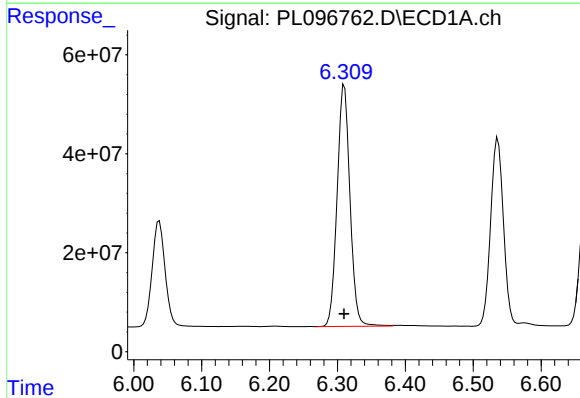


#13 Dieldrin

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 643186736
Conc: 178.56 ng/ml

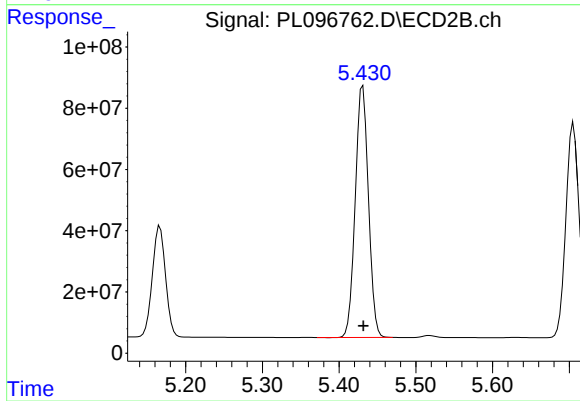

#13 Dieldrin


R.T.: 5.431 min
Delta R.T.: 0.000 min
Response: 989963748
Conc: 170.04 ng/ml

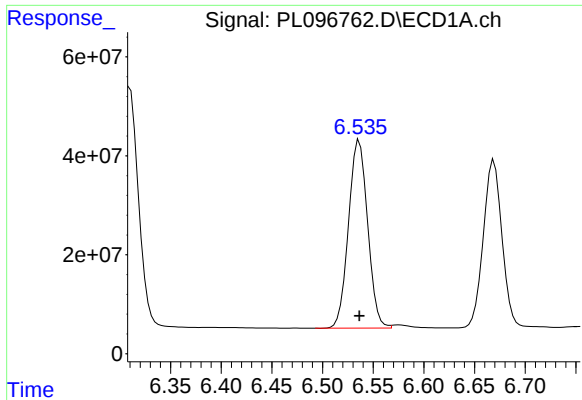

#14 Endrin


R.T.: 6.536 min
Delta R.T.: 0.000 min
Response: 499447013
Conc: 176.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

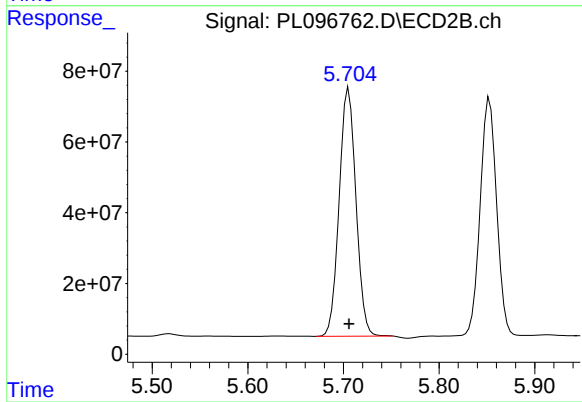


#14 Endrin

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 855986306
Conc: 170.30 ng/ml

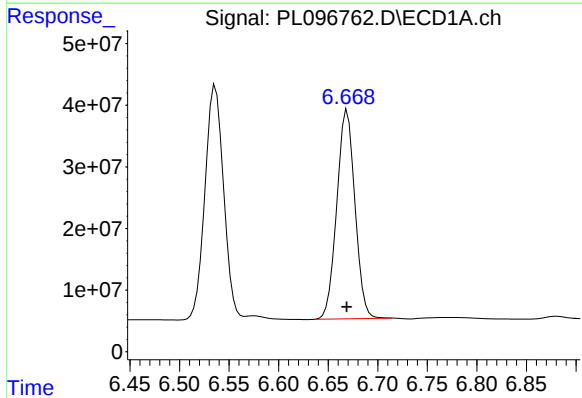


#16 4,4'-DDD

R.T.: 6.669 min
Delta R.T.: 0.000 min
Response: 432144727
Conc: 176.52 ng/ml

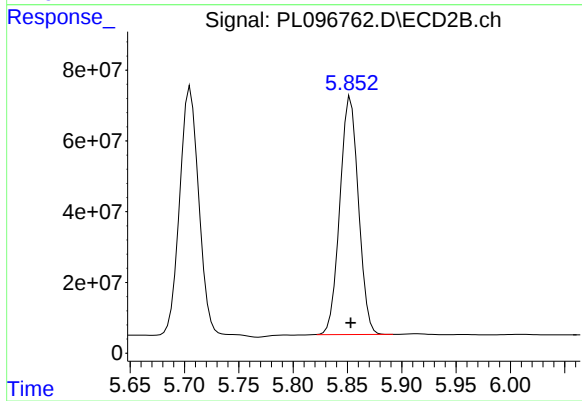

#16 4,4'-DDD


R.T.: 5.853 min
Delta R.T.: 0.000 min
Response: 801099742
Conc: 173.56 ng/ml

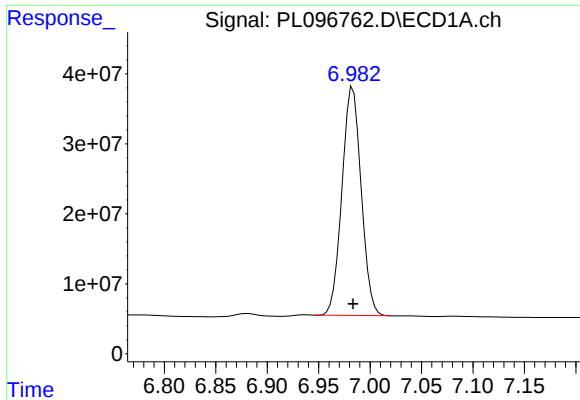

#17 4,4'-DDT


R.T.: 6.983 min
Delta R.T.: 0.000 min
Response: 424794961
Conc: 180.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

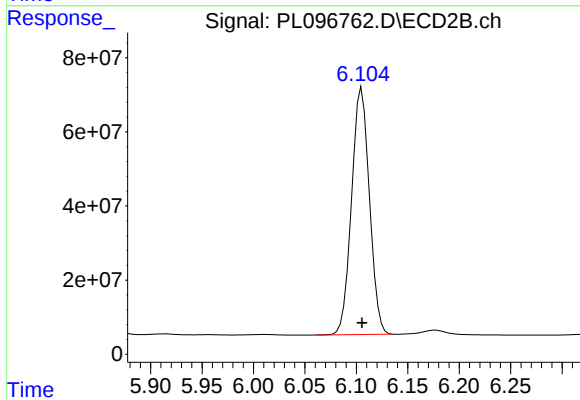


#17 4,4'-DDT

R.T.: 6.105 min
Delta R.T.: 0.000 min
Response: 803504434
Conc: 176.26 ng/ml

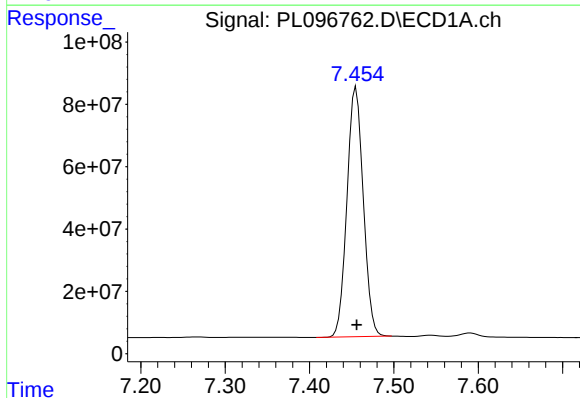


#20 Methoxychlor

R.T.: 7.455 min
Delta R.T.: 0.000 min
Response: 1077137774
Conc: 830.31 ng/ml

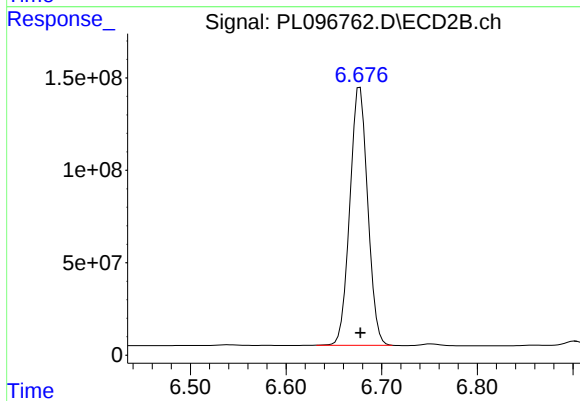

#20 Methoxychlor


R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 1817330145
Conc: 730.34 ng/ml

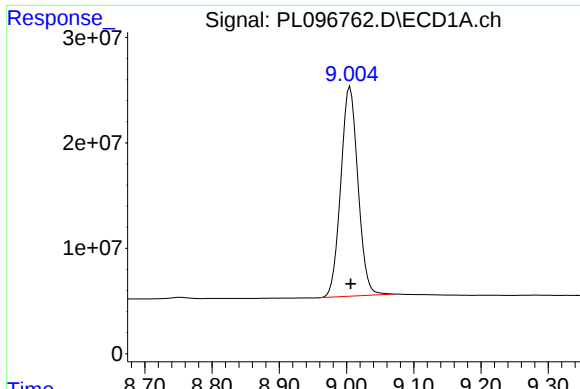

#27 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: -0.001 min
Response: 351991084
Conc: 157.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
INDA5305

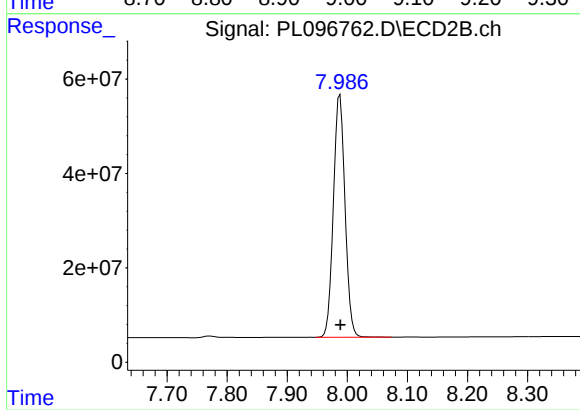

#27 Decachlorobiphenyl

R.T.: 7.988 min
Delta R.T.: 0.000 min
Response: 693330132
Conc: 155.43 ng/ml