

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
 Data File : PL039123.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2018 01:25
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 07:42:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 14 06:53:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	7.907f	0.000	52531790	0	7.480	N.D. #
Target Compounds							
2)	A alpha-BHC	3.698f	0.000	5604162	0	0.474	N.D. #
7)	B delta-BHC	4.406f	0.000	3165795	0	0.292	N.D. #
8)	B Heptachlo...	4.921f	0.000	8690162	0	0.910	N.D. #
10)	B gamma-Chl...	5.164	0.000	3487320	0	0.353	N.D. #
13)	MA Dieldrin	5.599f	0.000	5678818	0	0.582	N.D. #
14)	MA Endrin	5.782	0.000	3904987	0	0.436	N.D. #
17)	MA 4,4'-DDT	6.179	0.000	60351329	0	7.961	N.D. #
18)	B Endrin al...	6.179f	0.000	60351329	0	8.905	N.D. #
19)	B Endosulfa...	6.395f	0.000	9125859	0	1.122	N.D. #
20)	A Methoxychlor	6.640f	0.000	1906854	0	0.466	N.D. #
25)	Chlordane-3	5.164	0.000	3487320	0	3.193	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
Data File : PL039123.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2018 01:25
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 07:42:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Tue Aug 14 06:53:39 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

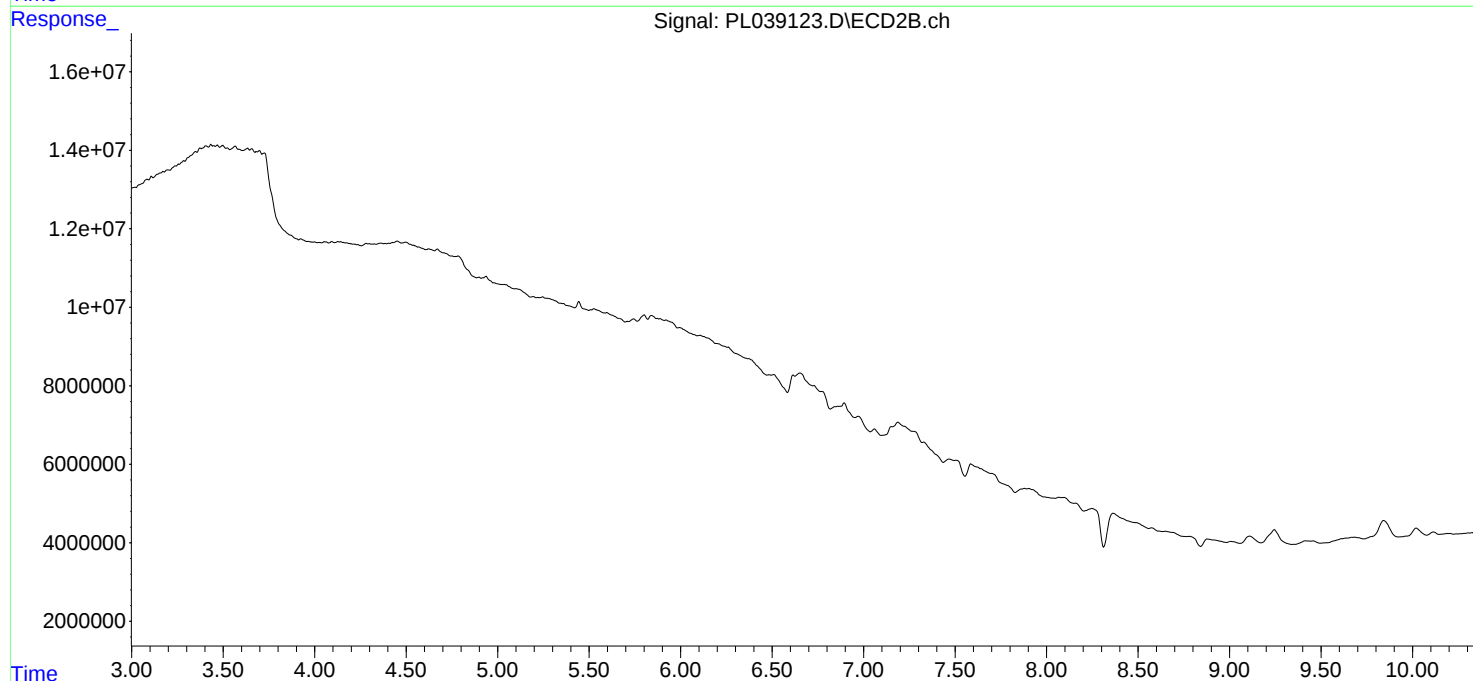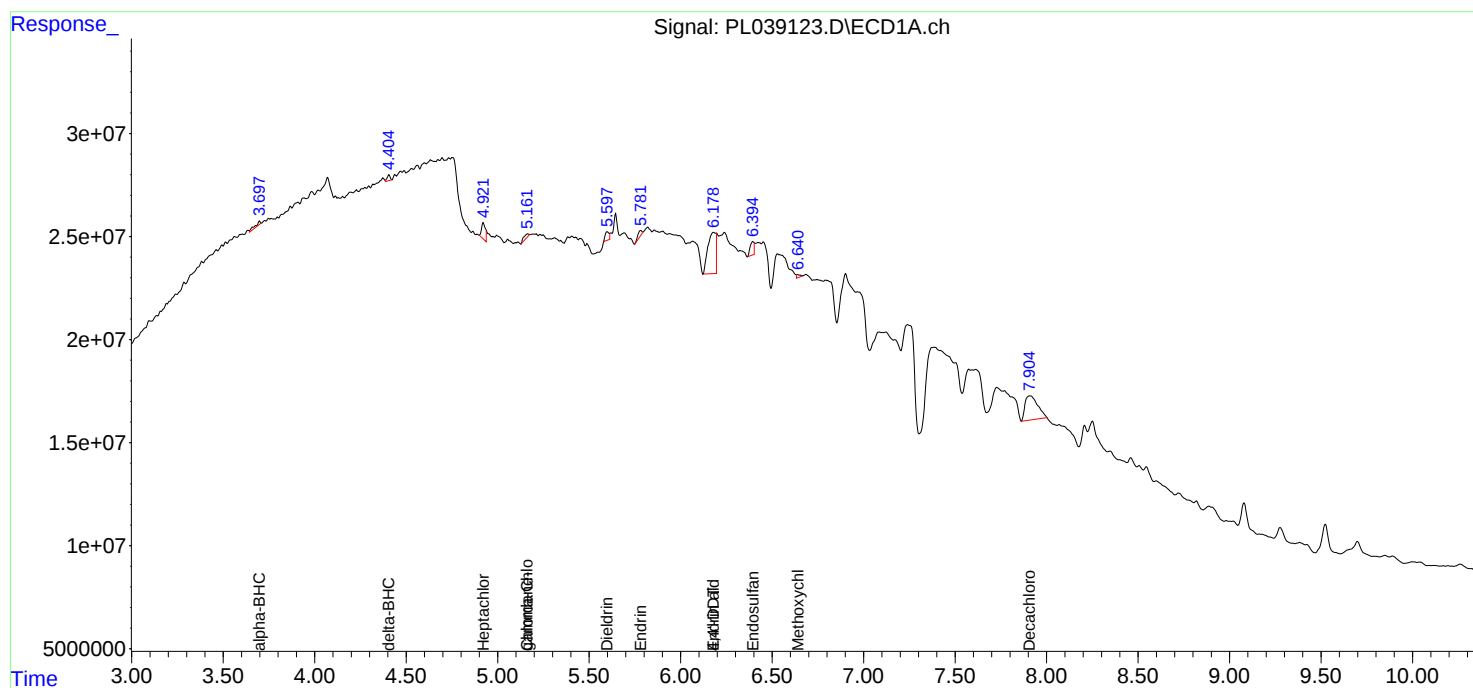


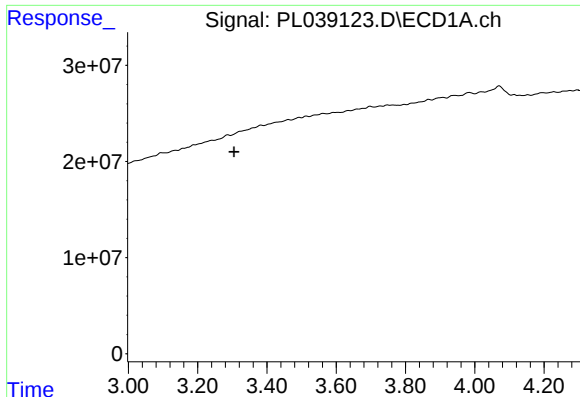

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.305 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

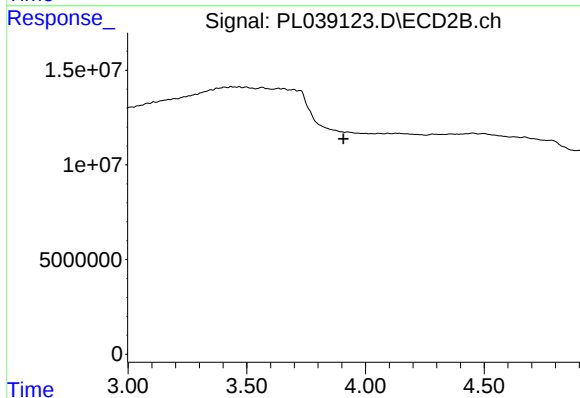


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.907 min
Response: 0
Conc: N.D.

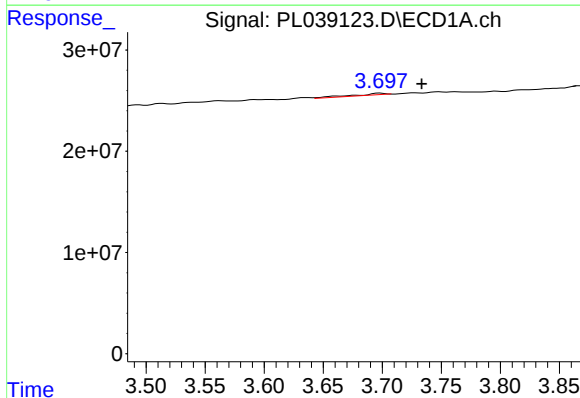


#2 alpha-BHC

R.T.: 3.698 min
Delta R.T.: -0.035 min
Response: 5604162
Conc: 0.47 ng/ml

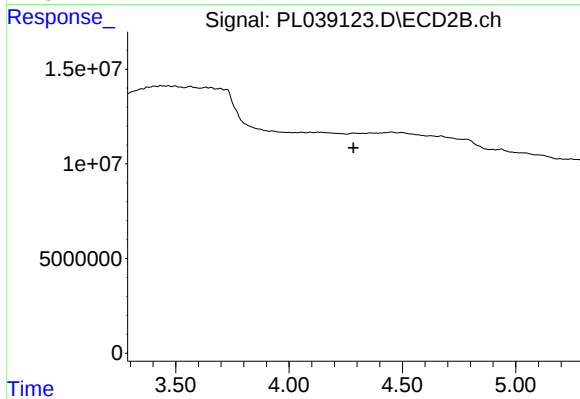

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.284 min
Response: 0
Conc: N.D.

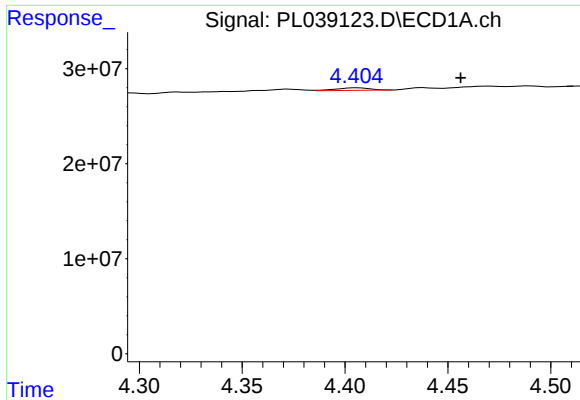

#7 delta-BHC


R.T.: 4.406 min
Delta R.T.: -0.050 min
Response: 3165795
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :

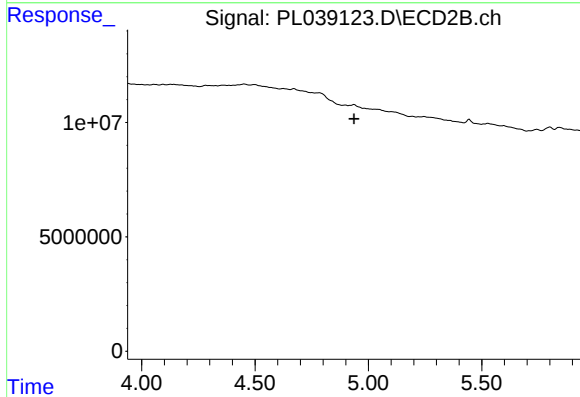


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.936 min
Response: 0
Conc: N.D.

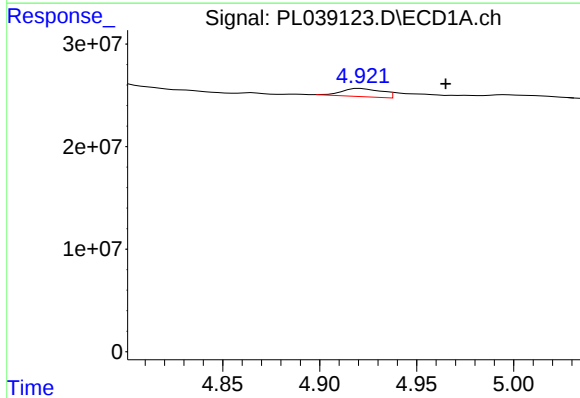


#8 Heptachlor epoxide

R.T.: 4.921 min
Delta R.T.: -0.044 min
Response: 8690162
Conc: 0.91 ng/ml

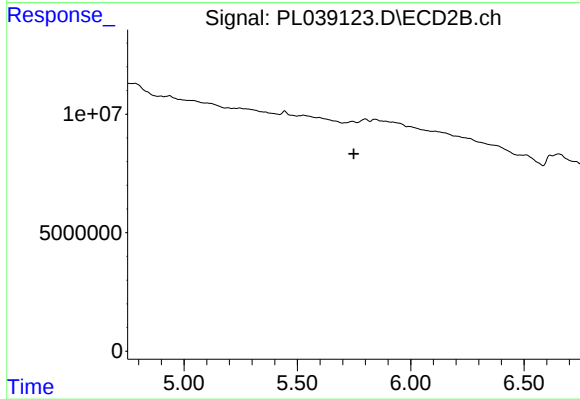

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.749 min
Response: 0
Conc: N.D.

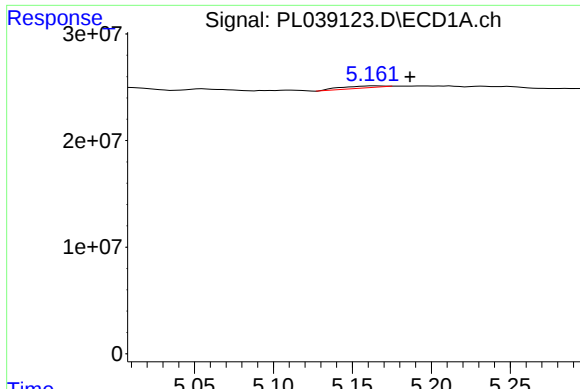

#10 gamma-Chlordane


R.T.: 5.164 min
Delta R.T.: -0.023 min
Response: 3487320
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

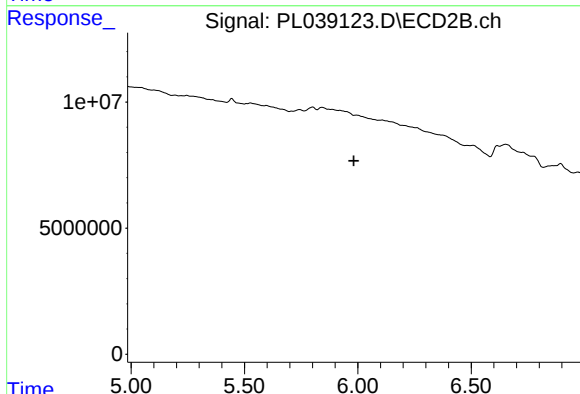


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.982 min
Response: 0
Conc: N.D.

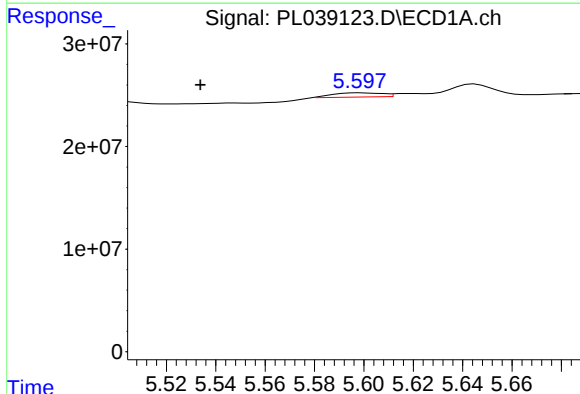


#13 Dieldrin

R.T.: 5.599 min
Delta R.T.: 0.065 min
Response: 5678818
Conc: 0.58 ng/ml

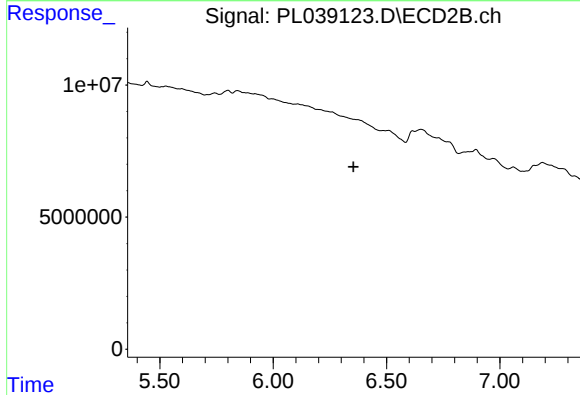

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.354 min
Response: 0
Conc: N.D.

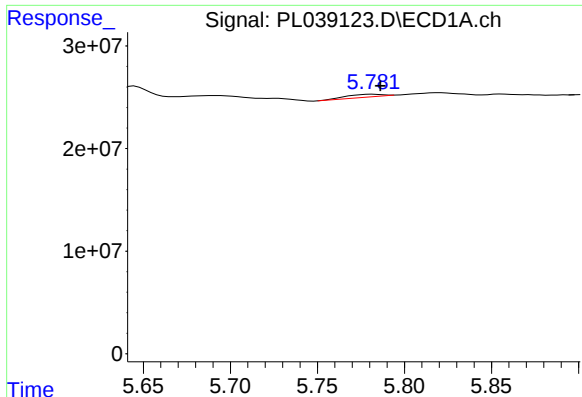

#14 Endrin


R.T.: 5.782 min
Delta R.T.: -0.004 min
Response: 3904987
Conc: 0.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

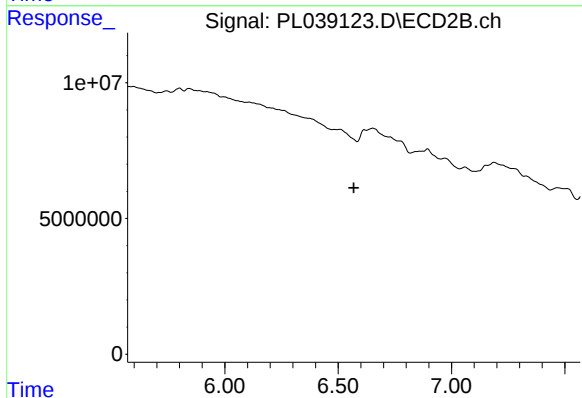


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.569 min
Response: 0
Conc: N.D.

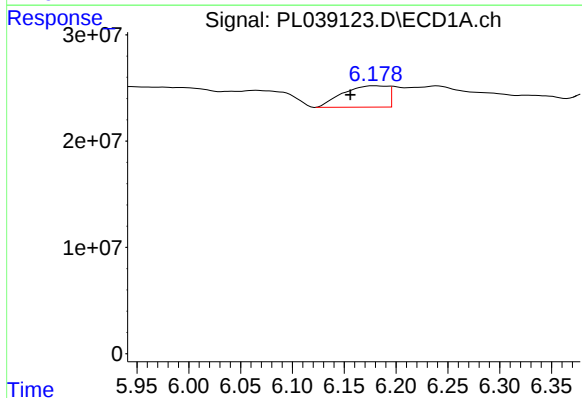


#17 4,4'-DDT

R.T.: 6.179 min
Delta R.T.: 0.023 min
Response: 60351329
Conc: 7.96 ng/ml

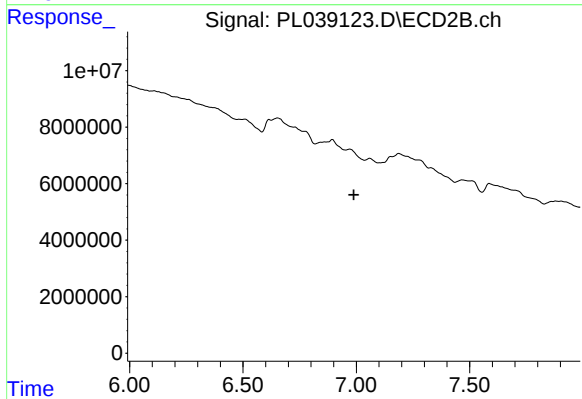

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.989 min
Response: 0
Conc: N.D.

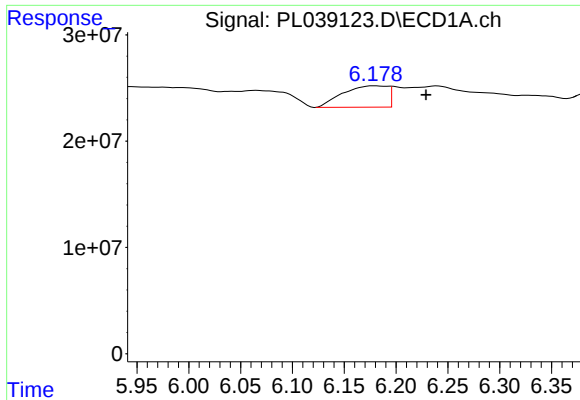

#18 Endrin aldehyde


R.T.: 6.179 min
Delta R.T.: -0.050 min
Response: 60351329
Conc: 8.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

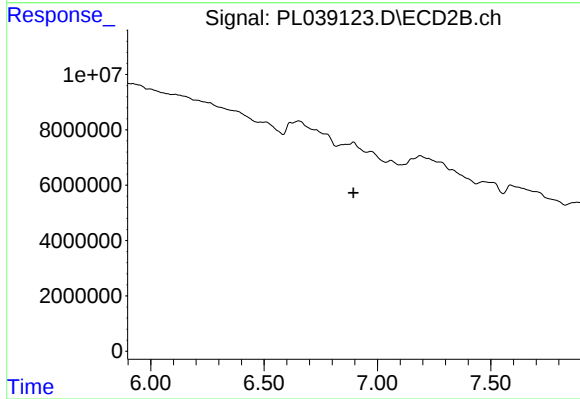


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.895 min
Response: 0
Conc: N.D.

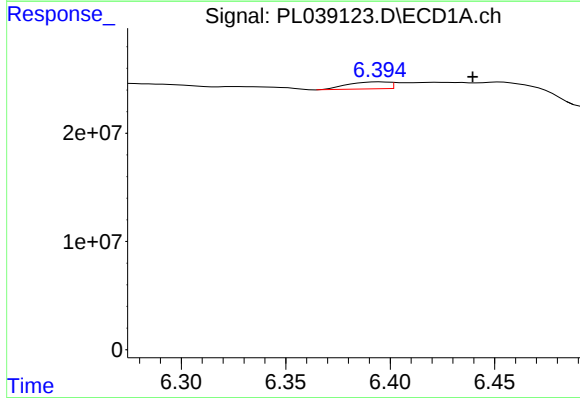


#19 Endosulfan Sulfate

R.T.: 6.395 min
Delta R.T.: -0.044 min
Response: 9125859
Conc: 1.12 ng/ml

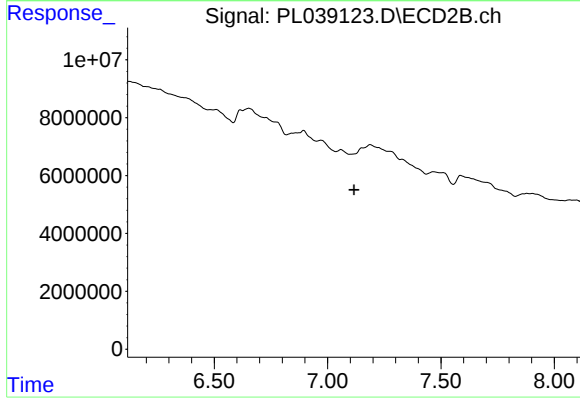

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

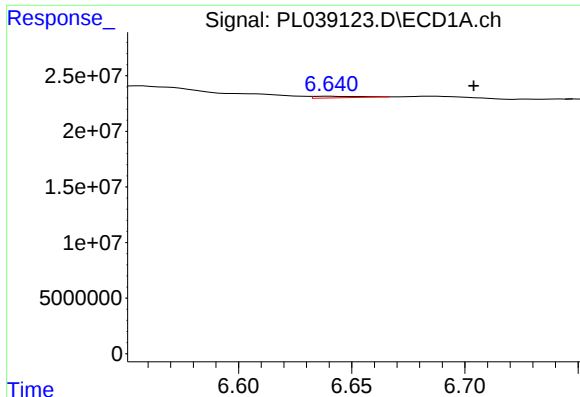

#20 Methoxychlor


R.T.: 6.640 min
Delta R.T.: -0.064 min
Response: 1906854
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

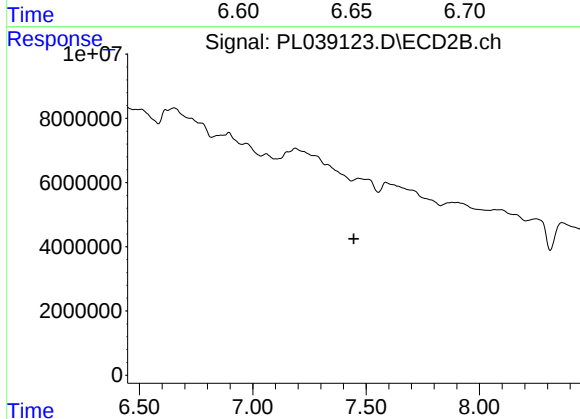


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.445 min
Response: 0
Conc: N.D.

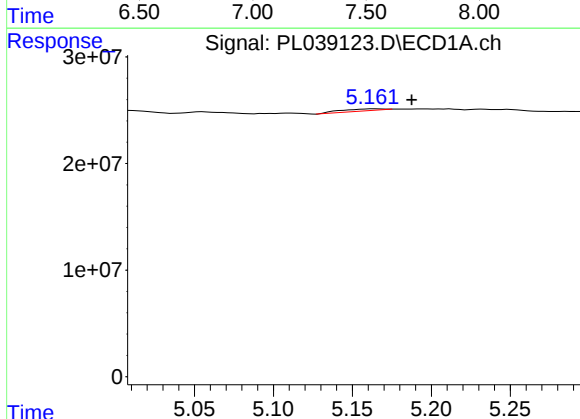


#25 Chlordane-3

R.T.: 5.164 min
Delta R.T.: -0.024 min
Response: 3487320
Conc: 3.19 ng/ml

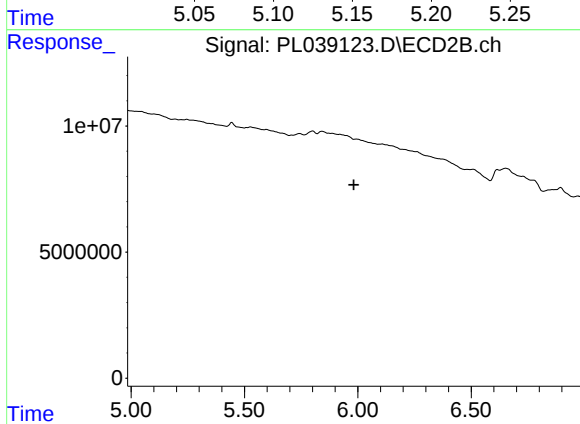

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.983 min
Response: 0
Conc: N.D.

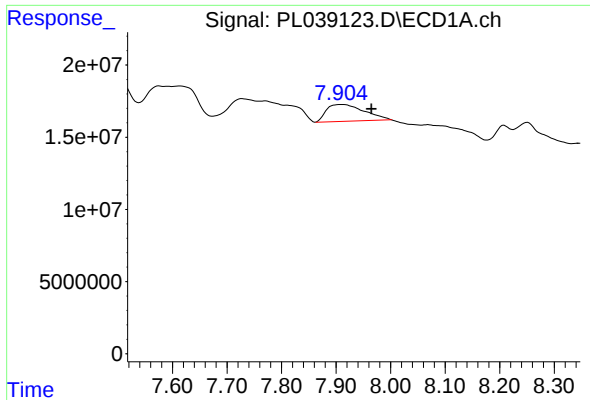

#28 Decachlorobiphenyl

R.T.: 7.907 min
Delta R.T.: -0.057 min
Response: 52531790
Conc: 7.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

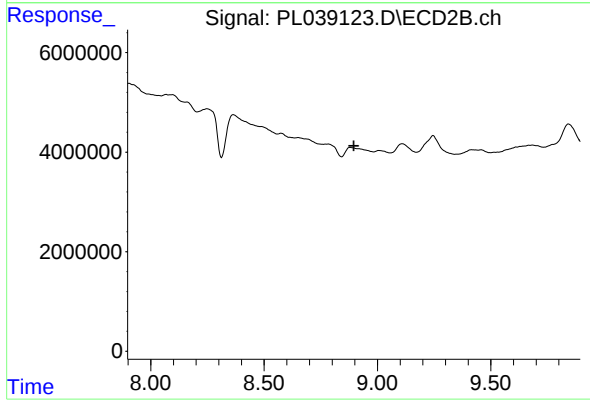

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.895 min
Response: 0
Conc: N.D.