

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
 Data File : PL039132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2018 03:33
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:46:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 14 06:46:06 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.306	3.907	724.8E6	272.8E6	102.078	101.195
28)	SA Decachlor...	7.965	8.896	674.2E6	220.7E6	95.415	94.359
Target Compounds							
23)	Chlordane-1	4.145	4.885	326.8E6	127.0E6	954.225	995.408
24)	Chlordane-2	4.635	5.346	343.7E6	120.6E6	961.710	958.796
25)	Chlordane-3	5.188	5.983	1062.8E6	436.5E6	939.284	996.885
26)	Chlordane-4	5.243	6.058	987.3E6	513.2E6	970.411	982.276
27)	Chlordane-5	6.063	6.848	331.1E6	92415183	978.129	991.042



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
Data File : PL039132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2018 03:33
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:46:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Tue Aug 14 06:46:06 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

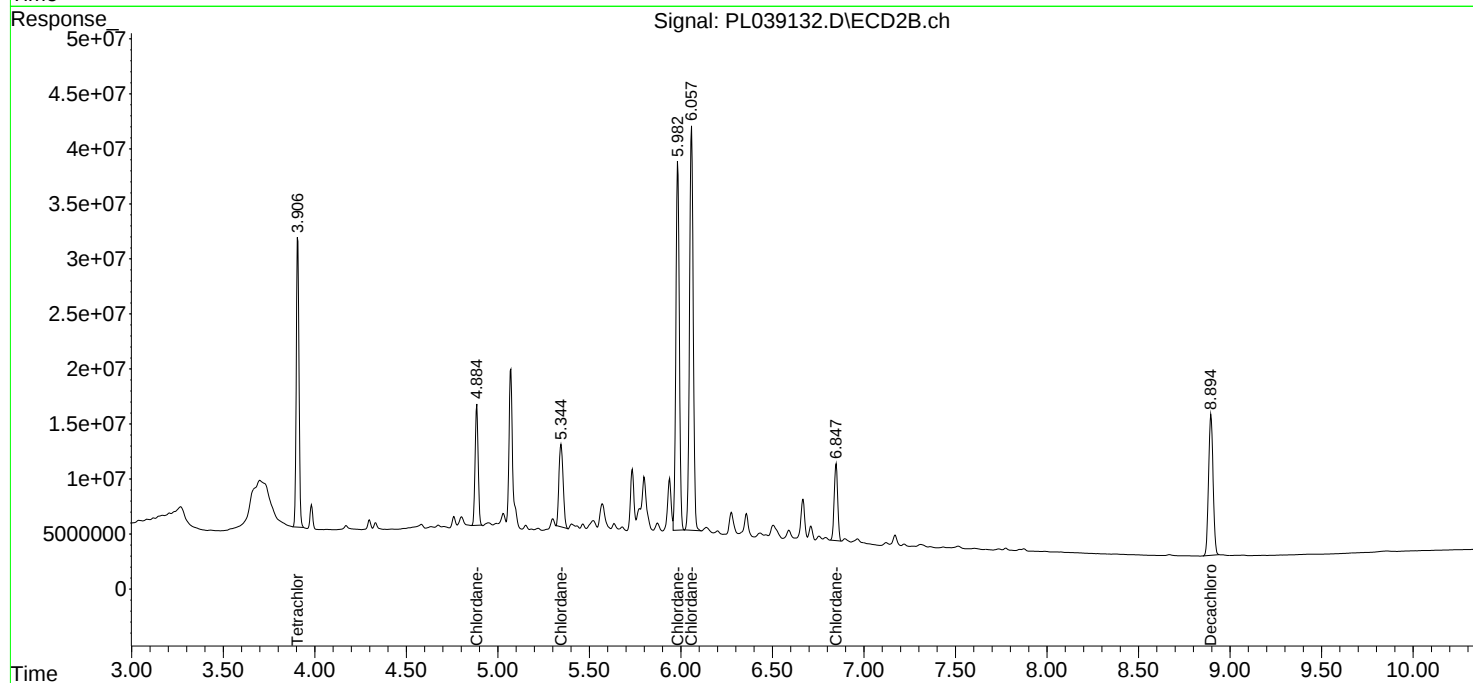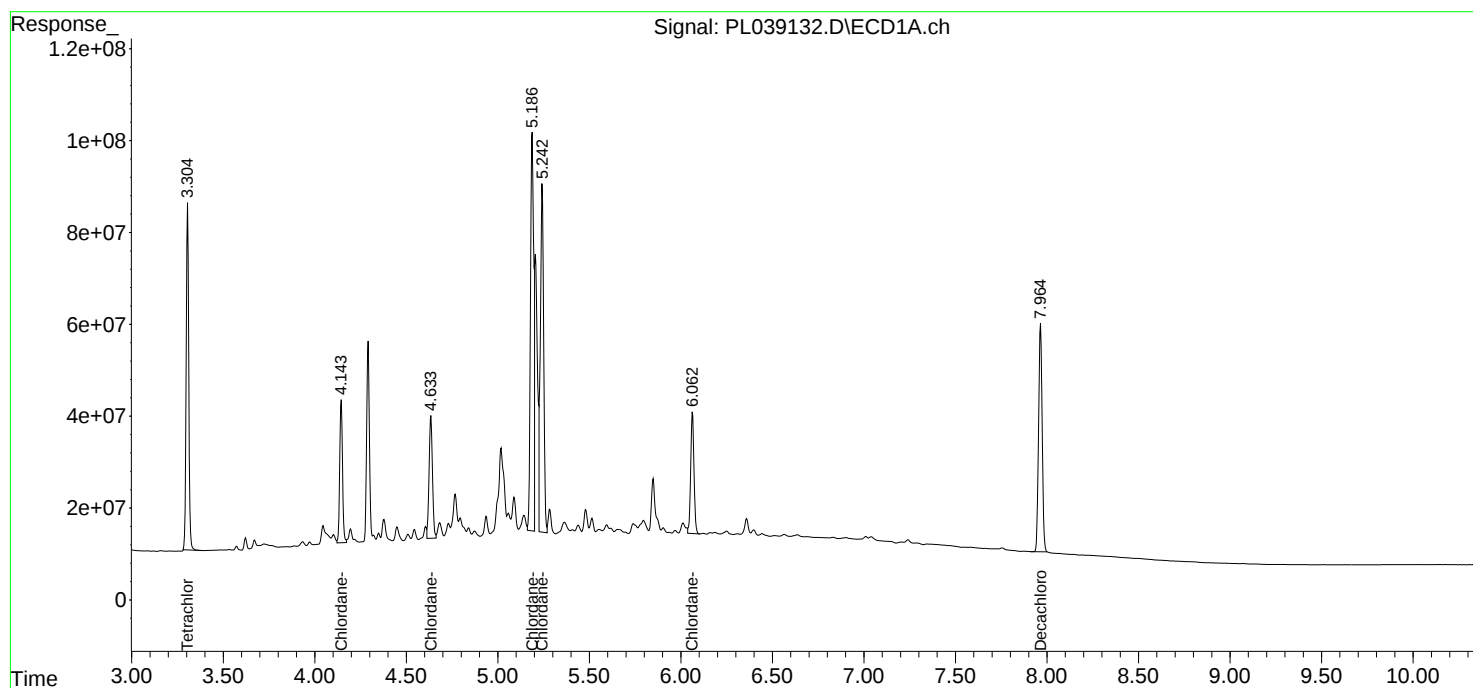


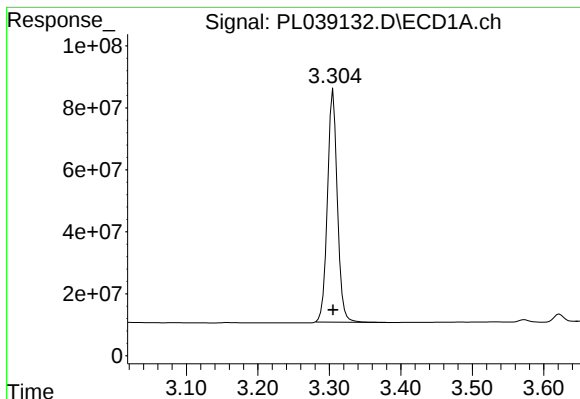

#1 Tetrachloro-m-xylene


R.T.: 3.306 min
Delta R.T.: 0.000 min
Response: 724795255
Conc: 102.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

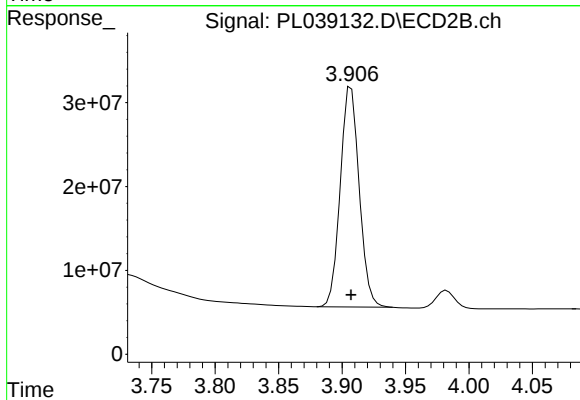


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 272829641
Conc: 101.20 ng/ml

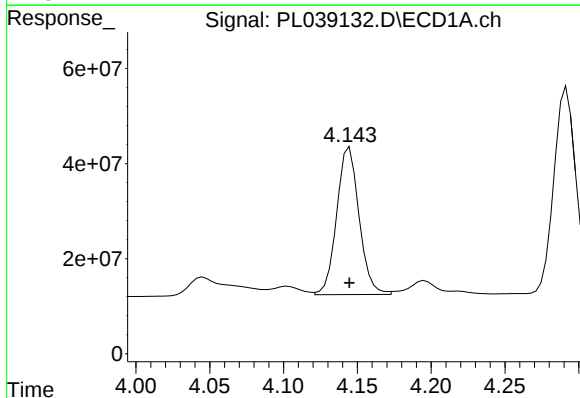


#23 Chlordane-1

R.T.: 4.145 min
Delta R.T.: 0.000 min
Response: 326752988
Conc: 954.23 ng/ml

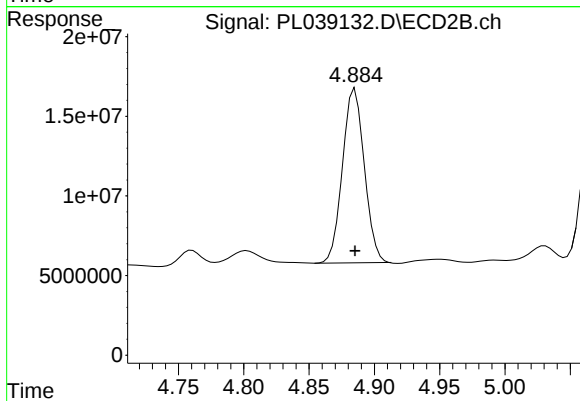

#23 Chlordane-1


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 126954279
Conc: 995.41 ng/ml

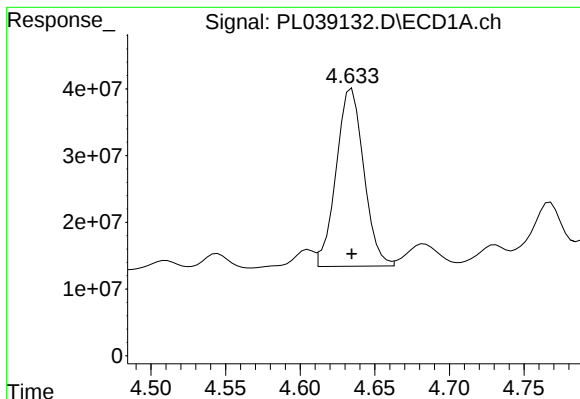

#24 Chlordane-2


R.T.: 4.635 min
Delta R.T.: 0.000 min
Response: 343659736
Conc: 961.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

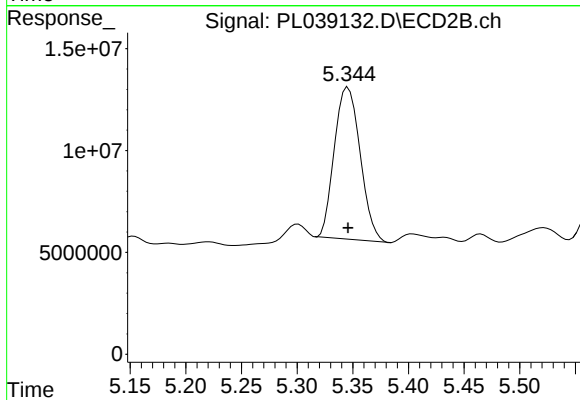


#24 Chlordane-2

R.T.: 5.346 min
Delta R.T.: 0.000 min
Response: 120591443
Conc: 958.80 ng/ml

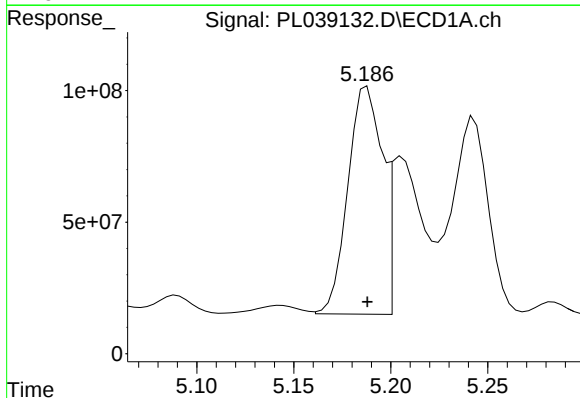


#25 Chlordane-3

R.T.: 5.188 min
Delta R.T.: 0.000 min
Response: 1062754471
Conc: 939.28 ng/ml

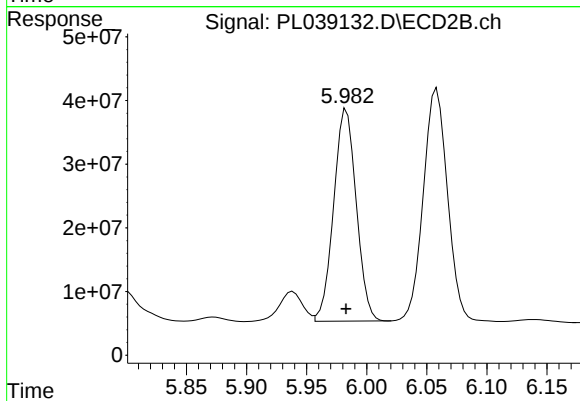

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 436538014
Conc: 996.89 ng/ml

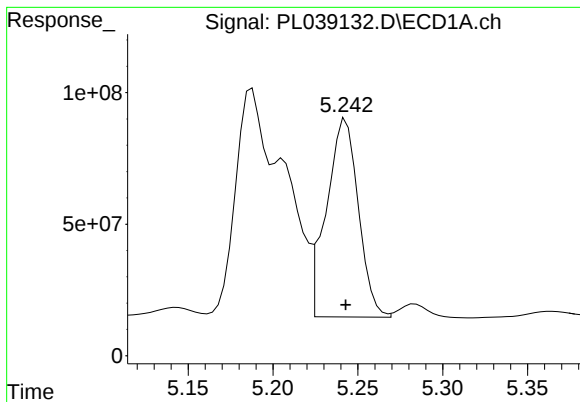

#26 Chlordane-4


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 987263624
Conc: 970.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

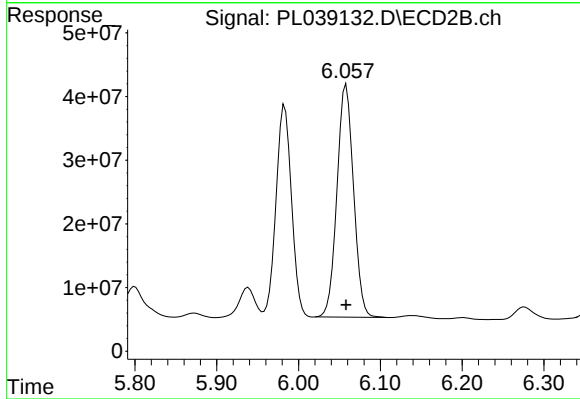


#26 Chlordane-4

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 513206373
Conc: 982.28 ng/ml

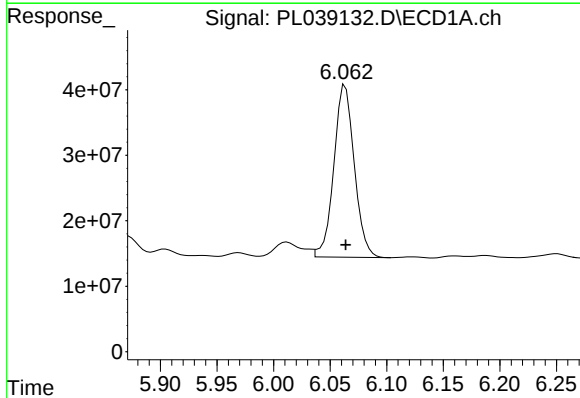


#27 Chlordane-5

R.T.: 6.063 min
Delta R.T.: 0.000 min
Response: 331106693
Conc: 978.13 ng/ml

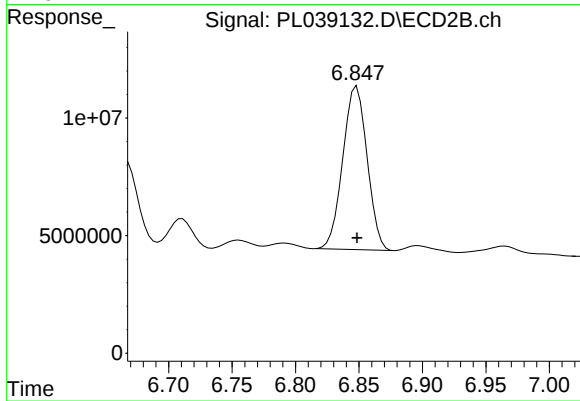

#27 Chlordane-5

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 92415183
Conc: 991.04 ng/ml

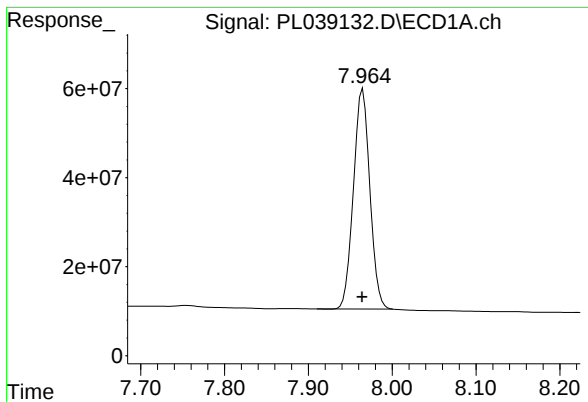

#28 Decachlorobiphenyl


R.T.: 7.965 min

Delta R.T.: 0.001 min

Response: 674189378

Conc: 95.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

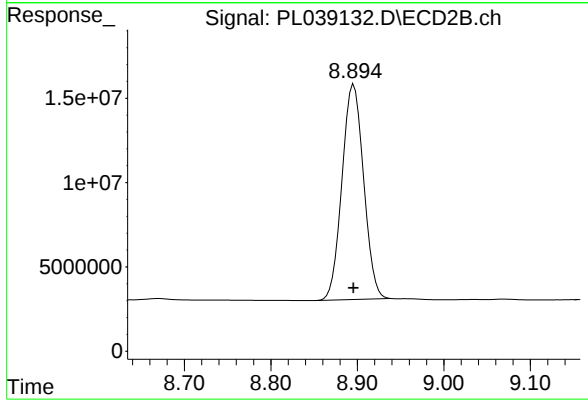

#28 Decachlorobiphenyl

R.T.: 8.896 min

Delta R.T.: 0.000 min

Response: 220698335

Conc: 94.36 ng/ml