

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
 Data File : PL039133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2018 03:47
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 06:46:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 14 06:46:06 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	545.4E6	205.3E6	76.808	76.165
28)	SA Decachlor...	7.965	8.896	513.6E6	169.7E6	72.689	72.536
Target Compounds							
23)	Chlordane-1	4.145	4.885	236.7E6	94118360	691.329	737.952
24)	Chlordane-2	4.635	5.346	261.5E6	92216932	731.891	733.196
25)	Chlordane-3	5.188	5.983	817.4E6	326.1E6	722.412	744.619
26)	Chlordane-4	5.243	6.058	752.2E6	384.5E6	739.337	735.983
27)	Chlordane-5	6.064	6.848	248.5E6	68393024	734.072	733.433



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081318\
Data File : PL039133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2018 03:47
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 06:46:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Tue Aug 14 06:46:06 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

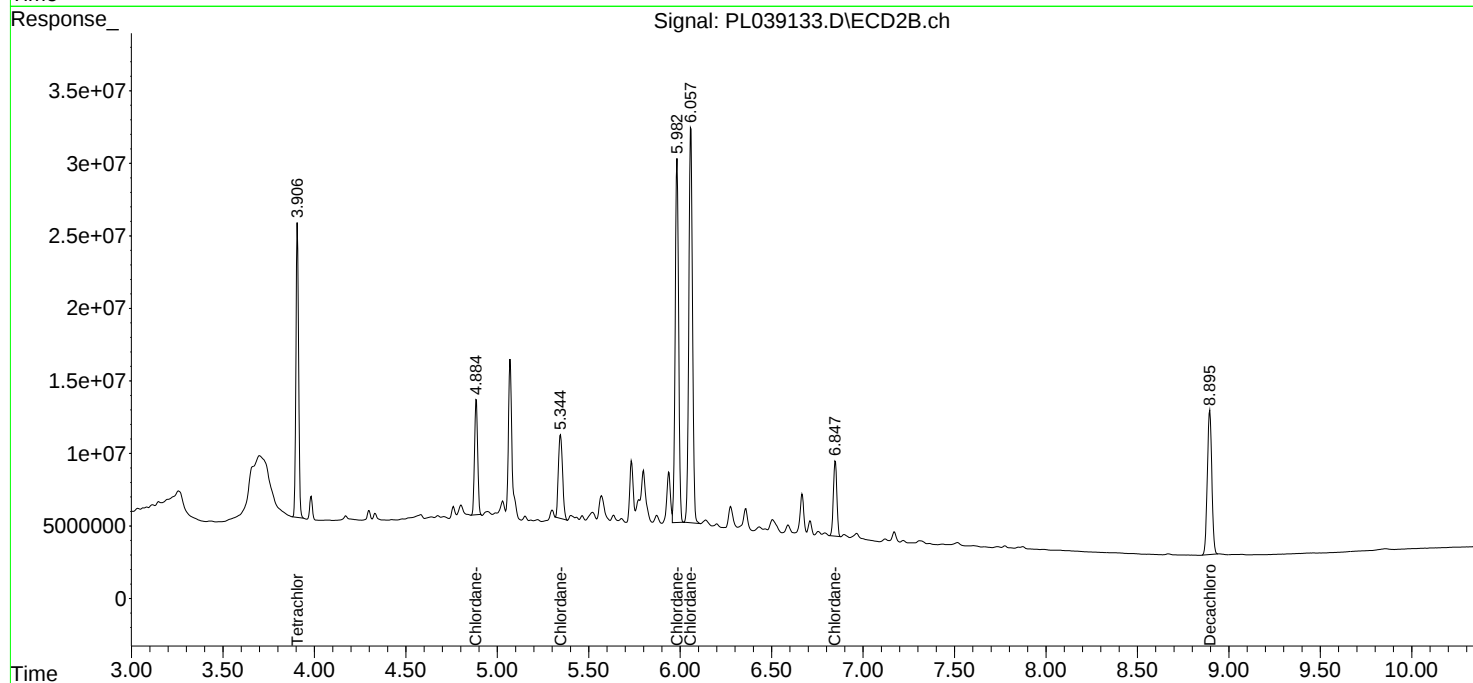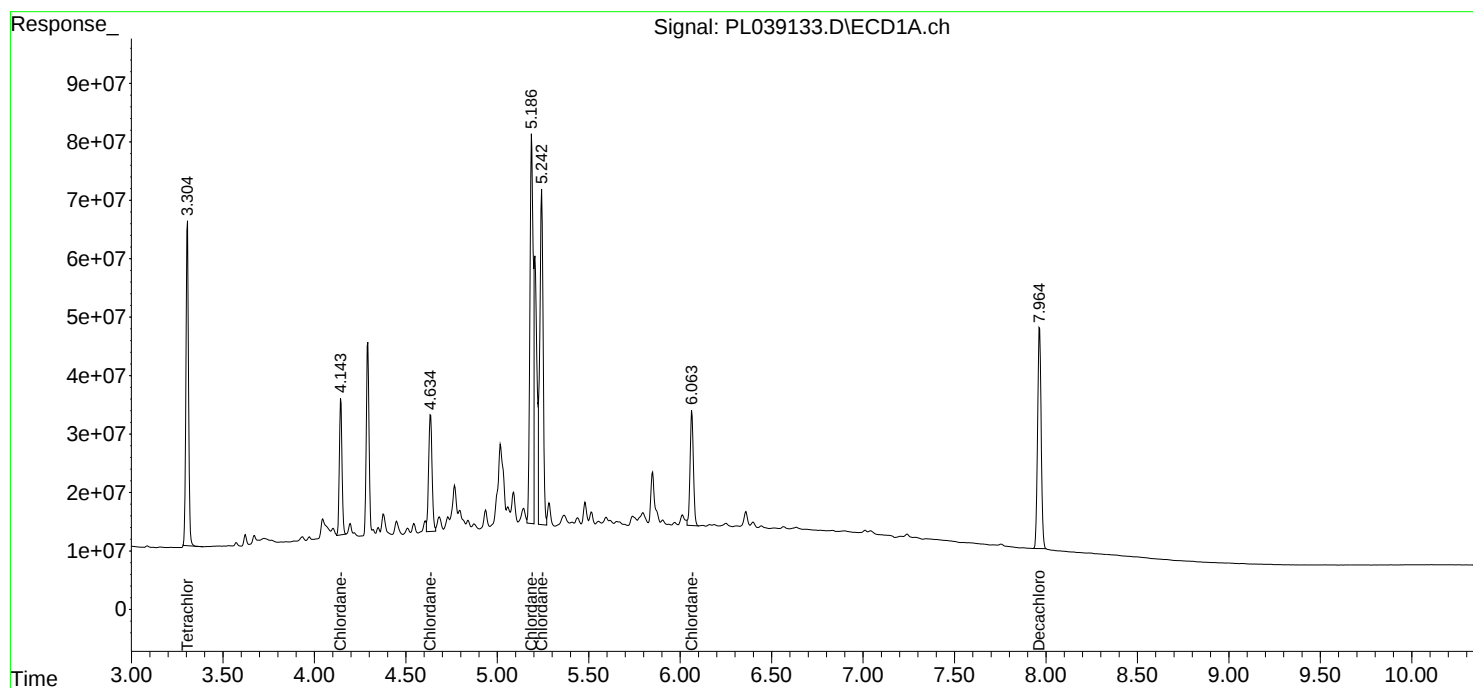


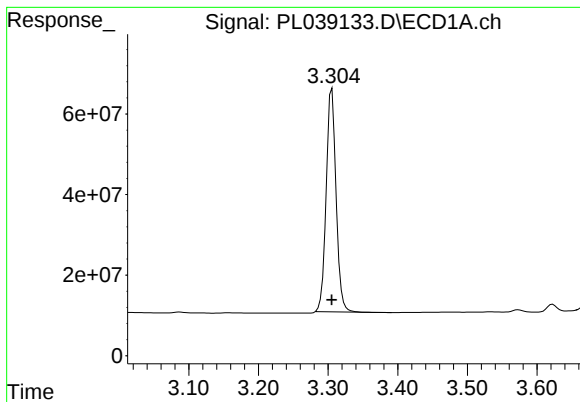

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: 0.000 min
Response: 545372539
Conc: 76.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

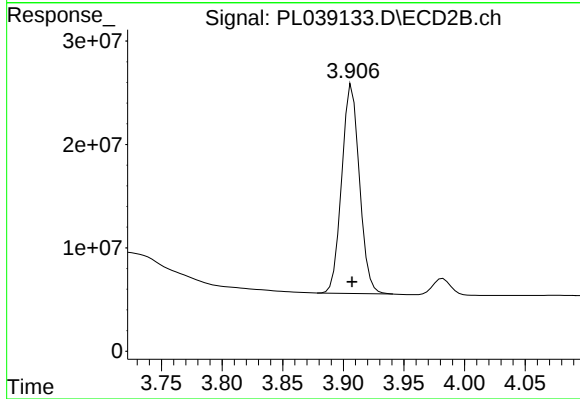


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 205346287
Conc: 76.16 ng/ml

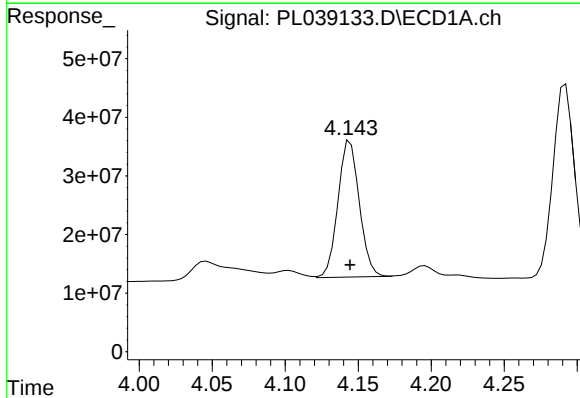


#23 Chlordane-1

R.T.: 4.145 min
Delta R.T.: 0.000 min
Response: 236730125
Conc: 691.33 ng/ml

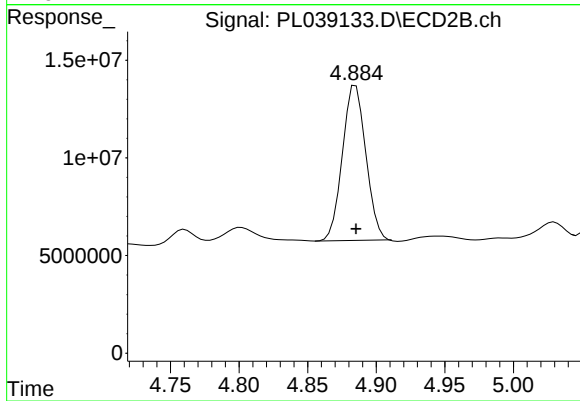

#23 Chlordane-1


R.T.: 4.885 min
Delta R.T.: 0.000 min
Response: 94118360
Conc: 737.95 ng/ml

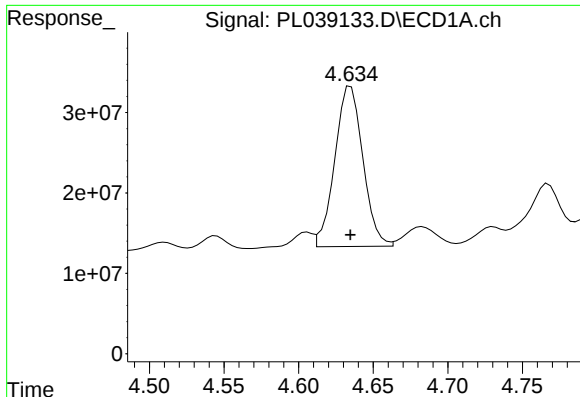

#24 Chlordane-2


R.T.: 4.635 min
Delta R.T.: 0.000 min
Response: 261535594
Conc: 731.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

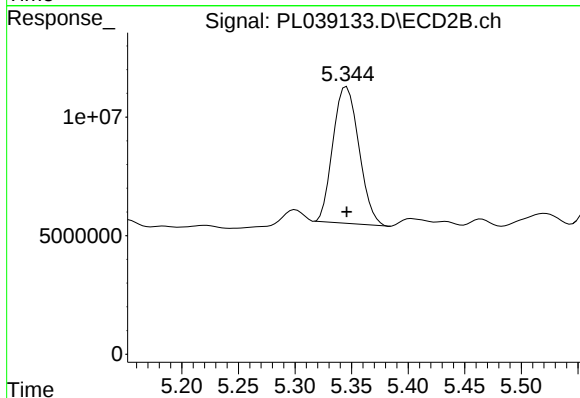


#24 Chlordane-2

R.T.: 5.346 min
Delta R.T.: 0.000 min
Response: 92216932
Conc: 733.20 ng/ml

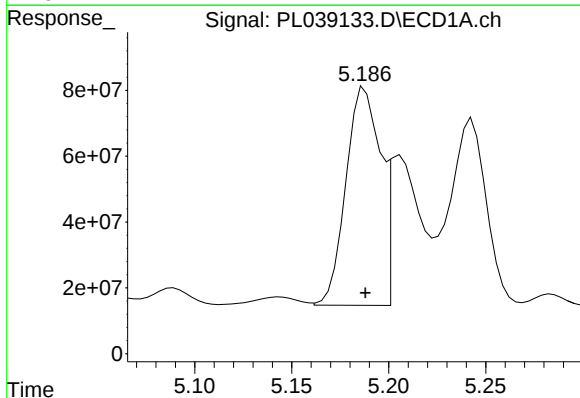


#25 Chlordane-3

R.T.: 5.188 min
Delta R.T.: 0.000 min
Response: 817374432
Conc: 722.41 ng/ml

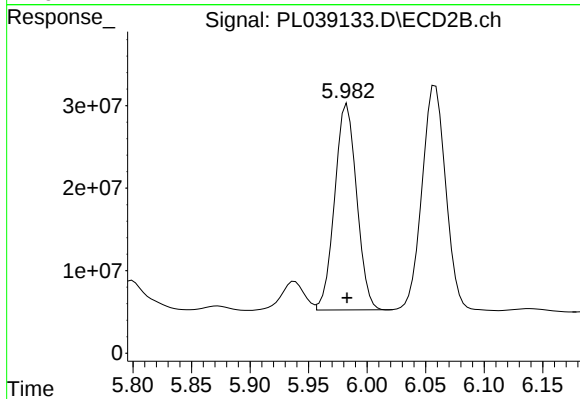

#25 Chlordane-3


R.T.: 5.983 min
Delta R.T.: 0.000 min
Response: 326070337
Conc: 744.62 ng/ml

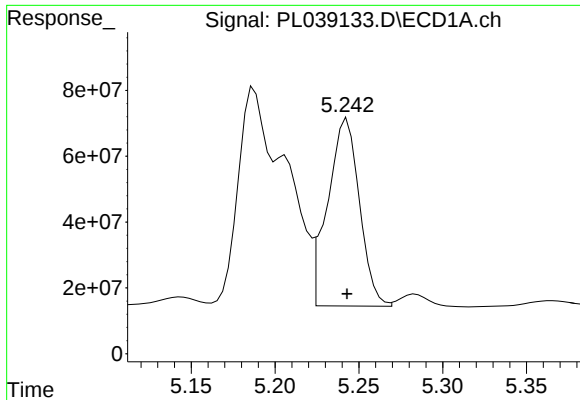

#26 Chlordane-4


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 752176218
Conc: 739.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

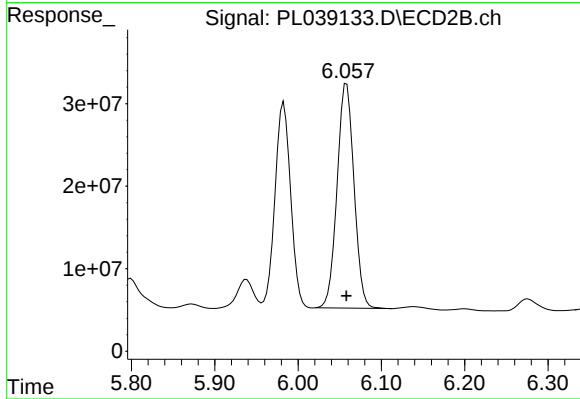


#26 Chlordane-4

R.T.: 6.058 min
Delta R.T.: 0.000 min
Response: 384526409
Conc: 735.98 ng/ml

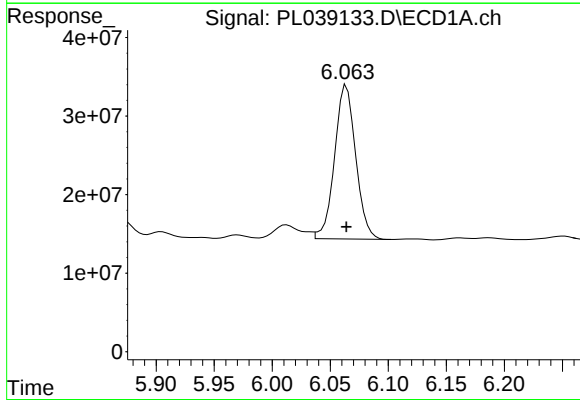


#27 Chlordane-5

R.T.: 6.064 min
Delta R.T.: 0.000 min
Response: 248490970
Conc: 734.07 ng/ml

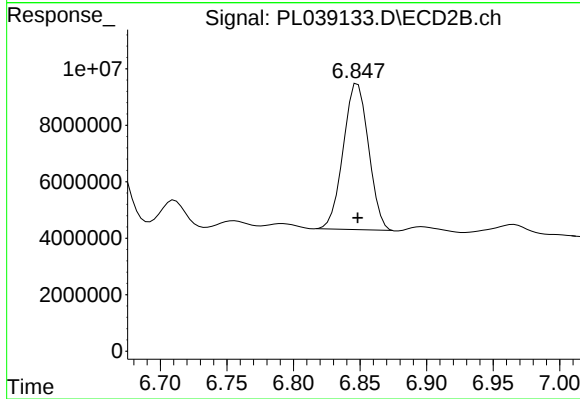

#27 Chlordane-5

R.T.: 6.848 min
Delta R.T.: 0.000 min
Response: 68393024
Conc: 733.43 ng/ml

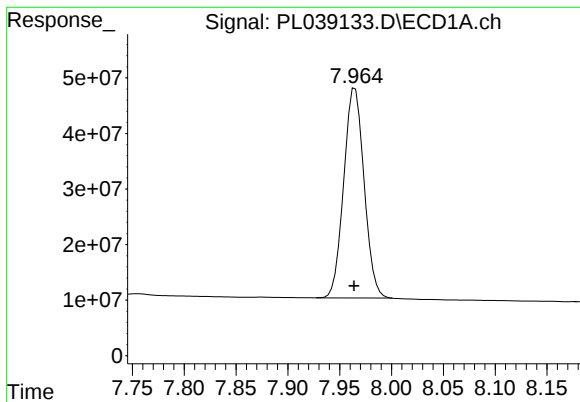

#28 Decachlorobiphenyl


R.T.: 7.965 min

Delta R.T.: 0.000 min

Response: 513611583

Conc: 72.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

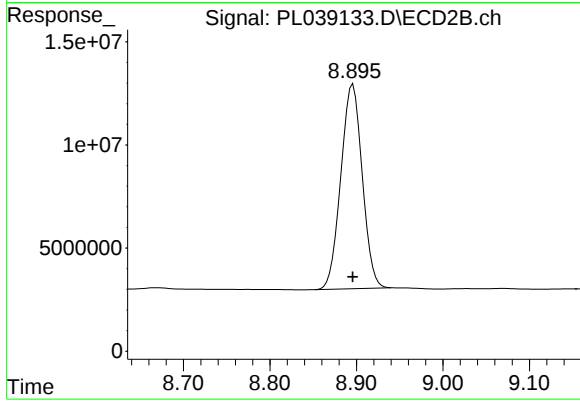

#28 Decachlorobiphenyl

R.T.: 8.896 min

Delta R.T.: 0.000 min

Response: 169656166

Conc: 72.54 ng/ml