

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
 Data File : PL051381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 08:57
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:36:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) MB Aldrin	4.549	0.000	91619552	0	5.914	N.D.	#
6) B beta-BHC	0.000	4.777	0	4038185	N.D.	2.336	#
7) B delta-BHC	4.475	0.000	16826456	0	1.025	N.D.	#
8) B Heptachlo...	0.000	5.790	0	18122085	N.D.	4.738	#
9) A Endosulfan I	5.338f	0.000	20927471	0	1.439	N.D.	#
10) B gamma-Chl...	5.208	0.000	99007079	0	6.273	N.D.	#
14) MA Endrin	5.820f	6.627	9625036	6949215	0.654	2.241	#
15) B Endosulfa...	6.081	0.000	5994676	0	0.428	N.D.	#
25) Chlordane-3	5.208	0.000	99007079	0	70.730	N.D.	#
27) Chlordane-5	6.081	0.000	5994676	0	11.802	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051381\
Data File : PL051381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 08:57
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:36:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

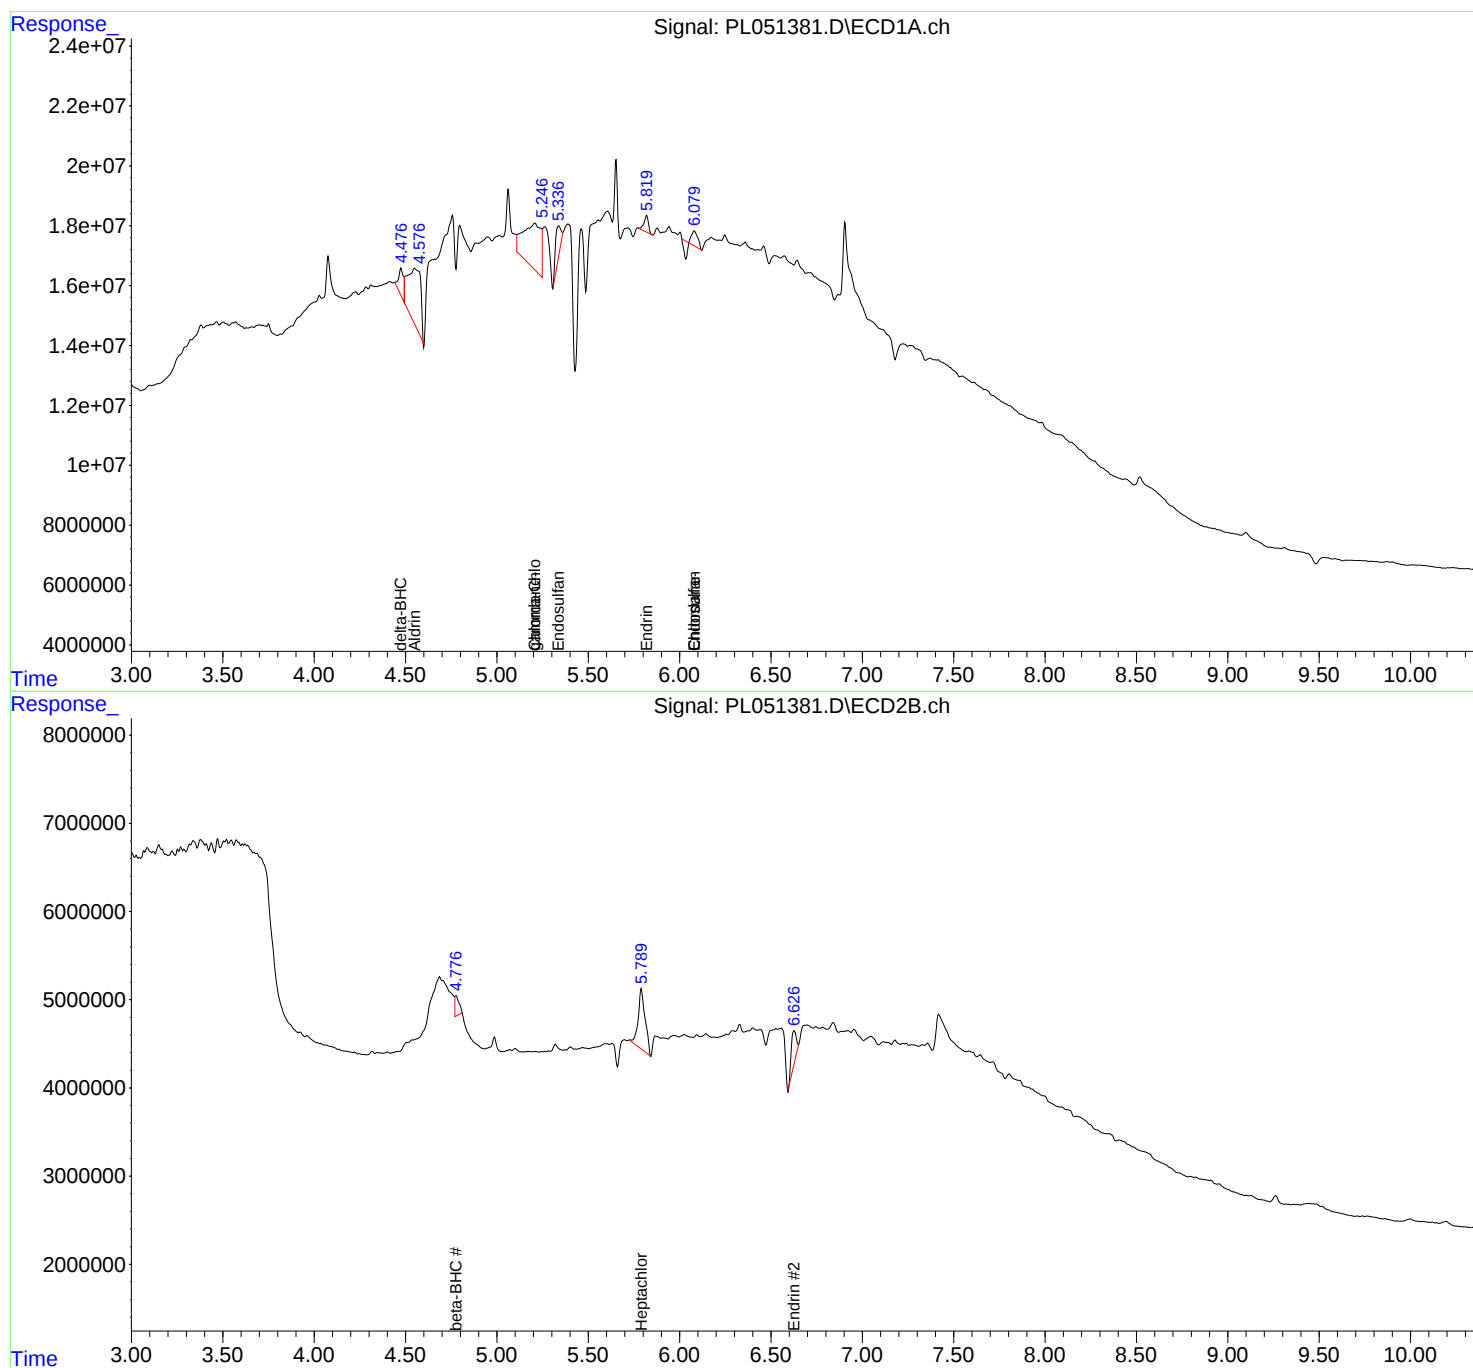


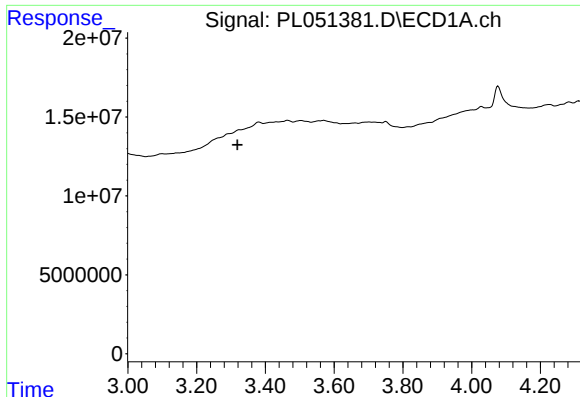

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.318 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

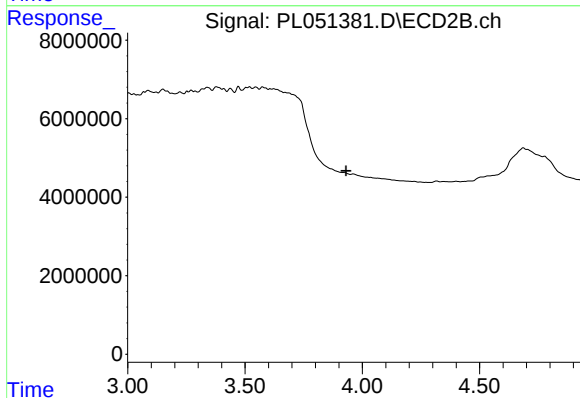


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.931 min
Response: 0
Conc: N.D.

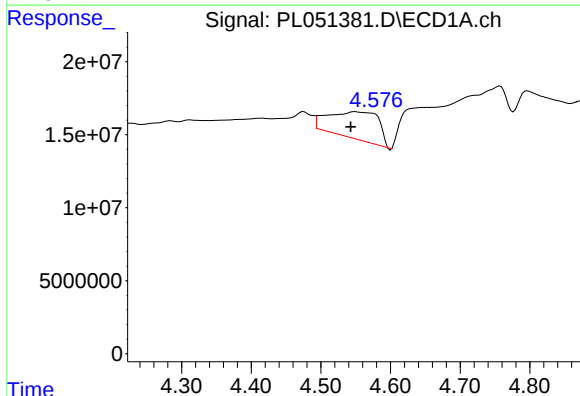


#5 Aldrin

R.T.: 4.549 min
Delta R.T.: 0.006 min
Response: 91619552
Conc: 5.91 ng/ml

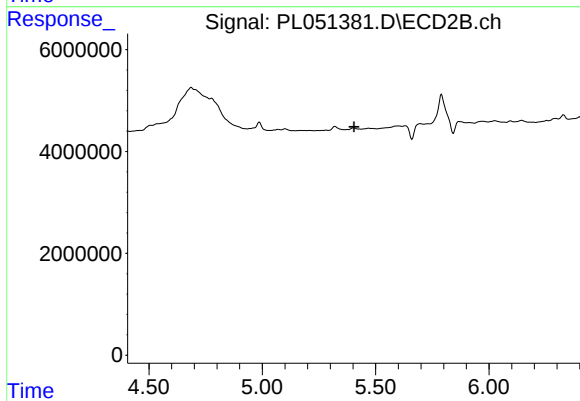

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.405 min
Response: 0
Conc: N.D.

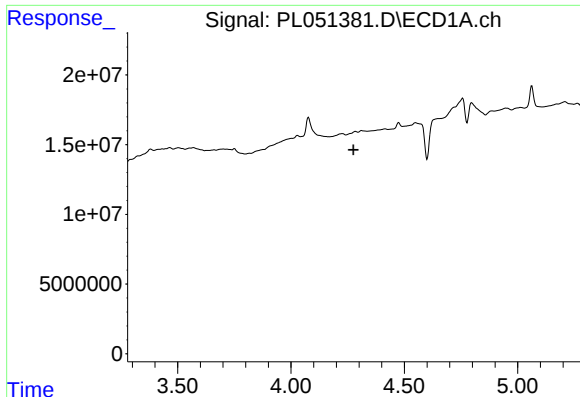

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

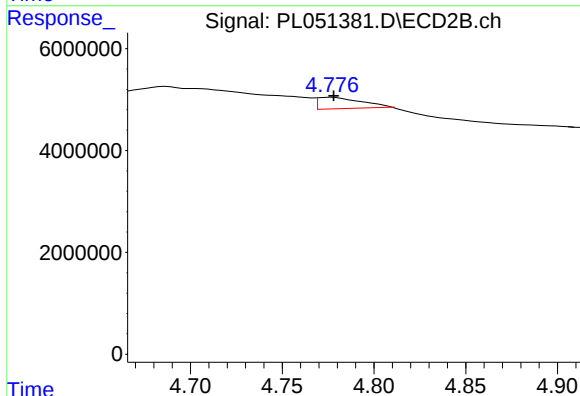


#6 beta-BHC

R.T.: 4.777 min
Delta R.T.: 0.000 min
Response: 4038185
Conc: 2.34 ng/ml

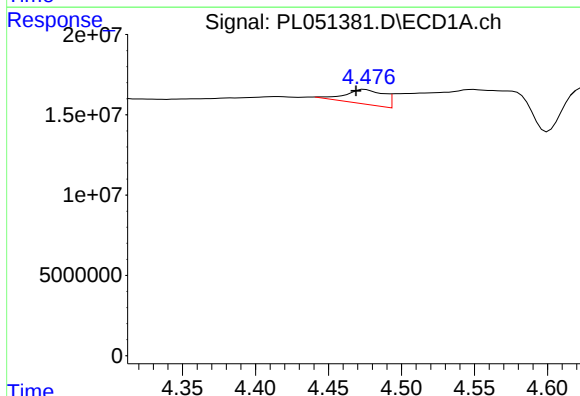


#7 delta-BHC

R.T.: 4.475 min
Delta R.T.: 0.006 min
Response: 16826456
Conc: 1.03 ng/ml

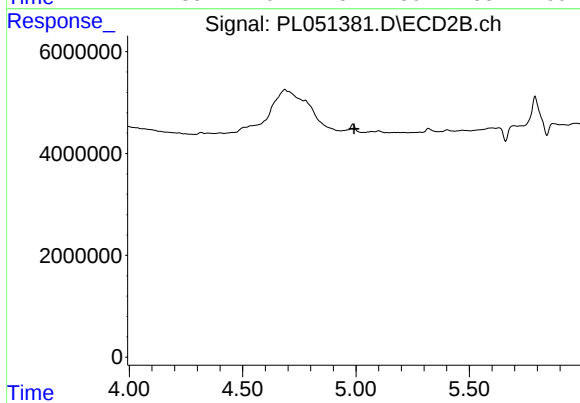

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.991 min
Response: 0
Conc: N.D.

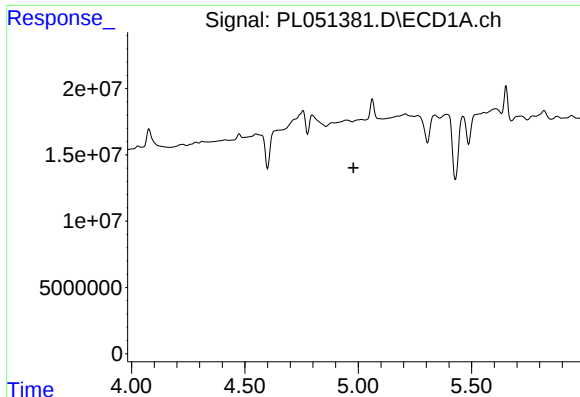

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

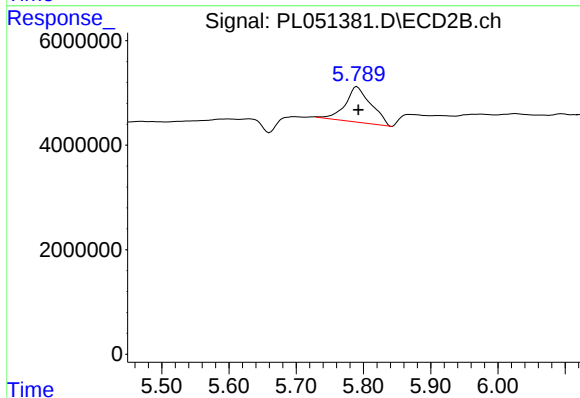


#8 Heptachlor epoxide

R.T.: 5.790 min
Delta R.T.: -0.002 min
Response: 18122085
Conc: 4.74 ng/ml

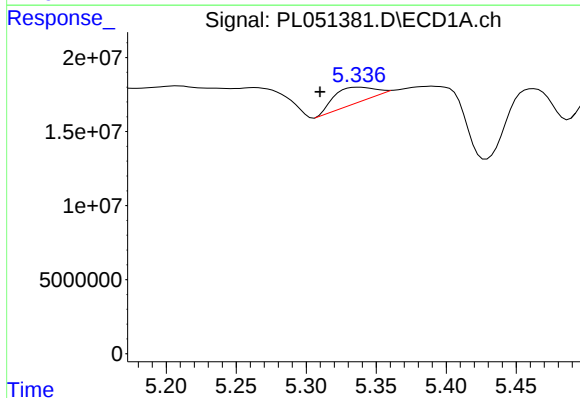


#9 Endosulfan I

R.T.: 5.338 min
Delta R.T.: 0.028 min
Response: 20927471
Conc: 1.44 ng/ml

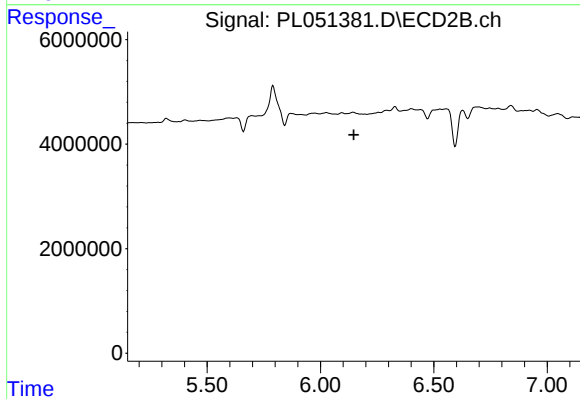

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.148 min
Response: 0
Conc: N.D.

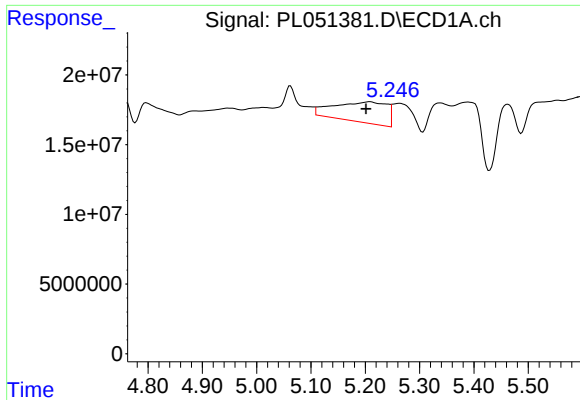

#10 gamma-Chlordane


R.T.: 5.208 min
Delta R.T.: 0.007 min
Response: 99007079
Conc: 6.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

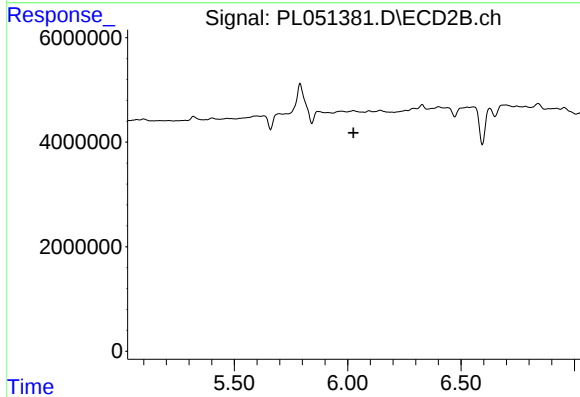


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

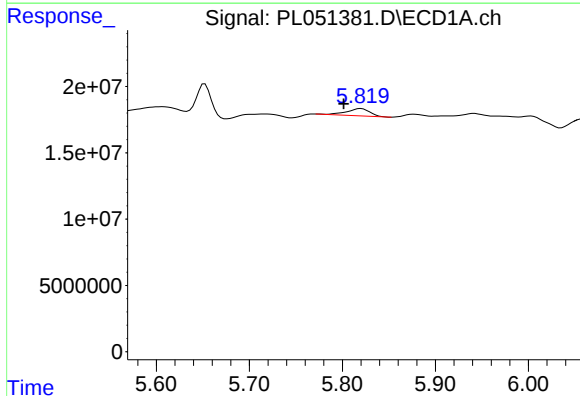


#14 Endrin

R.T.: 5.820 min
Delta R.T.: 0.019 min
Response: 9625036
Conc: 0.65 ng/ml

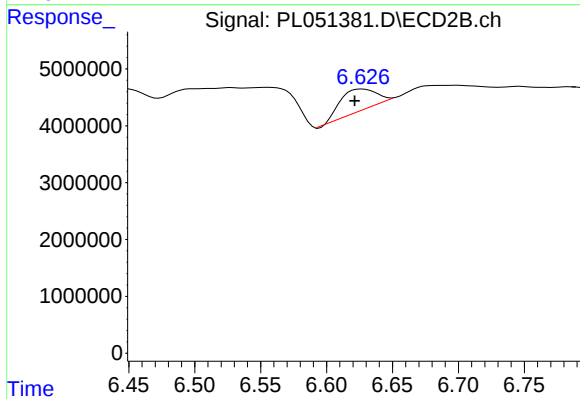

#14 Endrin


R.T.: 6.627 min
Delta R.T.: 0.006 min
Response: 6949215
Conc: 2.24 ng/ml

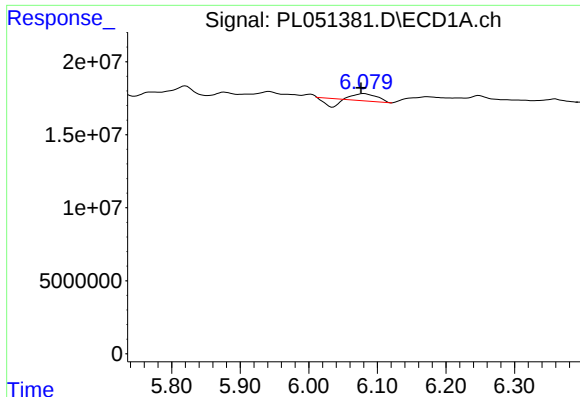

#15 Endosulfan II


R.T.: 6.081 min
Delta R.T.: 0.005 min
Response: 5994676
Conc: 0.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

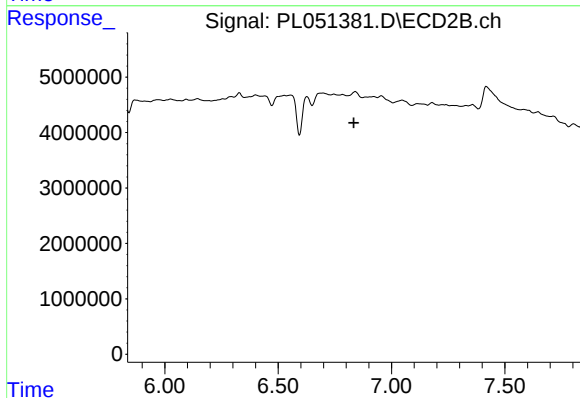


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.833 min
Response: 0
Conc: N.D.

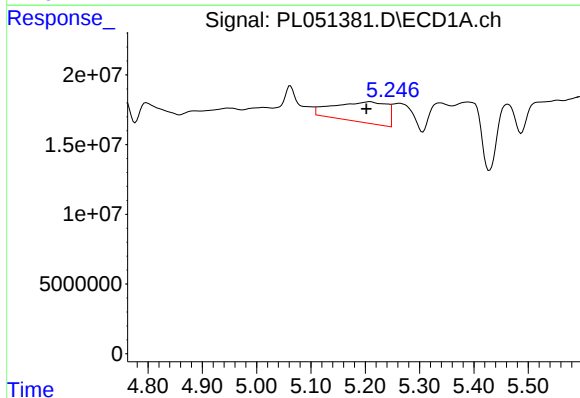


#25 Chlordane-3

R.T.: 5.208 min
Delta R.T.: 0.006 min
Response: 99007079
Conc: 70.73 ng/ml

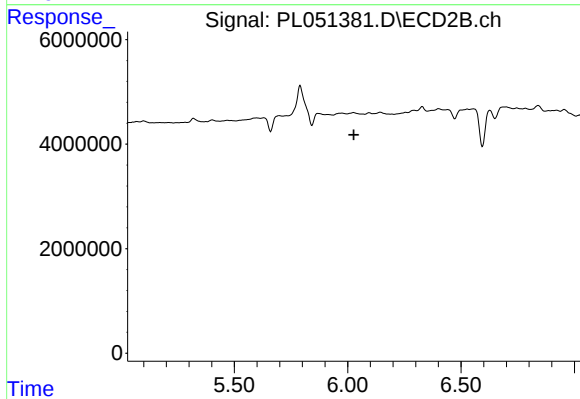

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

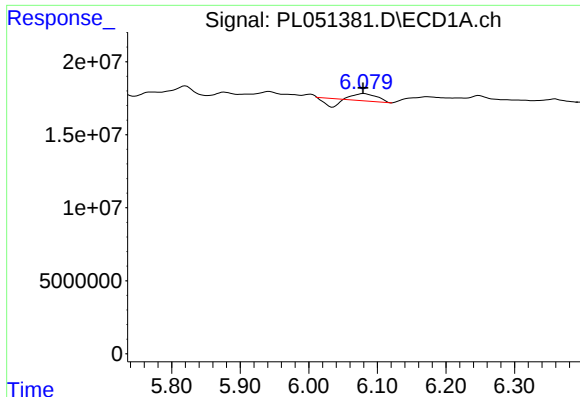

#27 Chlordane-5


R.T.: 6.081 min
Delta R.T.: 0.002 min
Response: 5994676
Conc: 11.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

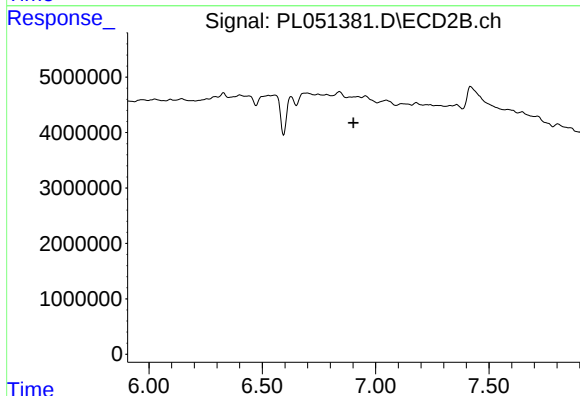


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.902 min
Response: 0
Conc: N.D.

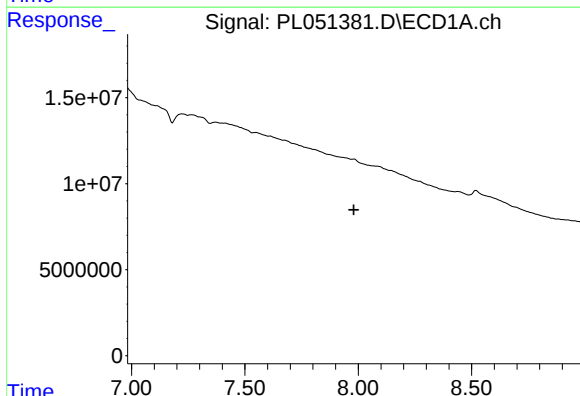

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.981 min
Response: 0
Conc: N.D.

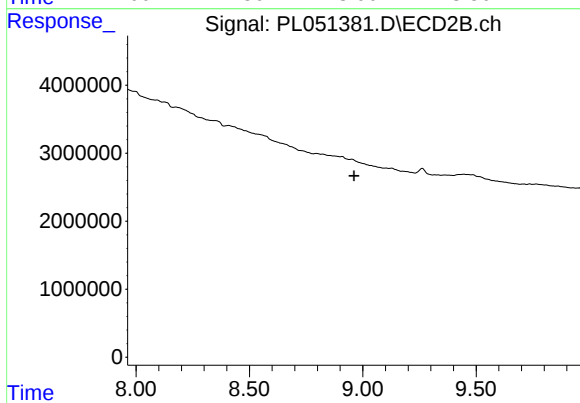

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.