

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
 Data File : PL051443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 23:49
 Operator : SM\AJ
 Sample : PB122219BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB122219BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:50:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	255.8E6	67568805	25.454	23.682
28)	SA Decachlor...	7.976	8.956	250.5E6	66292559	24.741	23.442
Target Compounds							
6)	B beta-BHC	0.000	4.803f	0	4131765	N.D.	2.390 #
8)	B Heptachlo...	0.000	5.803	0	3258423	N.D.	0.852 #
11)	B alpha-Chl...	5.244	0.000	10703025	0	0.702	N.D. #
15)	B Endosulfa...	0.000	6.846	0	7791588	N.D.	2.451 #
19)	B Endosulfa...	6.465	0.000	34909428	0	2.740	N.D. #
26)	Chlordane-4	5.244	0.000	10703025	0	8.115	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
Data File : PL051443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 23:49
Operator : SM\AJ
Sample : PB122219BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PB122219BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:50:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

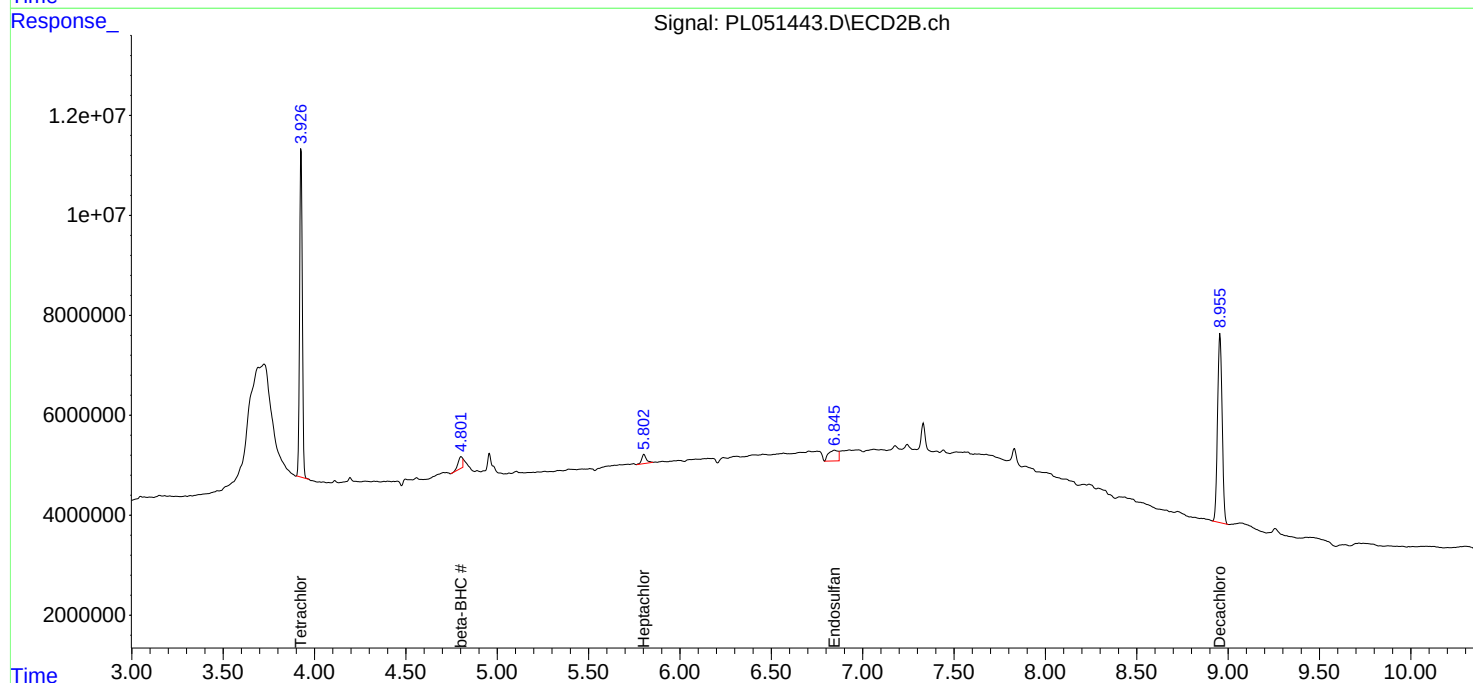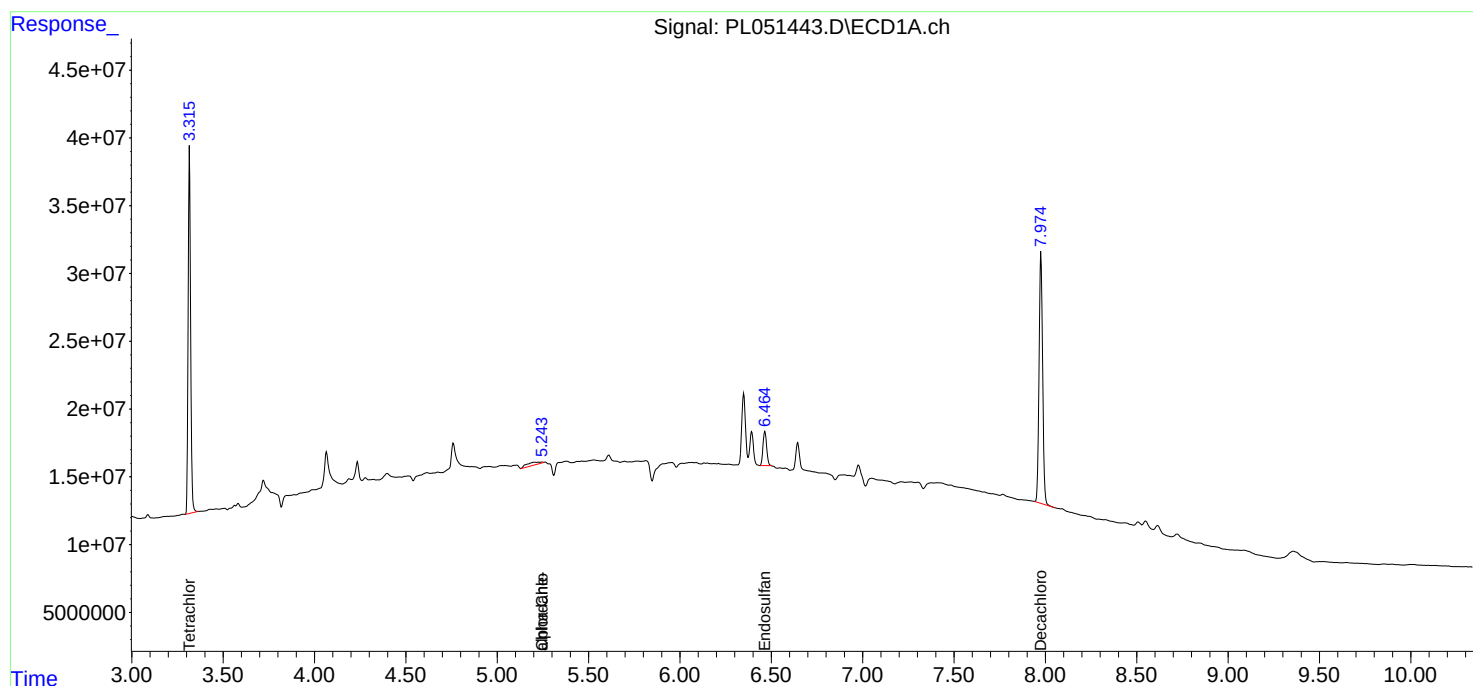


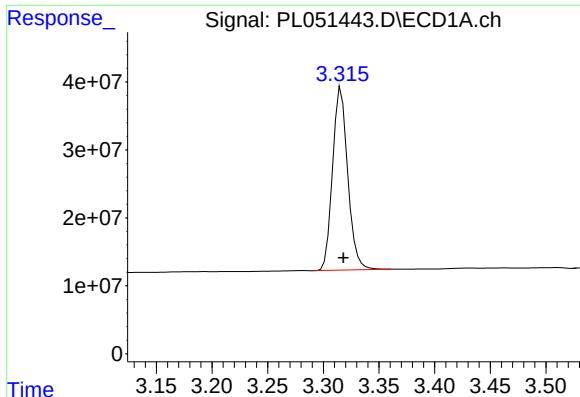

#1 Tetrachloro-m-xylene


R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 255761276
Conc: 25.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122219BL

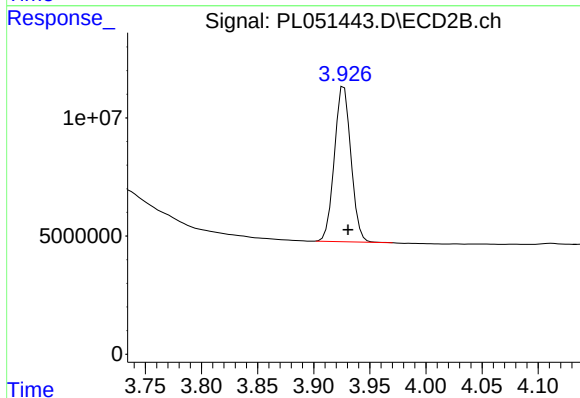


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.004 min
Response: 67568805
Conc: 23.68 ng/ml

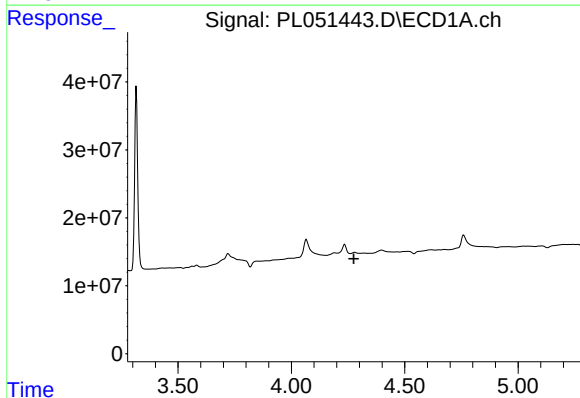


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.276 min
Response: 0
Conc: N.D.

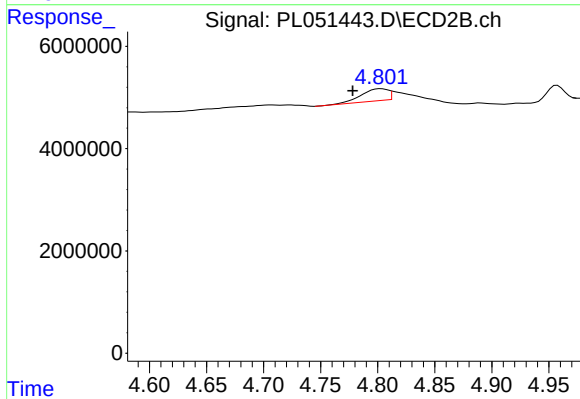

#6 beta-BHC


R.T.: 4.803 min
Delta R.T.: 0.025 min
Response: 4131765
Conc: 2.39 ng/ml

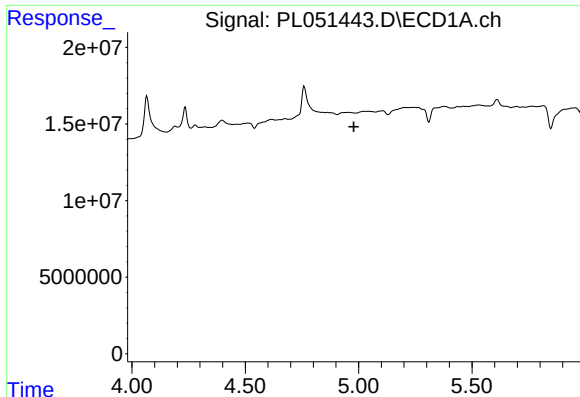

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 4.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122219BL

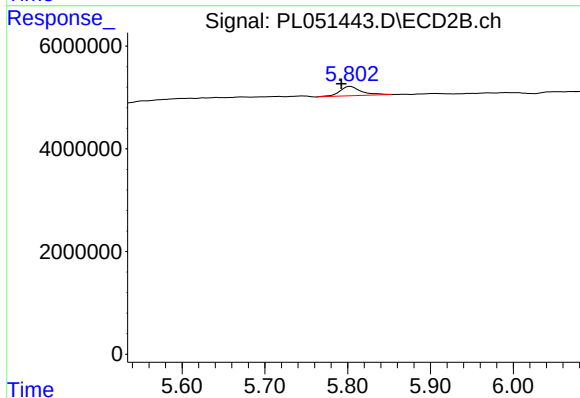


#8 Heptachlor epoxide

R.T.: 5.803 min
Delta R.T.: 0.011 min
Response: 3258423
Conc: 0.85 ng/ml

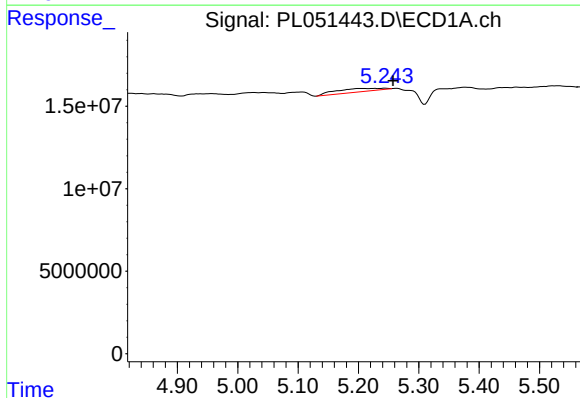


#11 alpha-Chlordane

R.T.: 5.244 min
Delta R.T.: -0.013 min
Response: 10703025
Conc: 0.70 ng/ml

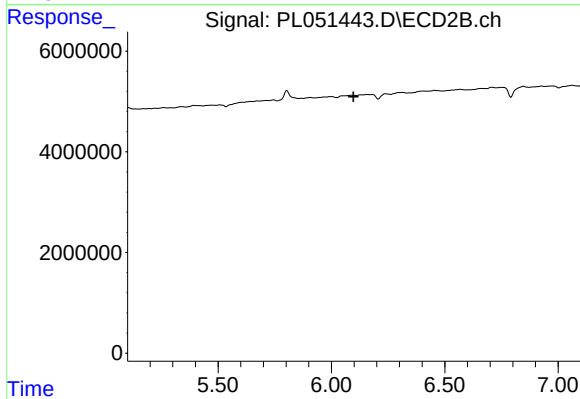

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.098 min
Response: 0
Conc: N.D.

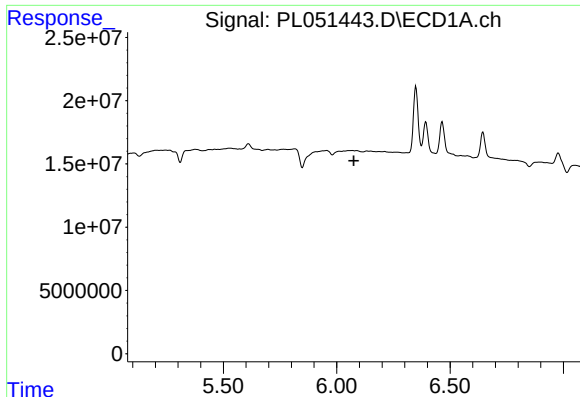

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB122219BL

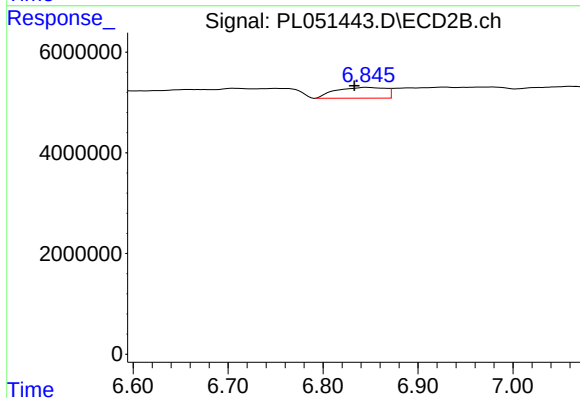


#15 Endosulfan II

R.T.: 6.846 min
Delta R.T.: 0.013 min
Response: 7791588
Conc: 2.45 ng/ml

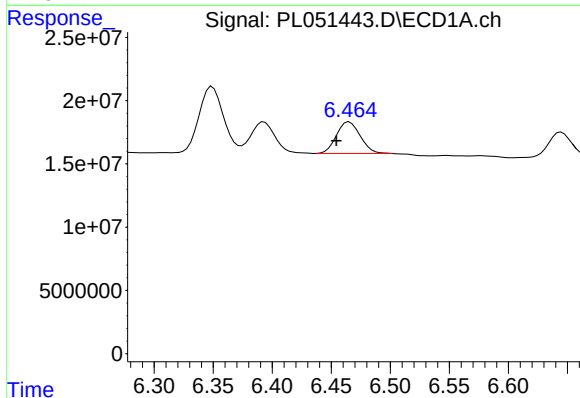


#19 Endosulfan Sulfate

R.T.: 6.465 min
Delta R.T.: 0.011 min
Response: 34909428
Conc: 2.74 ng/ml

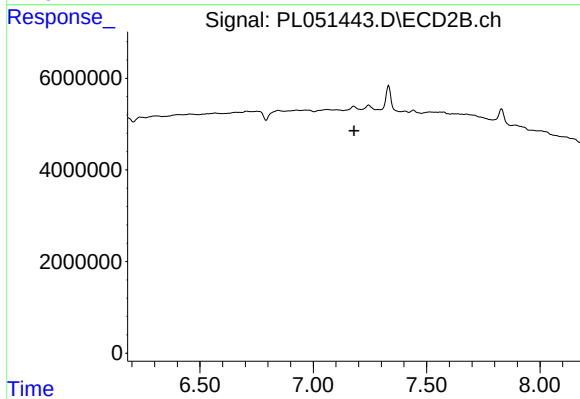

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.180 min
Response: 0
Conc: N.D.

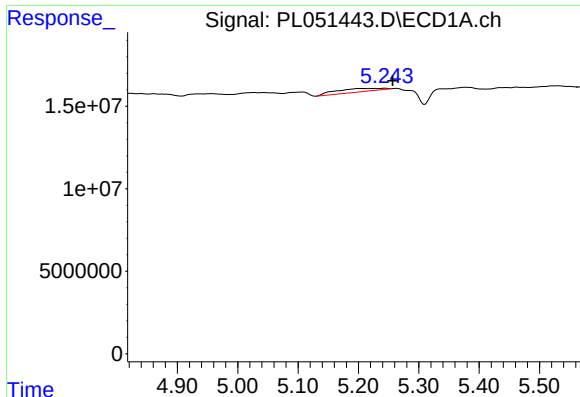

#26 Chlordane-4


R.T.: 5.244 min
Delta R.T.: -0.013 min
Response: 10703025
Conc: 8.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB122219BL

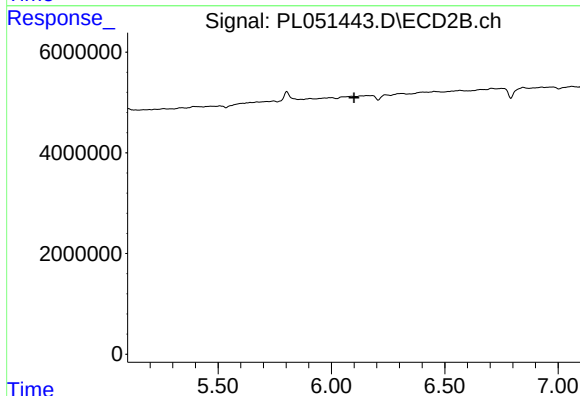


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 6.100 min
Response: 0
Conc: N.D.

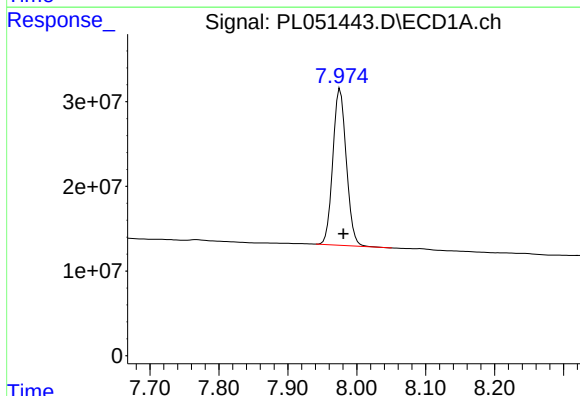

#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 250514963
Conc: 24.74 ng/ml

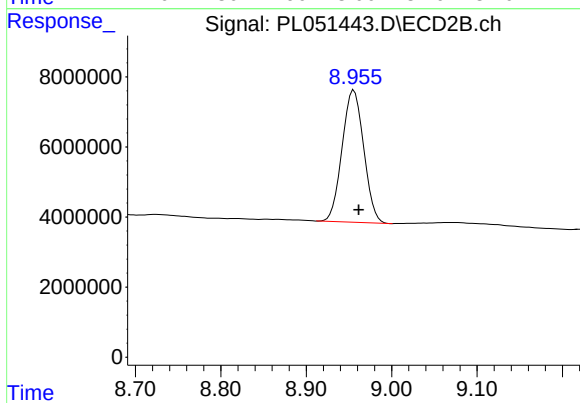

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.006 min
Response: 66292559
Conc: 23.44 ng/ml