

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
 Data File : PL051404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 14:35
 Operator : SM\AJ
 Sample : K4282-06 (Sig #1); K4288-06 (Sig #2)
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-035-B241-080819

Manual Integrations
 APPROVED

Ankita
 8/14/2019 4:53:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:41:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	197.6E6	51981688	19.664	18.219
28)	SA Decachlor...	7.976	8.956	128.7E6	32154658	12.711	11.370
Target Compounds							
17)	MA 4,4'-DDT	6.166	7.037	10023831	2615523	0.809m	0.969m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
Data File : PL051404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 14:35
Operator : SM\AJ
Sample : K4282-06 (Sig #1); K4288-06 (Sig #2)
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-035-B241-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:41:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

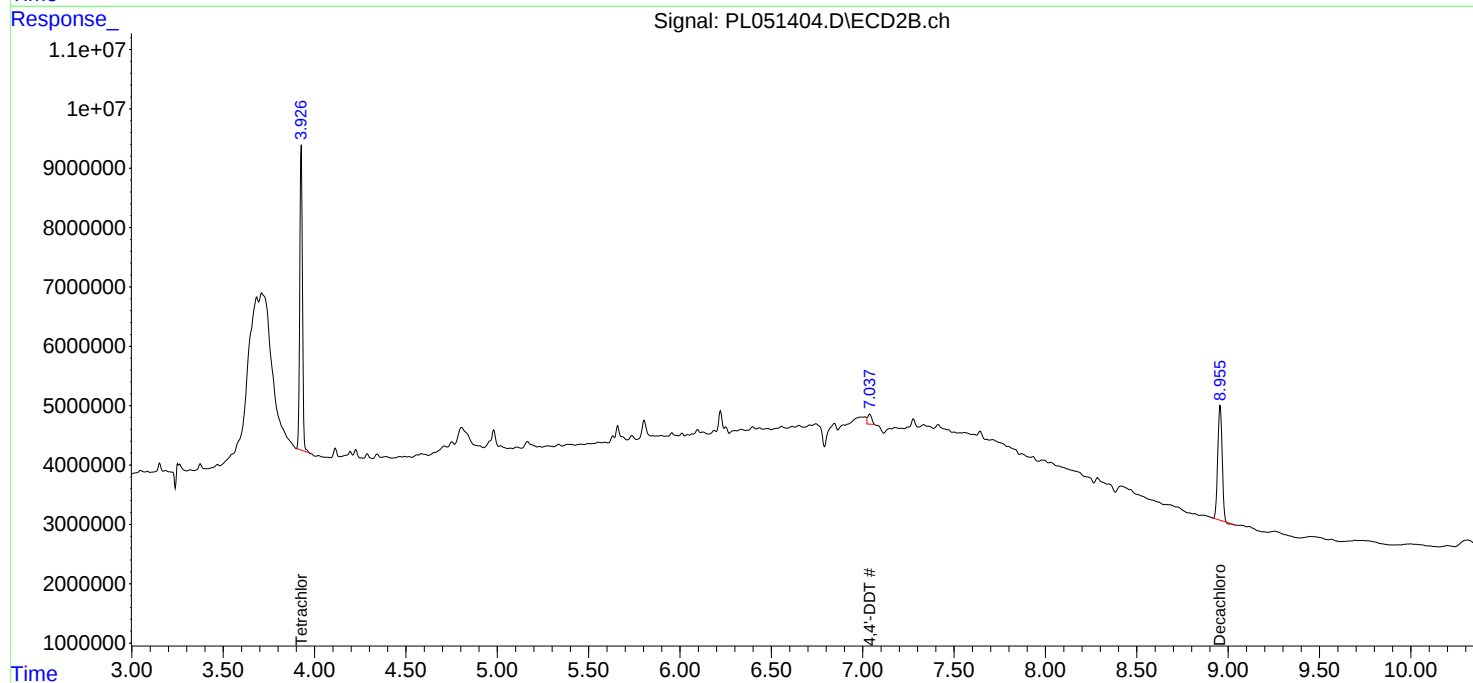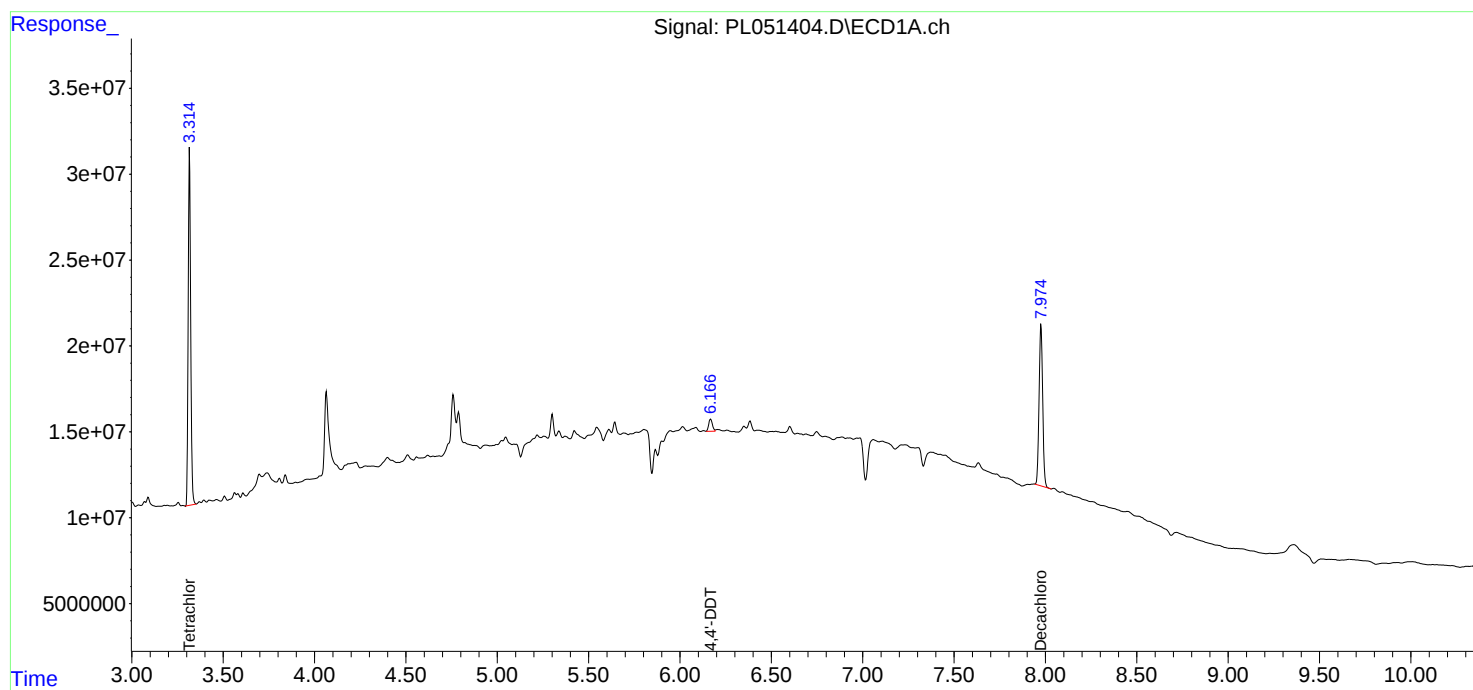

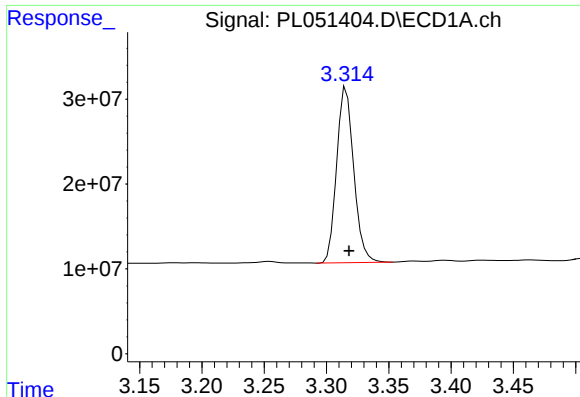


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 197577100
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B241-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:25 PM

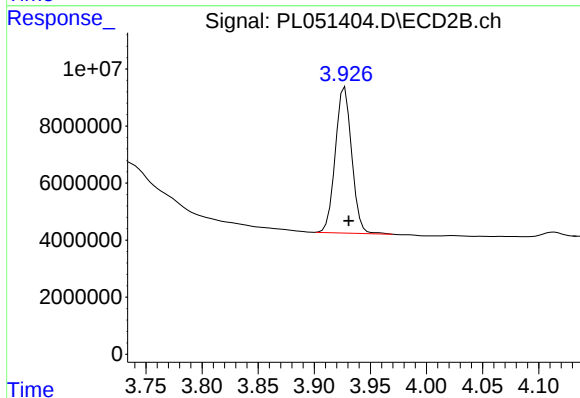


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 51981688
Conc: 18.22 ng/ml

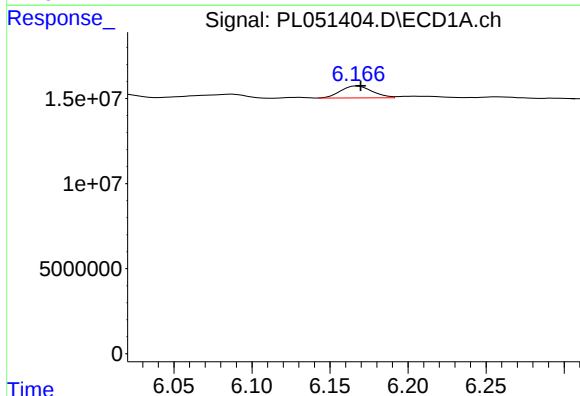


#17 4,4'-DDT

R.T.: 6.166 min
Delta R.T.: -0.003 min
Response: 10023831
Conc: 0.81 ng/ml m

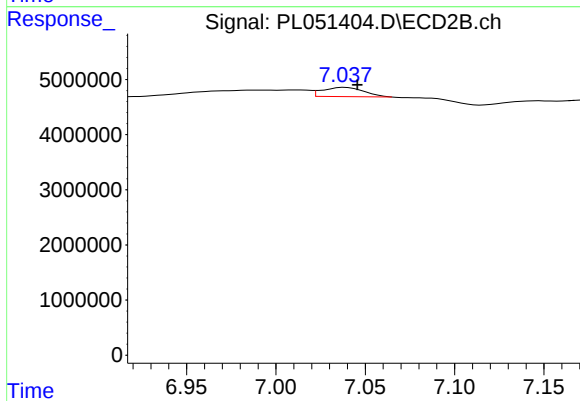

#17 4,4'-DDT

R.T.: 7.037 min
Delta R.T.: -0.008 min
Response: 2615523
Conc: 0.97 ng/ml m

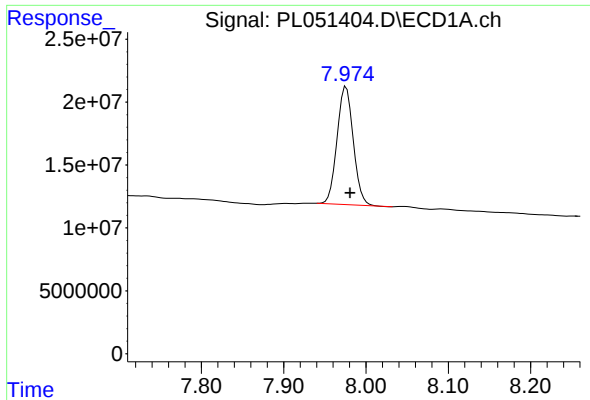


#28 Decachlorobiphenyl

R.T.: 7.976 min
Delta R.T.: -0.005 min
Response: 128700417
Conc: 12.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-035-B241-080819

Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:25 PM

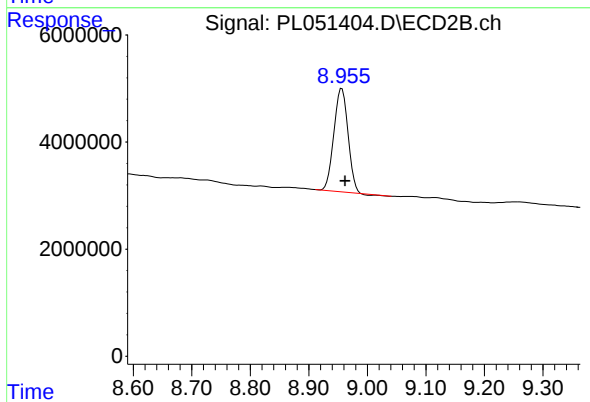

#28 Decachlorobiphenyl

R.T.: 8.956 min
Delta R.T.: -0.005 min
Response: 32154658
Conc: 11.37 ng/ml