

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
 Data File : PL051414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 16:58
 Operator : SM\AJ
 Sample : K4282-14
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-029-B216-080819

Manual Integrations
 APPROVED

Ankita
 8/14/2019 4:53:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:43:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	279.3E6	71809294	27.796	25.168
28)	SA Decachlor...	7.977	8.957	223.2E6	61597282	22.046	21.782
Target Compounds							
13)	MA Dieldrin	5.543	6.399	66239118	14407729	4.274m	4.069
17)	MA 4,4'-DDT	6.164	7.040	5596702	1107547	0.452m	0.410m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
Data File : PL051414.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 16:58
Operator : SM\AJ
Sample : K4282-14
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-029-B216-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:43:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

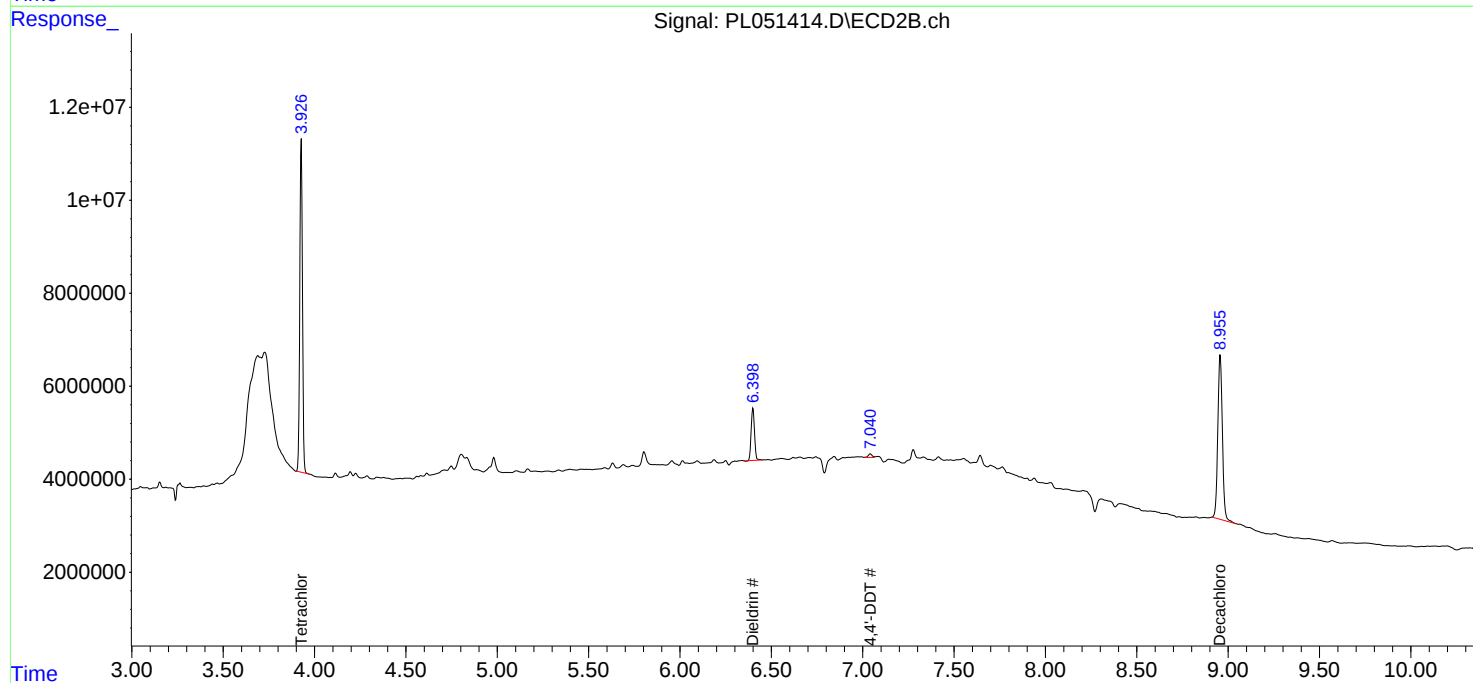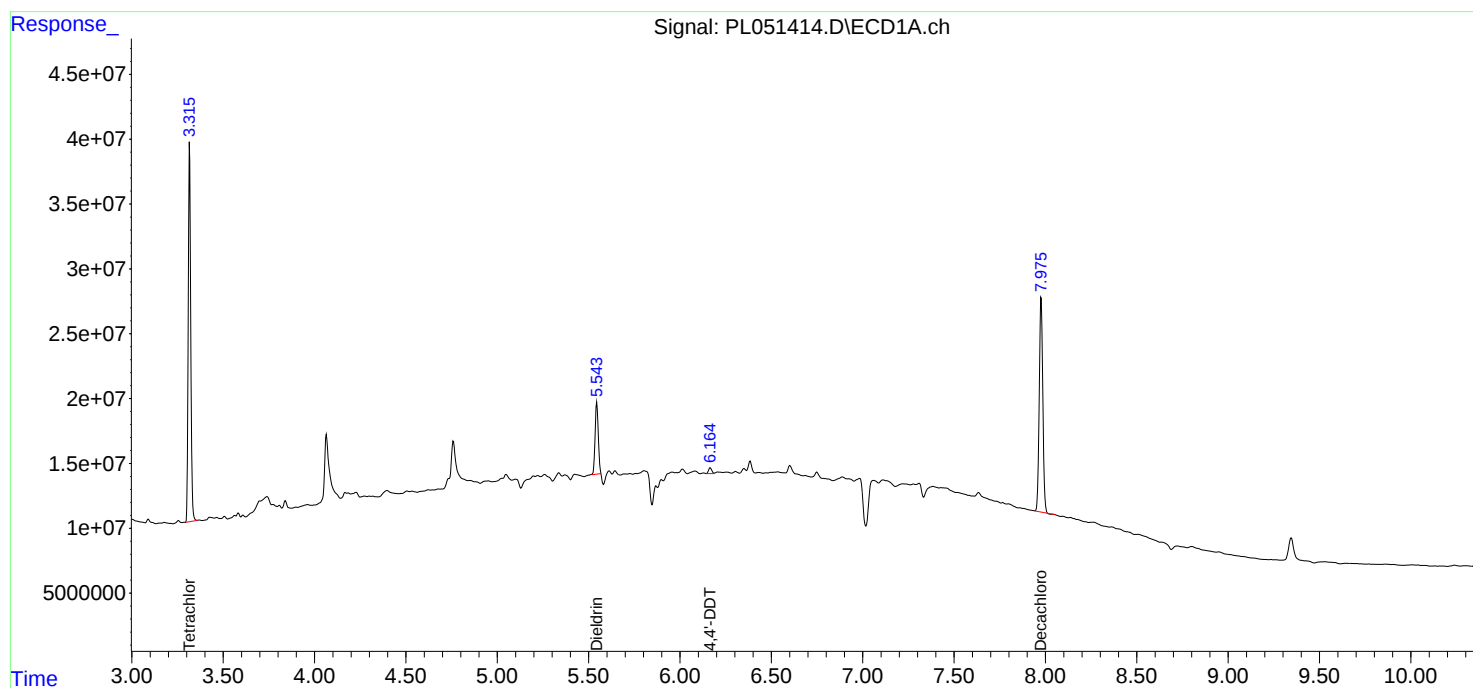

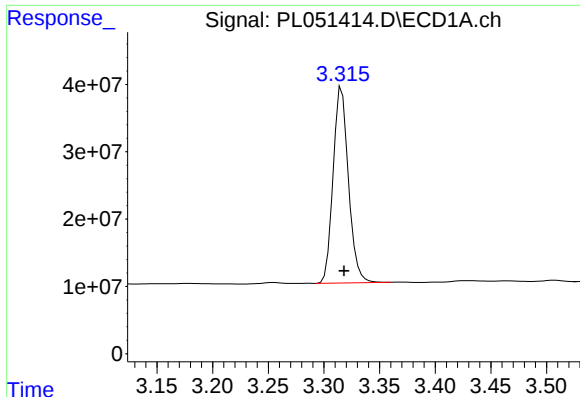


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 279286207
Conc: 27.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-029-B216-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:50 PM

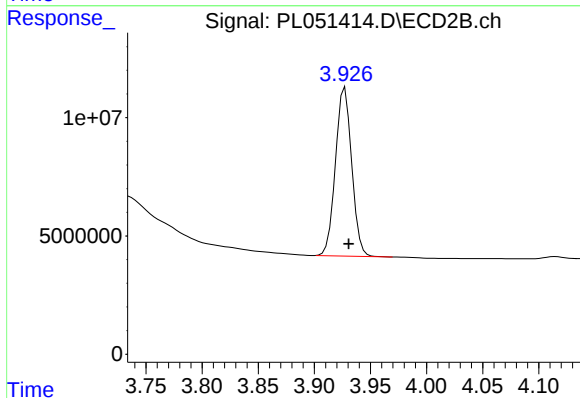


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 71809294
Conc: 25.17 ng/ml

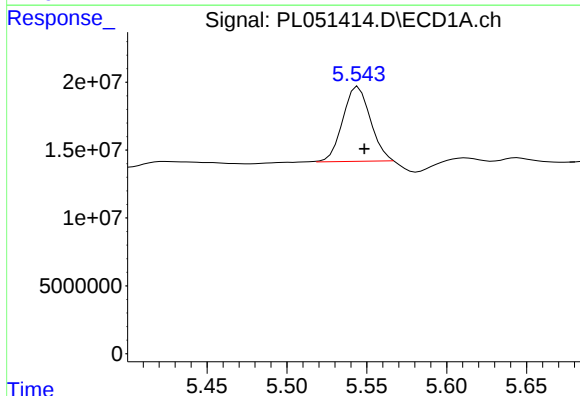


#13 Dieldrin

R.T.: 5.543 min
Delta R.T.: -0.005 min
Response: 66239118
Conc: 4.27 ng/ml m

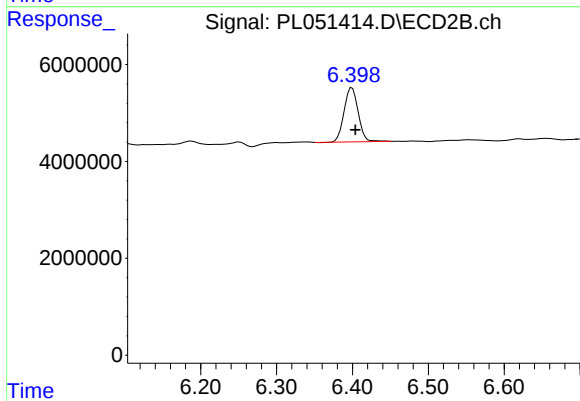

#13 Dieldrin

R.T.: 6.399 min
Delta R.T.: -0.004 min
Response: 14407729
Conc: 4.07 ng/ml

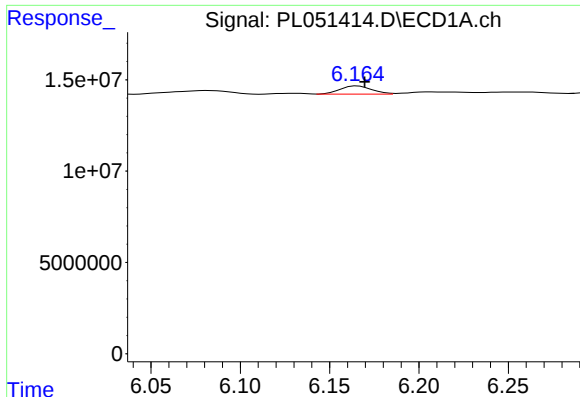


#17 4,4'-DDT

R.T.: 6.164 min
Delta R.T.: -0.005 min
Response: 5596702
Conc: 0.45 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PST-029-B216-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:50 PM

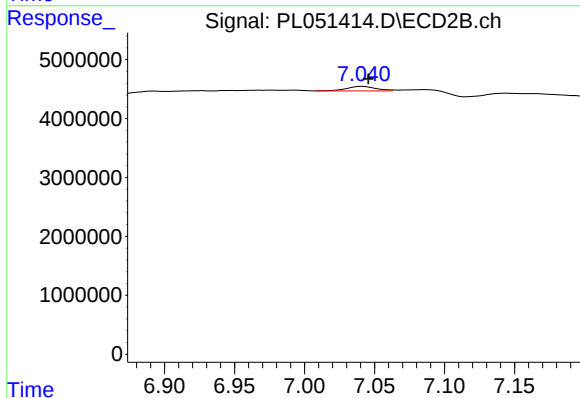


#17 4,4'-DDT

R.T.: 7.040 min
Delta R.T.: -0.005 min
Response: 1107547
Conc: 0.41 ng/ml m

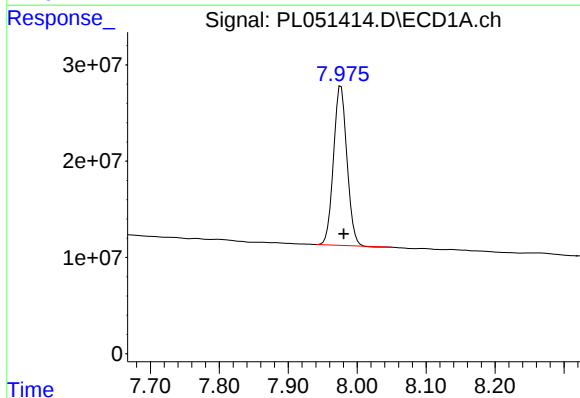

#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 223223707
Conc: 22.05 ng/ml

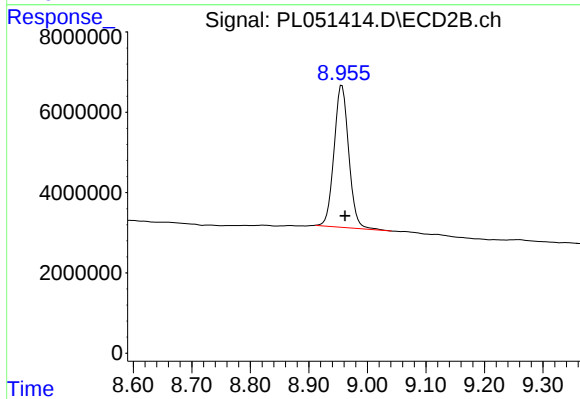

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 61597282
Conc: 21.78 ng/ml