

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
 Data File : PL051418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2019 17:54
 Operator : SM\AJ
 Sample : K4282-16
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-010-B225-080819

Manual Integrations
 APPROVED

Ankita
 8/14/2019 4:53:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 00:44:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 19 01:19:13 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.316	3.927	240.3E6	58562727	23.914	20.525
28)	SA Decachlor...	7.977	8.957	121.4E6	31570025	11.992	11.164
Target Compounds							
12)	B 4,4'-DDE	5.420	6.250	23067027	3250964	1.539m	0.902m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL081319\
Data File : PL051418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2019 17:54
Operator : SM\AJ
Sample : K4282-16
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-010-B225-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 00:44:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL071719.M
Quant Title : GC Extractables
QLast Update : Fri Jul 19 01:19:13 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

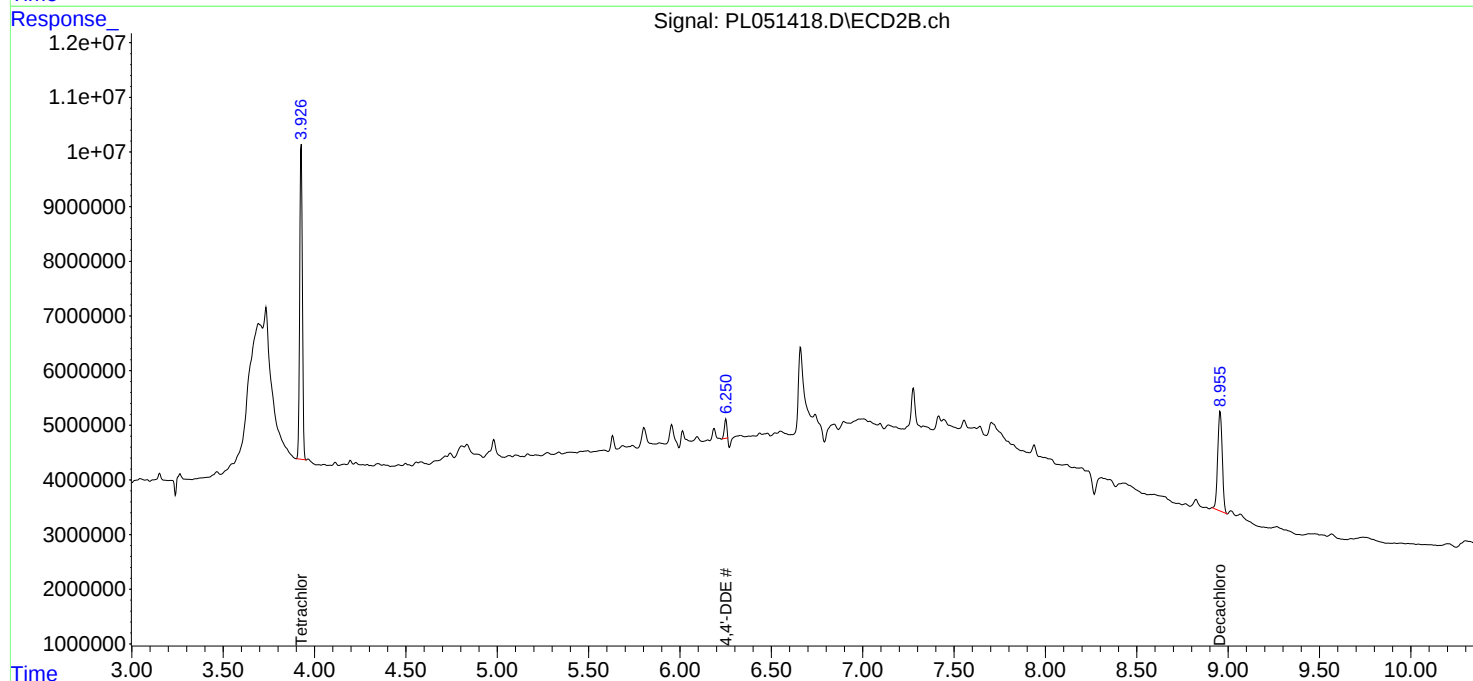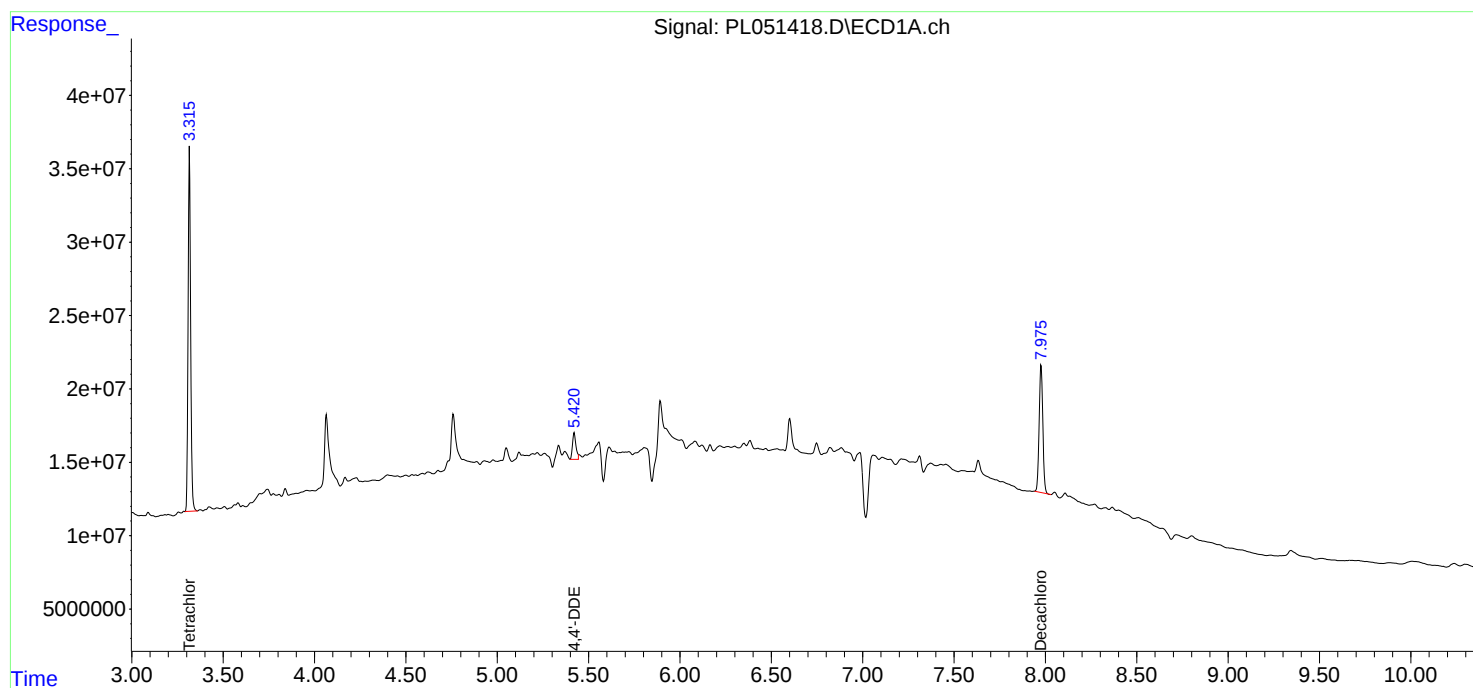

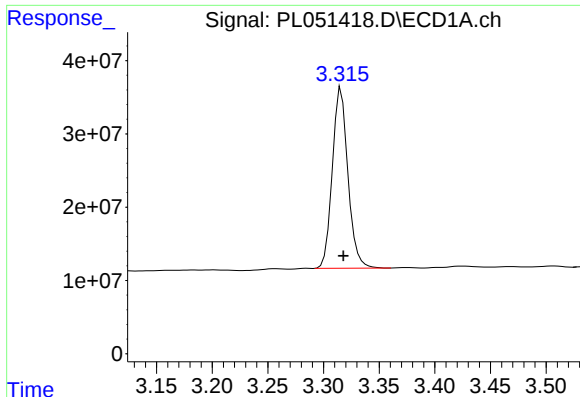


#1 Tetrachloro-m-xylene

R.T.: 3.316 min
Delta R.T.: -0.002 min
Response: 240286386
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-010-B225-080819


Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:57 PM

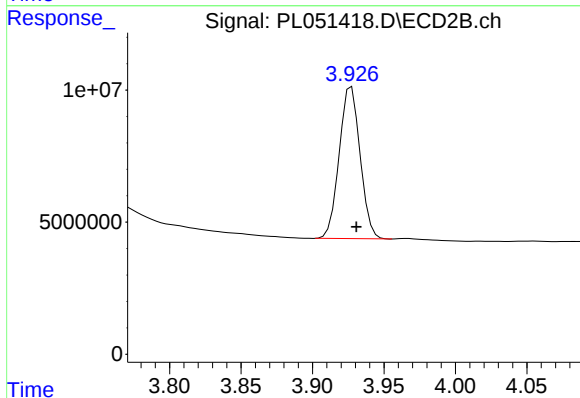


#1 Tetrachloro-m-xylene

R.T.: 3.927 min
Delta R.T.: -0.003 min
Response: 58562727
Conc: 20.53 ng/ml

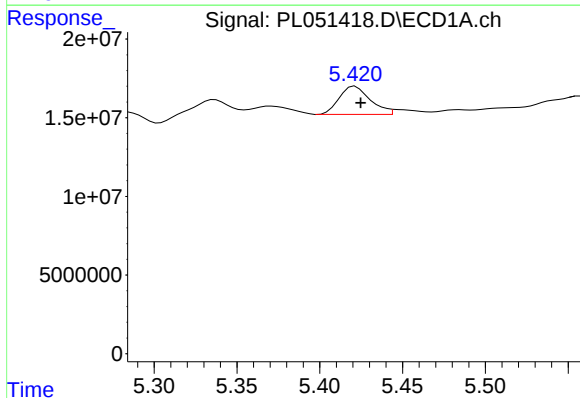


#12 4,4'-DDE

R.T.: 5.420 min
Delta R.T.: -0.005 min
Response: 23067027
Conc: 1.54 ng/ml m

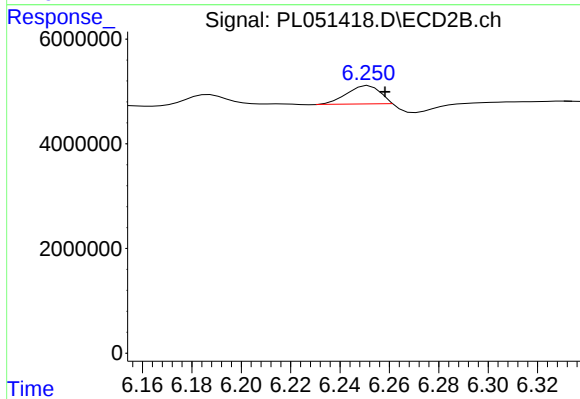

#12 4,4'-DDE

R.T.: 6.250 min
Delta R.T.: -0.008 min
Response: 3250964
Conc: 0.90 ng/ml m

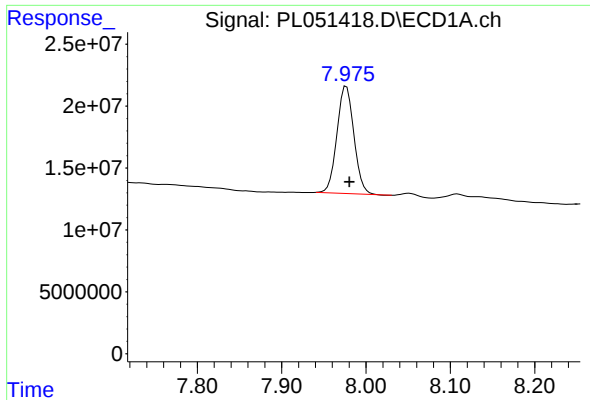


#28 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.004 min
Response: 121423243
Conc: 11.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-010-B225-080819

Manual Integrations
APPROVED

Ankita
8/14/2019 4:53:57 PM

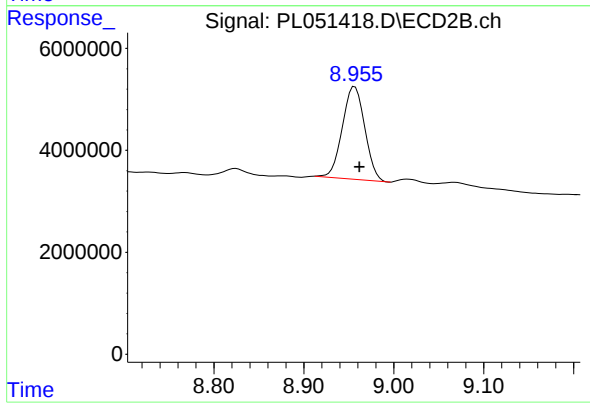

#28 Decachlorobiphenyl

R.T.: 8.957 min
Delta R.T.: -0.005 min
Response: 31570025
Conc: 11.16 ng/ml